

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048390.D
 Acq On : 01 Nov 2024 11:58
 Operator : RC/JU
 Sample : P4592-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H09

Quant Time: Nov 03 21:49:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4484	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.491	136	14709	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.349	164	8027	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.192	188	1119459	0.400	ng/ul	0.07
17) Chrysene-d12	21.292	240	10390	0.400	ng/ul	0.00
23) Perylene-d12	23.516	264	20215	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	24058	4.369	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.113	152	5814	0.311	ng/ul	-0.03
18) Fluoranthene-d10	19.123	212	14649	0.555	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.481	202	2166	0.056	ng/ul#	1
26) Benzo(a)pyrene	23.364	252	3999	0.062	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048390.D
Acq On : 01 Nov 2024 11:58
Operator : RC/JU
Sample : P4592-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H09

Quant Time: Nov 03 21:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

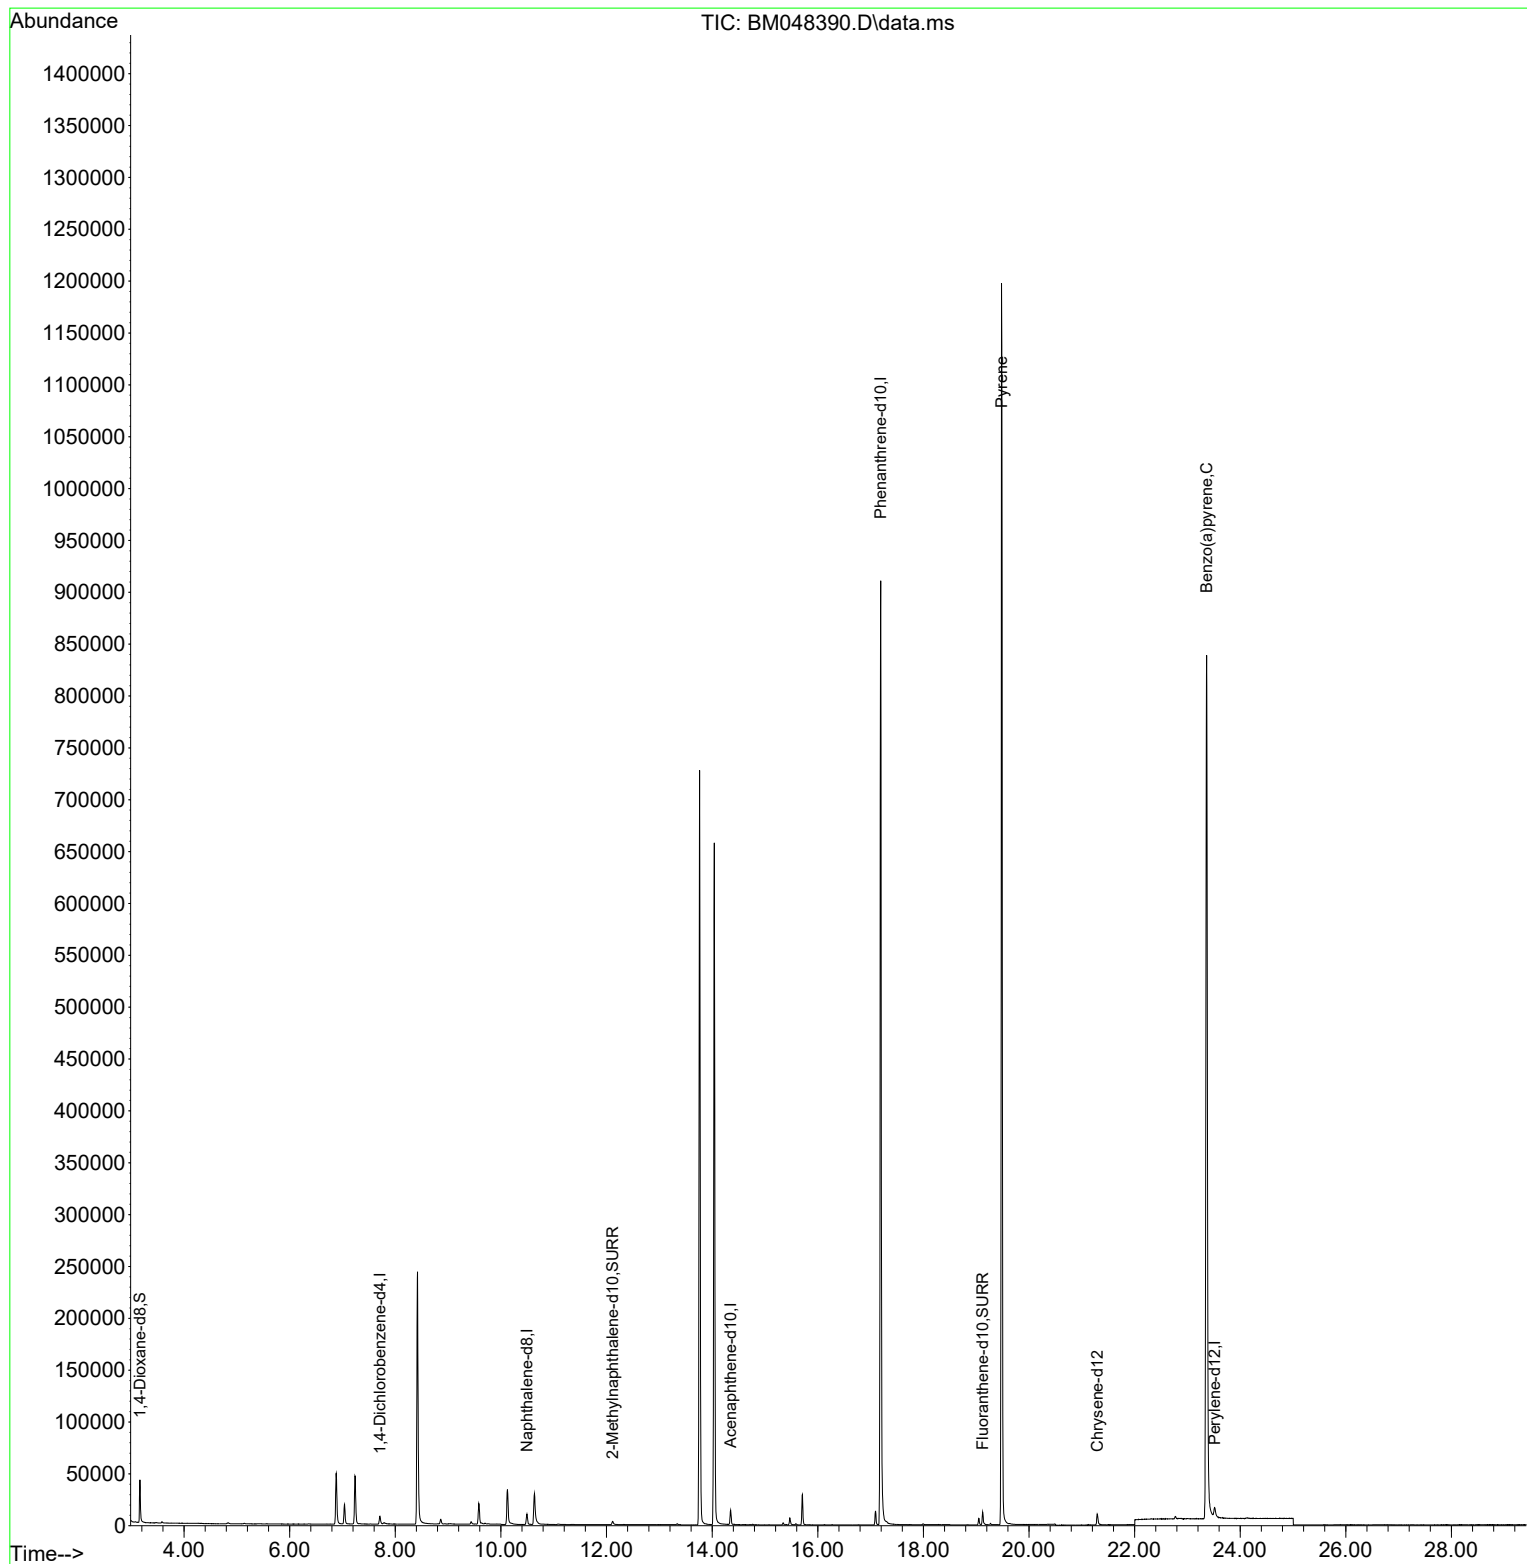

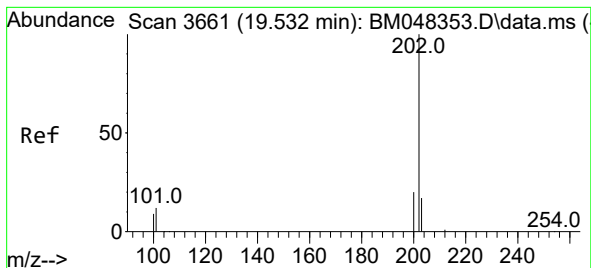

#20

Pyrene

Concen: 0.056 ng/ul

RT: 19.481 min Scan# 3

Delta R.T. -0.051 min

Lab File: BM048390.D

Acq: 01 Nov 2024 11:58

Instrument :

BNA_M

ClientSampleId :

F7H09





Tgt Ion:202 Resp: 2166

Ion Ratio Lower Upper

202 100

101 144.0 10.0 15.0#

100 1059.1 8.0 12.0#

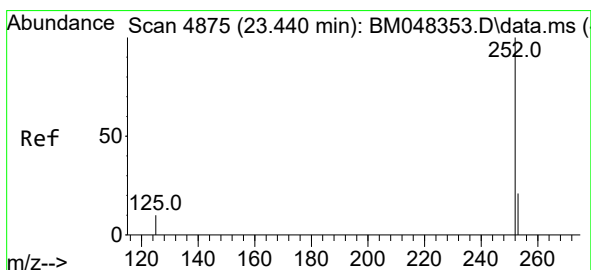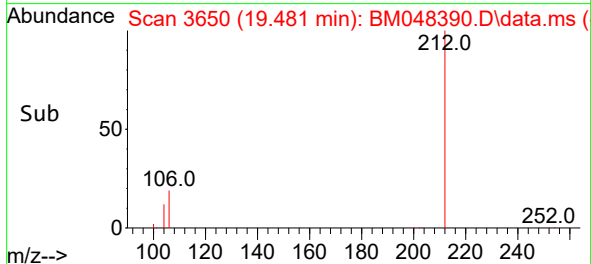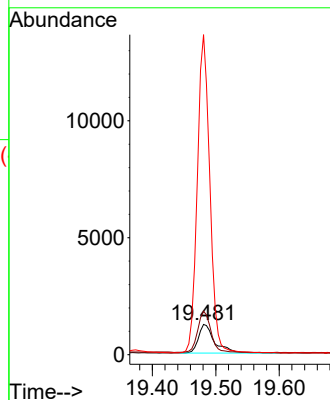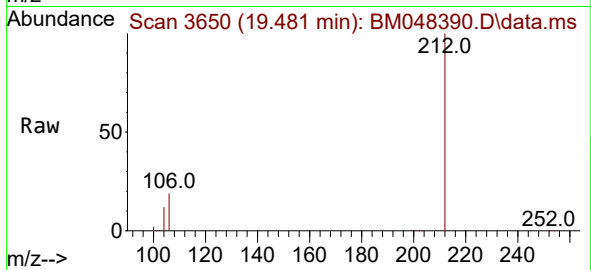

#26

Benzo(a)pyrene

Concen: 0.062 ng/ul

RT: 23.364 min Scan# 4849

Delta R.T. -0.076 min

Lab File: BM048390.D

Acq: 01 Nov 2024 11:58

Tgt Ion:252 Resp: 3999

Ion Ratio Lower Upper

252 100

253 49.3 27.7 41.5#

125 45.7 21.1 31.7#

