

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048395.D
 Acq On : 01 Nov 2024 15:00
 Operator : RC/JU
 Sample : P4534-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L67

Quant Time: Nov 03 21:49:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	3850	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.491	136	12538	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.350	164	6807	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.188	188	1214568	0.400	ng/ul	0.07
17) Chrysene-d12	21.298	240	9554	0.400	ng/ul	0.00
23) Perylene-d12	23.513	264	18047	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	24097	5.096	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.119	152	5816	0.365	ng/ul	-0.02
18) Fluoranthene-d10	19.123	212	15330	0.632	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.486	202	2020	0.057	ng/ul#	1
26) Benzo(a)pyrene	23.358	252	4441	0.077	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048395.D
Acq On : 01 Nov 2024 15:00
Operator : RC/JU
Sample : P4534-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L67

Quant Time: Nov 03 21:49:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

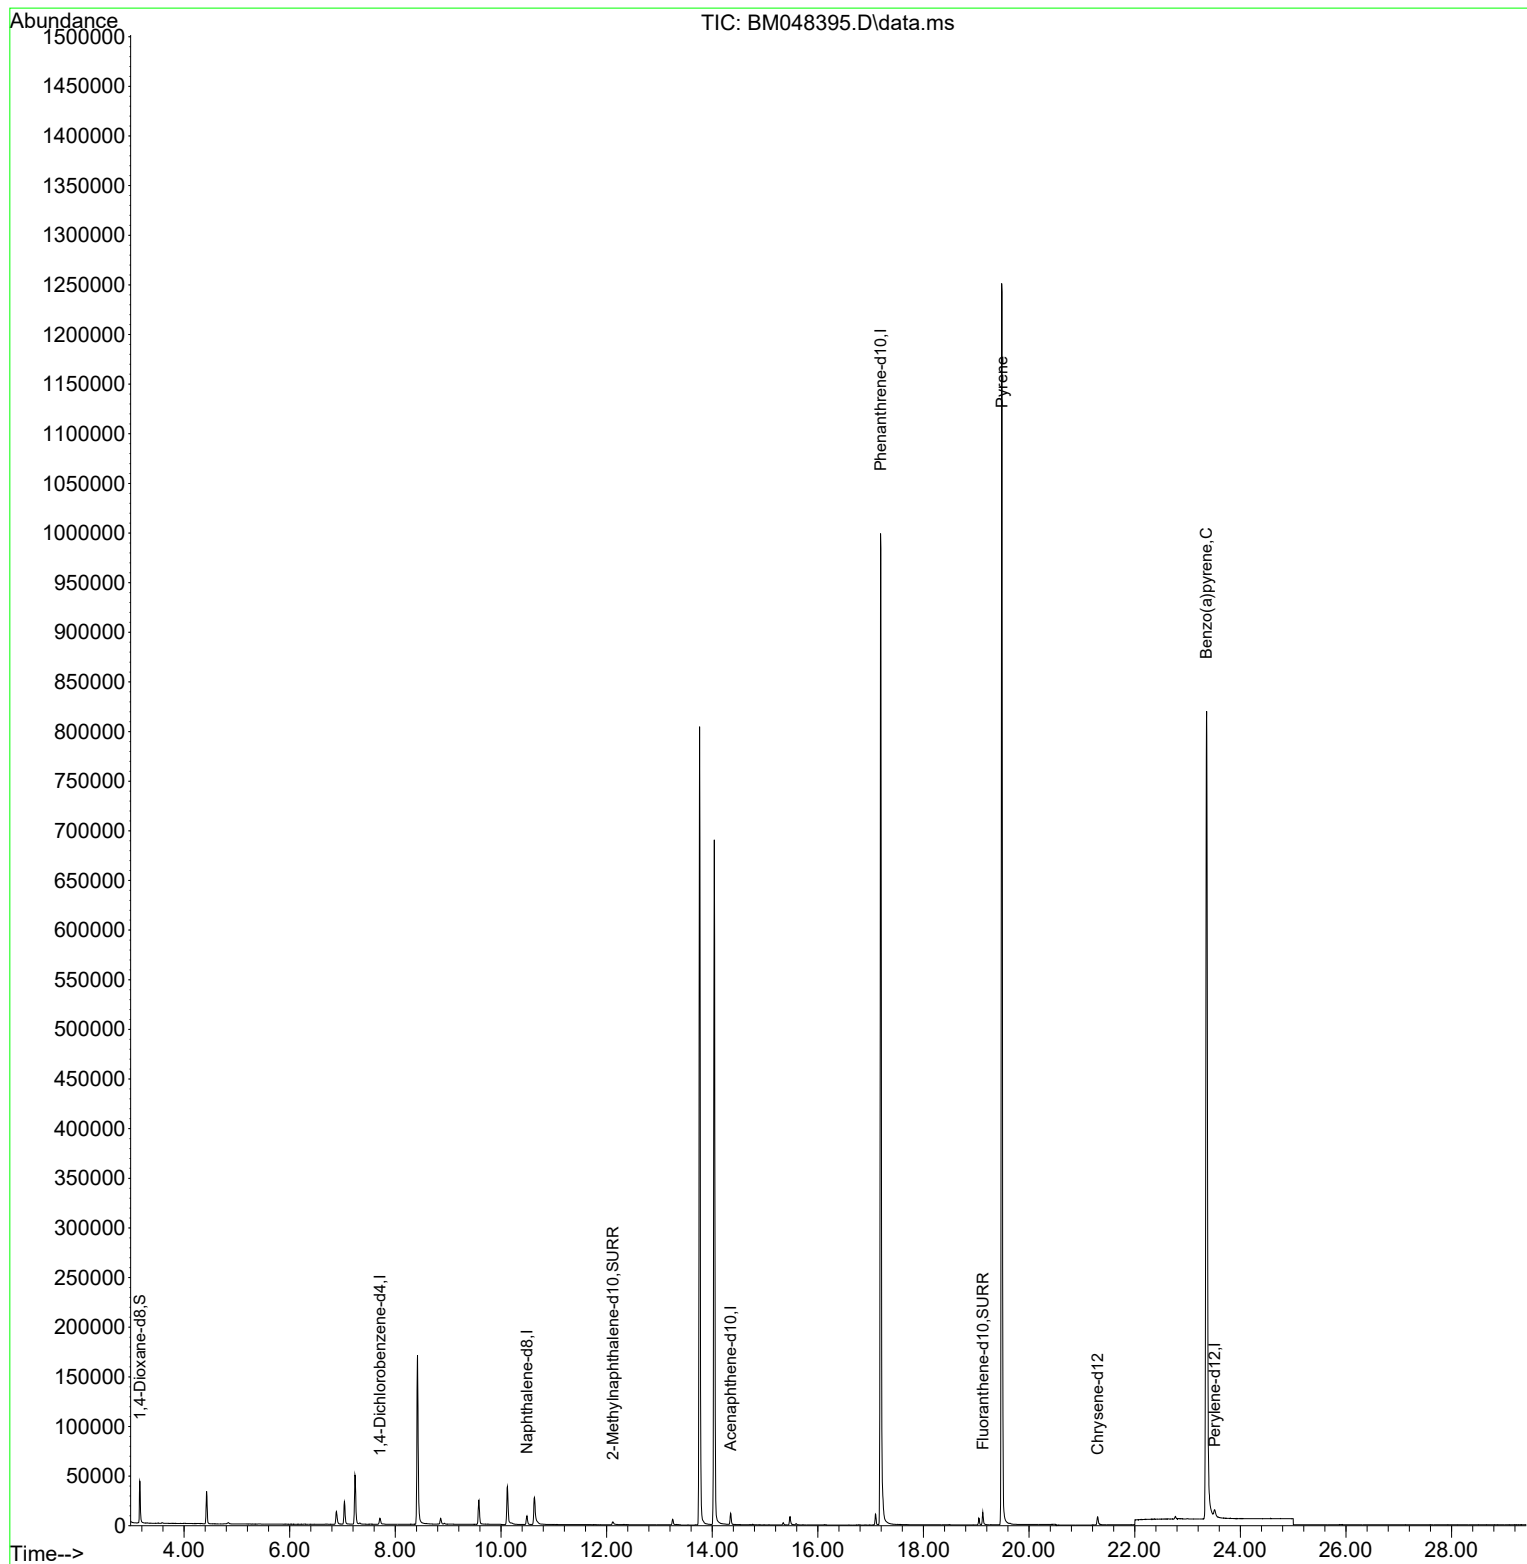

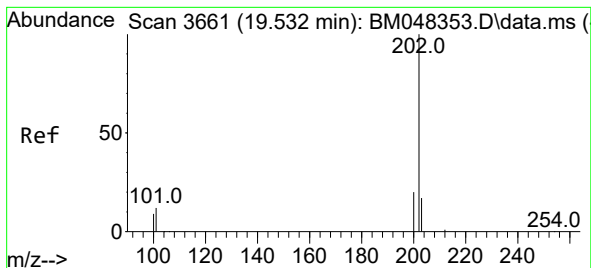

#20

Pyrene

Concen: 0.057 ng/ul

RT: 19.486 min Scan# 3

Delta R.T. -0.046 min

Lab File: BM048395.D

Acq: 01 Nov 2024 15:00

Instrument :

BNA_M

ClientSampleId :

E1L67





Tgt Ion:202 Resp: 2020

Ion Ratio Lower Upper

202 100

101 130.4 10.0 15.0#

100 912.3 8.0 12.0#

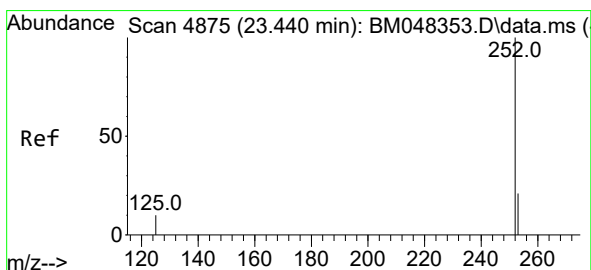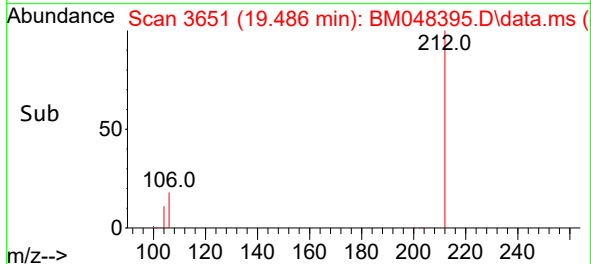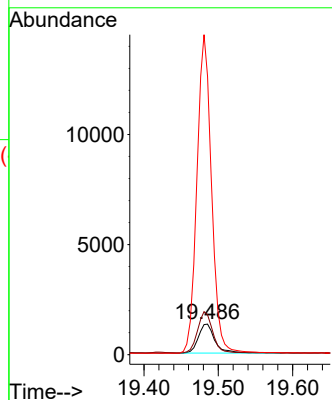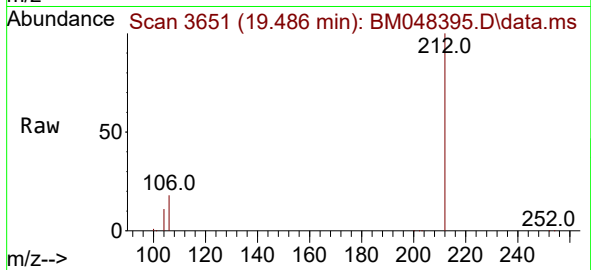

#26

Benzo(a)pyrene

Concen: 0.077 ng/ul

RT: 23.358 min Scan# 4847

Delta R.T. -0.082 min

Lab File: BM048395.D

Acq: 01 Nov 2024 15:00

Tgt Ion:252 Resp: 4441

Ion Ratio Lower Upper

252 100

253 50.4 27.7 41.5#

125 53.1 21.1 31.7#

