

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048396.D
 Acq On : 01 Nov 2024 15:37
 Operator : RC/JU
 Sample : P4534-07
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L78

Quant Time: Nov 03 21:49:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	3763	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.490	136	12224	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.348	164	6579	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.191	188	1263898	0.400	ng/ul	0.07
17) Chrysene-d12	21.295	240	8780	0.400	ng/ul	0.00
23) Perylene-d12	23.513	264	17500	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	23484	5.081	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	5586	0.359	ng/ul	-0.02
18) Fluoranthene-d10	19.122	212	16247	0.729	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.484	202	2156	0.066	ng/ul#	1
26) Benzo(a)pyrene	23.359	252	4707	0.084	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048396.D
Acq On : 01 Nov 2024 15:37
Operator : RC/JU
Sample : P4534-07
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L78

Quant Time: Nov 03 21:49:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

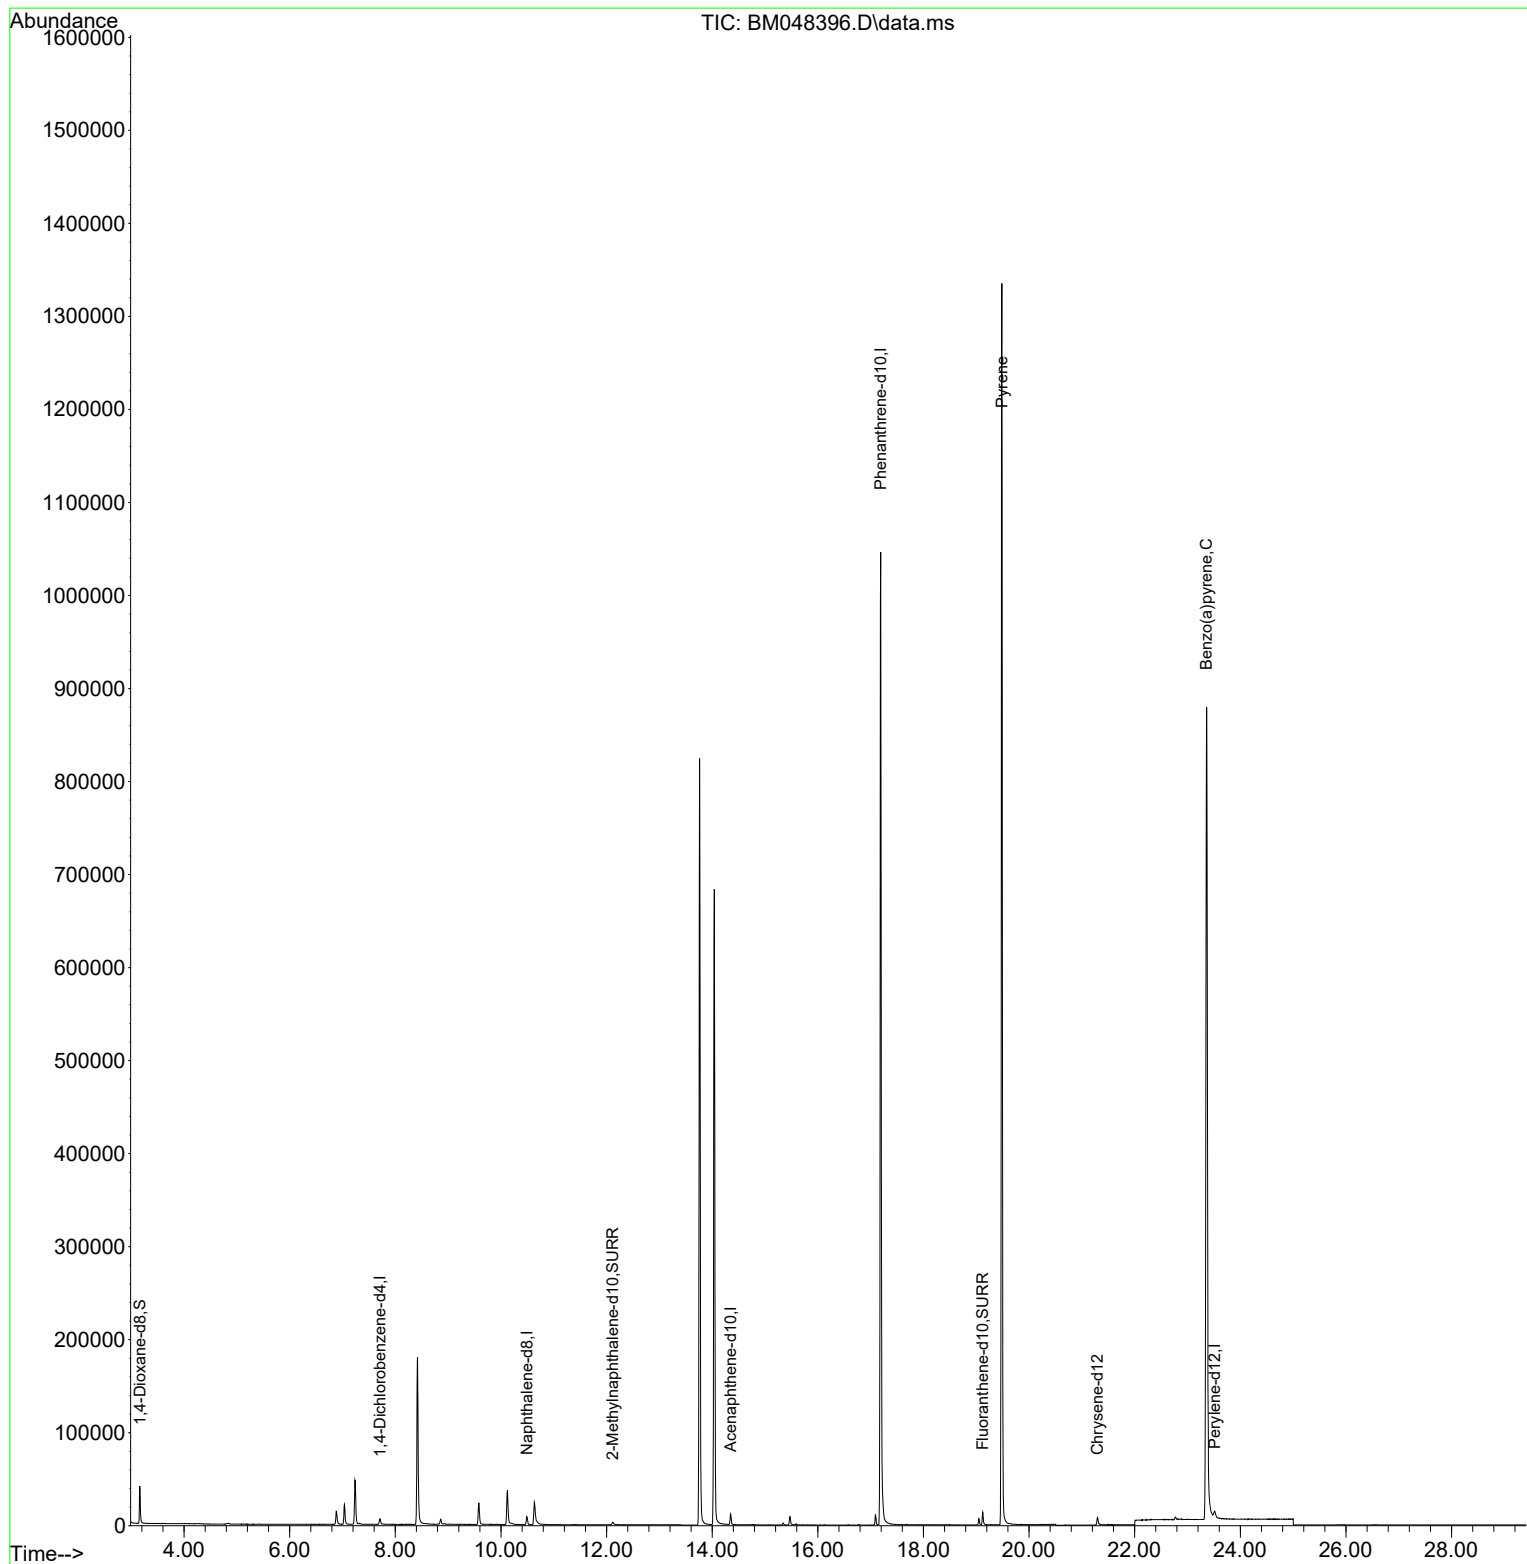

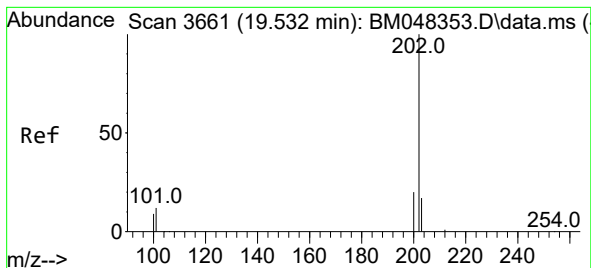

#20

Pyrene

Concen: 0.066 ng/ul

RT: 19.484 min Scan# 3

Delta R.T. -0.048 min

Lab File: BM048396.D

Acq: 01 Nov 2024 15:37

Instrument :

BNA_M

ClientSampleId :

E1L78





Tgt Ion:202 Resp: 2156

Ion Ratio Lower Upper

202 100

101 137.3 10.0 15.0#

100 959.0 8.0 12.0#

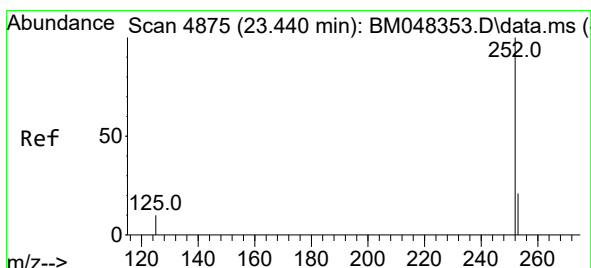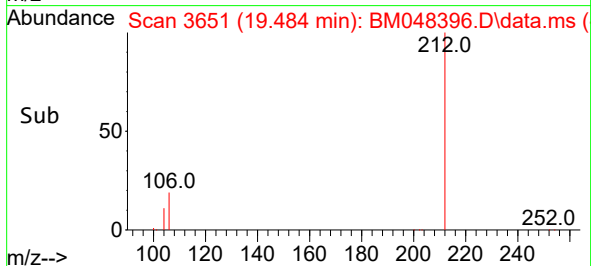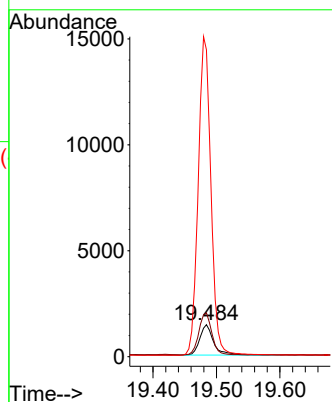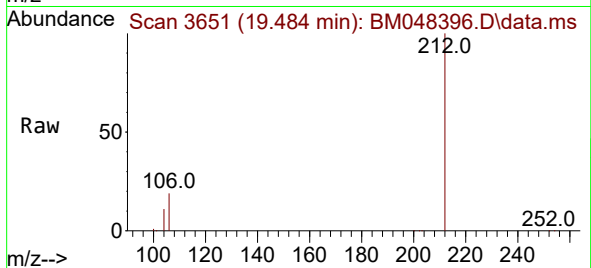

#26

Benzo(a)pyrene

Concen: 0.084 ng/ul

RT: 23.359 min Scan# 4847

Delta R.T. -0.081 min

Lab File: BM048396.D

Acq: 01 Nov 2024 15:37

Tgt Ion:252 Resp: 4707

Ion Ratio Lower Upper

252 100

253 48.4 27.7 41.5#

125 46.8 21.1 31.7#

