

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048398.D
 Acq On : 01 Nov 2024 16:50
 Operator : RC/JU
 Sample : P4534-08
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L98

Quant Time: Nov 03 21:50:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	3981	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.490	136	12921	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.348	164	6951	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.191	188	1320088	0.400	ng/ul	0.07
17) Chrysene-d12	21.301	240	9653	0.400	ng/ul	0.00
23) Perylene-d12	23.514	264	17316	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	24362	4.983	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	5968	0.363	ng/ul	-0.02
18) Fluoranthene-d10	19.122	212	16338	0.667	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.484	202	2164	0.061	ng/ul#	1
26) Benzo(a)pyrene	23.361	252	4605	0.083	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048398.D
Acq On : 01 Nov 2024 16:50
Operator : RC/JU
Sample : P4534-08
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L98

Quant Time: Nov 03 21:50:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

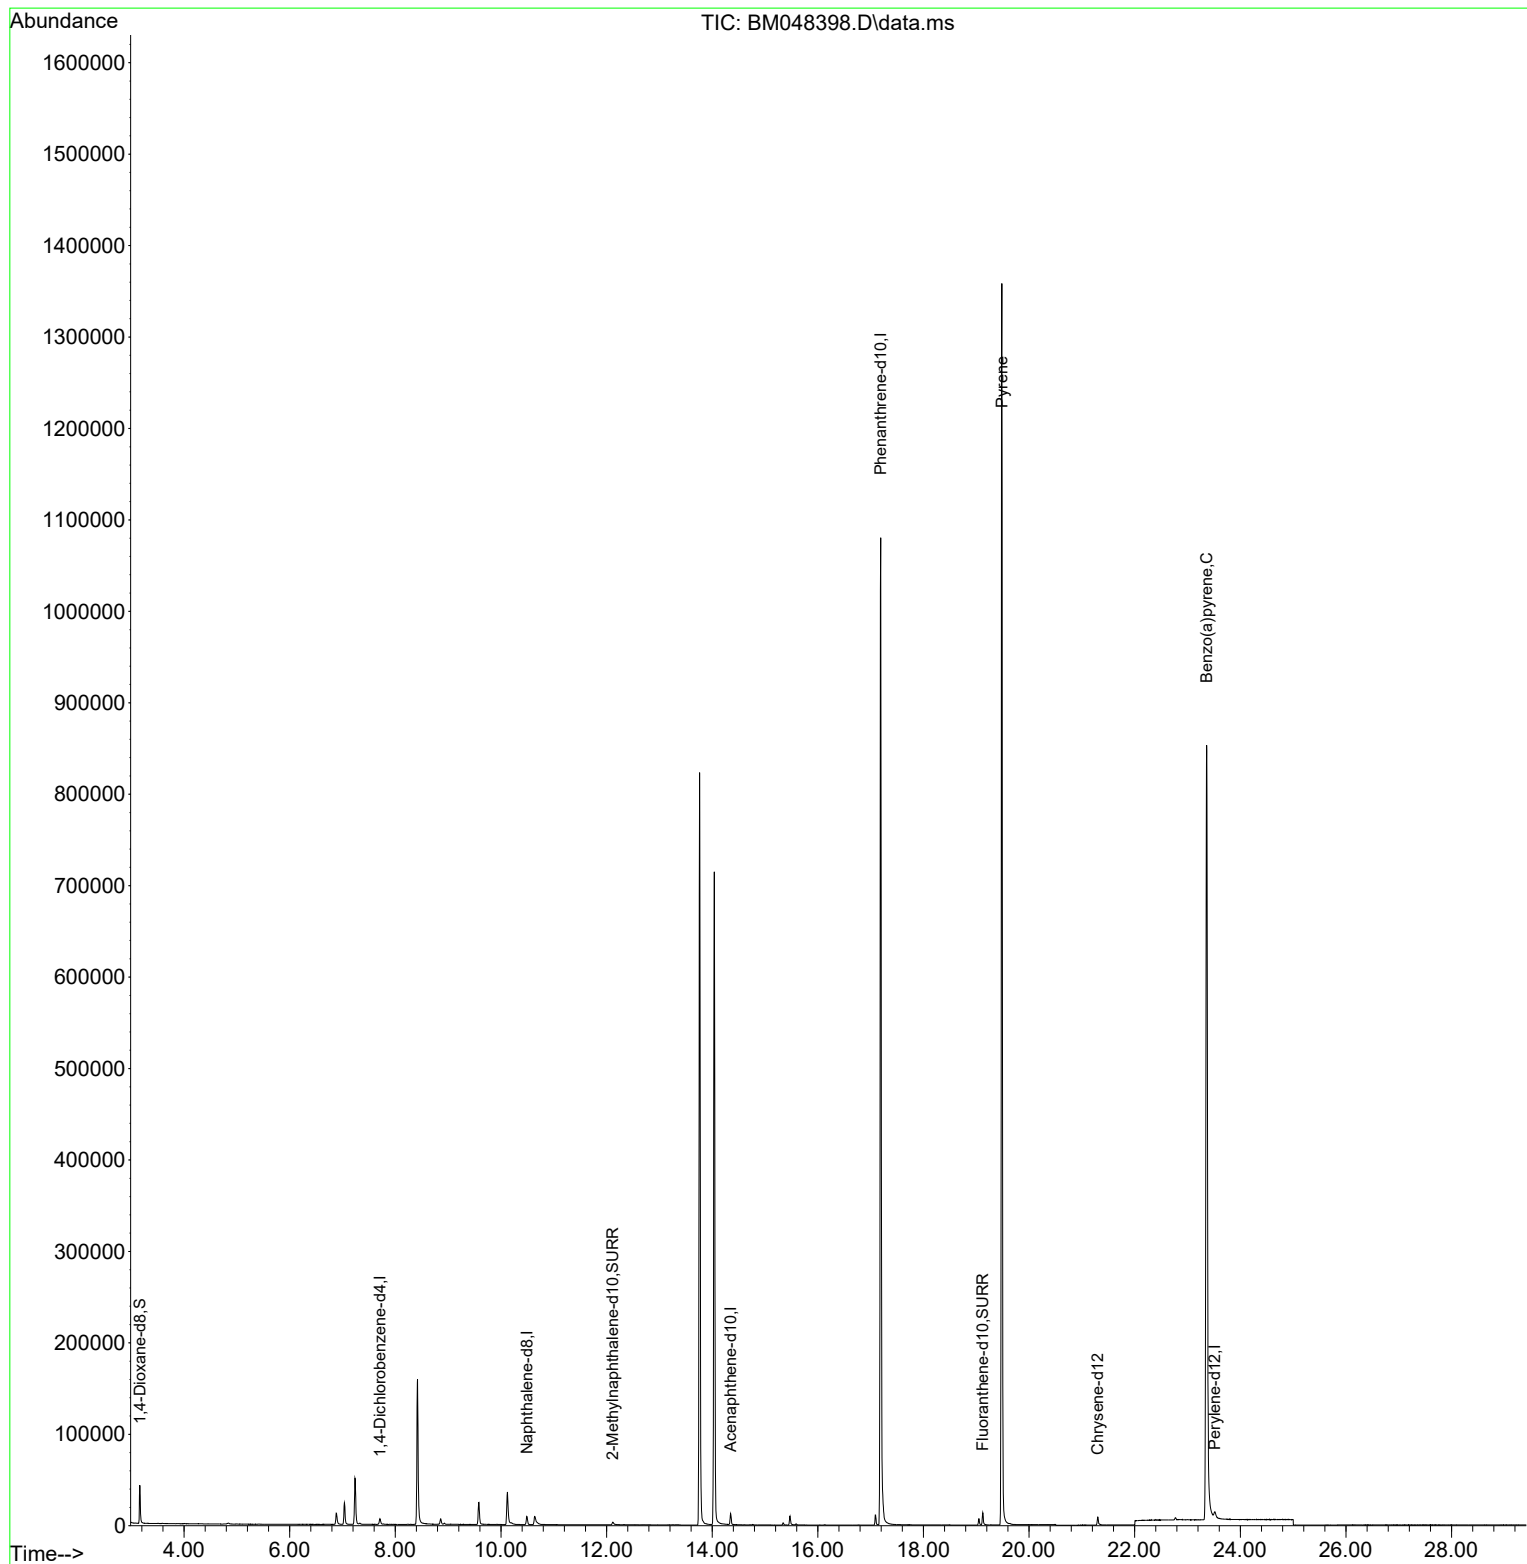

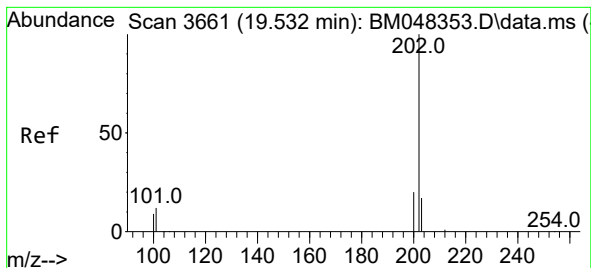

#20

Pyrene

Concen: 0.061 ng/ul

RT: 19.484 min Scan# 3

Delta R.T. -0.048 min

Lab File: BM048398.D

Acq: 01 Nov 2024 16:50

Instrument :

BNA_M

ClientSampleId :

E1L98





Tgt Ion:202 Resp: 2164

Ion Ratio Lower Upper

202 100

101 137.6 10.0 15.0#

100 959.4 8.0 12.0#

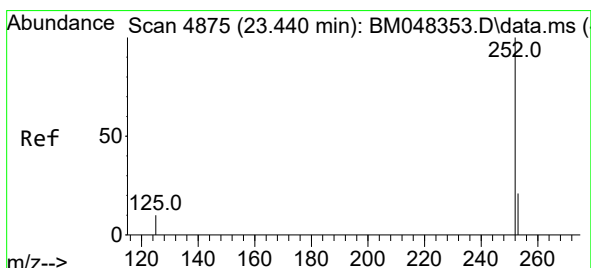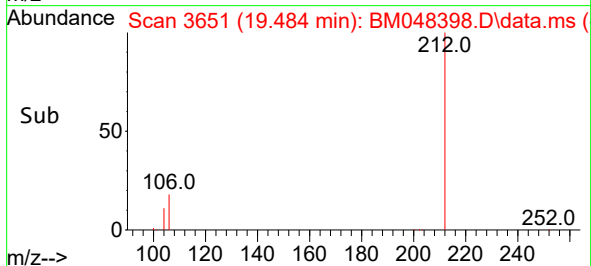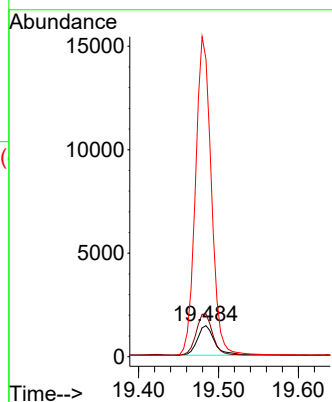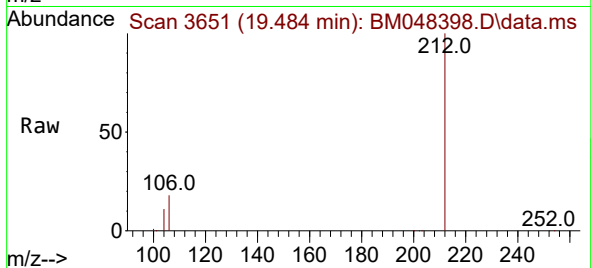

#26

Benzo(a)pyrene

Concen: 0.083 ng/ul

RT: 23.361 min Scan# 4848

Delta R.T. -0.078 min

Lab File: BM048398.D

Acq: 01 Nov 2024 16:50

Tgt Ion:252 Resp: 4605

Ion Ratio Lower Upper

252 100

253 47.7 27.7 41.5#

125 45.1 21.1 31.7#

