

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048402.D
 Acq On : 01 Nov 2024 19:52
 Operator : RC/JU
 Sample : PB164517BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK517

Quant Time: Nov 03 21:50:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4629	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.490	136	14688	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.348	164	7837	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.191	188	1049985	0.400	ng/ul	0.07
17) Chrysene-d12	21.304	240	11622	0.400	ng/ul	0.01
23) Perylene-d12	23.516	264	20979	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	30756	5.410	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	5878	0.315	ng/ul	-0.02
18) Fluoranthene-d10	19.122	212	12462	0.422	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.484	202	1687	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.364	252	3477	0.052	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048402.D
Acq On : 01 Nov 2024 19:52
Operator : RC/JU
Sample : PB164517BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK517

Quant Time: Nov 03 21:50:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

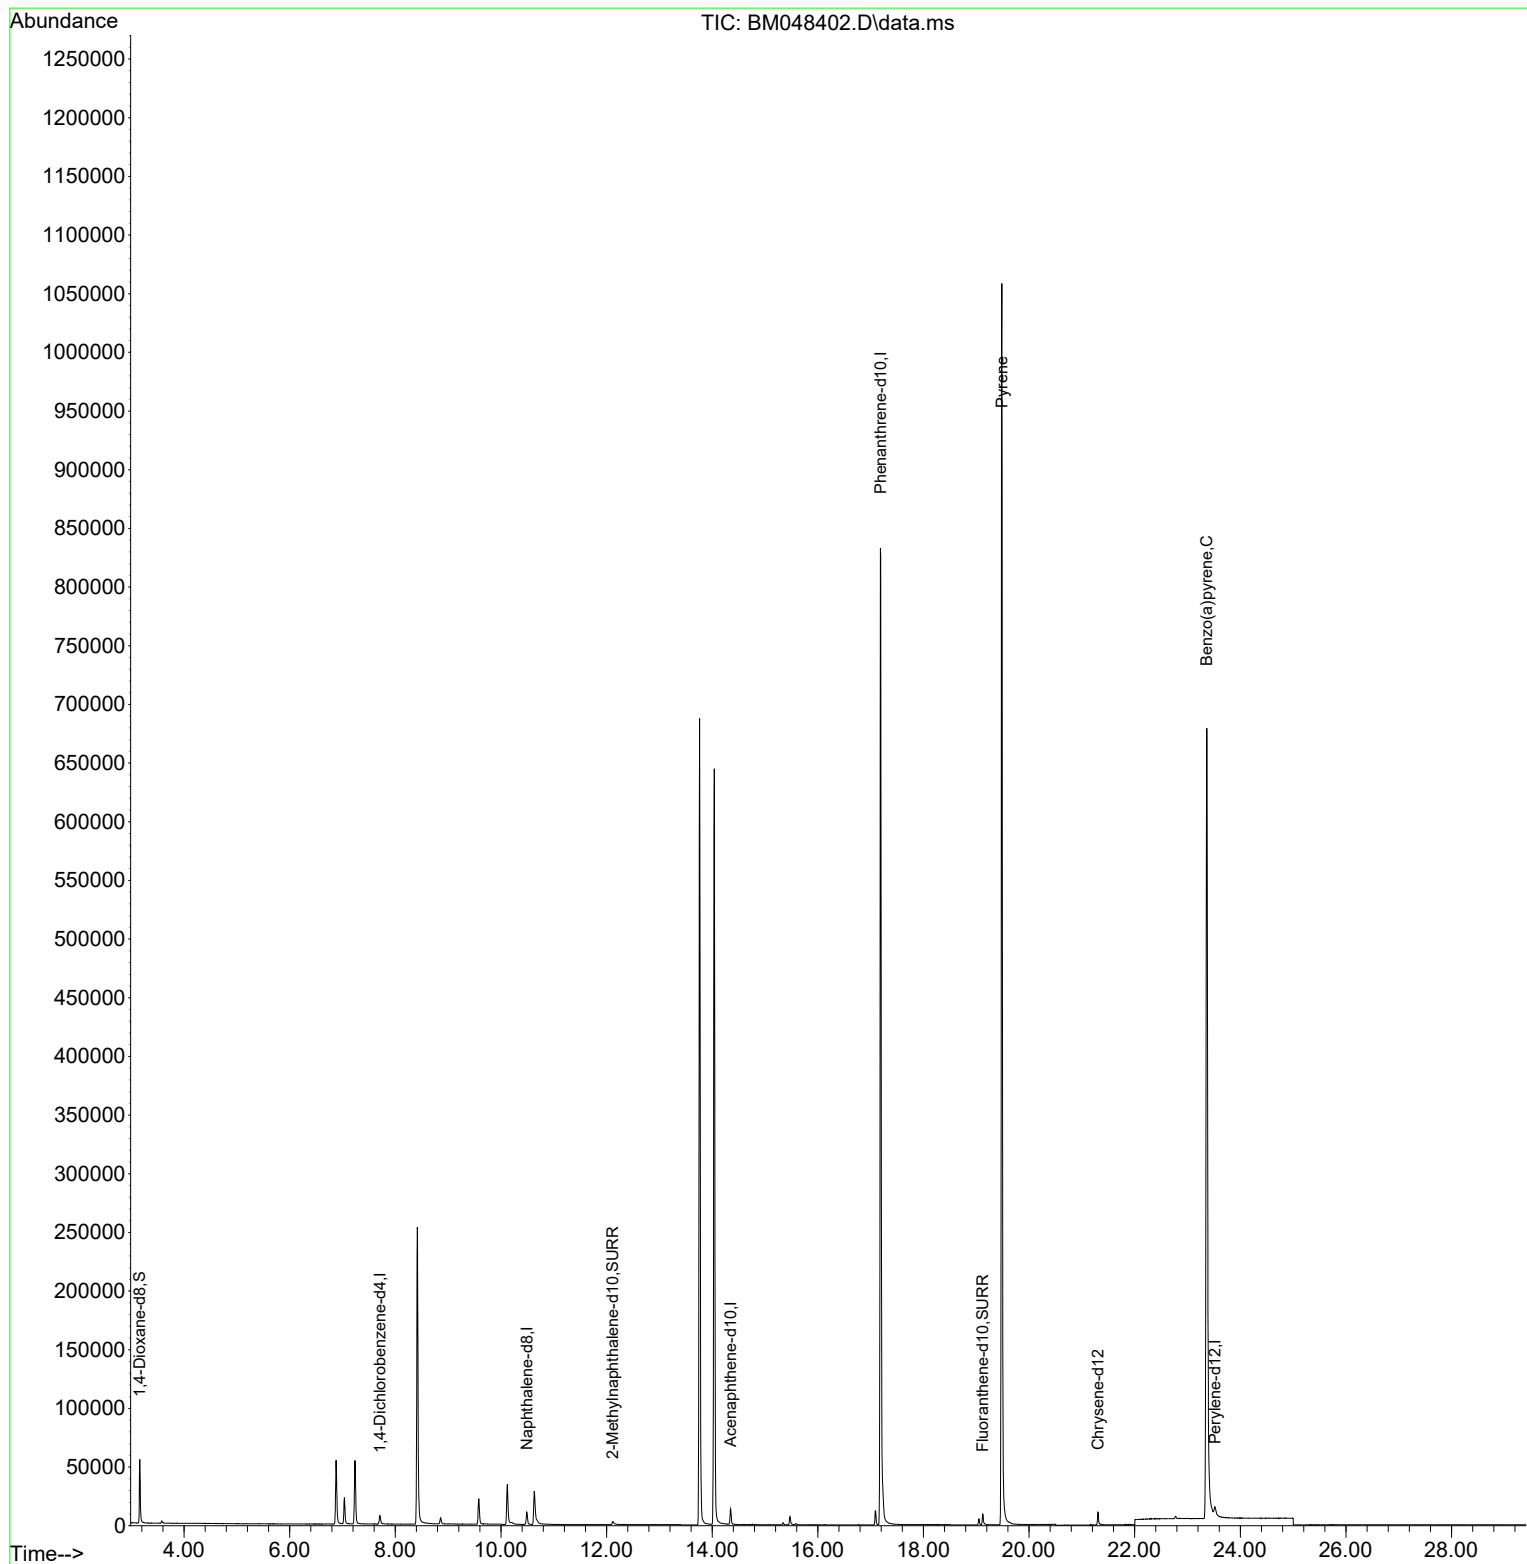

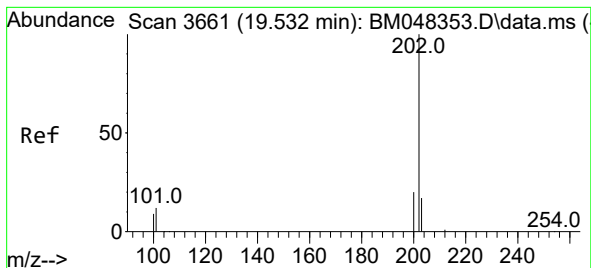

#20

Pyrene

Concen: 0.039 ng/ul

RT: 19.484 min Scan# 3

Delta R.T. -0.048 min

Lab File: BM048402.D

Acq: 01 Nov 2024 19:52

Instrument :

BNA_M

ClientSampleId :

SBLK517





Tgt Ion:202 Resp: 1687

Ion Ratio Lower Upper

202 100

101 139.4 10.0 15.0#

100 979.8 8.0 12.0#

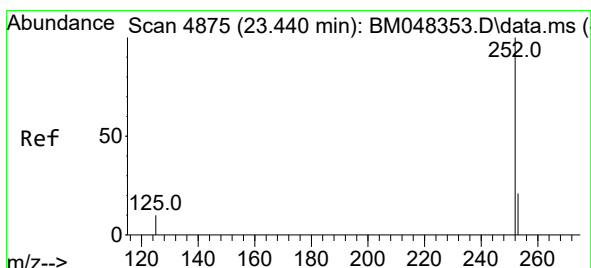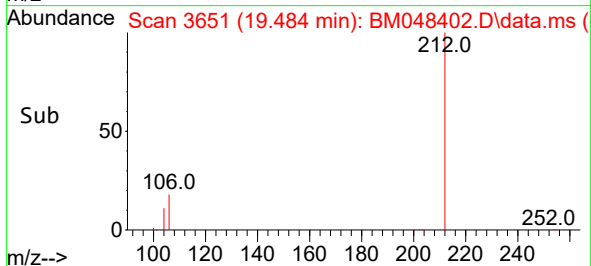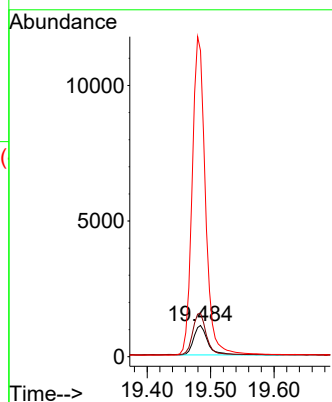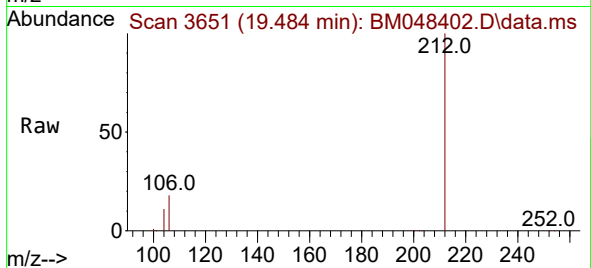

#26

Benzo(a)pyrene

Concen: 0.052 ng/ul

RT: 23.364 min Scan# 4849

Delta R.T. -0.076 min

Lab File: BM048402.D

Acq: 01 Nov 2024 19:52

Tgt Ion:252 Resp: 3477

Ion Ratio Lower Upper

252 100

253 53.7 27.7 41.5#

125 49.6 21.1 31.7#

