

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048403.D
 Acq On : 01 Nov 2024 20:28
 Operator : RC/JU
 Sample : PB164490BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK490

Quant Time: Nov 03 21:50:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4574	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.491	136	14563	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.349	164	7798	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.188	188	1099480	0.400	ng/ul	0.07
17) Chrysene-d12	21.306	240	10437	0.400	ng/ul	0.01
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.53
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	32413	5.770	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.119	152	6311	0.341	ng/ul	-0.02
18) Fluoranthene-d10	19.123	212	12748	0.481	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.485	202	1724	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048403.D
Acq On : 01 Nov 2024 20:28
Operator : RC/JU
Sample : PB164490BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK490

Quant Time: Nov 03 21:50:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

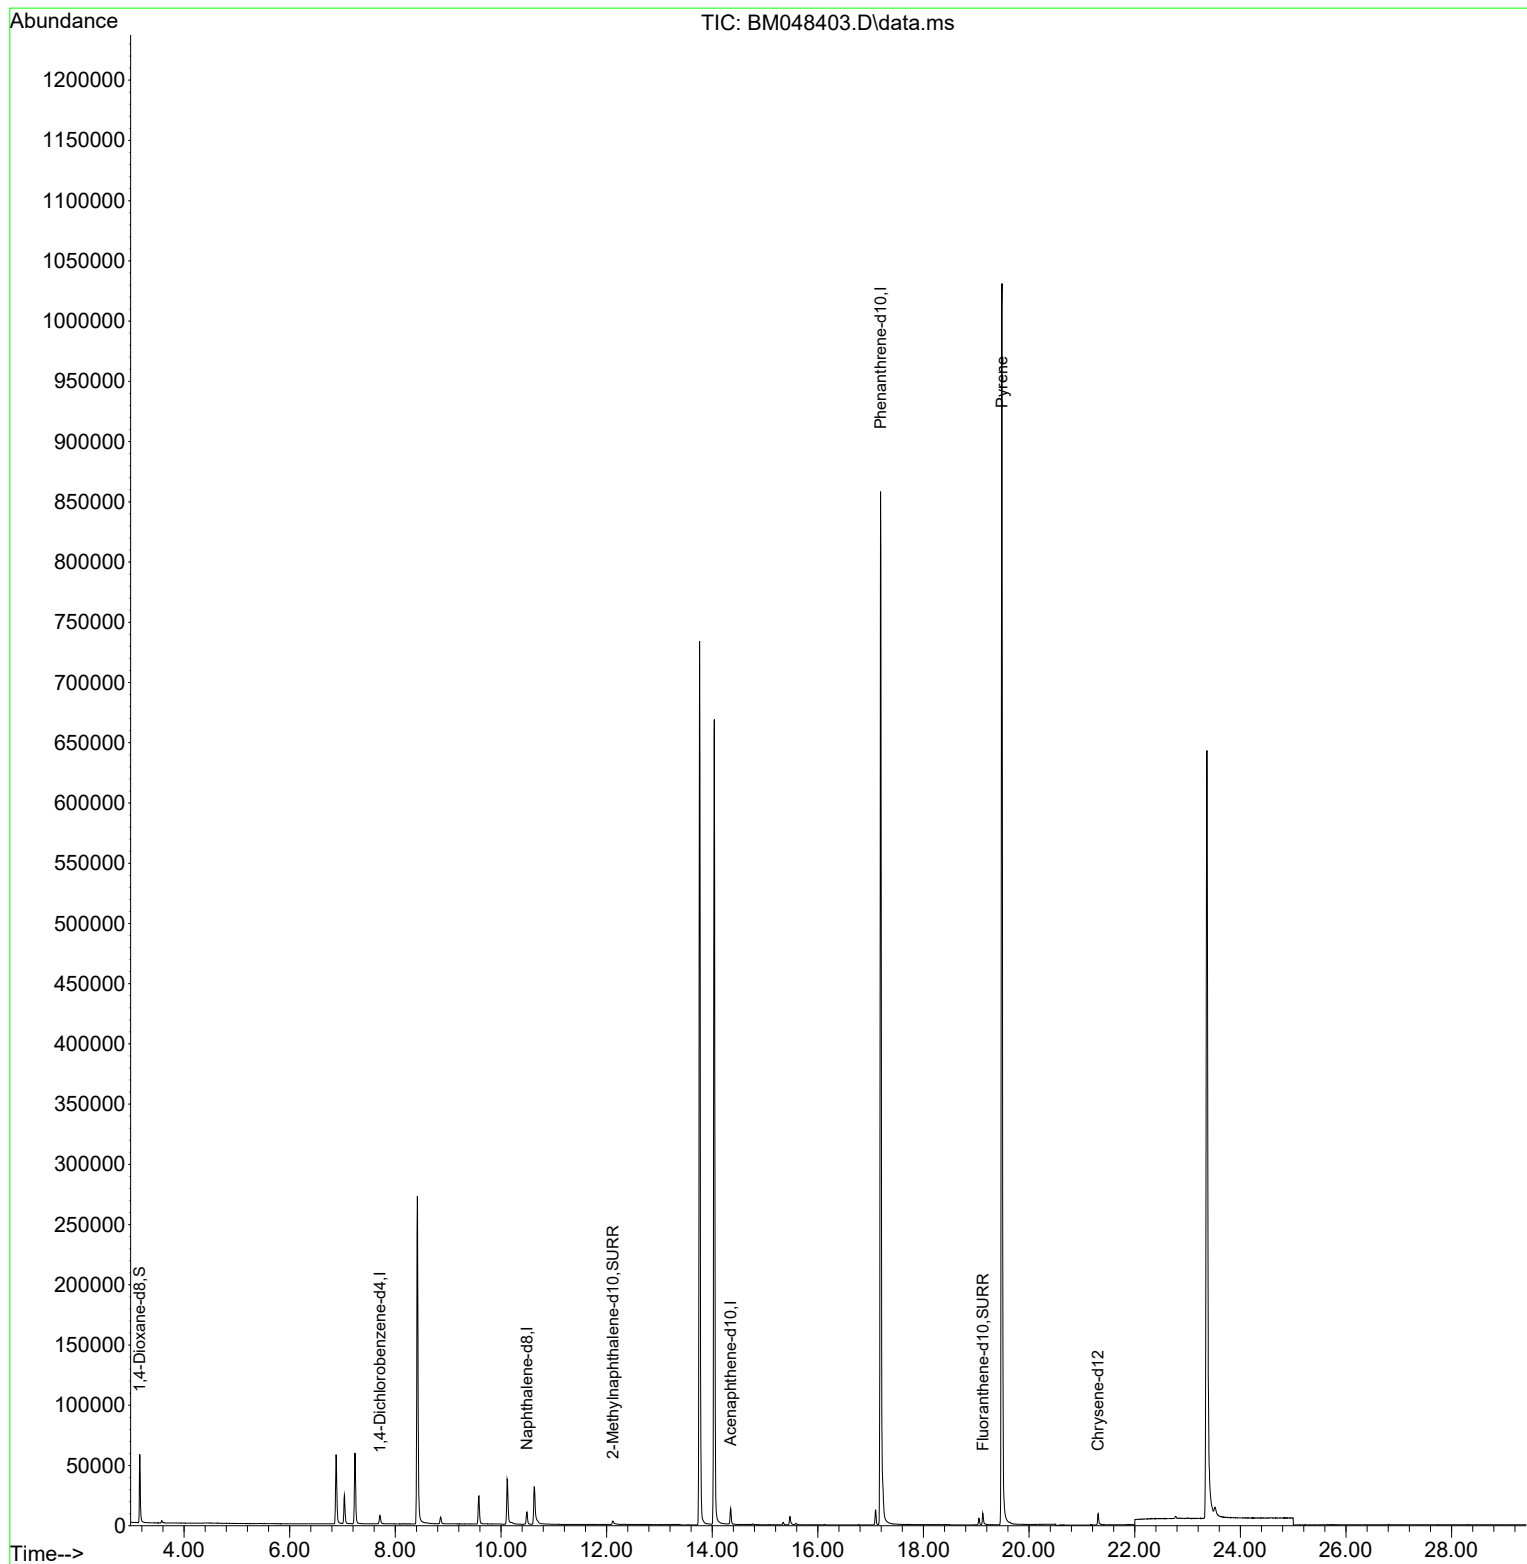

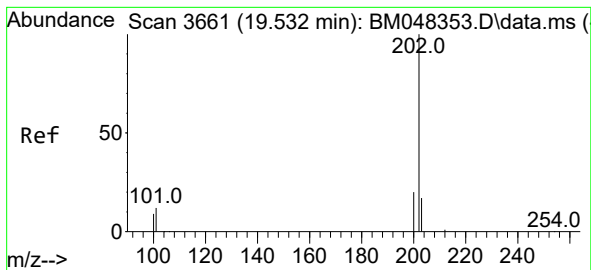

#20

Pyrene

Concen: 0.045 ng/ul

RT: 19.485 min Scan# 30

Delta R.T. -0.047 min

Lab File: BM048403.D


Acq: 01 Nov 2024 20:28

Instrument :

BNA_M

ClientSampleId :

SBLK490

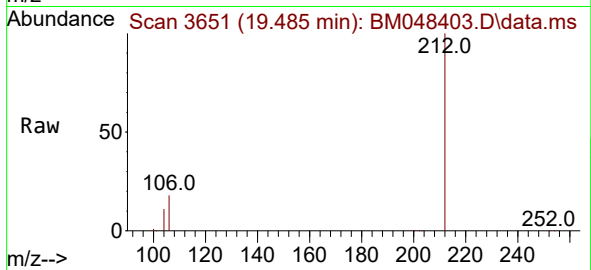

Tgt Ion:202 Resp: 1724

Ion Ratio Lower Upper

202 100

101 135.2 10.0 15.0#

100 937.1 8.0 12.0#

