

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048408.D
 Acq On : 01 Nov 2024 23:31
 Operator : RC/JU
 Sample : P4558-03
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L81

Quant Time: Nov 03 21:51:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4622	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.490	136	15519	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.348	164	8526	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.186	188	1406791	0.400	ng/ul	0.07
17) Chrysene-d12	21.295	240	13553	0.400	ng/ul	0.00
23) Perylene-d12	23.514	264	25711	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	23625	4.162	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	6440	0.326	ng/ul	-0.02
18) Fluoranthene-d10	19.122	212	18123	0.527	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.480	202	2388	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.359	252	5485	0.066	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048408.D
Acq On : 01 Nov 2024 23:31
Operator : RC/JU
Sample : P4558-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L81

Quant Time: Nov 03 21:51:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration




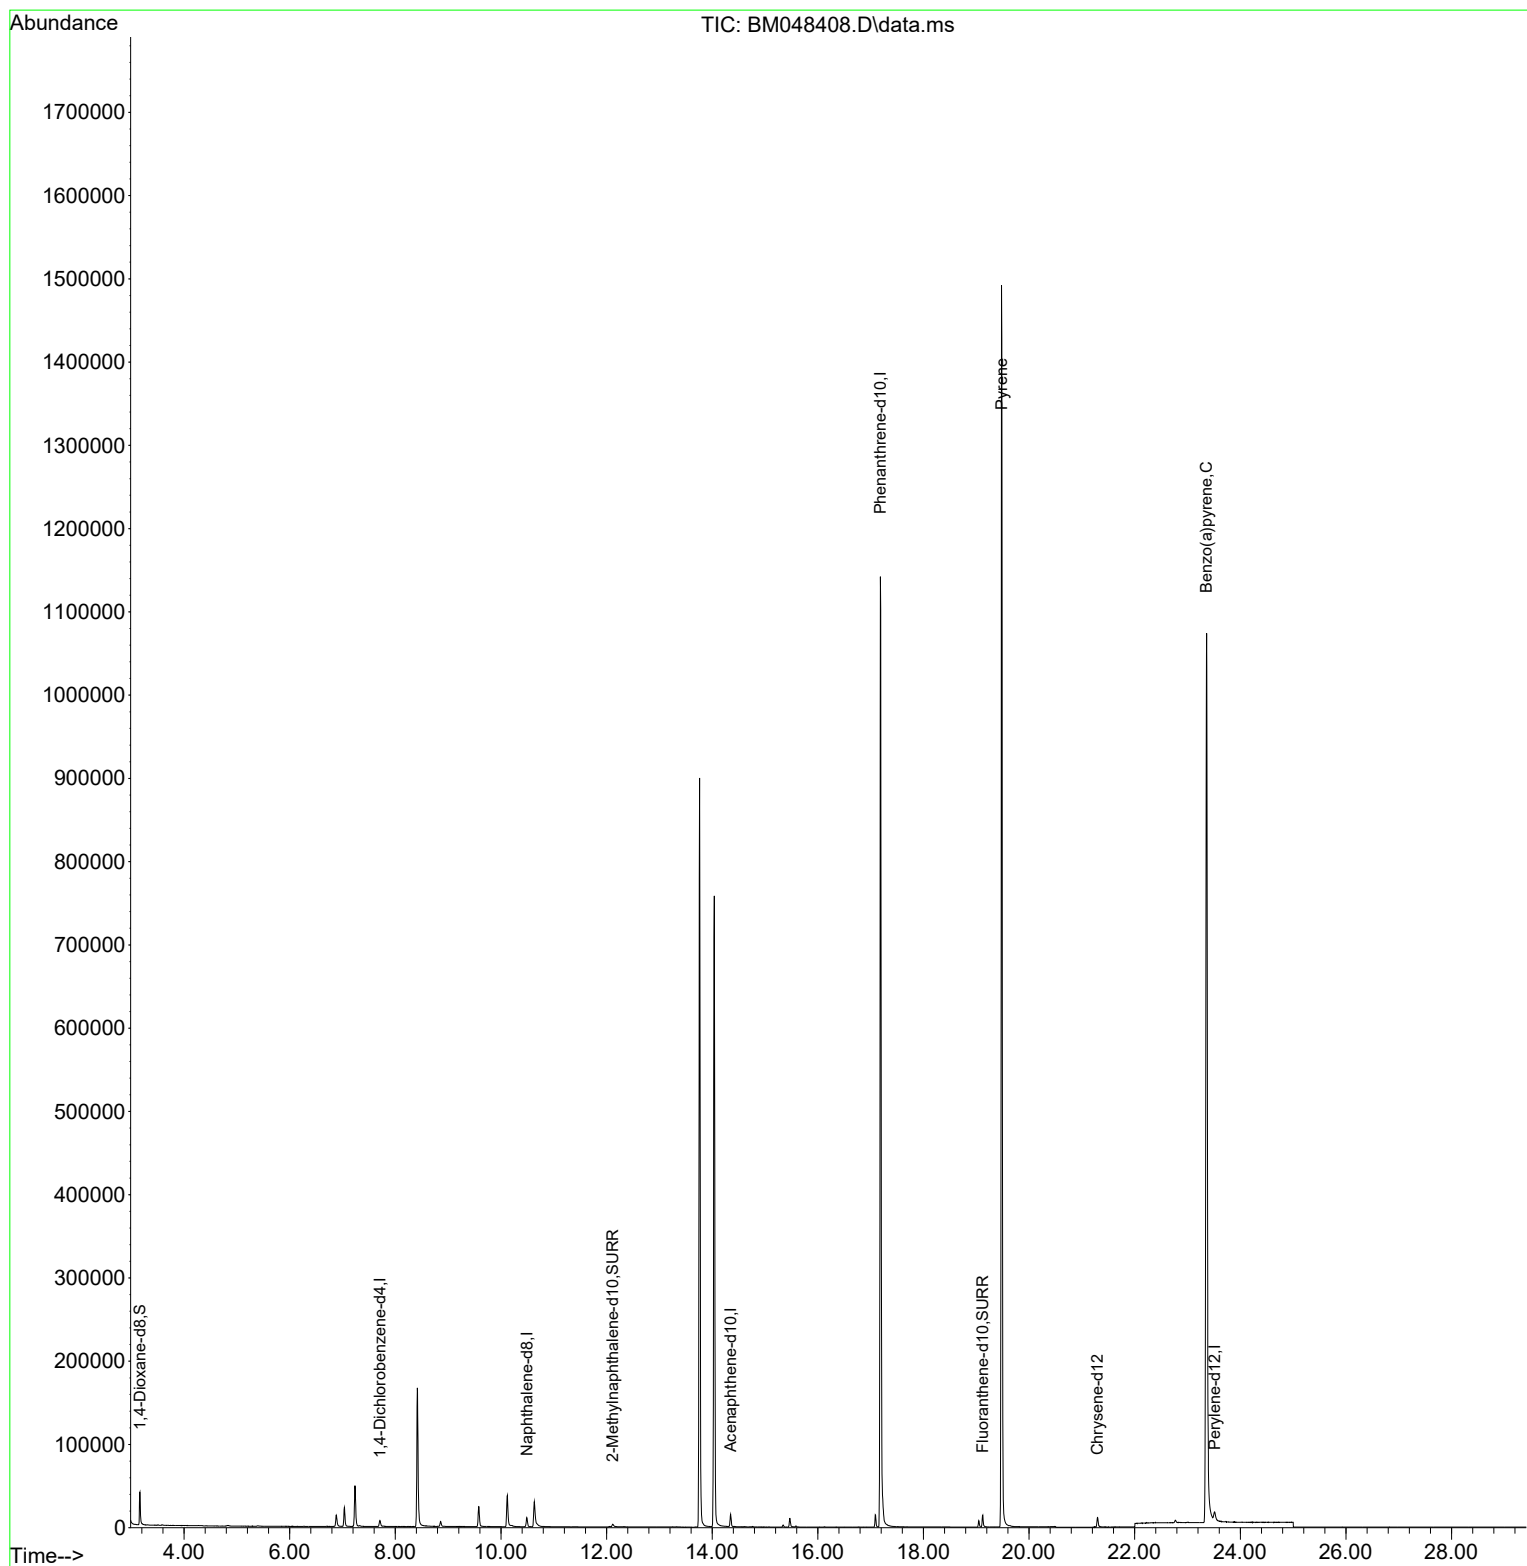


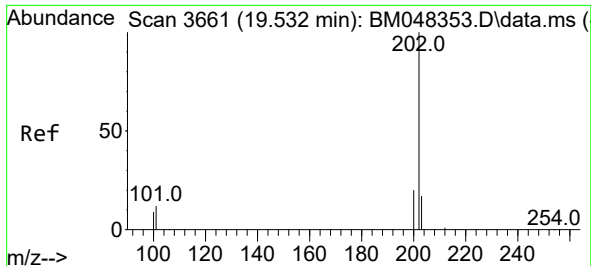

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.480 min Scan# 30
Delta R.T. -0.052 min
Lab File: BM048408.D
Acq: 01 Nov 2024 23:31

Instrument :
BNA_M
ClientSampleId :
E1L81

Tgt Ion:202 Resp: 2388
Ion Ratio Lower Upper
202 100
101 144.8 10.0 15.0#
100 1085.5 8.0 12.0#

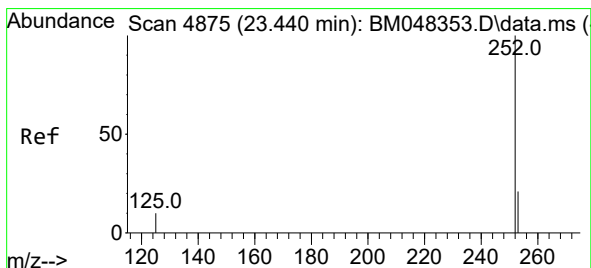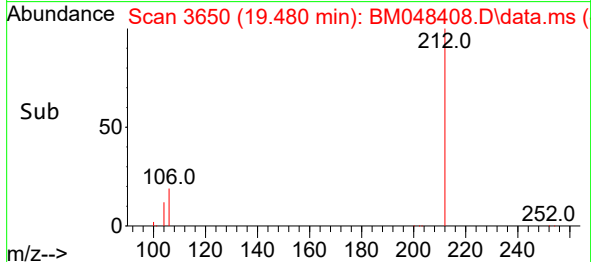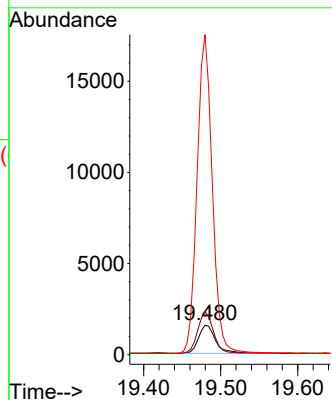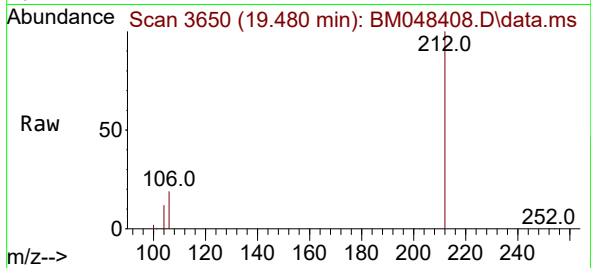

#26
Benzo(a)pyrene
Concen: 0.066 ng/ul
RT: 23.359 min Scan# 4847
Delta R.T. -0.081 min
Lab File: BM048408.D
Acq: 01 Nov 2024 23:31

Tgt Ion:252 Resp: 5485
Ion Ratio Lower Upper
252 100
253 44.0 27.7 41.5#
125 40.2 21.1 31.7#

