

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048410.D
 Acq On : 02 Nov 2024 00:44
 Operator : RC/JU
 Sample : P4558-05
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L89

Quant Time: Nov 03 21:51:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	5043	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.490	136	16177	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.348	164	8315	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.186	188	1415357	0.400	ng/ul	0.07
17) Chrysene-d12	21.295	240	11503	0.400	ng/ul	0.00
23) Perylene-d12	23.511	264	22324	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	29378	4.743	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	7931	0.385	ng/ul	-0.02
18) Fluoranthene-d10	19.122	212	18020	0.617	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.480	202	2375	0.056	ng/ul#	1
26) Benzo(a)pyrene	23.359	252	5381	0.075	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048410.D
Acq On : 02 Nov 2024 00:44
Operator : RC/JU
Sample : P4558-05
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L89

Quant Time: Nov 03 21:51:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

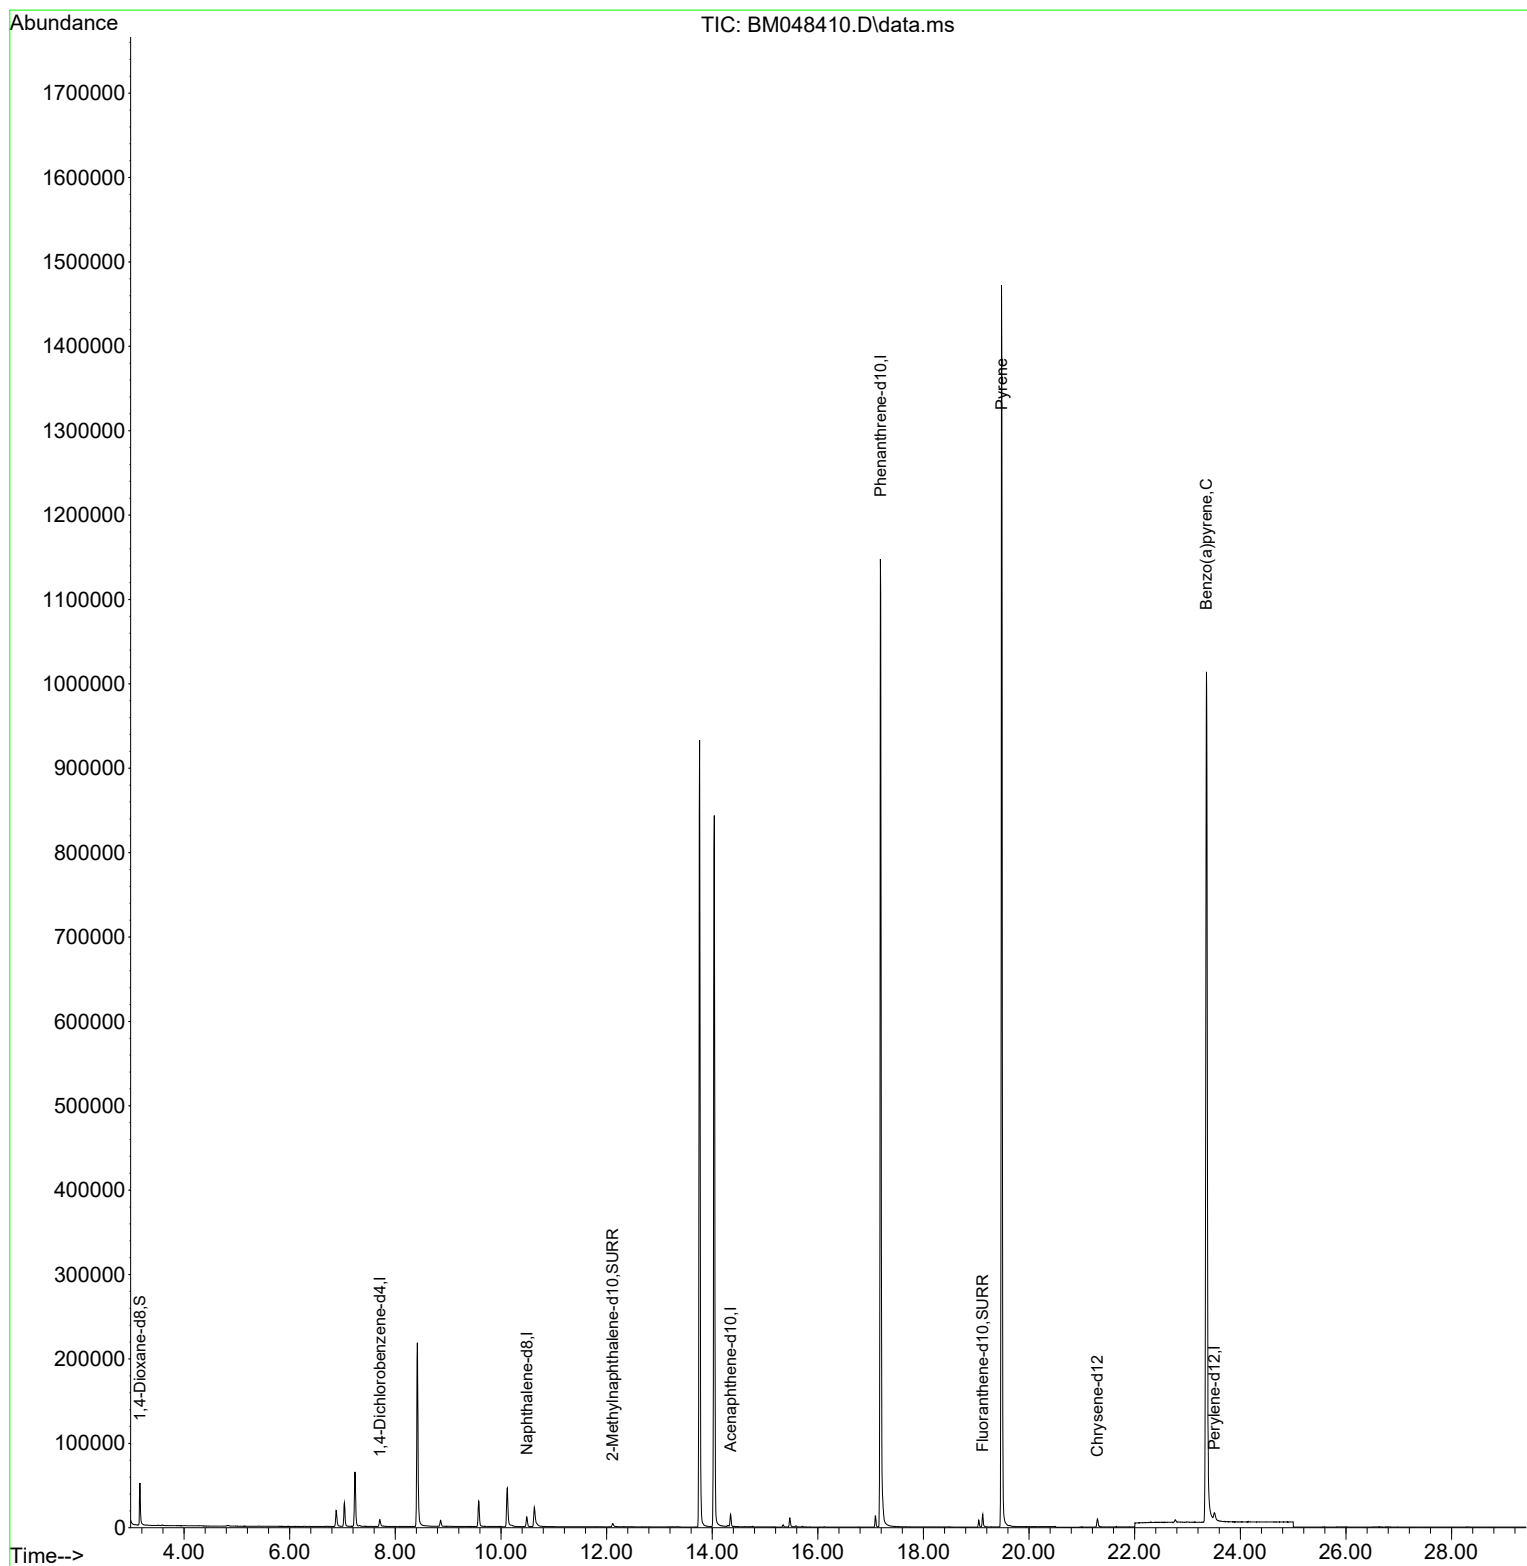

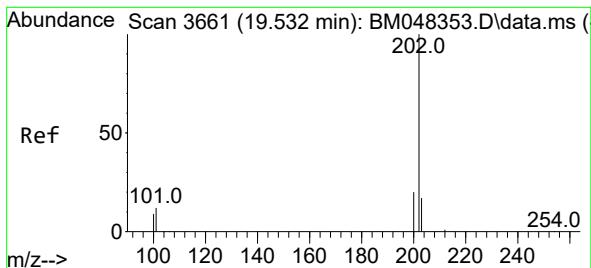

#20

Pyrene

Concen: 0.056 ng/ul

RT: 19.480 min Scan# 3

Delta R.T. -0.052 min

Lab File: BM048410.D

Acq: 02 Nov 2024 00:44

Instrument :

BNA_M

ClientSampleId :

E1L89





Tgt Ion:202 Resp: 2375

Ion Ratio Lower Upper

202 100

101 144.5 10.0 15.0#

100 1070.5 8.0 12.0#

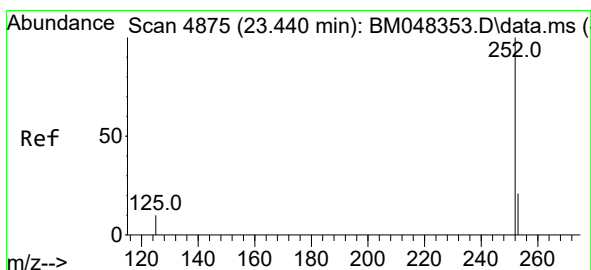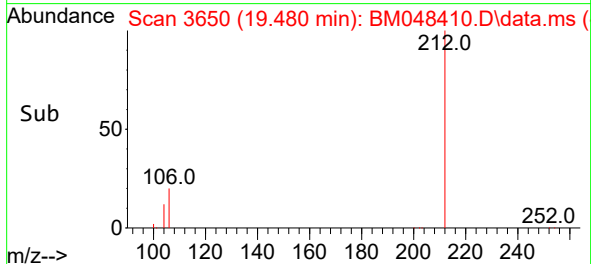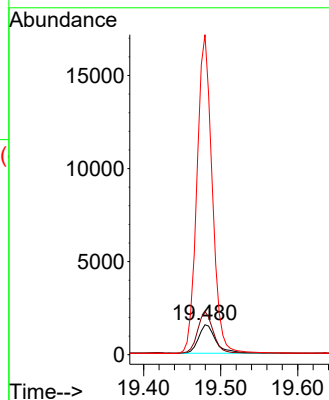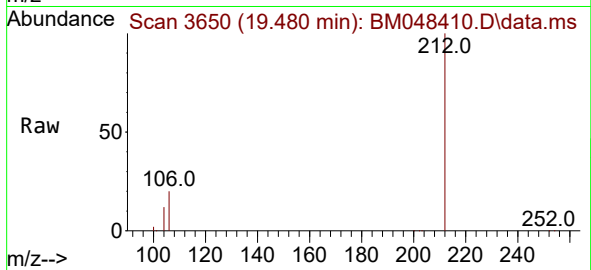

#26

Benzo(a)pyrene

Concen: 0.075 ng/ul

RT: 23.359 min Scan# 4847

Delta R.T. -0.081 min

Lab File: BM048410.D

Acq: 02 Nov 2024 00:44

Tgt Ion:252 Resp: 5381

Ion Ratio Lower Upper

252 100

253 46.9 27.7 41.5#

125 42.0 21.1 31.7#

