

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048411.D
 Acq On : 02 Nov 2024 01:21
 Operator : RC/JU
 Sample : P4558-06
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L91

Quant Time: Nov 03 21:51:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4509	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.490	136	14432	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.348	164	7897	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.186	188	1199230	0.400	ng/ul	0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.29
23) Perylene-d12	23.505	264	22402	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	23833	4.304	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.106	152	5836	0.318	ng/ul	-0.03
18) Fluoranthene-d10	19.122	212	18027	0.000	ng/ul	-0.02
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.193	88	345	0.057	ng/ul#	56
26) Benzo(a)pyrene	23.358	252	4575	0.064	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048411.D
Acq On : 02 Nov 2024 01:21
Operator : RC/JU
Sample : P4558-06
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L91

Quant Time: Nov 03 21:51:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration




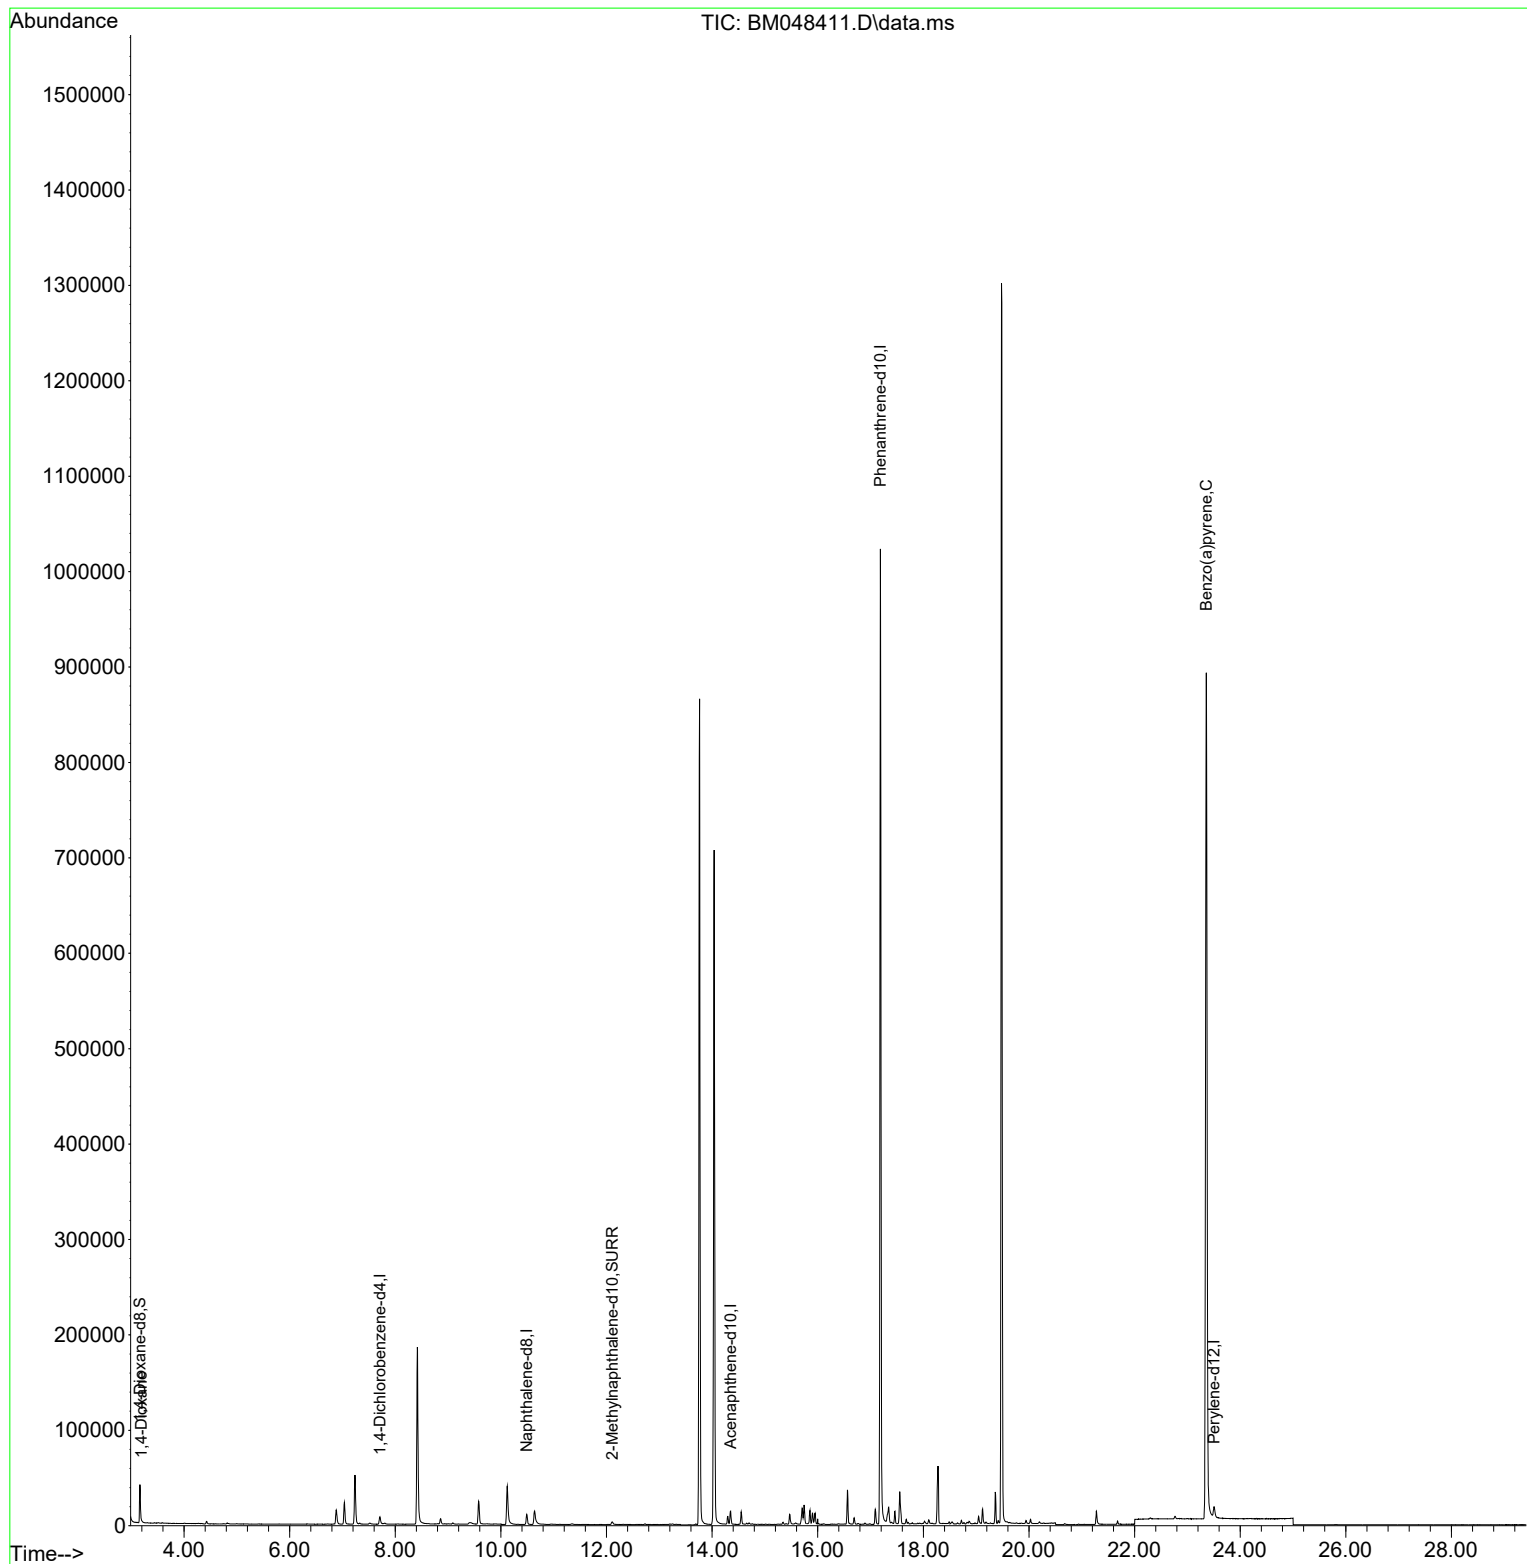


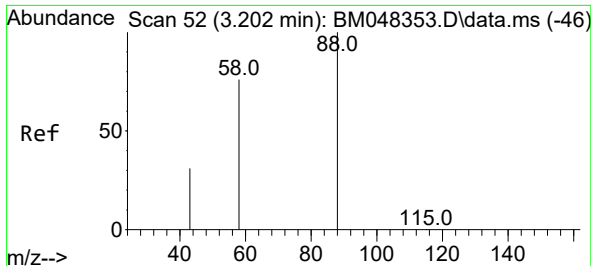

#2
1,4-Dioxane
Concen: 0.057 ng/ul
RT: 3.193 min Scan# 50
Delta R.T. -0.009 min
Lab File: BM048411.D
Acq: 02 Nov 2024 01:21

Instrument :
BNA_M
ClientSampleId :
E1L91

Tgt Ion: 88 Resp: 345
Ion Ratio Lower Upper
88 100
43 57.2 36.2 54.4#
58 11.9 47.4 71.0#

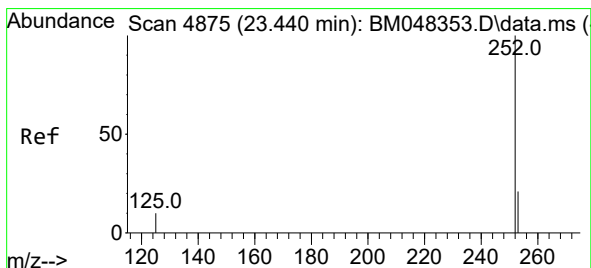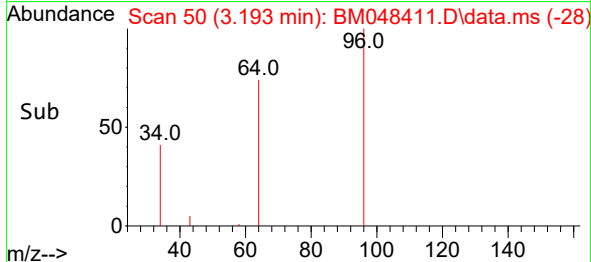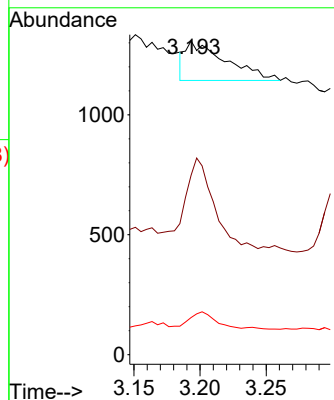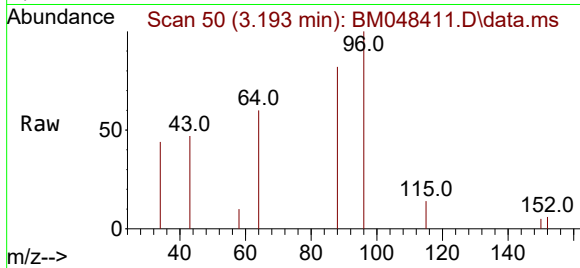

#26
Benzo(a)pyrene
Concen: 0.064 ng/ul
RT: 23.358 min Scan# 4847
Delta R.T. -0.082 min
Lab File: BM048411.D
Acq: 02 Nov 2024 01:21

Tgt Ion: 252 Resp: 4575
Ion Ratio Lower Upper
252 100
253 51.9 27.7 41.5#
125 50.9 21.1 31.7#

