

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048414.D
 Acq On : 02 Nov 2024 03:10
 Operator : RC/JU
 Sample : P4558-07
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L92

Quant Time: Nov 03 21:52:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4155	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.491	136	13270	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.349	164	7078	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.188	188	1289051	0.400	ng/ul	0.07
17) Chrysene-d12	21.298	240	10424	0.400	ng/ul	0.00
23) Perylene-d12	23.510	264	19995	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	25704	5.037	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.119	152	5335	0.316	ng/ul	-0.02
18) Fluoranthene-d10	19.123	212	15998	0.605	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.481	202	2211	0.057	ng/ul#	1
26) Benzo(a)pyrene	23.358	252	4696	0.073	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048414.D
Acq On : 02 Nov 2024 03:10
Operator : RC/JU
Sample : P4558-07
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L92

Quant Time: Nov 03 21:52:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration




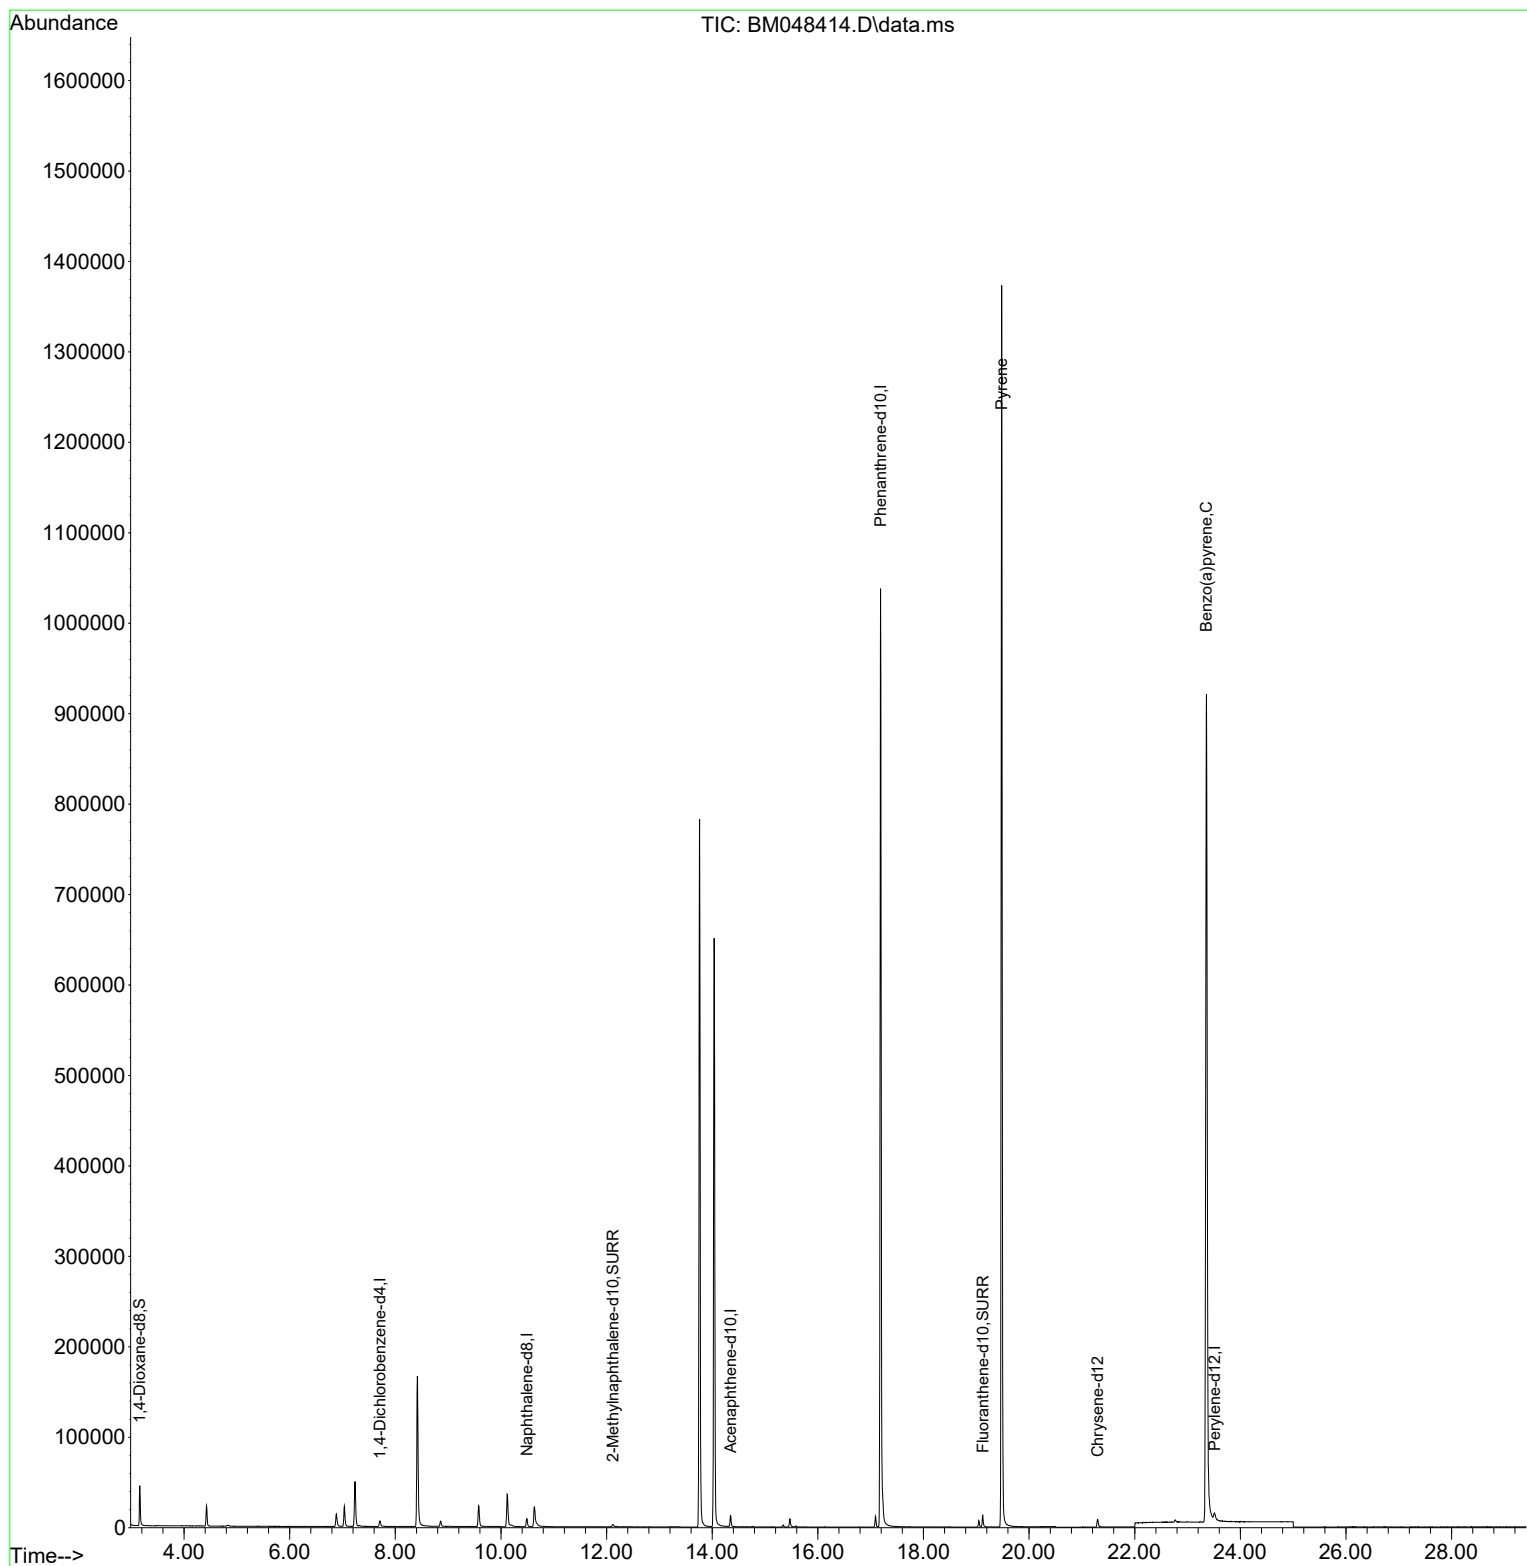


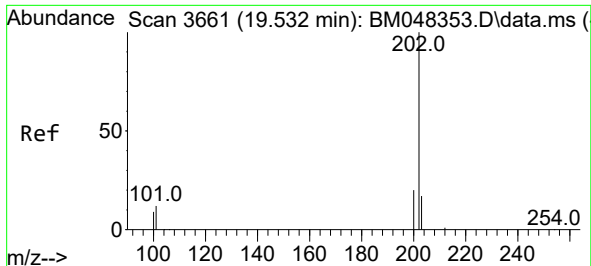

#20
Pyrene
Concen: 0.057 ng/ul
RT: 19.481 min Scan# 30
Delta R.T. -0.051 min
Lab File: BM048414.D
Acq: 02 Nov 2024 03:10

Instrument :
BNA_M
ClientSampleId :
E1L92

Tgt Ion:202 Resp: 2211
Ion Ratio Lower Upper
202 100
101 137.0 10.0 15.0#
100 978.4 8.0 12.0#

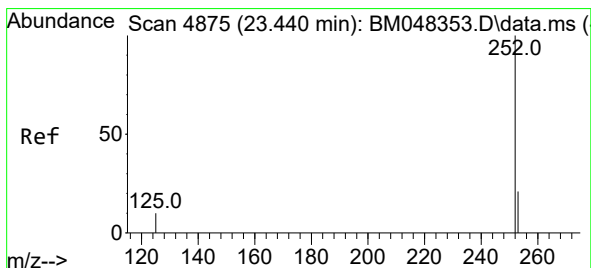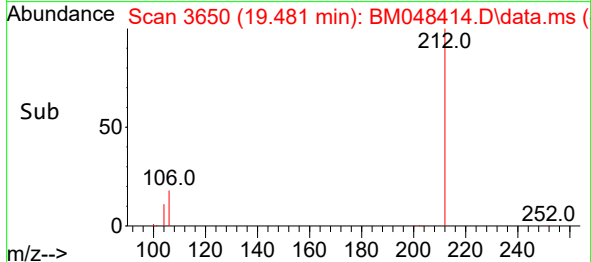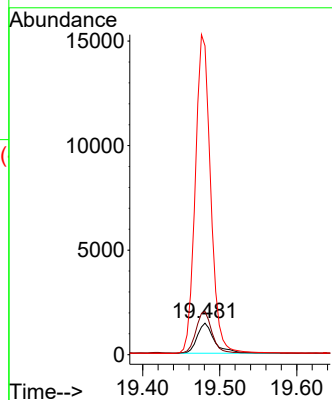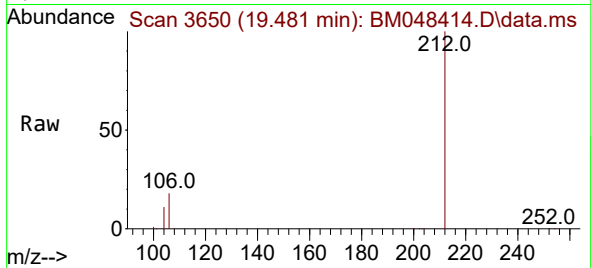

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.358 min Scan# 4847
Delta R.T. -0.082 min
Lab File: BM048414.D
Acq: 02 Nov 2024 03:10

Tgt Ion:252 Resp: 4696
Ion Ratio Lower Upper
252 100
253 47.7 27.7 41.5#
125 42.2 21.1 31.7#

