

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048415.D
 Acq On : 02 Nov 2024 03:47
 Operator : RC/JU
 Sample : P4558-08MS
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L92MS

Quant Time: Nov 03 21:52:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.788	152	2382	0.400	ng/ul	0.04
4) Naphthalene-d8	10.551	136	9484	0.400	ng/ul	0.02
9) Acenaphthene-d10	14.363	164	5637	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	10595	0.400	ng/ul	0.00
17) Chrysene-d12	21.289	240	10171	0.400	ng/ul	0.00
23) Perylene-d12	23.528	264	10160	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.168	96	1241	0.424	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.152	152	4638	0.384	ng/ul	0.01
18) Fluoranthene-d10	19.137	212	13909	0.539	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.197	88	3763	1.186	ng/ul#	89
5) Naphthalene	10.595	128	8809	0.355	ng/ul	96
7) 2-Methylnaphthalene	12.229	142	4847	0.329	ng/ul	97
8) 1-Methylnaphthalene	12.421	142	5898	0.375	ng/ul	98
10) Acenaphthylene	14.095	152	7981	0.366	ng/ul	98
11) Acenaphthene	14.428	153	6749	0.386	ng/ul	98
12) Fluorene	15.436	166	7521	0.387	ng/ul	97
14) Pentachlorophenol	16.782	266	2643	0.896	ng/ul	95
15) Phenanthrene	17.162	178	12045	0.457	ng/ul	99
16) Anthracene	17.268	178	10543	0.428	ng/ul	98
19) Fluoranthene	19.169	202	17472	0.498	ng/ul	99
20) Pyrene	19.527	202	18538	0.493	ng/ul	100
21) Benzo(a)anthracene	21.280	228	12690	0.417	ng/ul	99
22) Chrysene	21.324	228	21572	0.514	ng/ul	100
24) Benzo(b)fluoranthene	22.852	252	16248	0.468	ng/ul	98
25) Benzo(k)fluoranthene	22.896	252	21378	0.520	ng/ul	100
26) Benzo(a)pyrene	23.437	252	15207	0.466	ng/ul	100
27) Indeno(1,2,3-cd)pyrene	25.816	276	21051	0.462	ng/ul#	98
28) Dibenzo(a,h)anthracene	25.836	278	16209	0.456	ng/ul	100
29) Benzo(g,h,i)perylene	26.496	276	18410	0.479	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048415.D
Acq On : 02 Nov 2024 03:47
Operator : RC/JU
Sample : P4558-08MS
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L92MS

Quant Time: Nov 03 21:52:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration




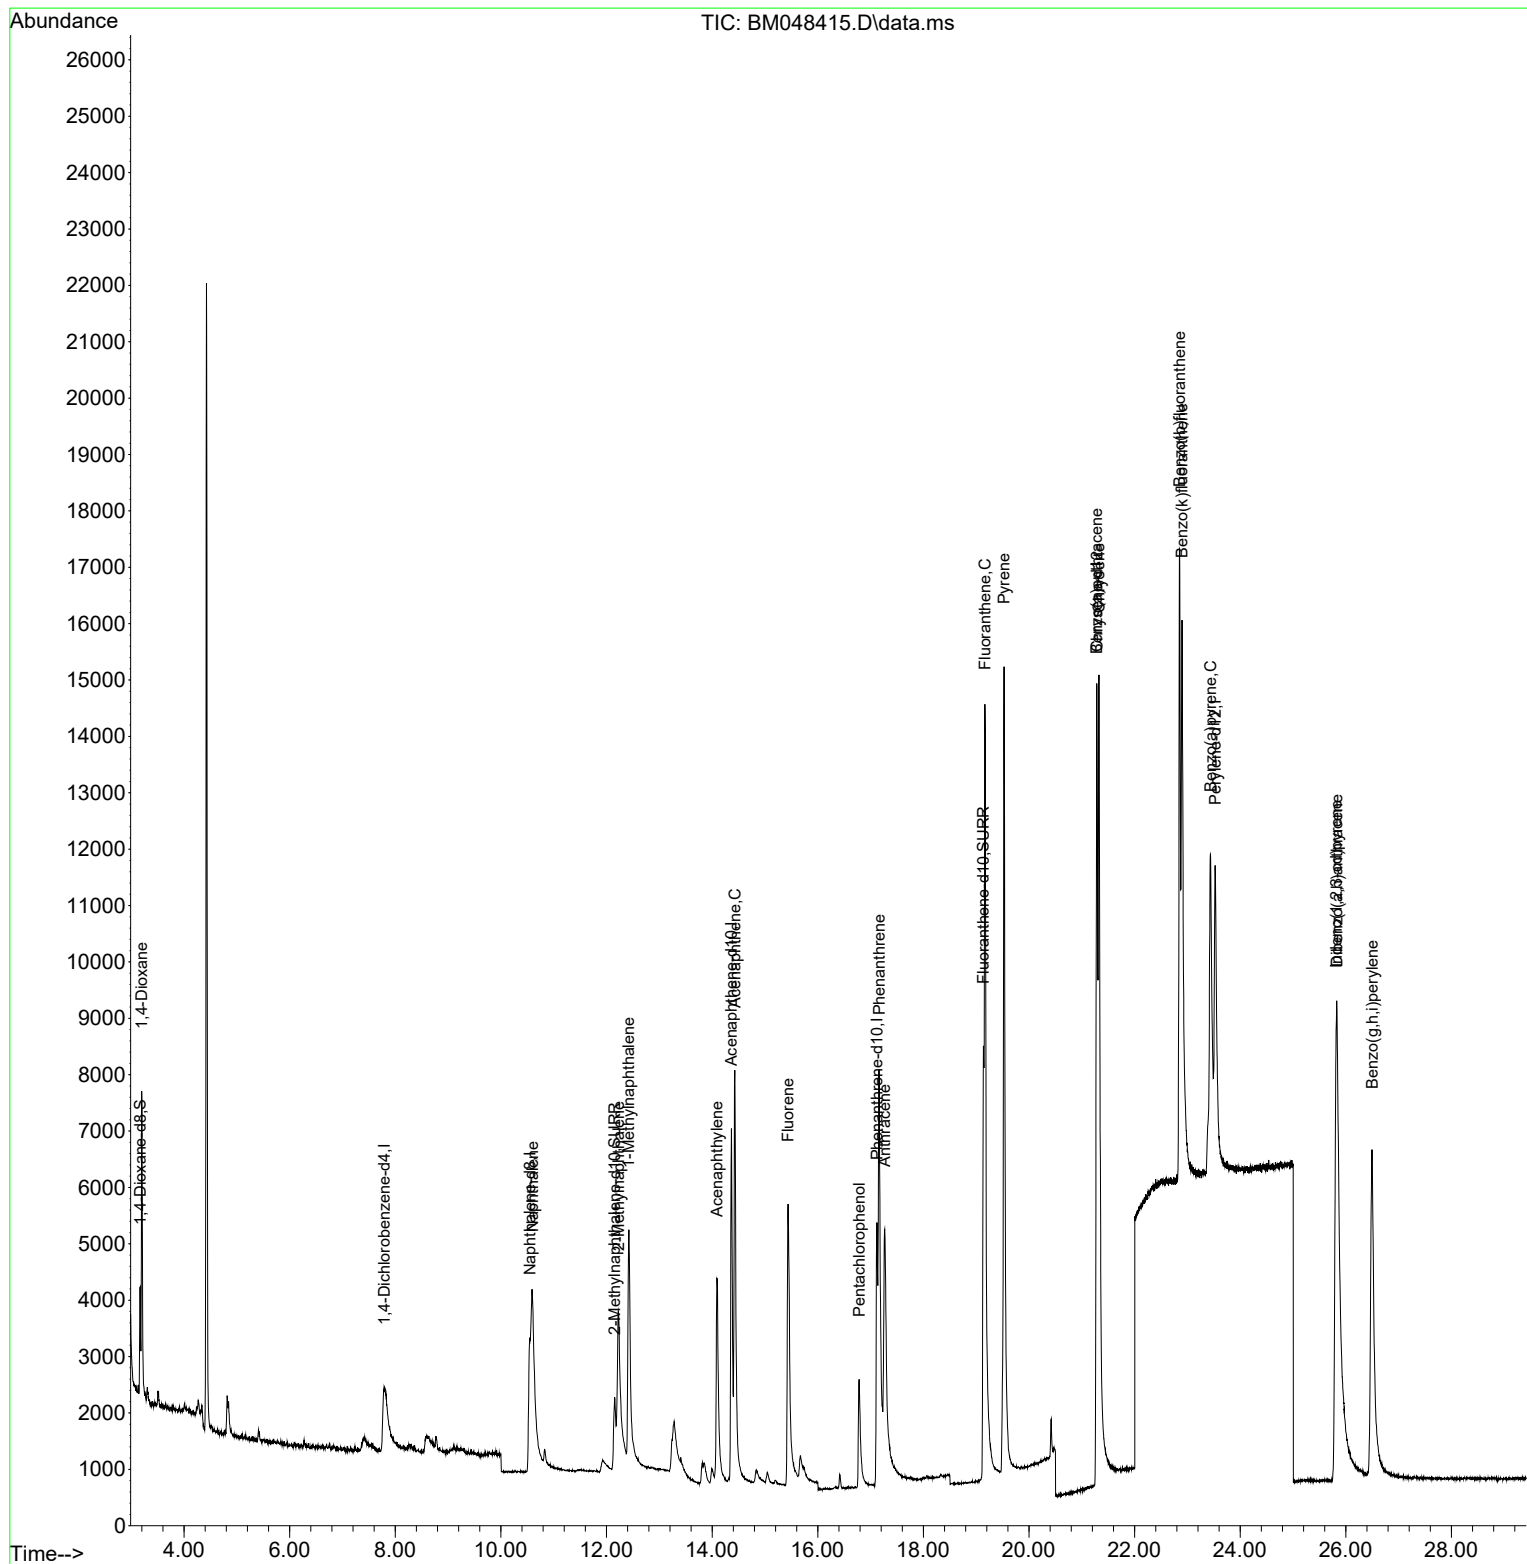


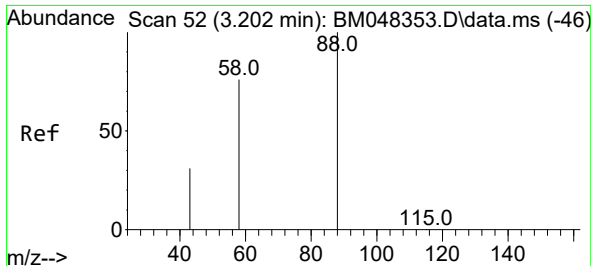

#2
1,4-Dioxane
Concen: 1.186 ng/ul
RT: 3.197 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47




Instrument :
BNA_M
ClientSampleId :
E1L92MS


Tgt Ion: 88 Resp: 3763
Ion Ratio Lower Upper
88 100
43 36.2 36.2 54.4#
58 65.8 47.4 71.0

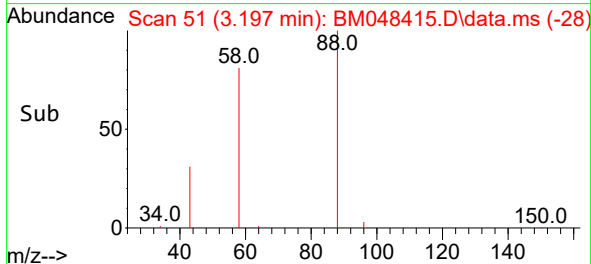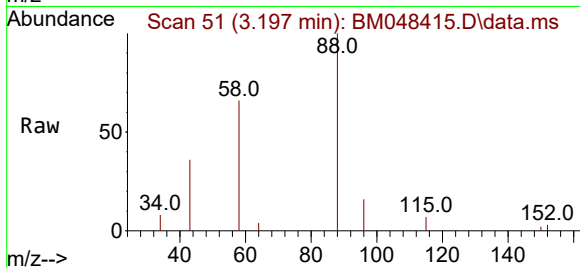

#5
Naphthalene
Concen: 0.355 ng/ul
RT: 10.595 min Scan# 1775
Delta R.T. 0.016 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Tgt Ion: 128 Resp: 8809
Ion Ratio Lower Upper
128 100
129 14.6 10.6 15.8
127 16.1 11.4 17.2


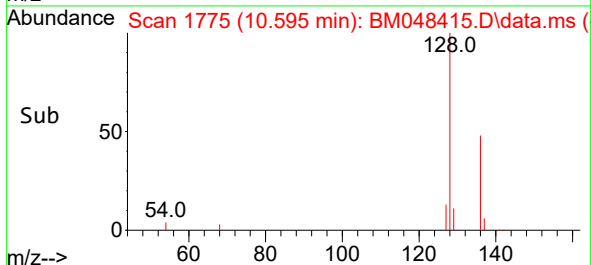

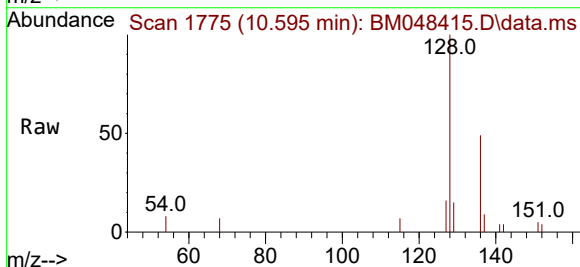




#7
2-Methylnaphthalene
Concen: 0.329 ng/ul
RT: 12.229 min Scan# 2069
Delta R.T. 0.016 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47




Instrument :
BNA_M
ClientSampleId :
E1L92MS


Tgt Ion:142 Resp: 4847
Ion Ratio Lower Upper
142 100
141 93.0 72.2 108.2

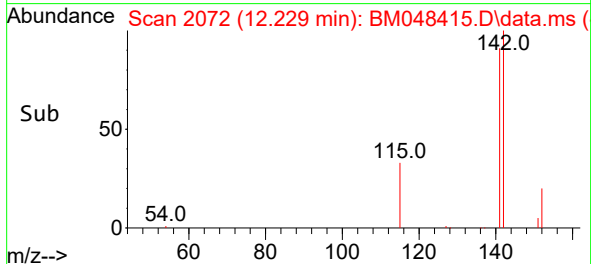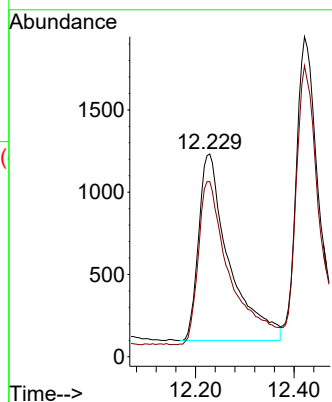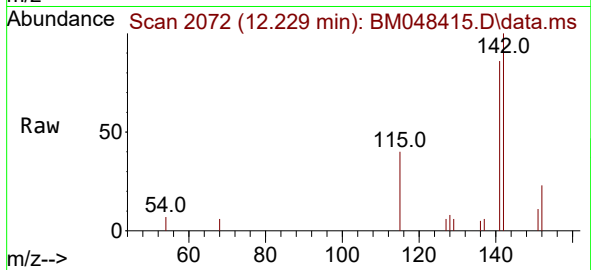

#8
1-Methylnaphthalene
Concen: 0.375 ng/ul
RT: 12.421 min Scan# 2107
Delta R.T. 0.005 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Tgt Ion:142 Resp: 5898
Ion Ratio Lower Upper
142 100
141 92.2 75.5 113.3


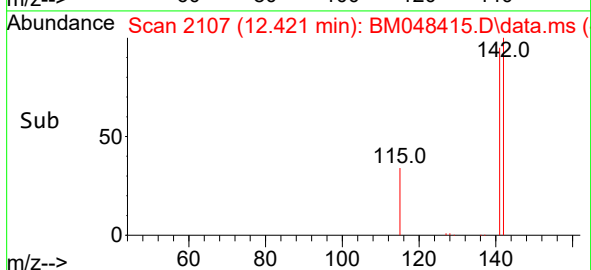

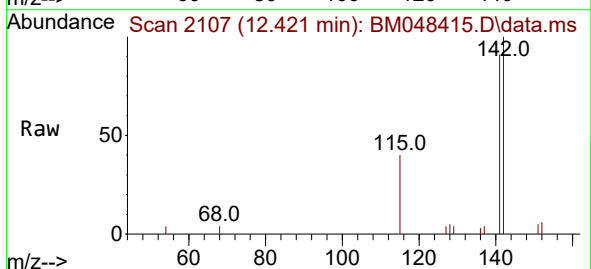


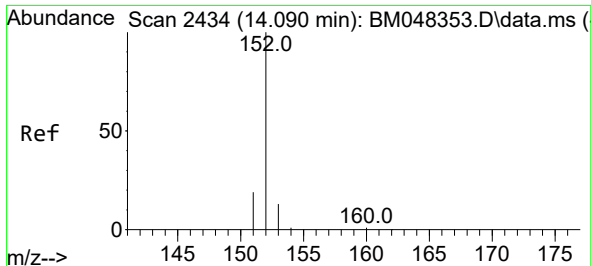

#10
Acenaphthylene
Concen: 0.366 ng/ul
RT: 14.095 min Scan# 2434
Delta R.T. 0.005 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47




Instrument :
BNA_M
ClientSampleId :
E1L92MS


Tgt Ion:152 Resp: 7981
Ion Ratio Lower Upper
152 100
151 21.6 16.6 24.8
153 15.6 11.8 17.6

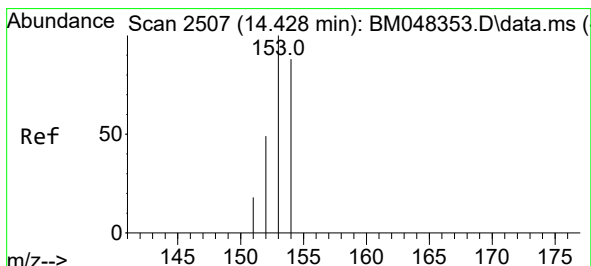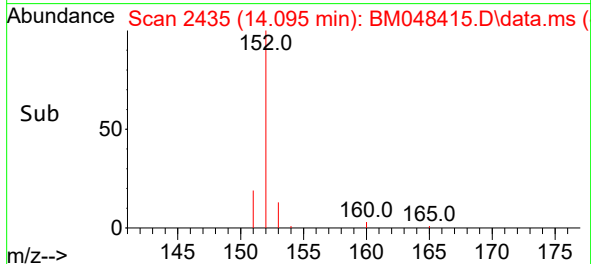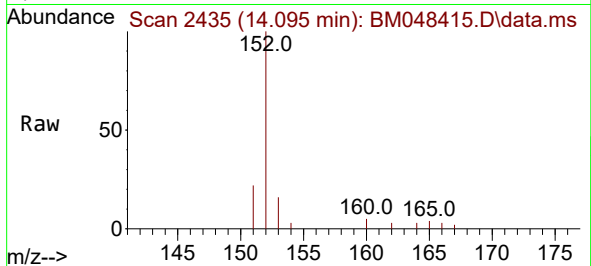

#11
Acenaphthene
Concen: 0.386 ng/ul
RT: 14.428 min Scan# 2507
Delta R.T. -0.000 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Tgt Ion:153 Resp: 6749
Ion Ratio Lower Upper
153 100
152 52.6 40.7 61.1
154 87.0 70.6 106.0

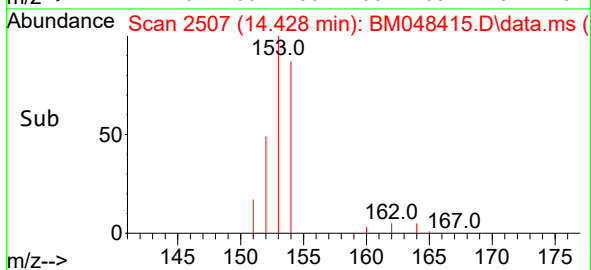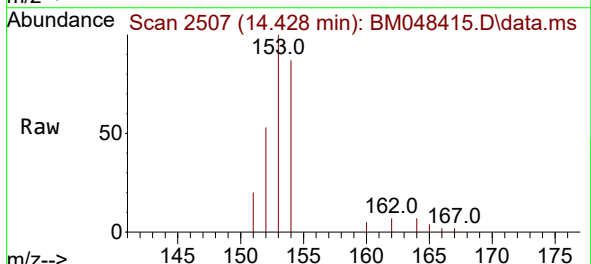



#12

Fluorene

Concen: 0.387 ng/ul

RT: 15.436 min Scan# 21

Delta R.T. 0.005 min

Lab File: BM048415.D

Acq: 02 Nov 2024 03:47

Instrument :

BNA_M

ClientSampleId :

E1L92MS





Tgt Ion:166 Resp: 7521

Ion Ratio Lower Upper

166 100

165 102.0 78.6 118.0

167 15.8 12.1 18.1

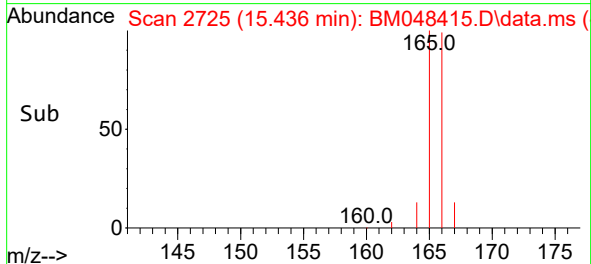

#14

Pentachlorophenol

Concen: 0.896 ng/ul

RT: 16.782 min Scan# 3032

Delta R.T. -0.004 min

Lab File: BM048415.D

Acq: 02 Nov 2024 03:47




Tgt Ion:266 Resp: 2643


Ion Ratio Lower Upper

266 100

264 60.0 48.3 72.5

268 65.5 46.2 69.4


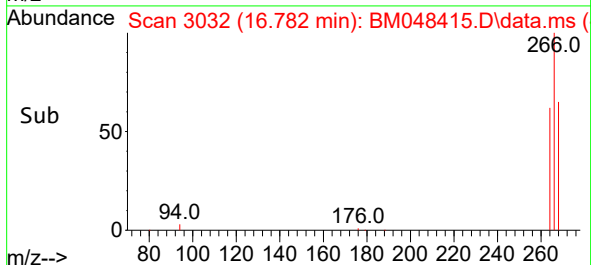

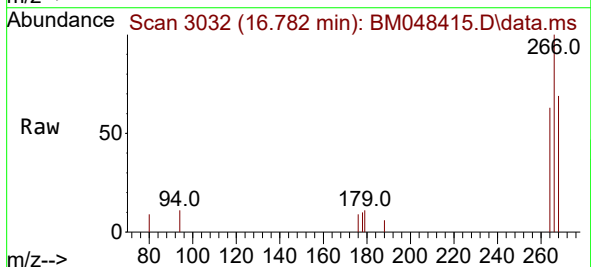


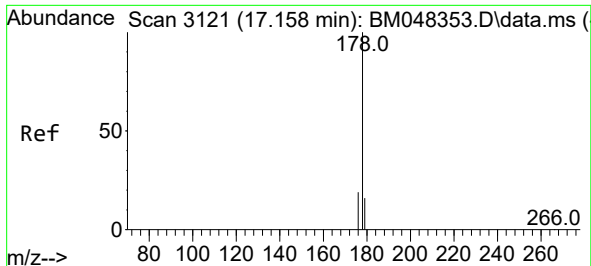

#15
Phenanthrene
Concen: 0.457 ng/ul
RT: 17.162 min Scan# 3122
Delta R.T. 0.004 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47




Instrument :
BNA_M
ClientSampleId :
E1L92MS


Tgt Ion:178 Resp: 12045
Ion Ratio Lower Upper
178 100
179 16.8 13.9 20.9
176 20.1 16.0 24.0

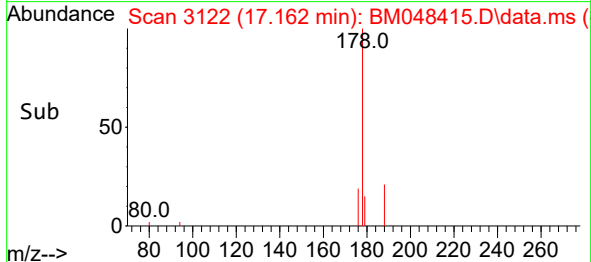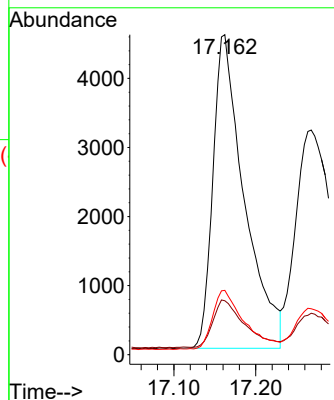

#16
Anthracene
Concen: 0.428 ng/ul
RT: 17.268 min Scan# 3147
Delta R.T. 0.008 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Tgt Ion:178 Resp: 10543
Ion Ratio Lower Upper
178 100
179 18.5 14.2 21.2
176 20.4 15.8 23.6


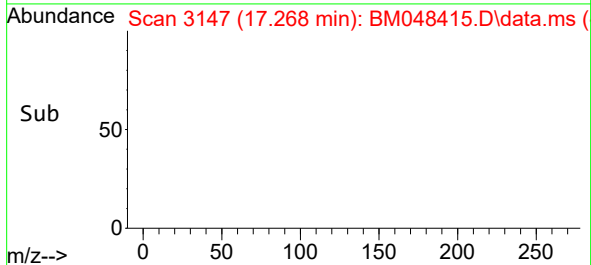
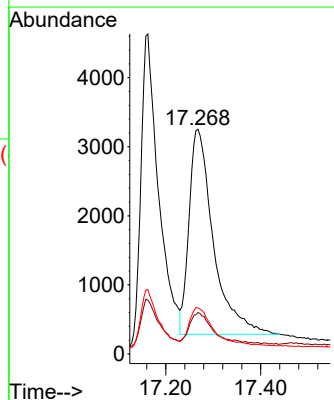
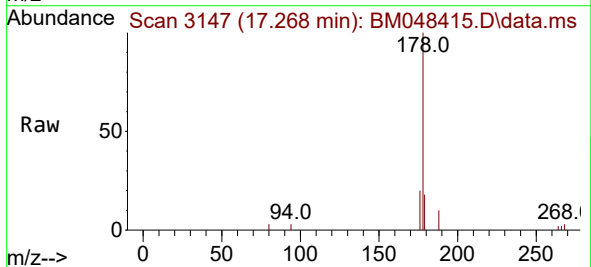




#19
Fluoranthene
Concen: 0.498 ng/ul
RT: 19.169 min Scan# 3583
Delta R.T. -0.000 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47




Instrument :
BNA_M
ClientSampleId :
E1L92MS


Tgt Ion:202 Resp: 17472
Ion Ratio Lower Upper
202 100
101 11.0 9.0 13.4
100 8.5 6.6 10.0

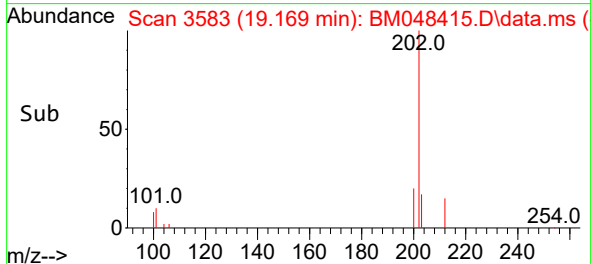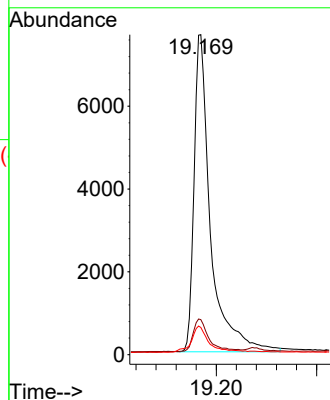

#20
Pyrene
Concen: 0.493 ng/ul
RT: 19.527 min Scan# 3660
Delta R.T. -0.005 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Tgt Ion:202 Resp: 18538
Ion Ratio Lower Upper
202 100
101 12.5 10.0 15.0
100 10.3 8.0 12.0


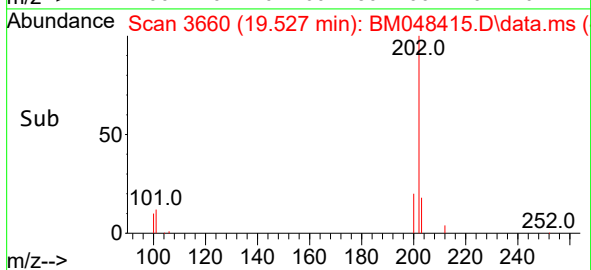
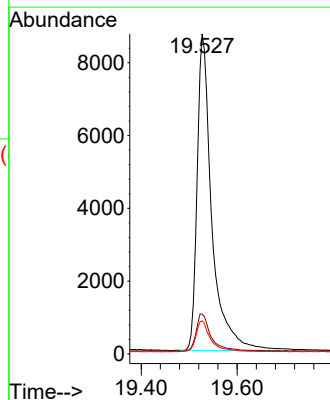
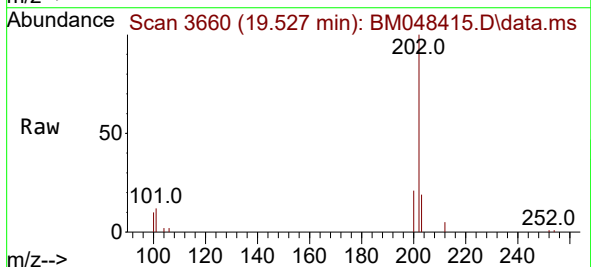


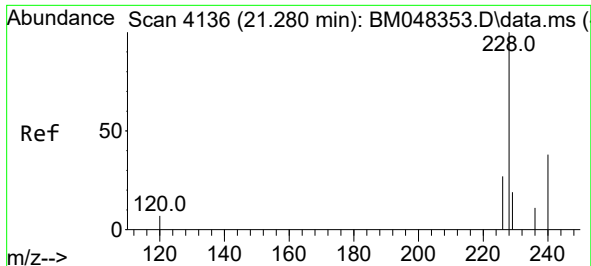

#21
Benzo(a)anthracene
Concen: 0.417 ng/ul
RT: 21.280 min Scan# 4136
Delta R.T. -0.000 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47




Instrument :
BNA_M
ClientSampleId :
E1L92MS


Tgt Ion:228 Resp: 12690
Ion Ratio Lower Upper
228 100
229 20.5 15.9 23.9
226 27.4 22.1 33.1

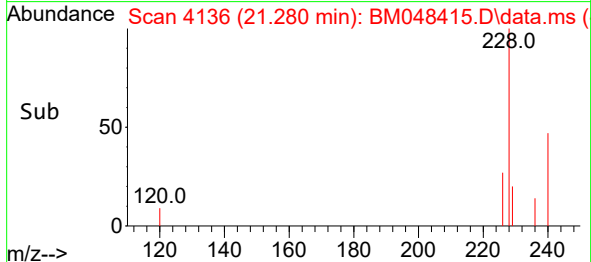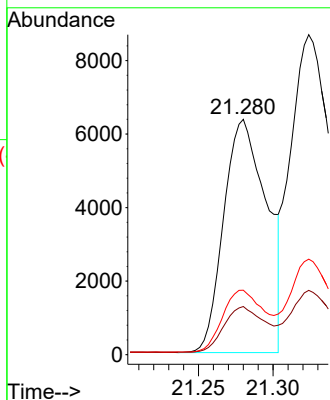

#22
Chrysene
Concen: 0.514 ng/ul
RT: 21.324 min Scan# 4151
Delta R.T. -0.003 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Tgt Ion:228 Resp: 21572
Ion Ratio Lower Upper
228 100
226 29.8 24.1 36.1
229 20.1 15.9 23.9


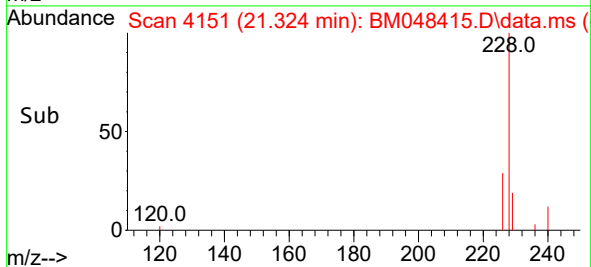
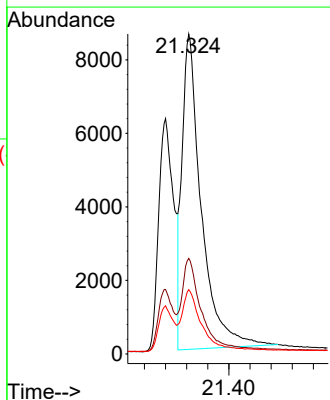
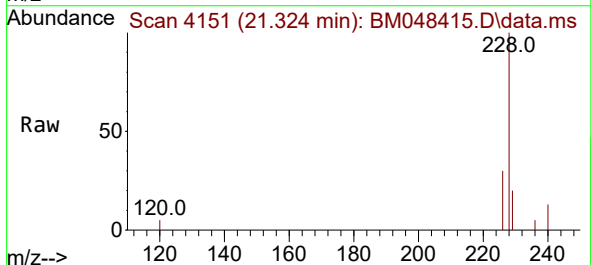


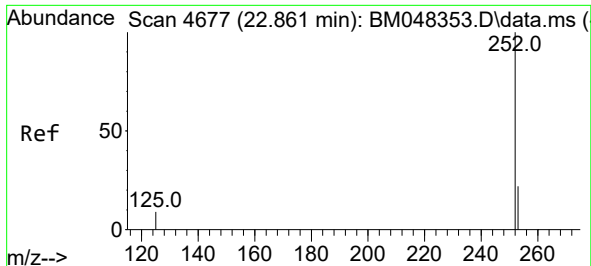

#24
Benzo(b)fluoranthene
Concen: 0.468 ng/ul
RT: 22.852 min Scan# 4674
Delta R.T. -0.009 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47




Instrument :
BNA_M
ClientSampleId :
E1L92MS


Tgt Ion:252 Resp: 16248
Ion Ratio Lower Upper
252 100
253 28.5 0.0 59.4
125 18.0 0.0 38.0

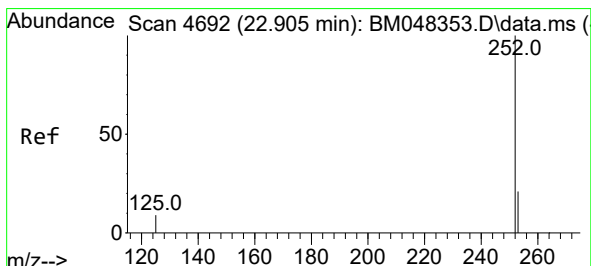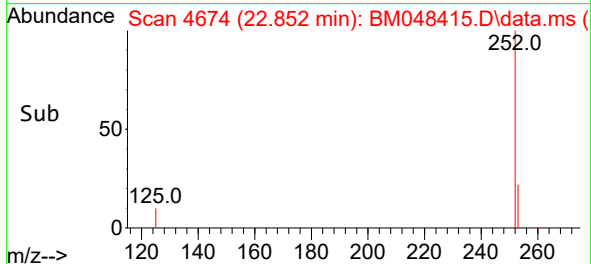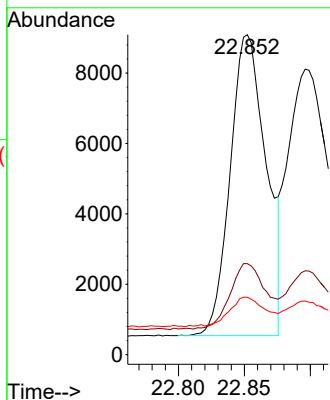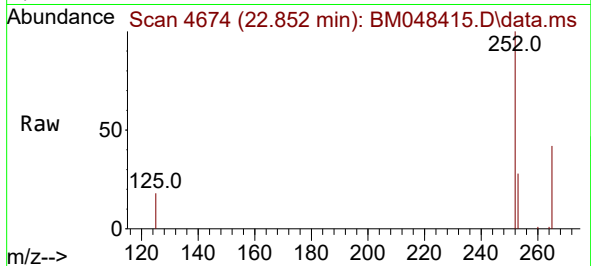

#25
Benzo(k)fluoranthene
Concen: 0.520 ng/ul
RT: 22.896 min Scan# 4689
Delta R.T. -0.009 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Tgt Ion:252 Resp: 21378
Ion Ratio Lower Upper
252 100
253 29.4 23.4 35.0
125 18.8 15.3 22.9

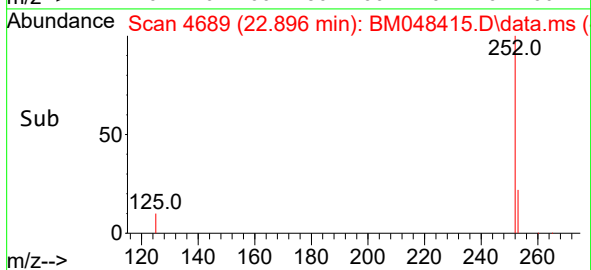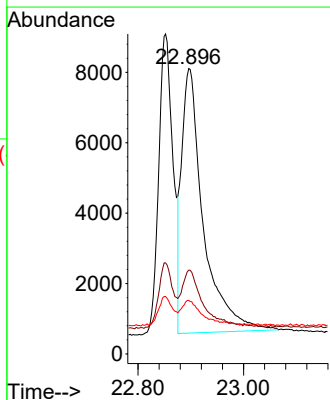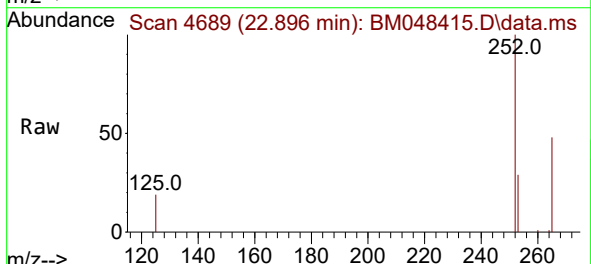



#26

Benzo(a)pyrene

Concen: 0.466 ng/ul

RT: 23.437 min Scan# 4875

Delta R.T. -0.003 min

Lab File: BM048415.D

Acq: 02 Nov 2024 03:47

Instrument :

BNA_M

ClientSampleId :

E1L92MS





Tgt Ion:252 Resp: 15207

Ion Ratio Lower Upper

252 100

253 34.6 27.7 41.5

125 25.9 21.1 31.7

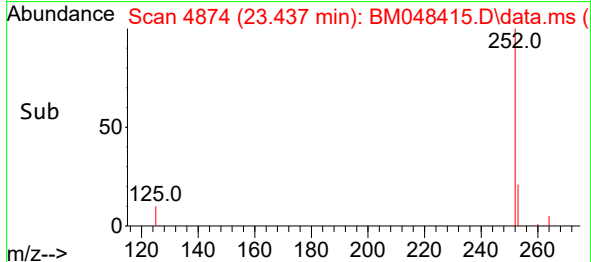

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.462 ng/ul

RT: 25.816 min Scan# 5652

Delta R.T. 0.003 min

Lab File: BM048415.D

Acq: 02 Nov 2024 03:47




Tgt Ion:276 Resp: 21051


Ion Ratio Lower Upper

276 100

138 23.7 19.6 29.4

227 0.0 0.1 0.1#


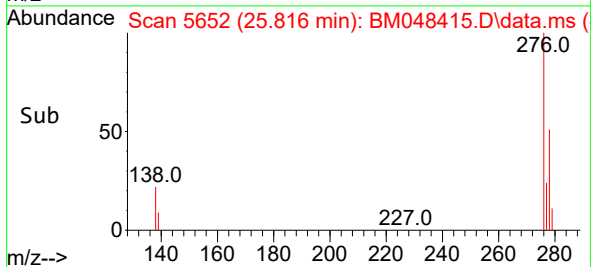

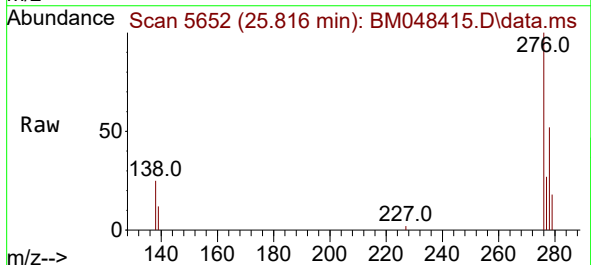




#28
Dibenzo(a,h)anthracene
Concen: 0.456 ng/ul
RT: 25.836 min Scan# 5658
Delta R.T. -0.000 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Instrument :
BNA_M
ClientSampleId :
E1L92MS

Tgt Ion:278 Resp: 16209
Ion Ratio Lower Upper
278 100
139 19.9 15.6 23.4
279 32.9 26.4 39.6

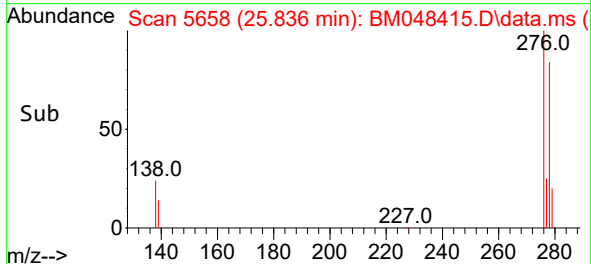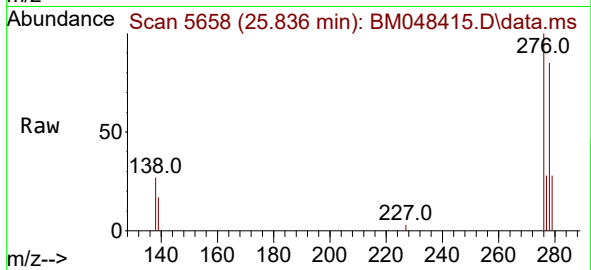

#29
Benzo(g,h,i)perylene
Concen: 0.479 ng/ul
RT: 26.496 min Scan# 5855
Delta R.T. -0.003 min
Lab File: BM048415.D
Acq: 02 Nov 2024 03:47

Tgt Ion:276 Resp: 18410
Ion Ratio Lower Upper
276 100
138 22.5 19.0 28.6
277 25.6 20.6 31.0

