

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048417.D
 Acq On : 02 Nov 2024 05:00
 Operator : RC/JU
 Sample : PB164513BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK513

Quant Time: Nov 03 21:52:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4364	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.490	136	13799	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.348	164	7287	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.186	188	954698	0.400	ng/ul	0.07
17) Chrysene-d12	21.301	240	10546	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.53
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	29485	5.501	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	5417	0.309	ng/ul	-0.02
18) Fluoranthene-d10	19.122	212	11353	0.424	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.480	202	1518	0.039	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048417.D
Acq On : 02 Nov 2024 05:00
Operator : RC/JU
Sample : PB164513BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513


Quant Time: Nov 03 21:52:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

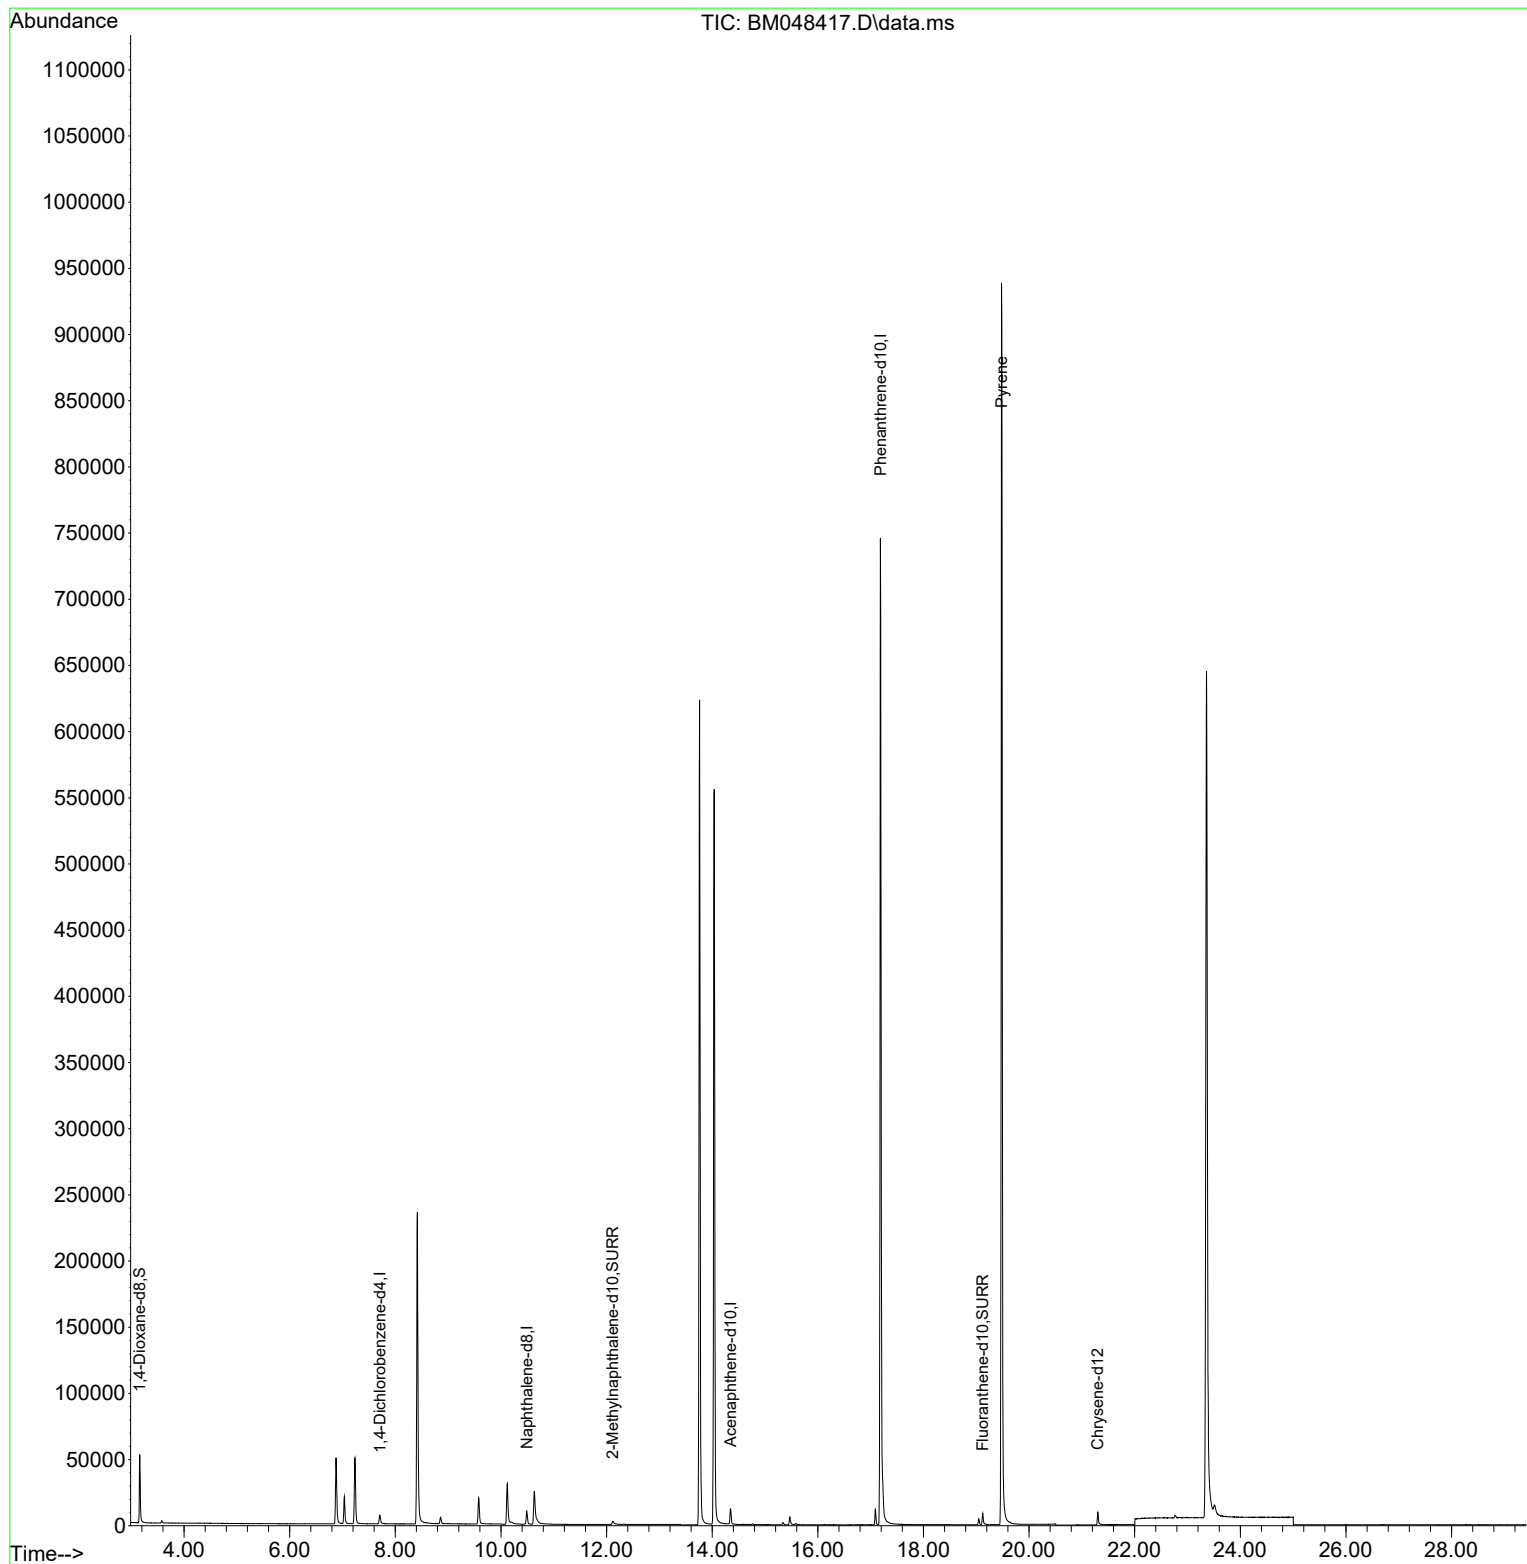

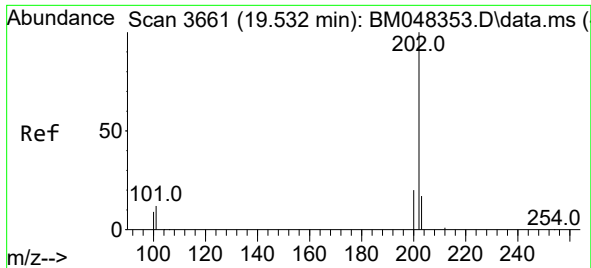

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.480 min Scan# 30
Delta R.T. -0.052 min
Lab File: BM048417.D
Acq: 02 Nov 2024 05:00

Instrument :
BNA_M
ClientSampleId :
SBLK513

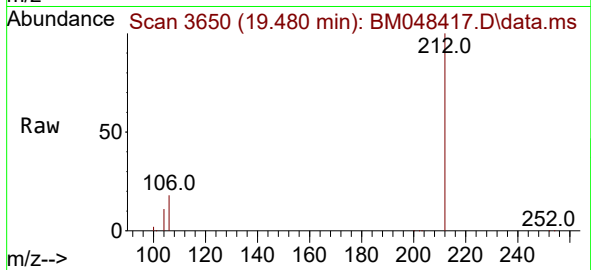

Tgt Ion:202 Resp: 1518
Ion Ratio Lower Upper
202 100
101 139.8 10.0 15.0#
100 1042.8 8.0 12.0#

