




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

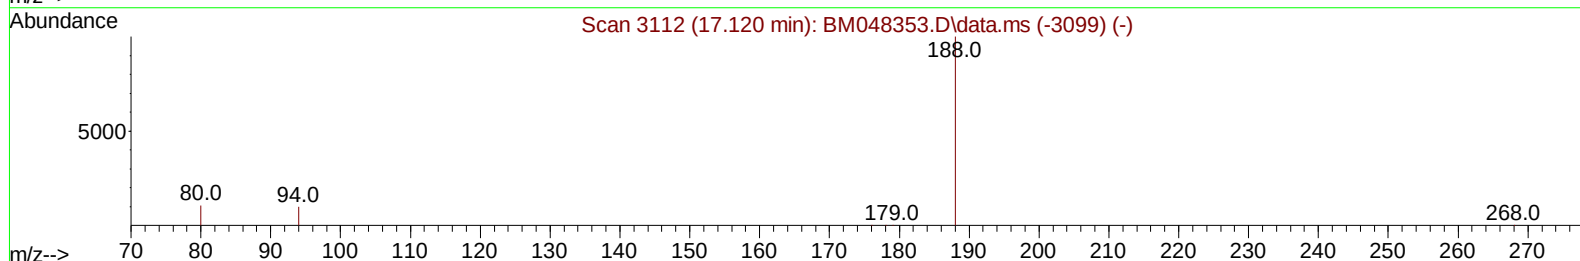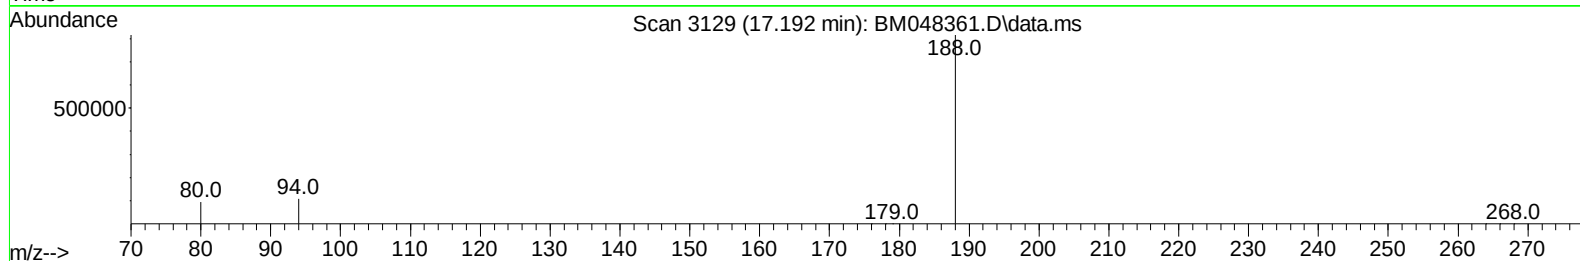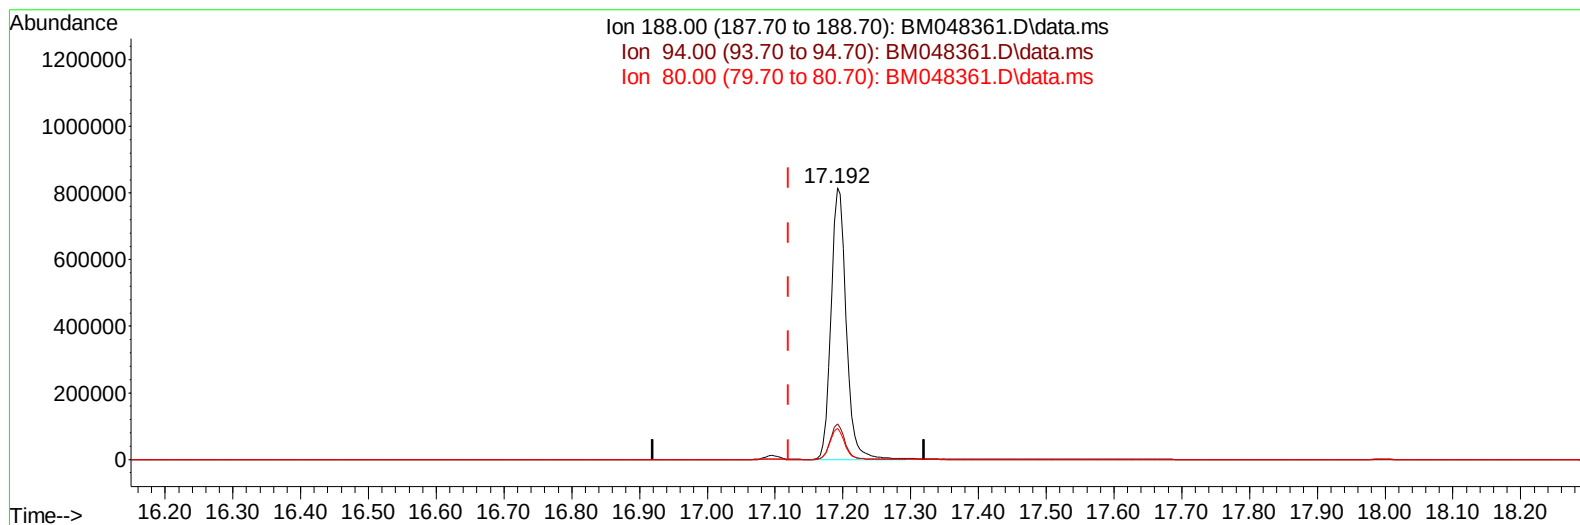

TIC: BM048361.D\data.ms

(13) Phenanthrene-d10 (I)

17.192min (+ 0.072) 0.40 ng/ul

response 1258698

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.50	13.14
80.00	12.10	11.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

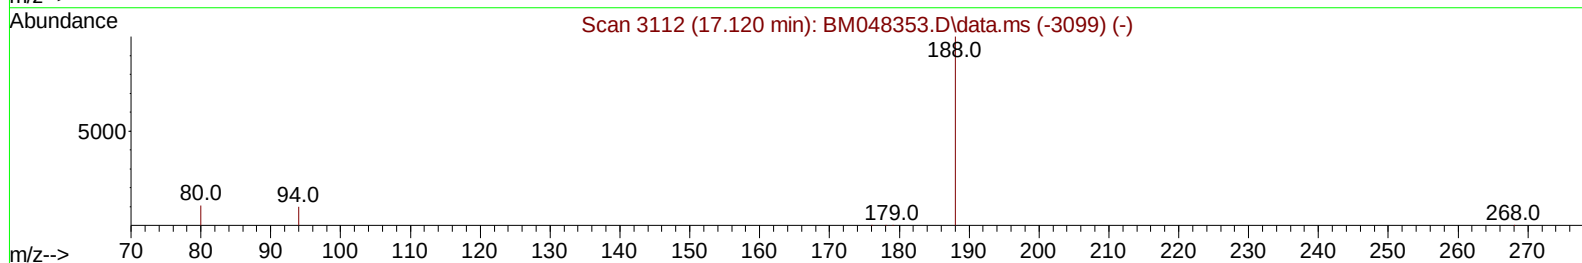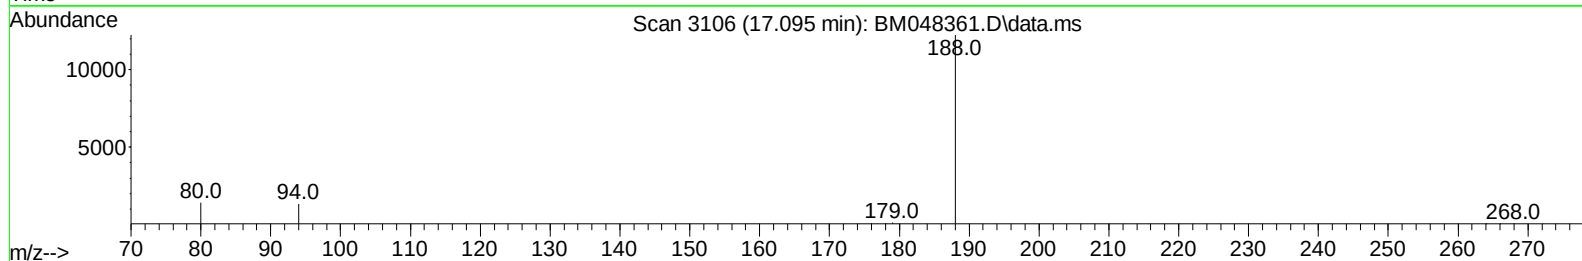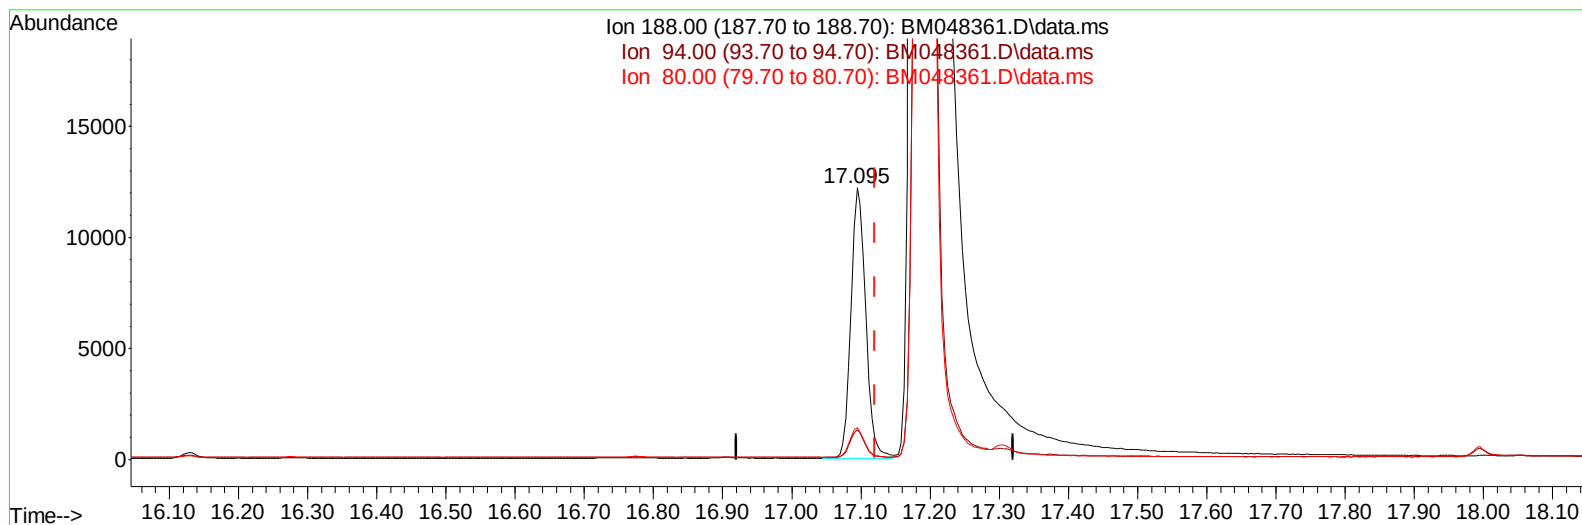

TIC: BM048361.D\data.ms

(13) Phenanthrene-d10 (I)

17.095min (-0.025) 0.40 ng/ul m

response 18048

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.50	10.87
80.00	12.10	11.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

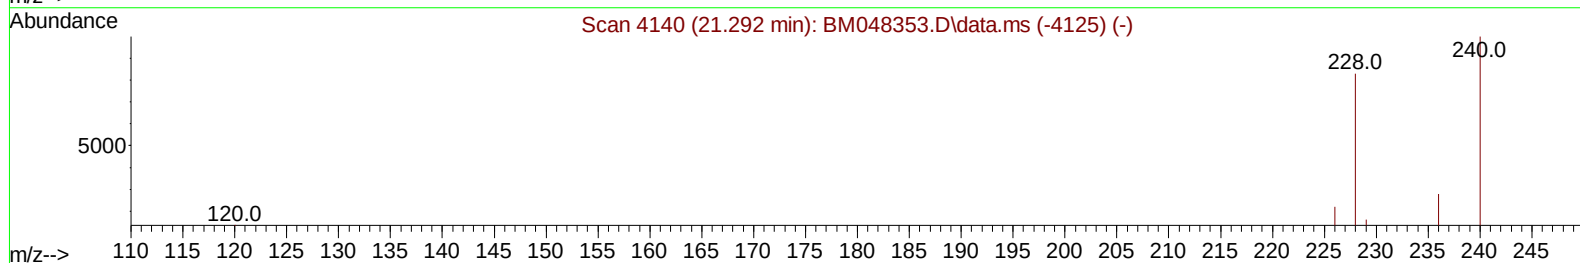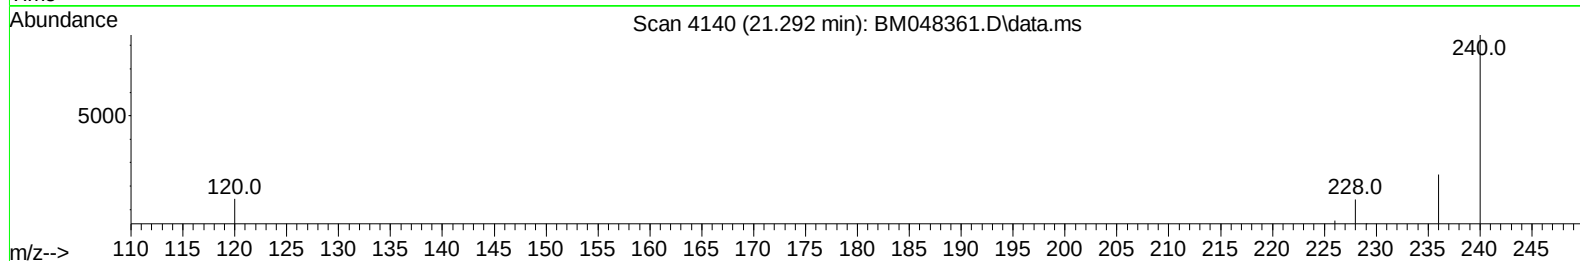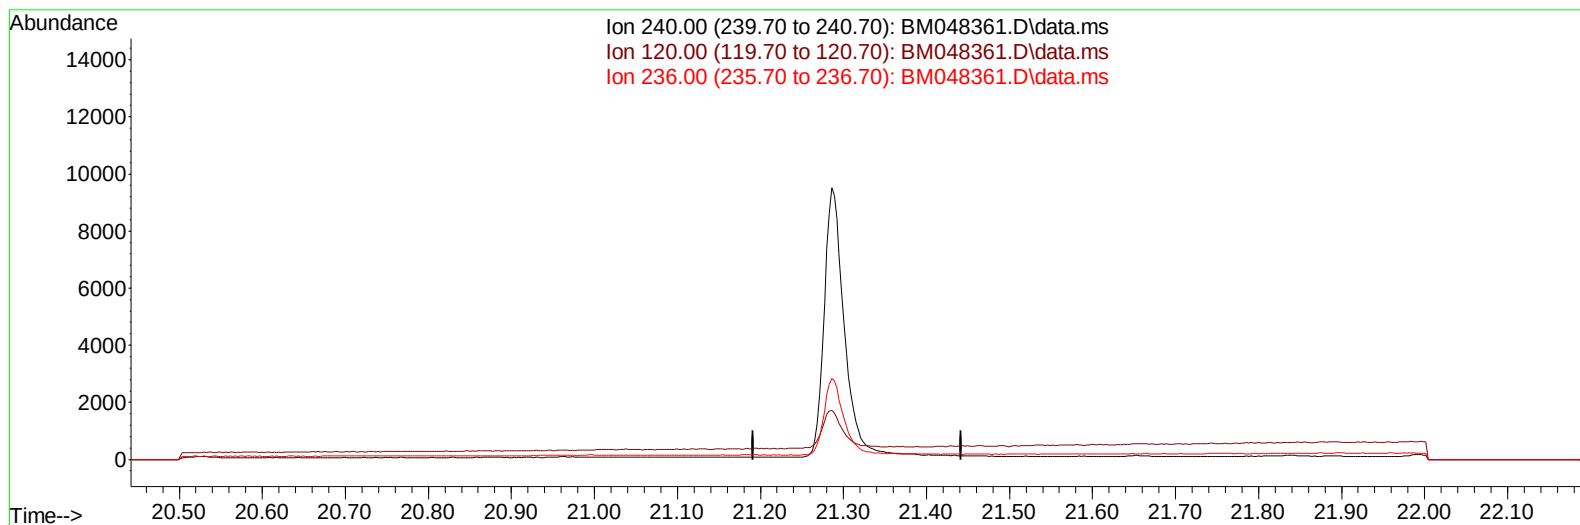

TIC: BM048361.D\data.ms

(17) Chrysene-d12

21.292min (-21.292) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	19.00	0.00#
236.00	29.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

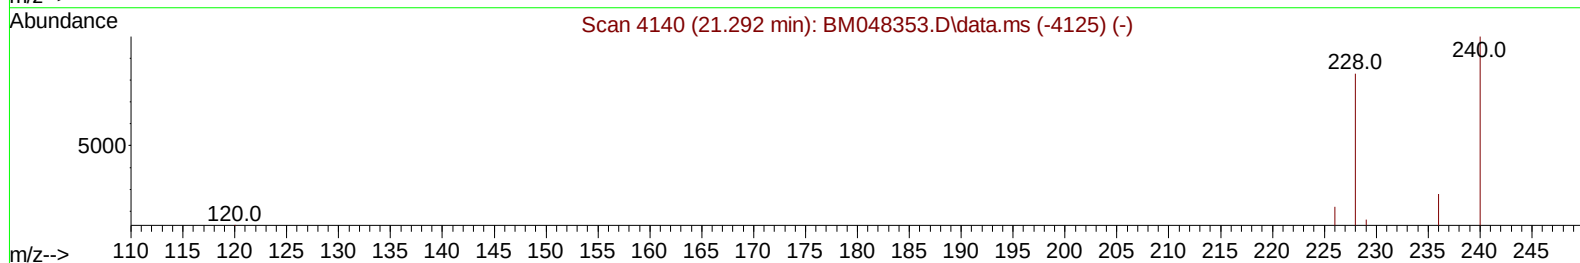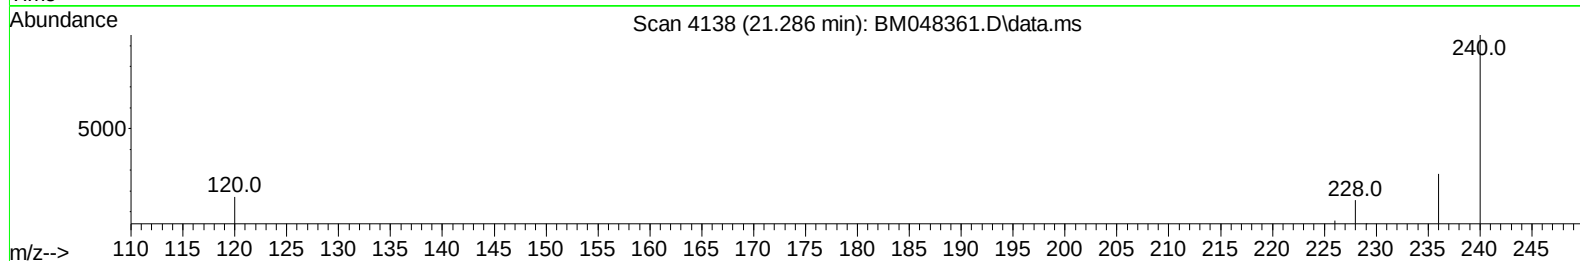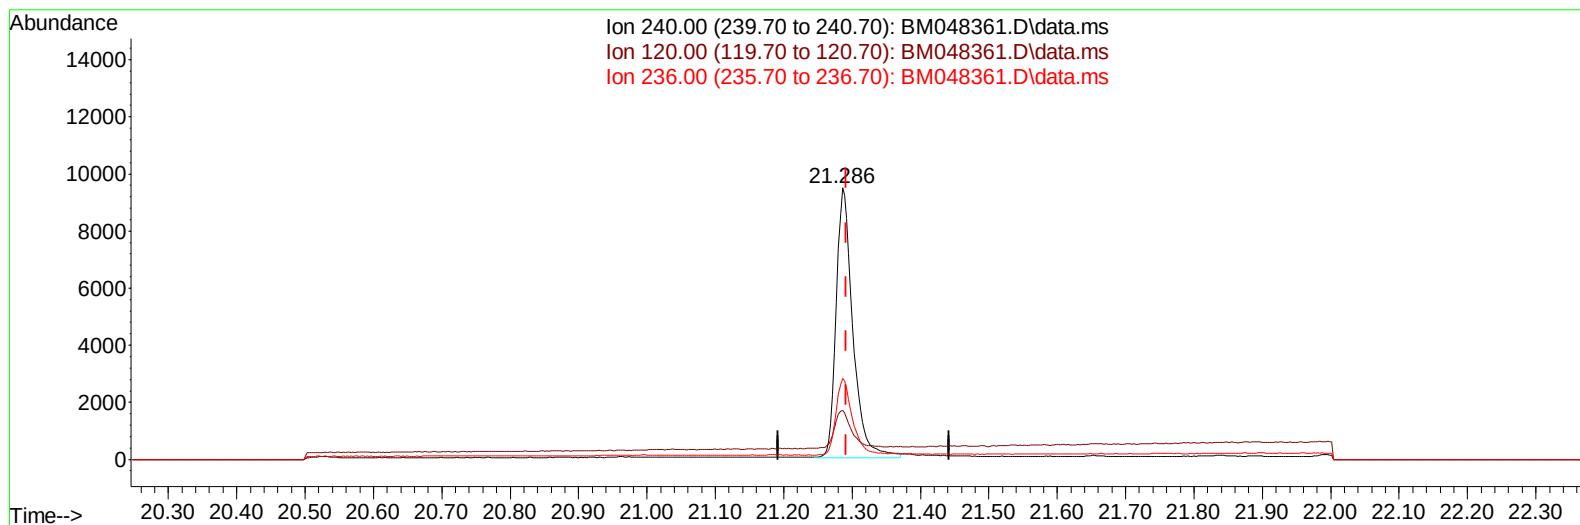

TIC: BM048361.D\data.ms

(17) Chrysene-d12

21.286min (-0.006) 0.40 ng/ul m

response 16109

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	19.00	18.16
236.00	29.90	29.74
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

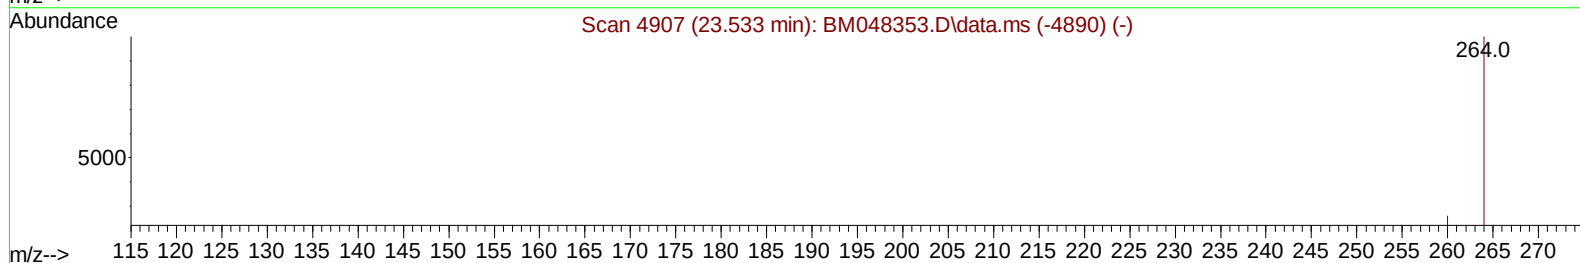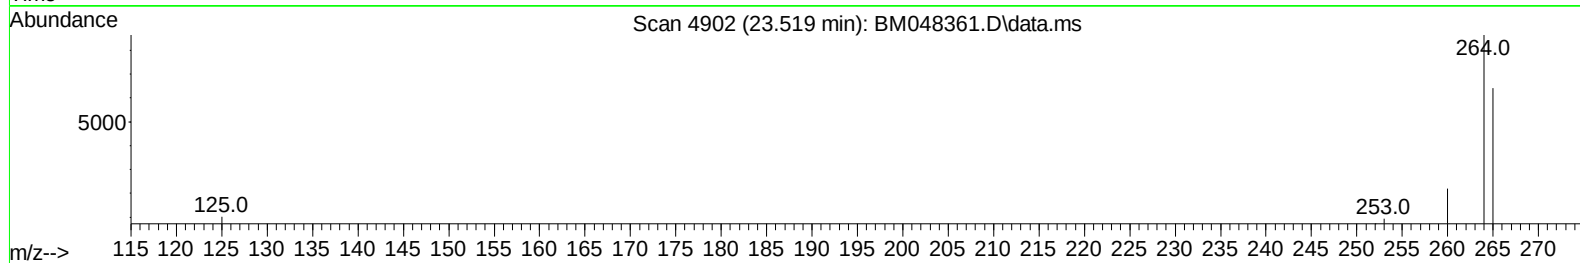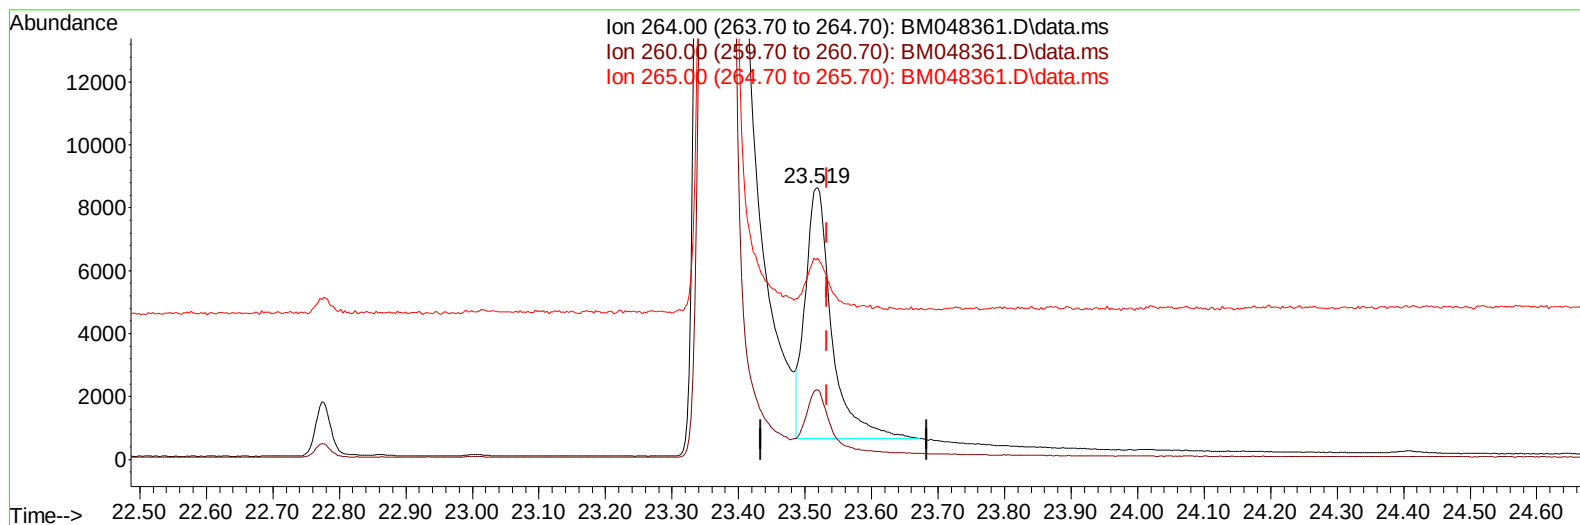

TIC: BM048361.D\data.ms

(23) Perylene-d12 (I)

23.519min (-0.015) 0.40 ng/u1

response 22156

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.51
265.00	120.80	74.27#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

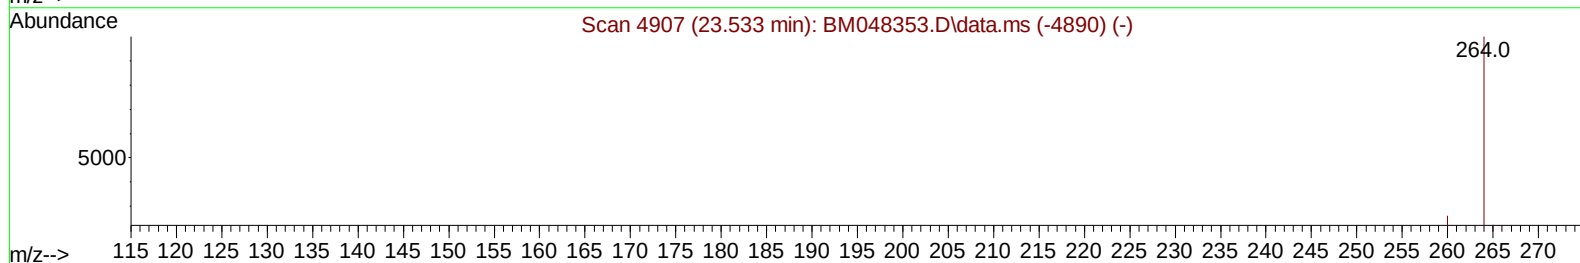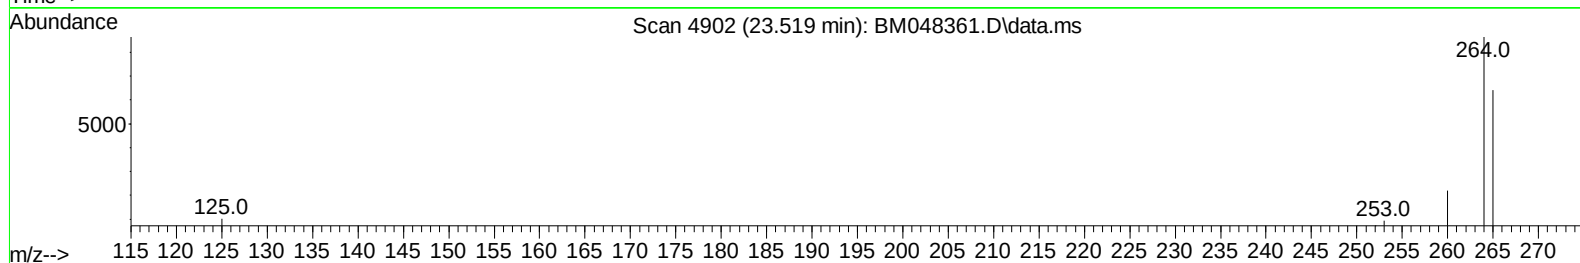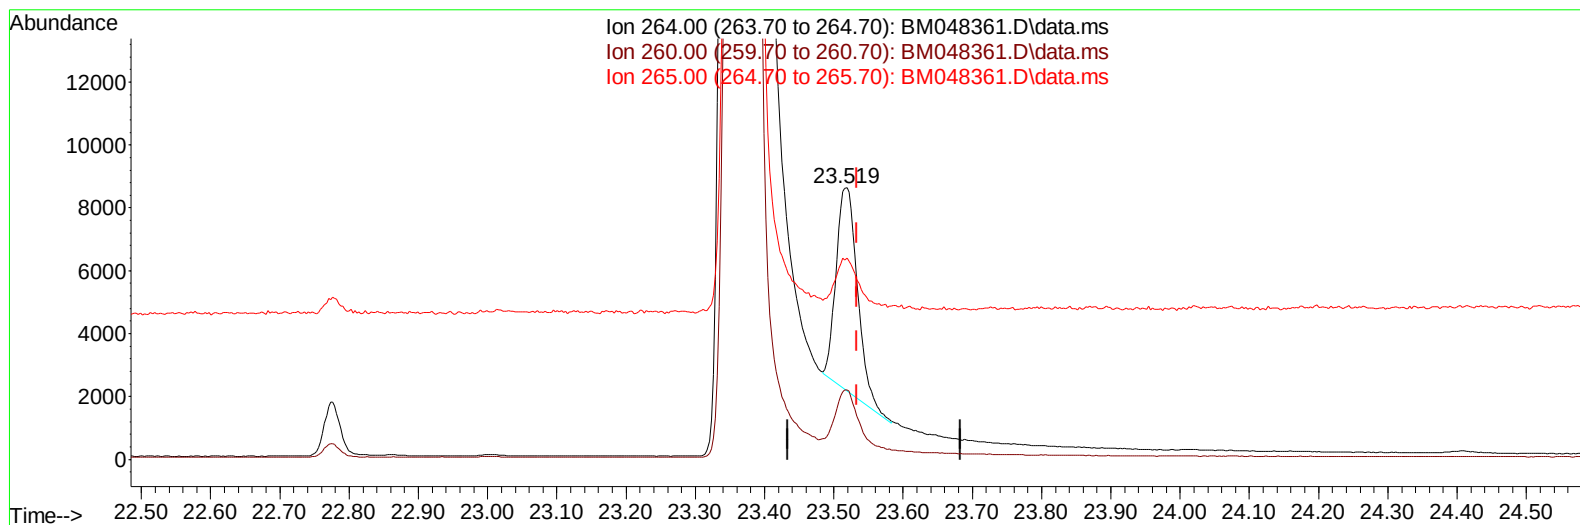

TIC: BM048361.D\data.ms

(23) Perylene-d12 (I)

23.519min (-0.015) 0.40 ng/ul m

response 13720

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.51
265.00	120.80	74.27#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

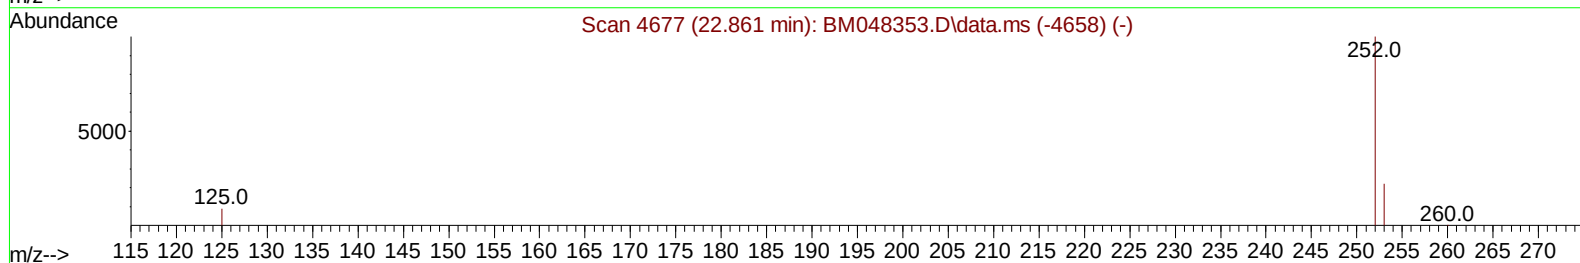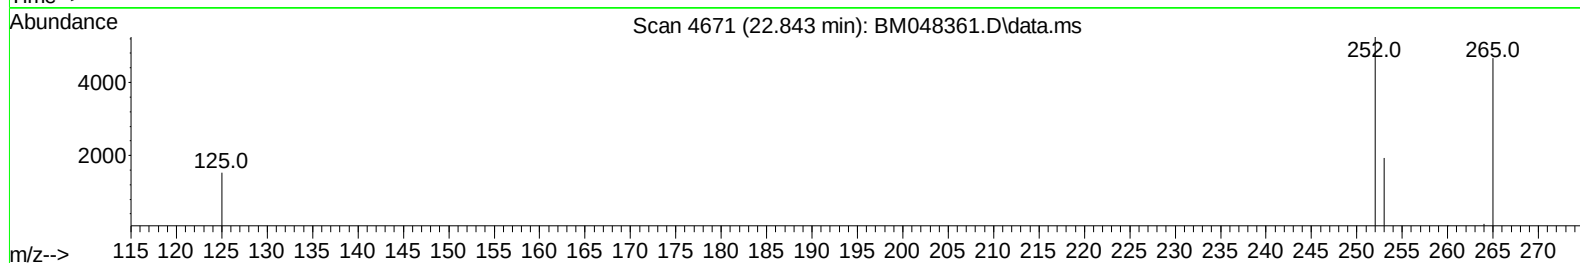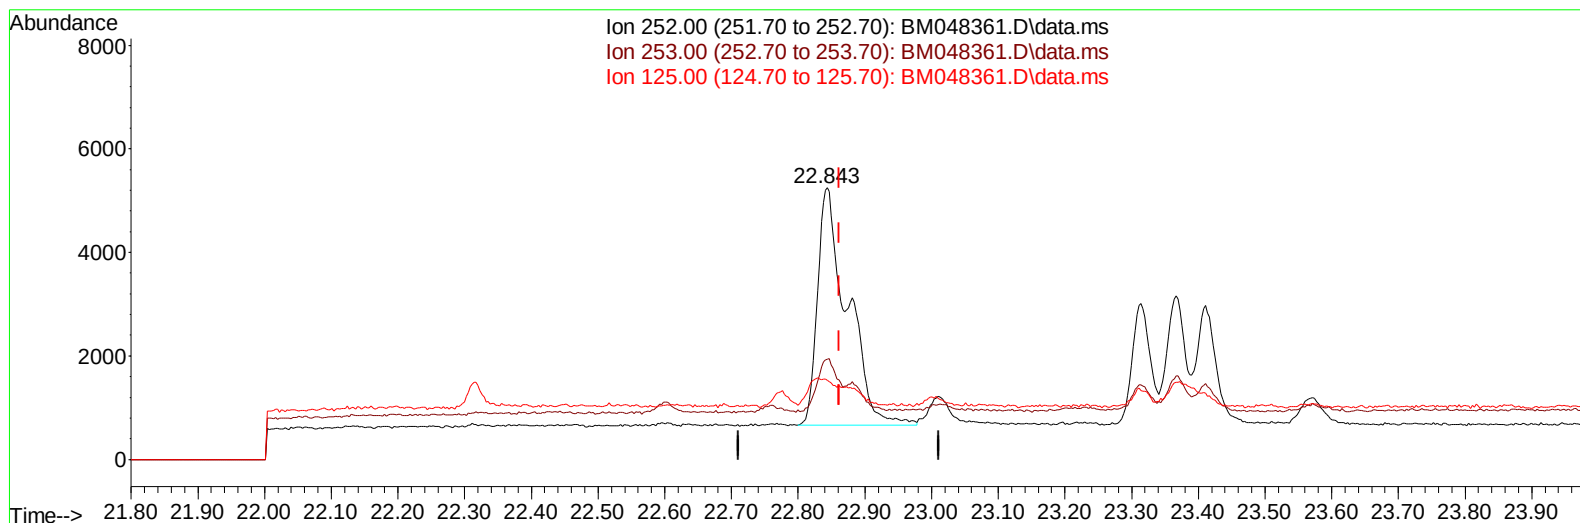

TIC: BM048361.D\data.ms

(24) Benzo(b)fluoranthene

22.843min (-0.018) 0.30 ng/u1

response 14249

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.70	36.98
125.00	19.00	29.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

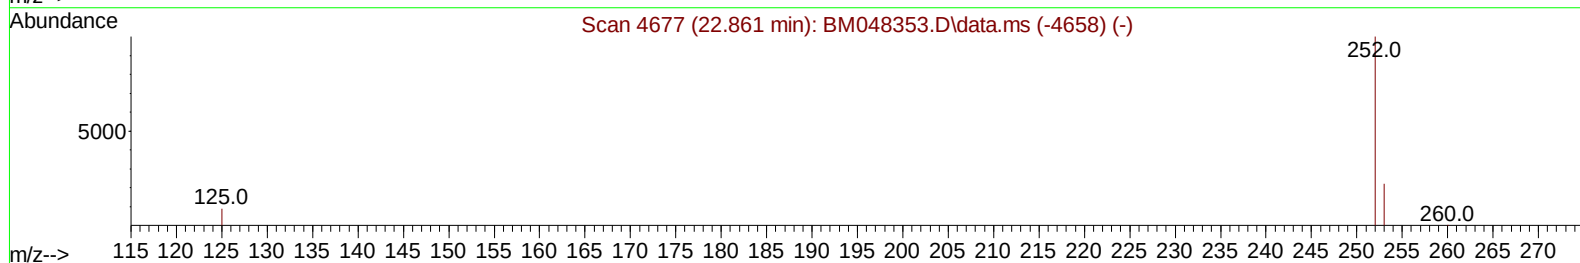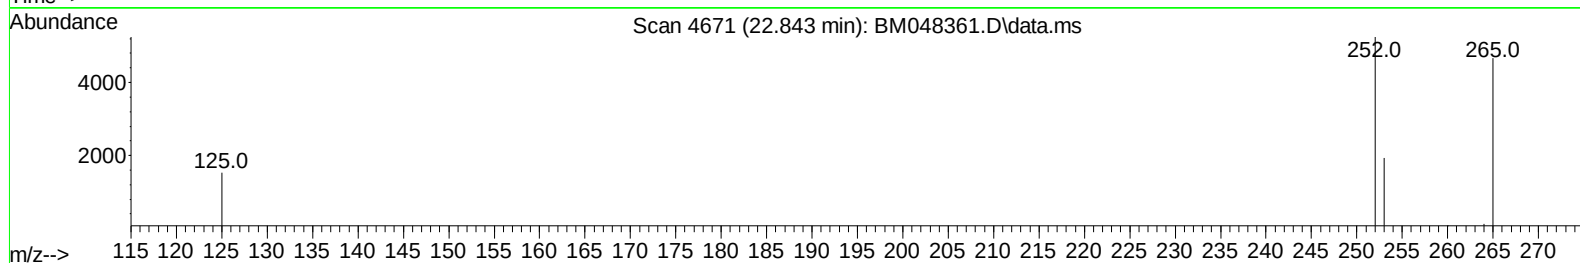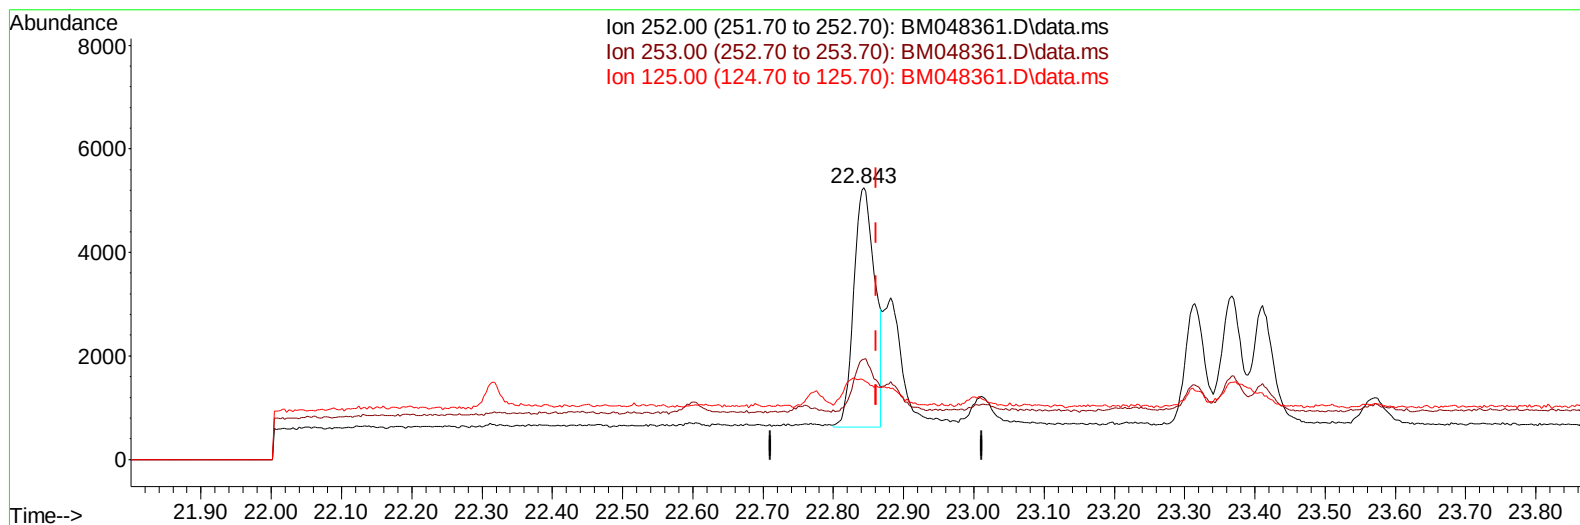

TIC: BM048361.D\data.ms

(24) Benzo(b)fluoranthene

22.843min (-0.018) 0.20 ng/ul m

response 9586

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.70	36.98
125.00	19.00	29.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

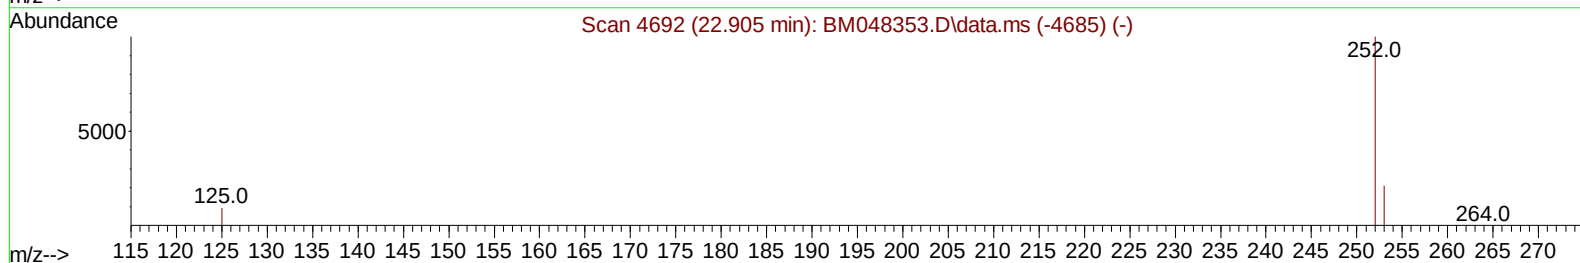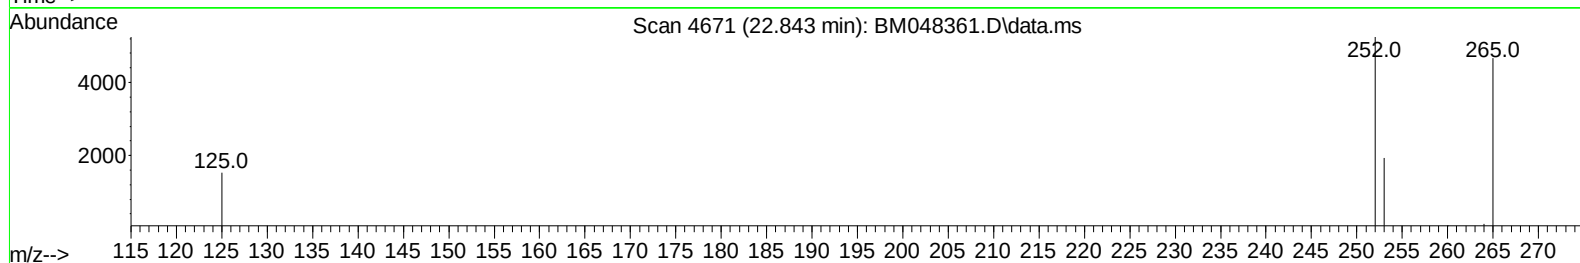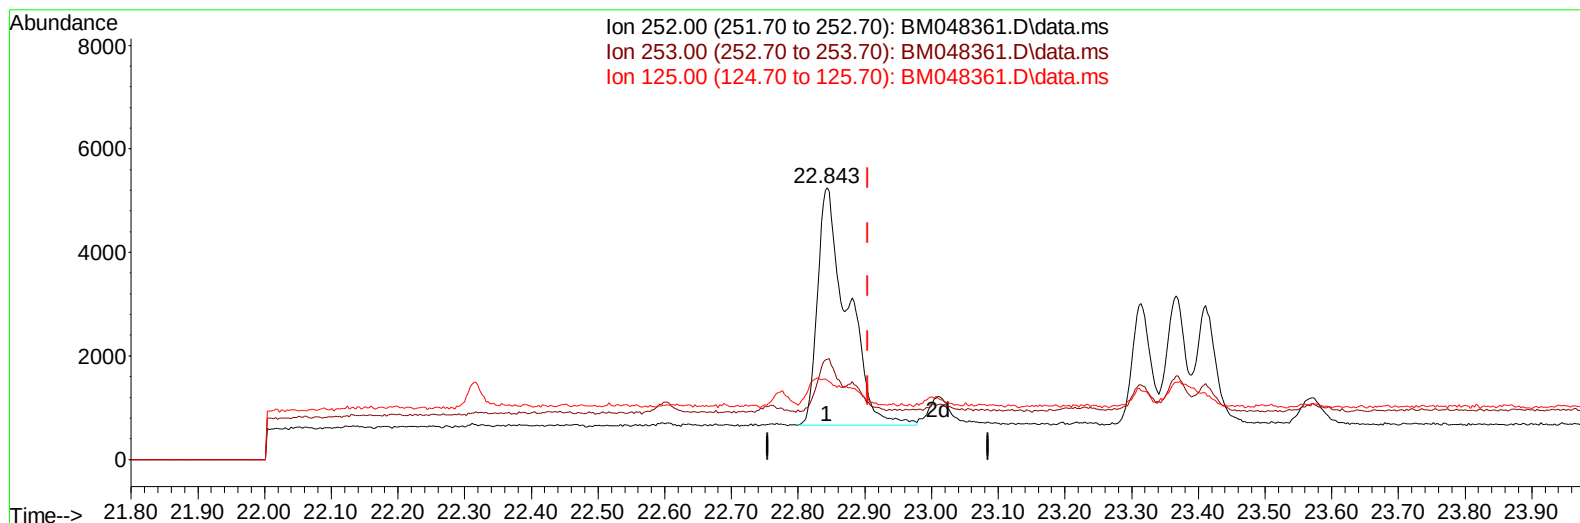

TIC: BM048361.D\data.ms

(25) Benzo(k)fluoranthene

22.843min (-0.061) 0.26 ng/u1

response 14249

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.20	36.98#
125.00	19.10	29.17#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

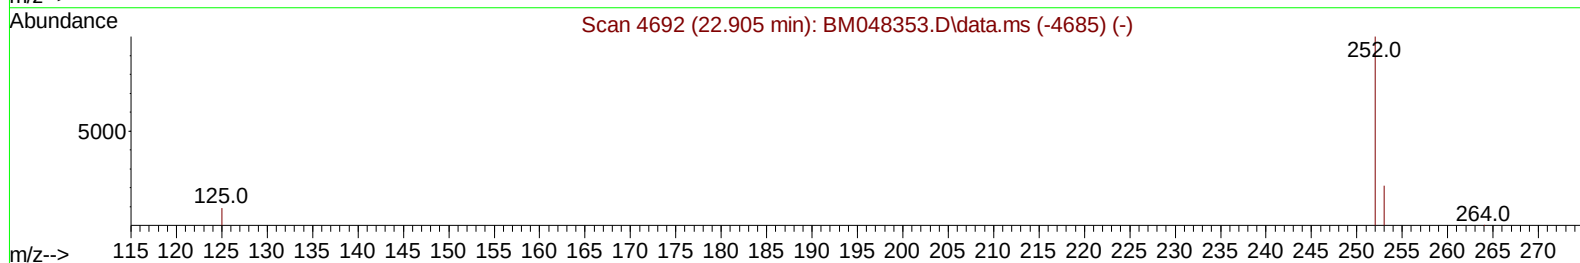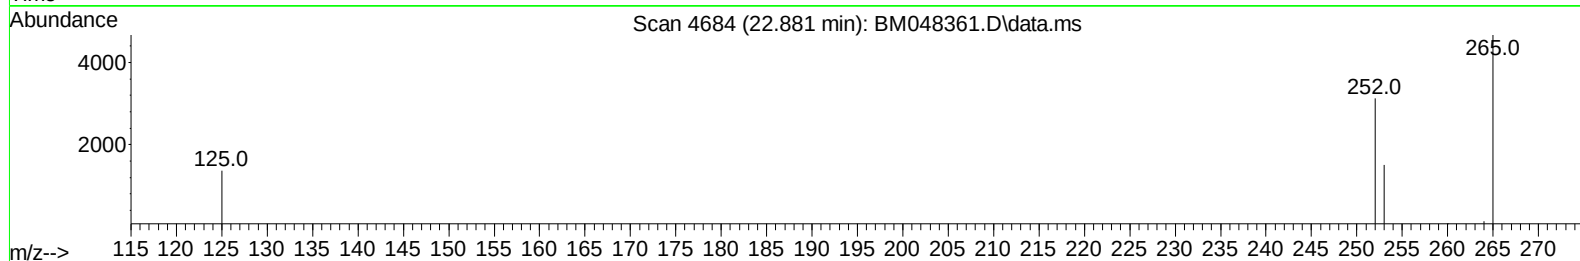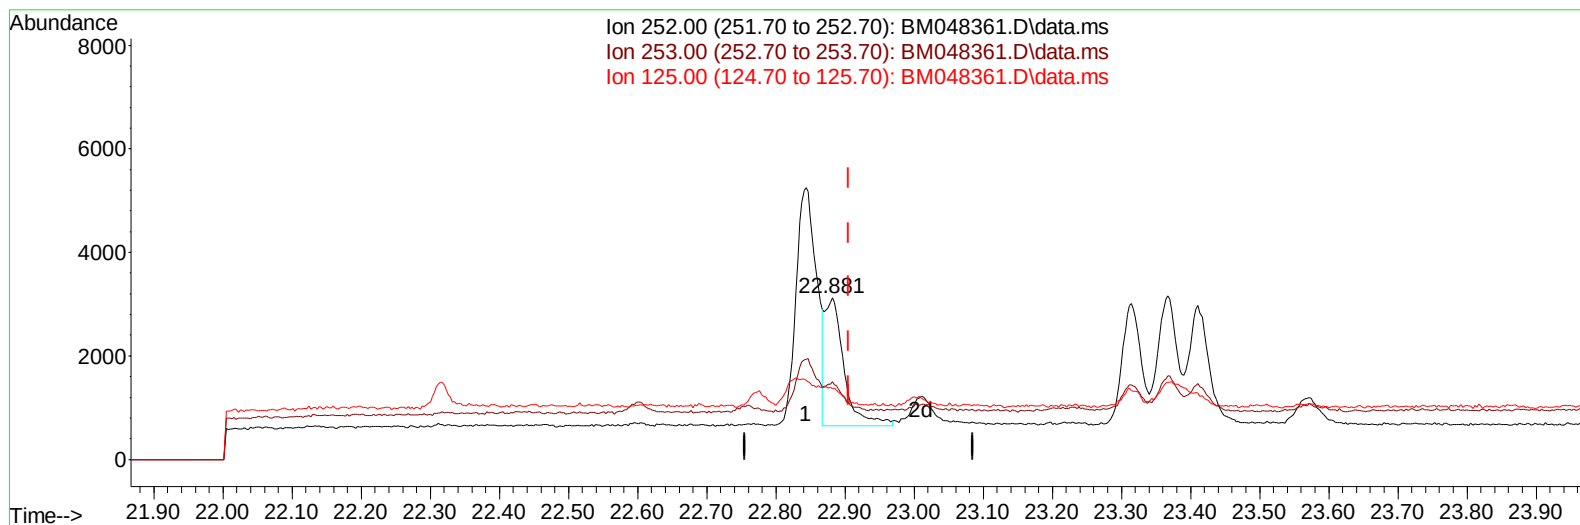

TIC: BM048361.D\data.ms

(25) Benzo(k)fluoranthene

22.881min (-0.023) 0.09 ng/ul m

response 4778

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.20	48.11#
125.00	19.10	43.78#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048361.D
 Acq On : 31 Oct 2024 17:11
 Operator : RC/JU
 Sample : P4530-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H28

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/04/2024

Quant Time: Oct 31 18:02:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.712	152		5006	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.497	136		16087	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.354	164		8718	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.095	188		18048m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.286	240		16109m	0.400	ng/ul	0.00
23) Perylene-d12	23.519	264		13720m	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.164	96		29394	4.781	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.113	152		7009	0.342	ng/ul	-0.03
18) Fluoranthene-d10	19.128	212		16807	0.411	ng/ul	0.00
Target Compounds							Qvalue
7) 2-Methylnaphthalene	12.190	142		1393	0.056	ng/ul	100
8) 1-Methylnaphthalene	12.405	142		799	0.030	ng/ul	92
19) Fluoranthene	19.155	202		3777	0.068	ng/ul#	81
20) Pyrene	19.513	202		6580	0.110	ng/ul#	86
21) Benzo(a)anthracene	21.274	228		4659	0.097	ng/ul#	91
22) Chrysene	21.321	228		3761	0.057	ng/ul	93
24) Benzo(b)fluoranthene	22.843	252		9586m	0.204	ng/ul	
25) Benzo(k)fluoranthene	22.881	252		4778m	0.086	ng/ul	
26) Benzo(a)pyrene	23.411	252		4375	0.099	ng/ul#	72
27) Indeno(1,2,3-cd)pyrene	25.822	276		3842	0.062	ng/ul#	95
28) Dibenzo(a,h)anthracene	25.822	278		1041	0.022	ng/ul#	1
29) Benzo(g,h,i)perylene	26.513	276		3584	0.069	ng/ul#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048361.D
Acq On : 31 Oct 2024 17:11
Operator : RC/JU
Sample : P4530-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H28

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

