




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

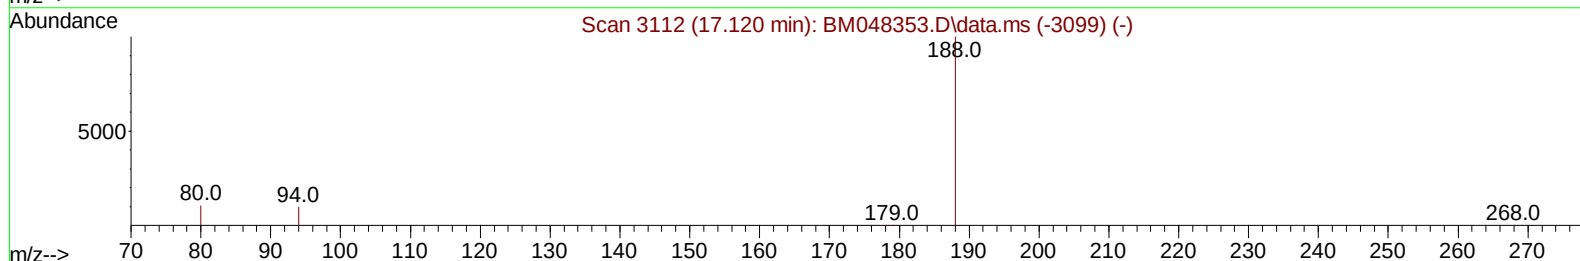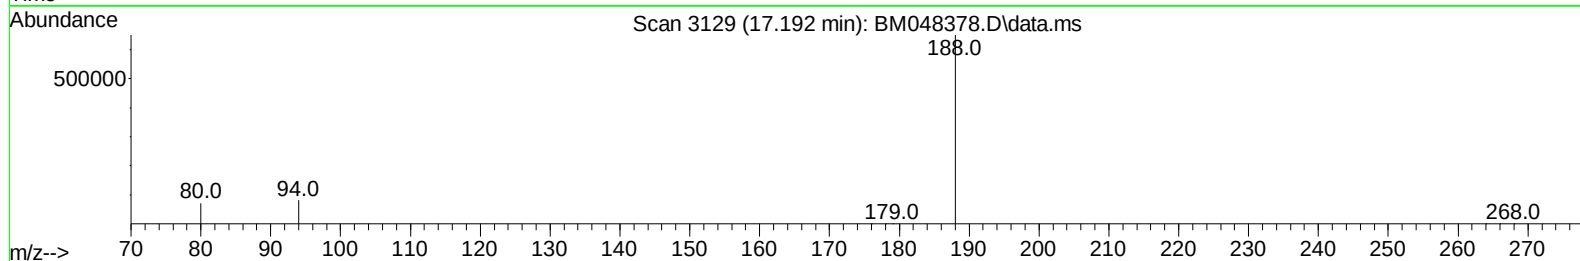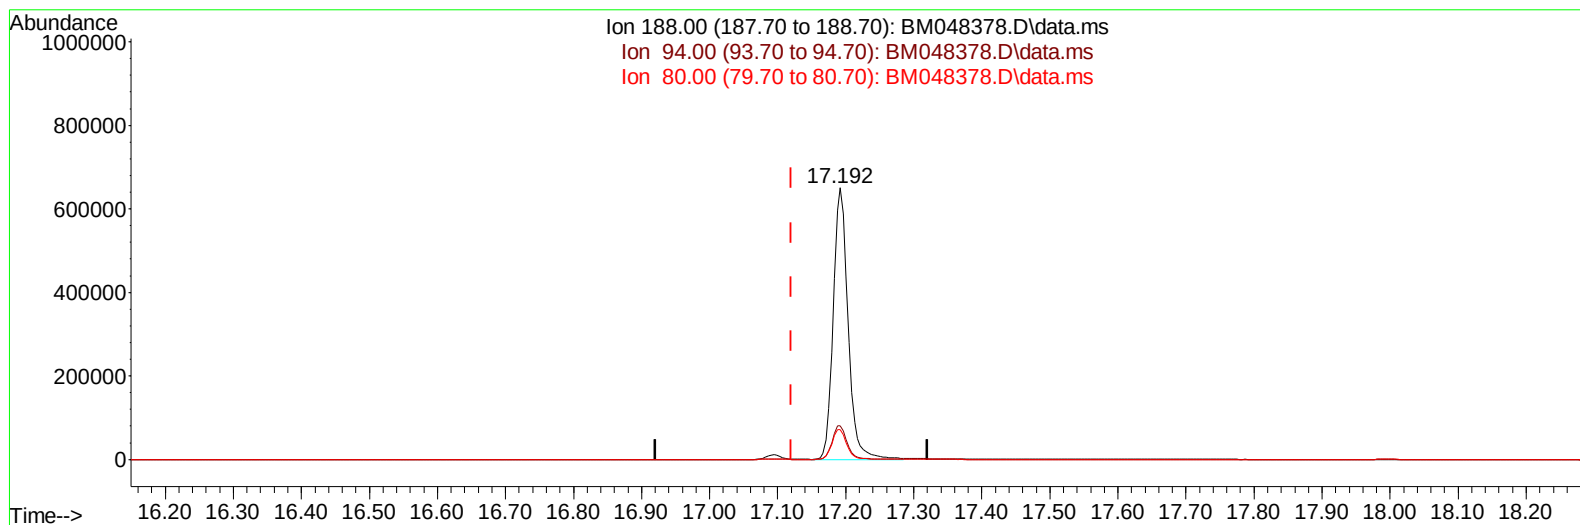

TIC: BM048378.D\data.ms

(13) Phenanthrene-d10 (I)

17.192min (+ 0.072) 0.40 ng/u1

response 983463

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.50	12.48
80.00	12.10	10.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

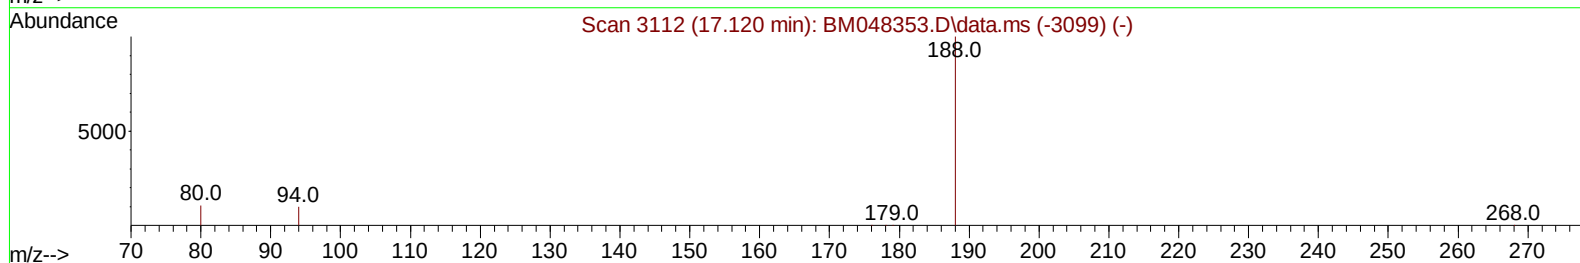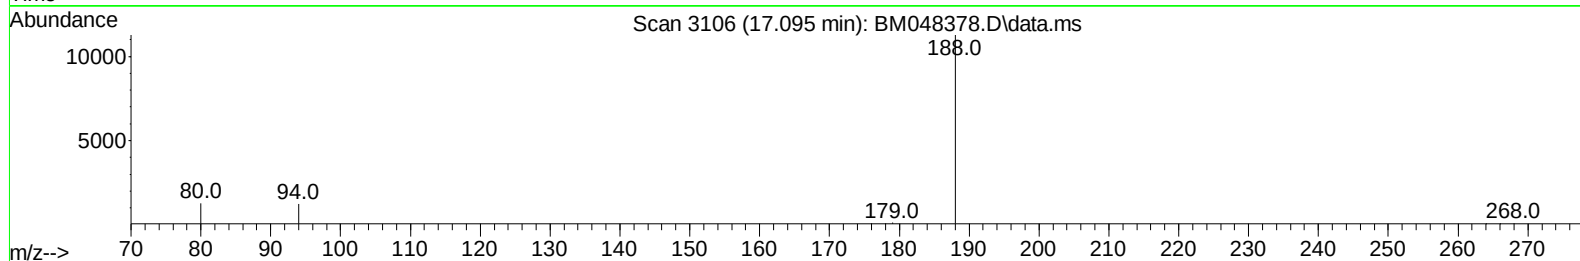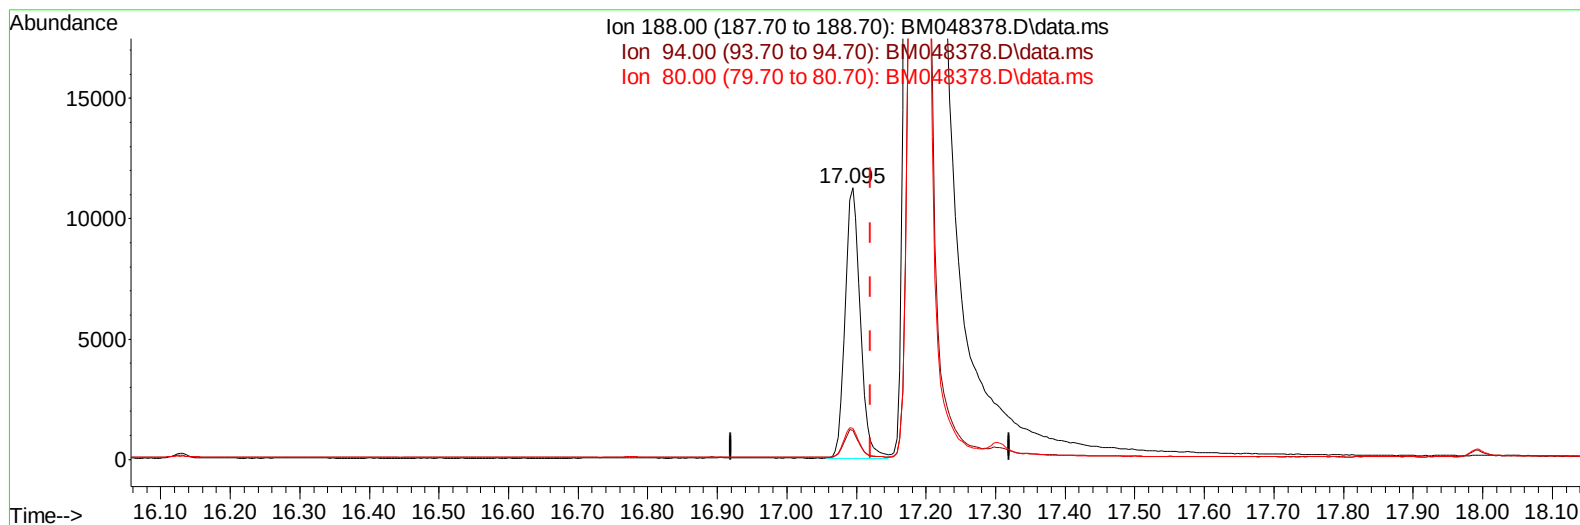

TIC: BM048378.D\data.ms

(13) Phenanthrene-d10 (I)

17.095min (-0.025) 0.40 ng/ul m

response 16905

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.50	10.78
80.00	12.10	11.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

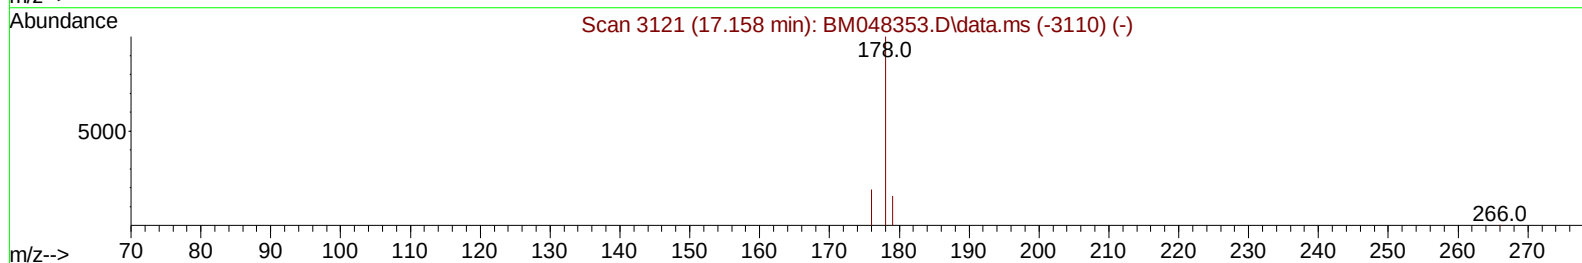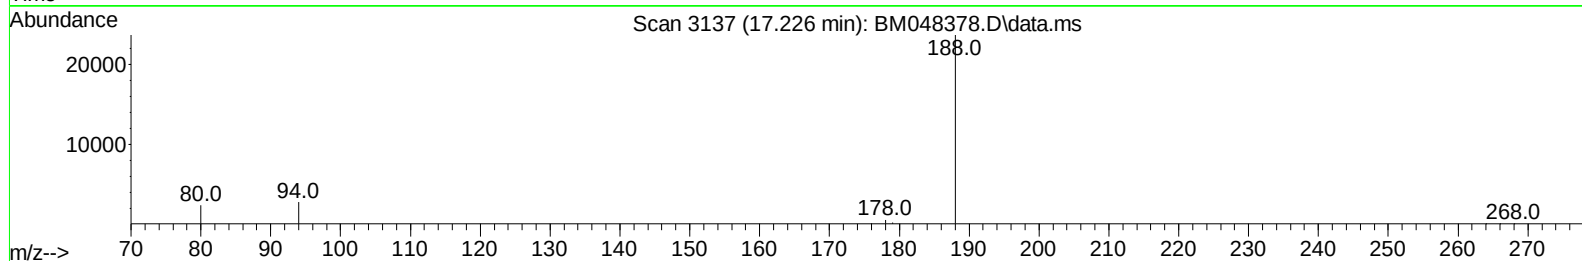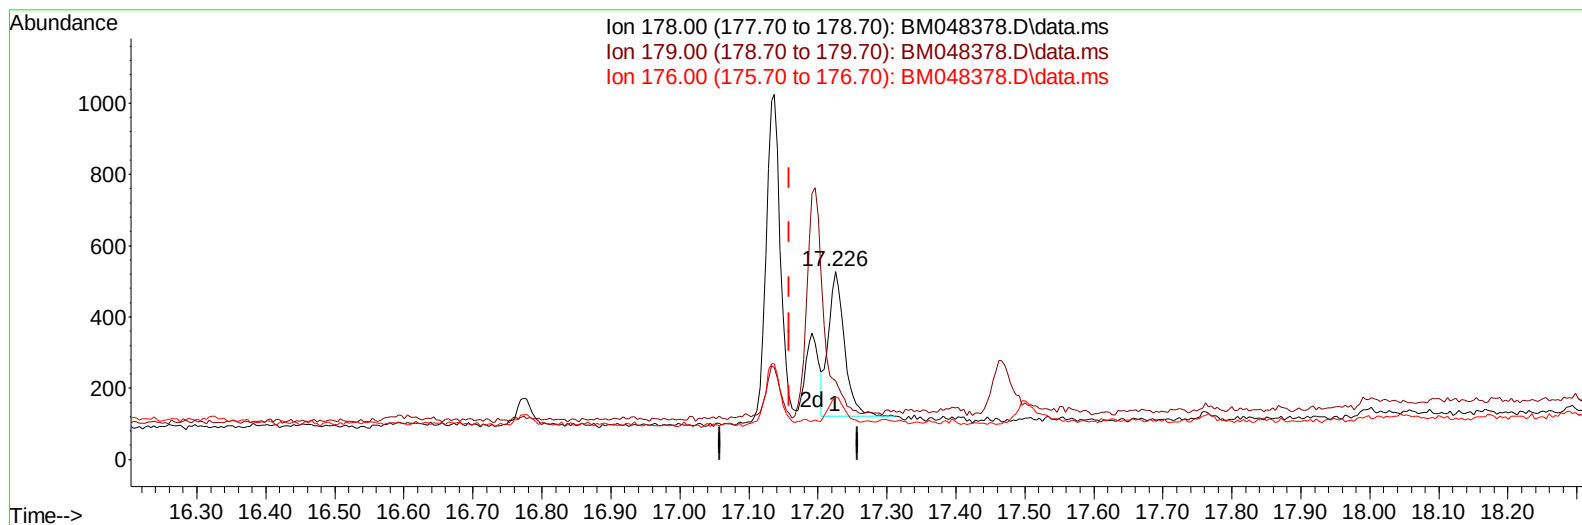

TIC: BM048378.D\data.ms

(15) Phenanthrene

17.226min (+ 0.067) 0.02 ng/u1

response 653

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.40	41.86#
176.00	20.00	33.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048378.D
 Acq On : 01 Nov 2024 04:05
 Operator : RC/JU
 Sample : P4592-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/04/2024

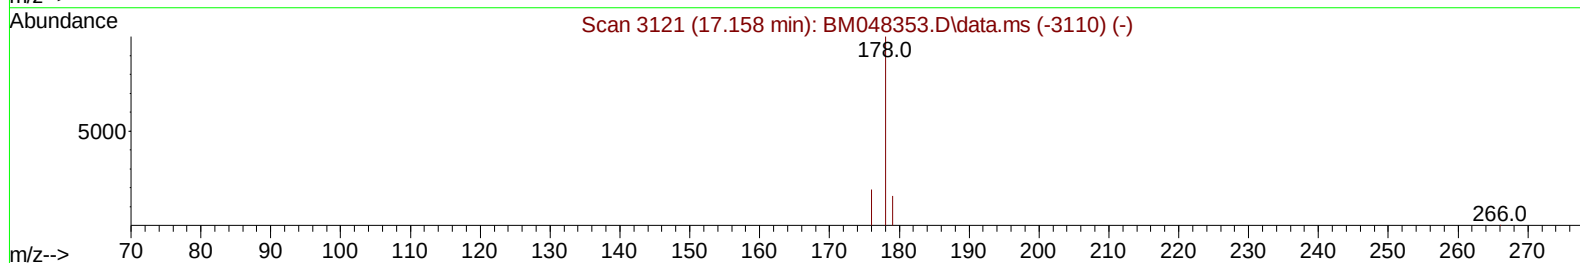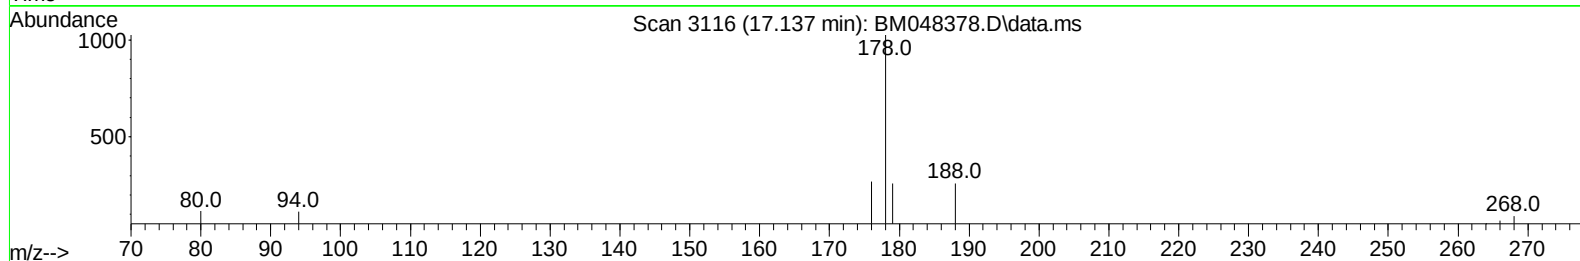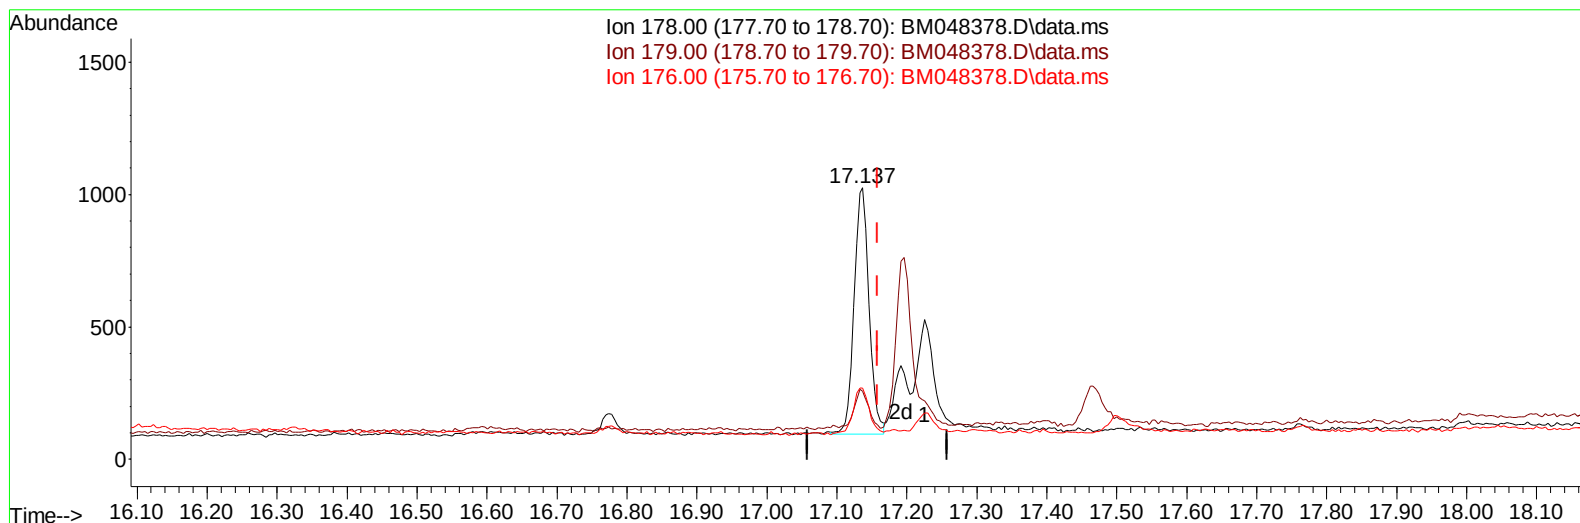

TIC: BM048378.D\data.ms

(15) Phenanthrene

17.137min (-0.021) 0.03 ng/ul m

response 1365

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.40	25.17#
176.00	20.00	26.24#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

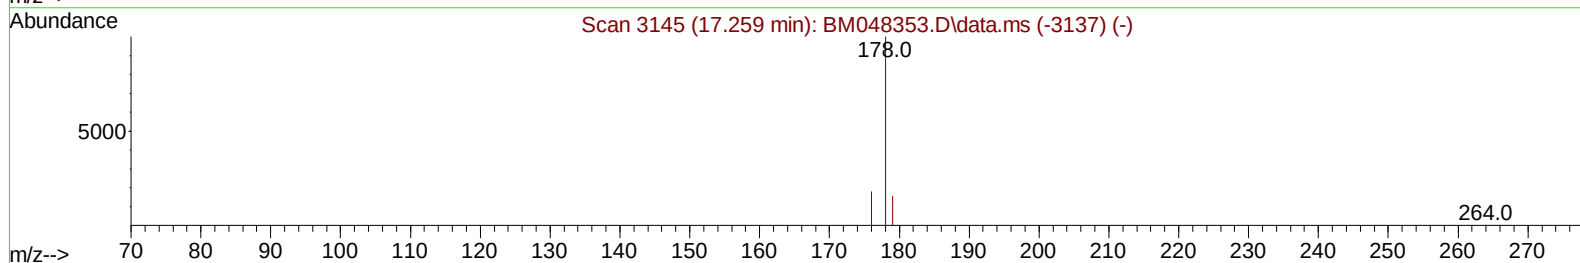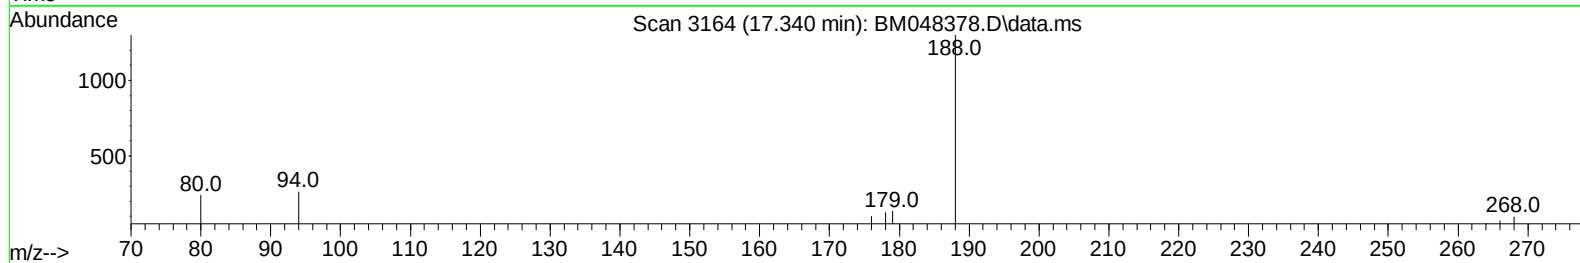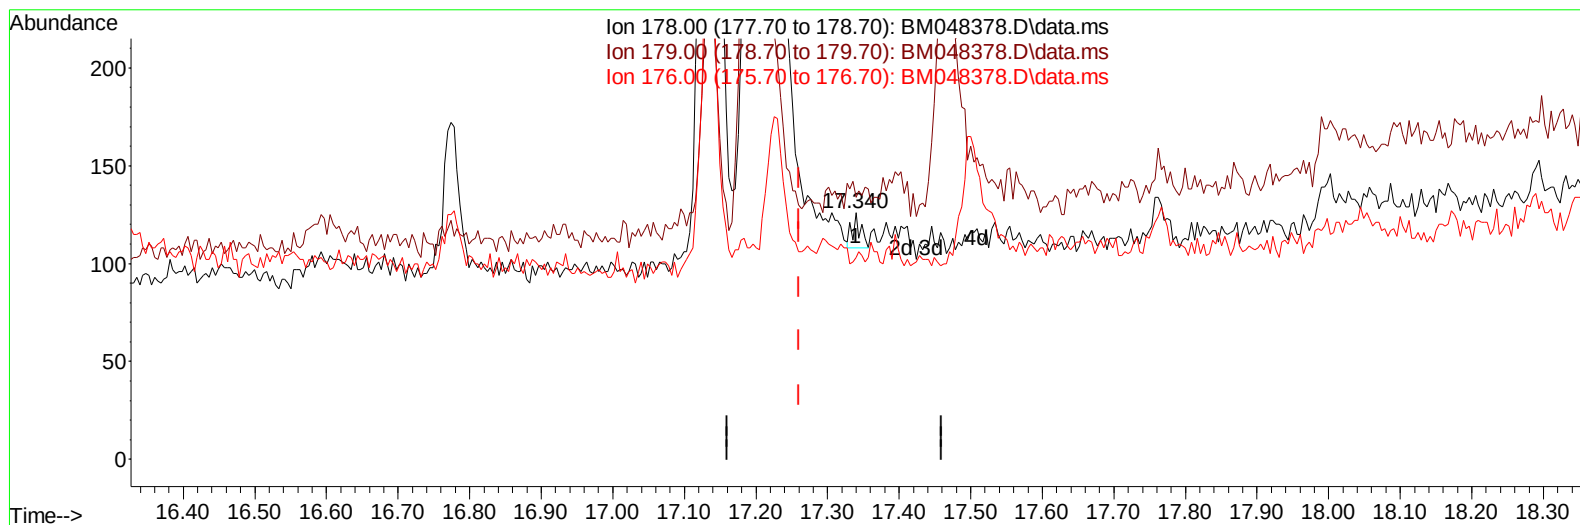

TIC: BM048378.D\data.ms

(16) Anthracene

17.340min (+ 0.080) 0.00 ng/u1

response 14

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	106.35#
176.00	19.70	81.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

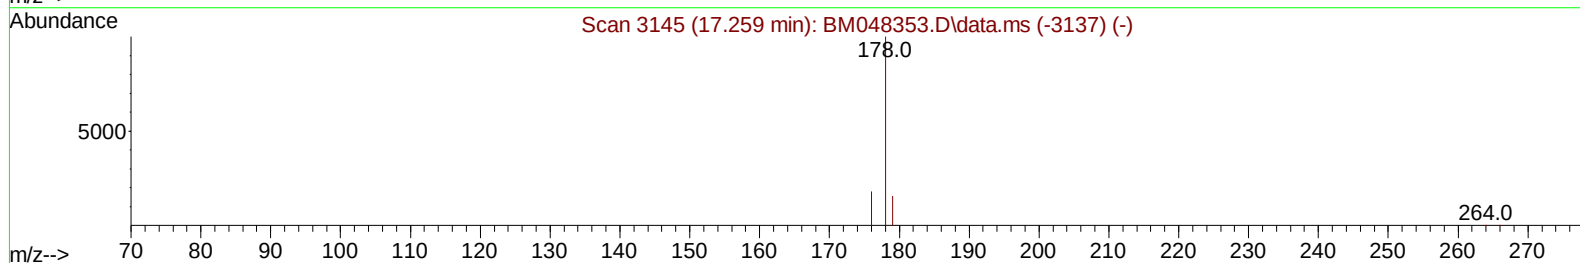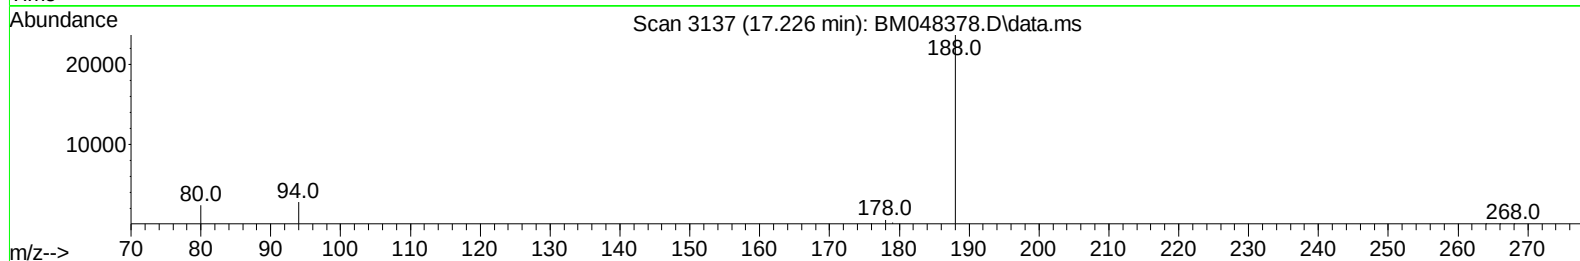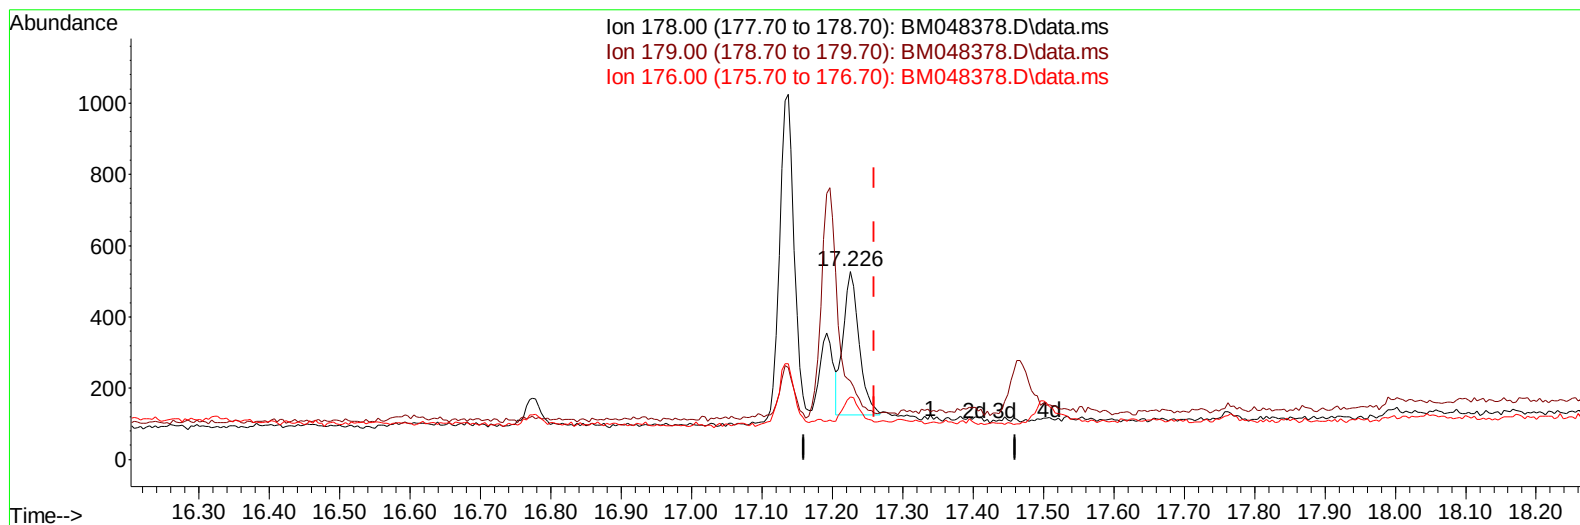

TIC: BM048378.D\data.ms

(16) Anthracene

17.226min (-0.034) 0.02 ng/ul m

response 632

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	41.86#
176.00	19.70	33.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

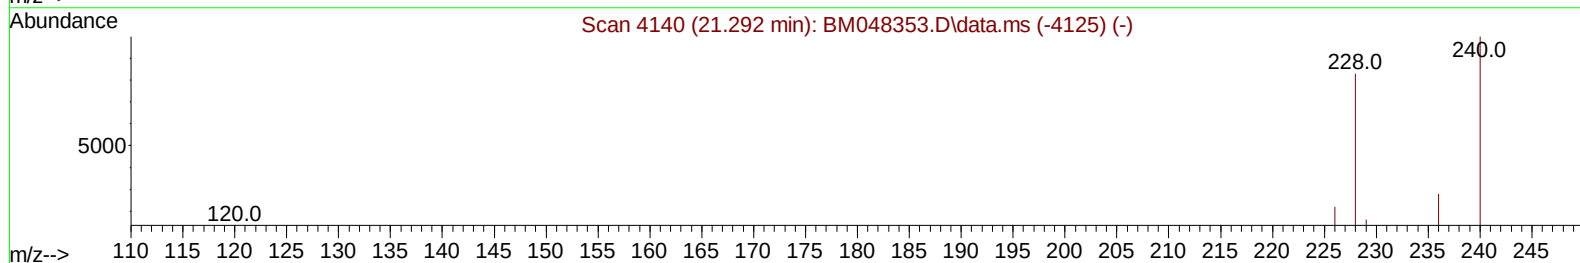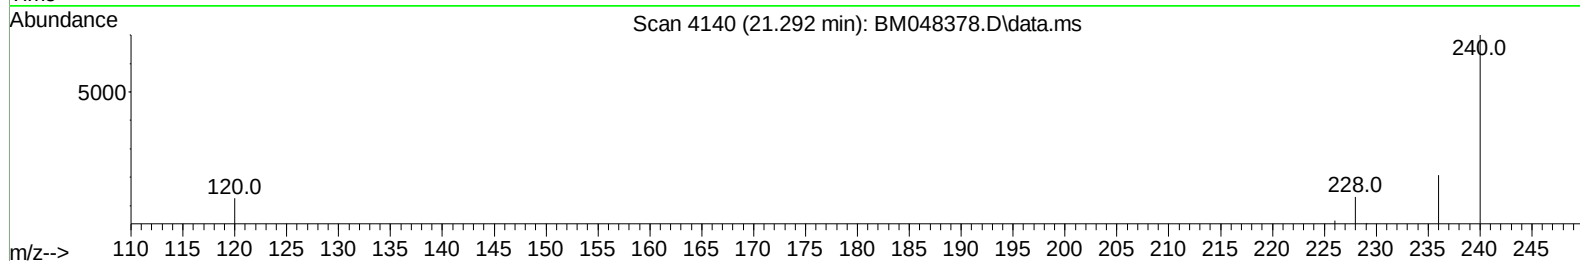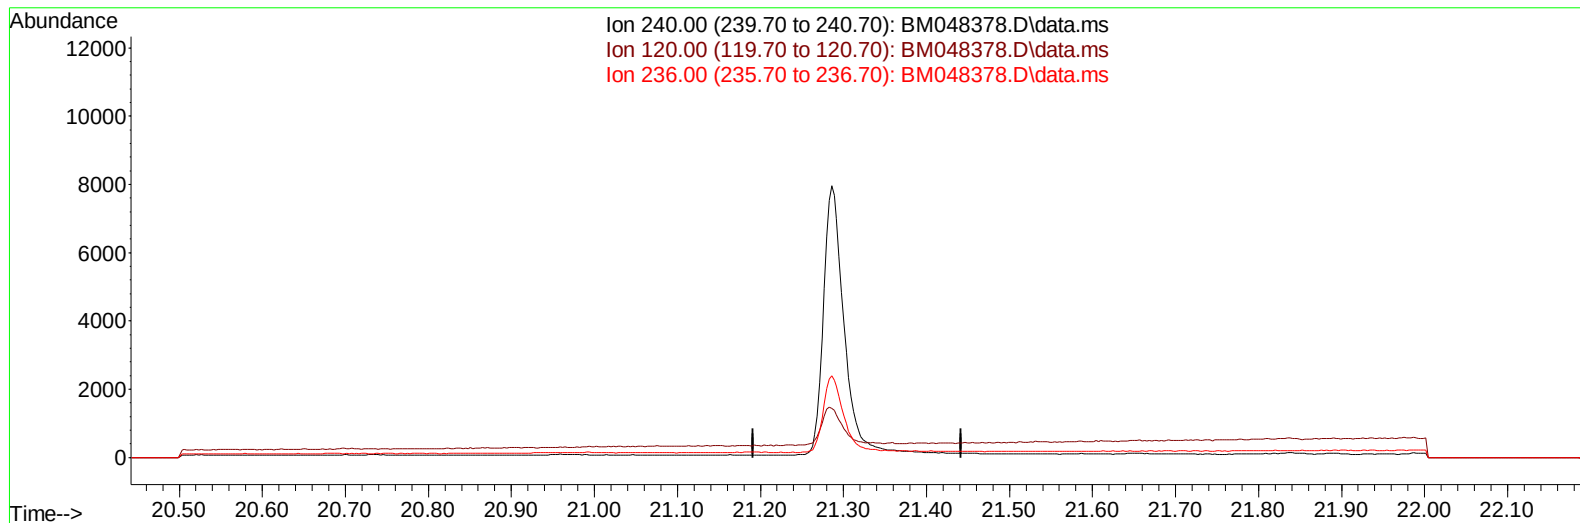

TIC: BM048378.D\data.ms

(17) Chrysene-d12

21.292min (-21.292) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	19.00	0.00#
236.00	29.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

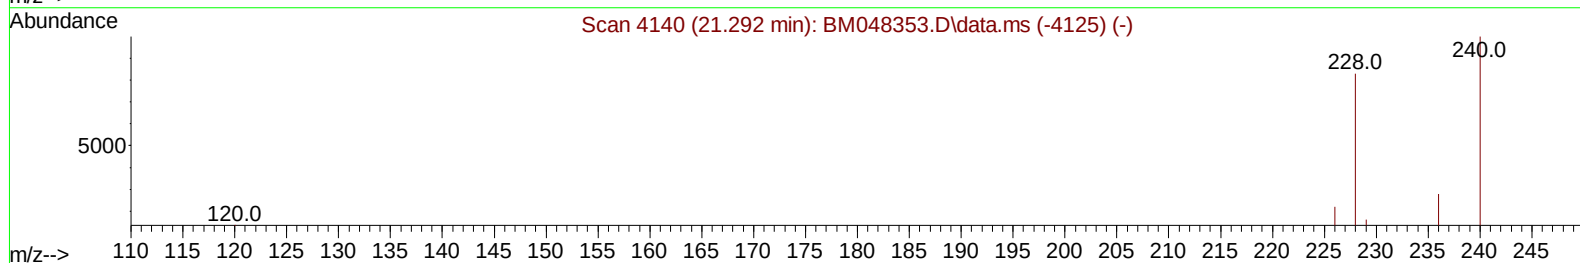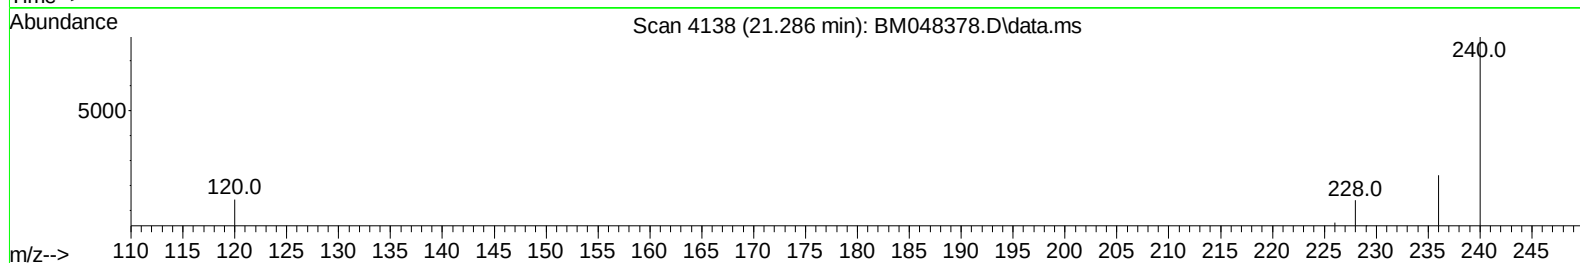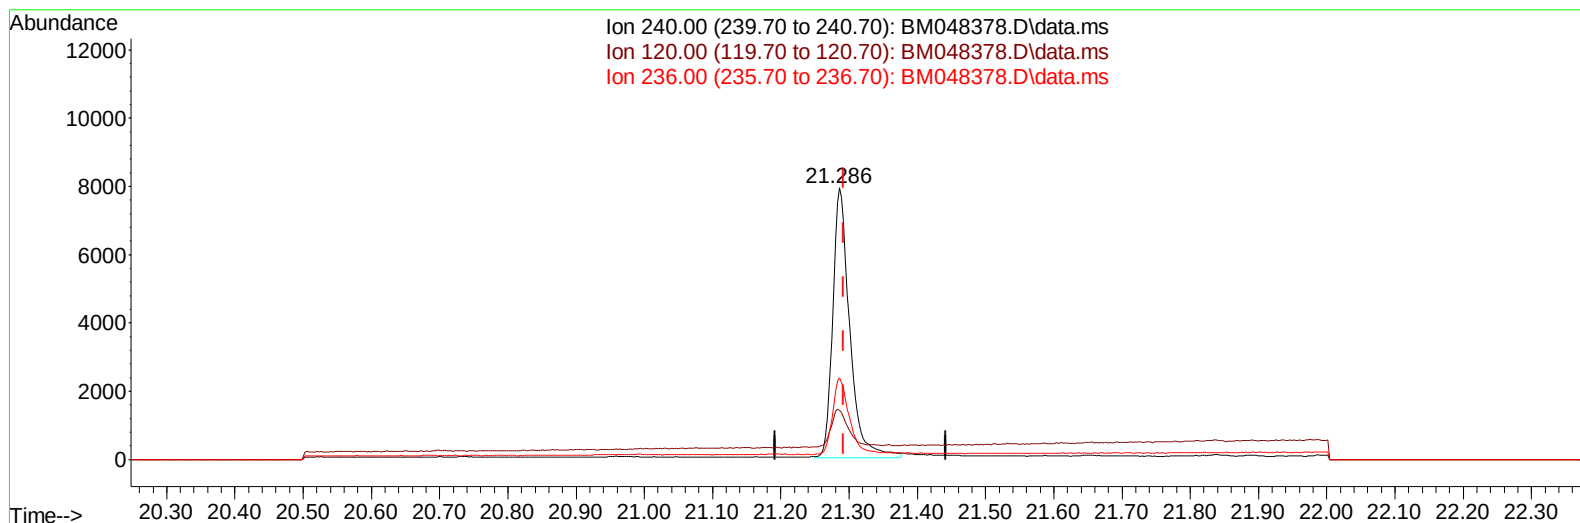

TIC: BM048378.D\data.ms

(17) Chrysene-d12

21.286min (-0.006) 0.40 ng/ul m

response 13838

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	19.00	17.99
236.00	29.90	30.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

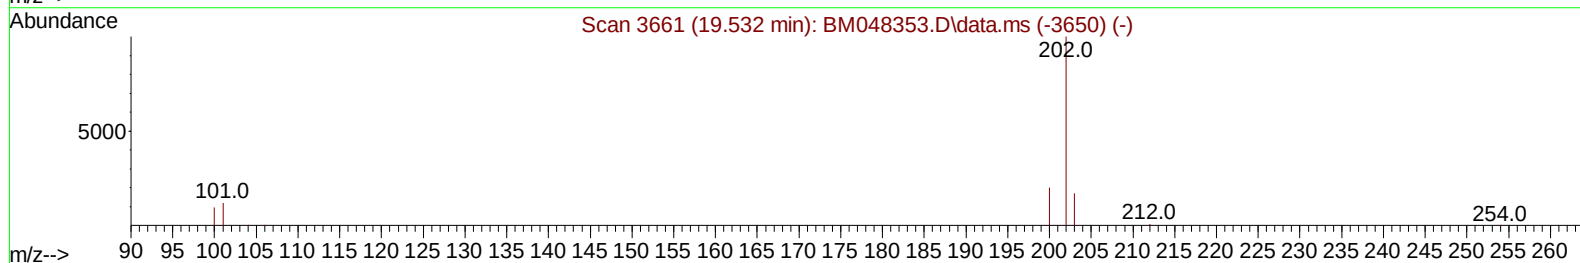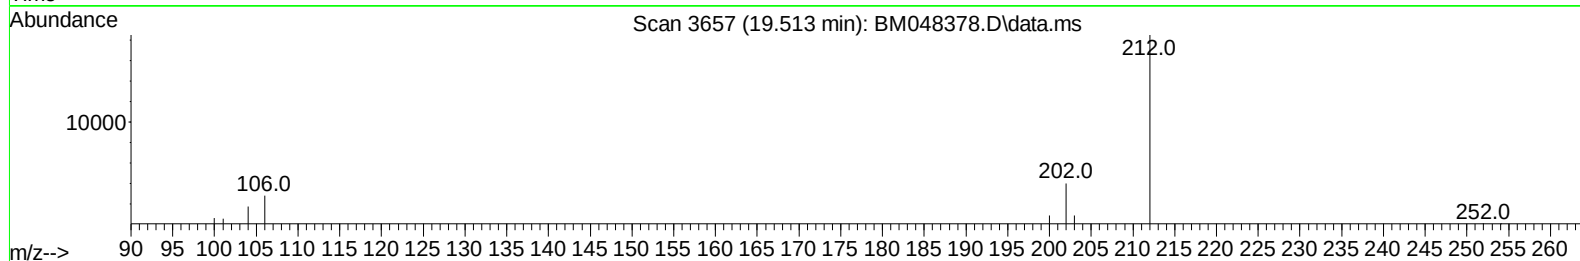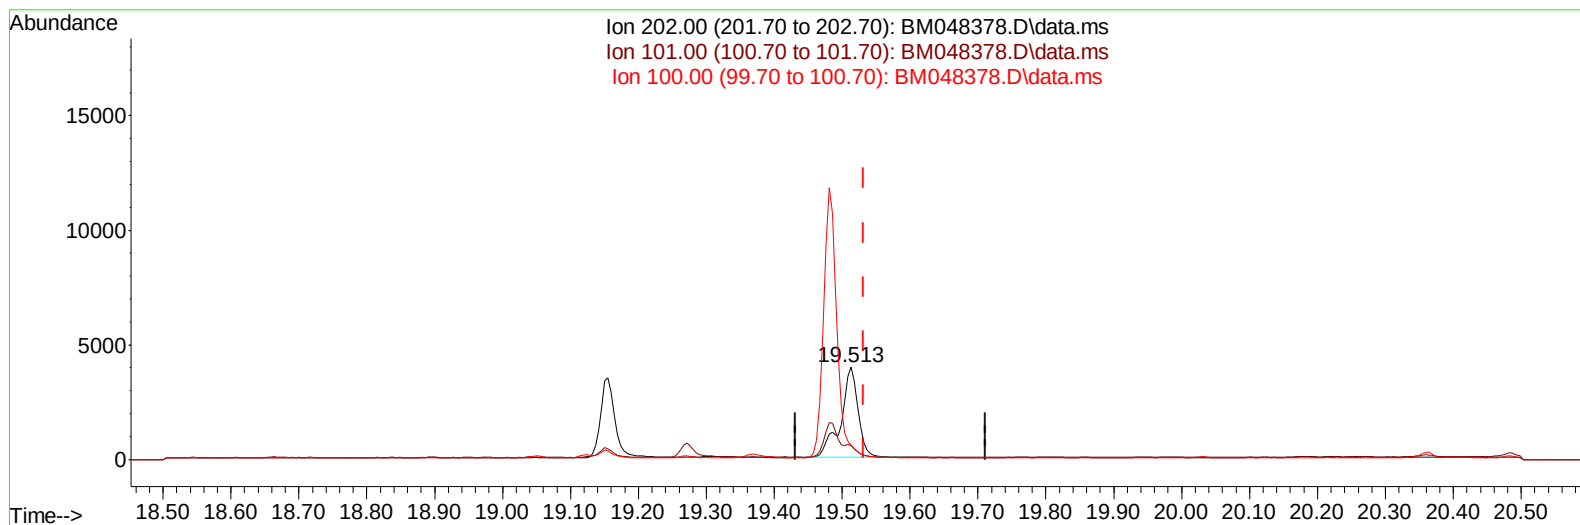

TIC: BM048378.D\data.ms

(20) Pyrene

19.513min (-0.019) 0.14 ng/u1

response 6990

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.50	15.05#
100.00	10.00	15.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

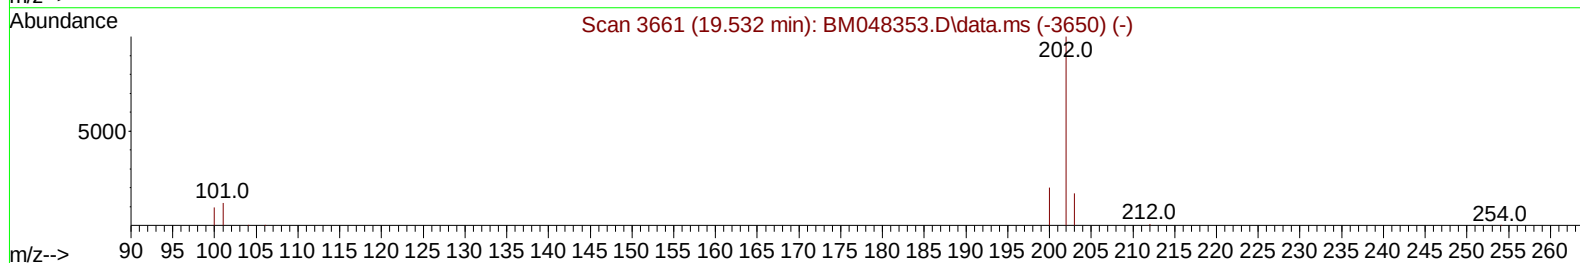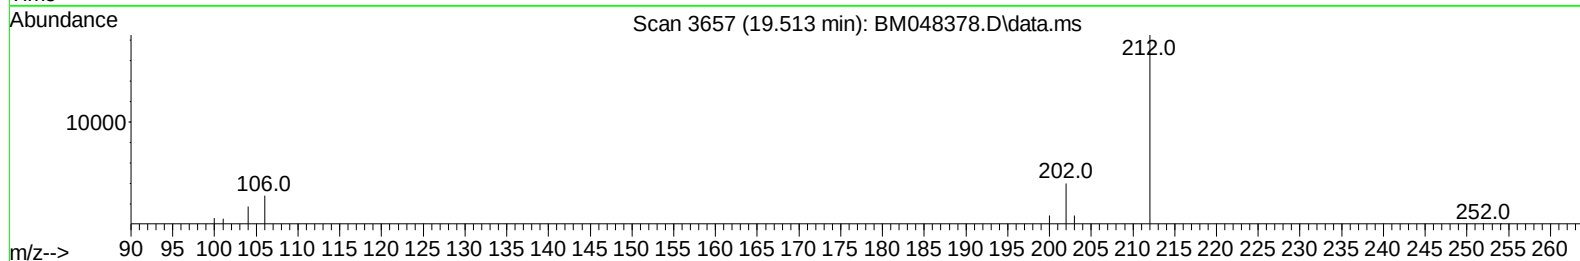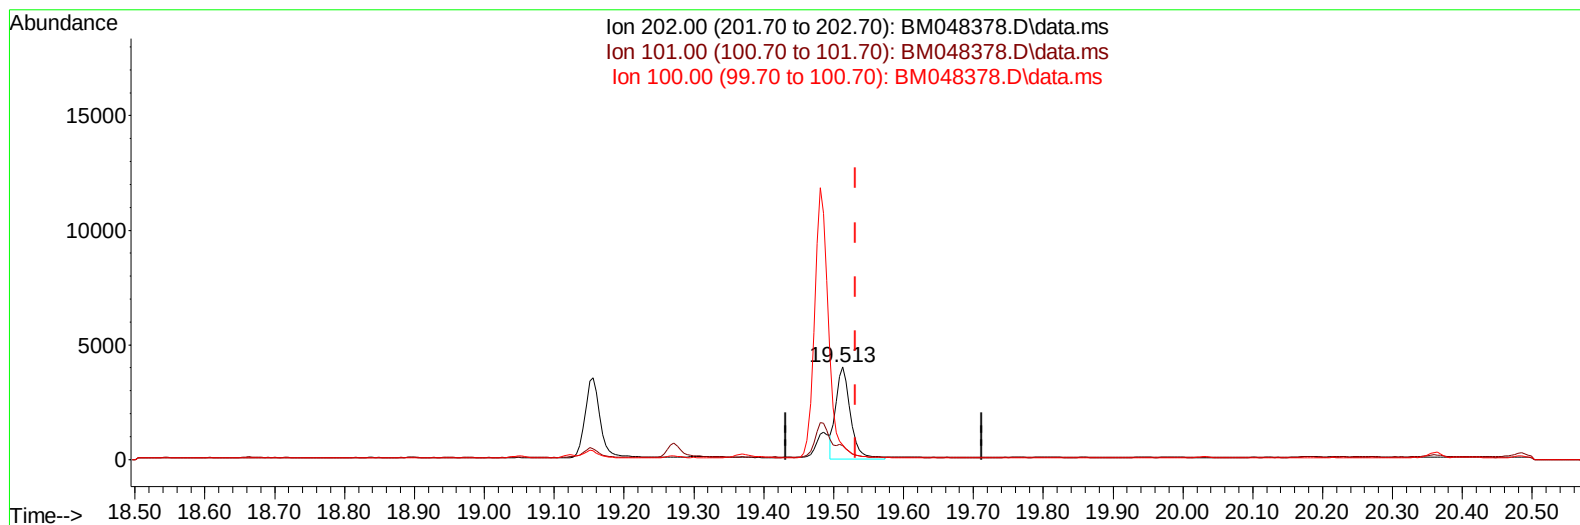

TIC: BM048378.D\data.ms

(20) Pyrene

19.513min (-0.019) 0.11 ng/ul m

response 5803

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.50	15.05#
100.00	10.00	15.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

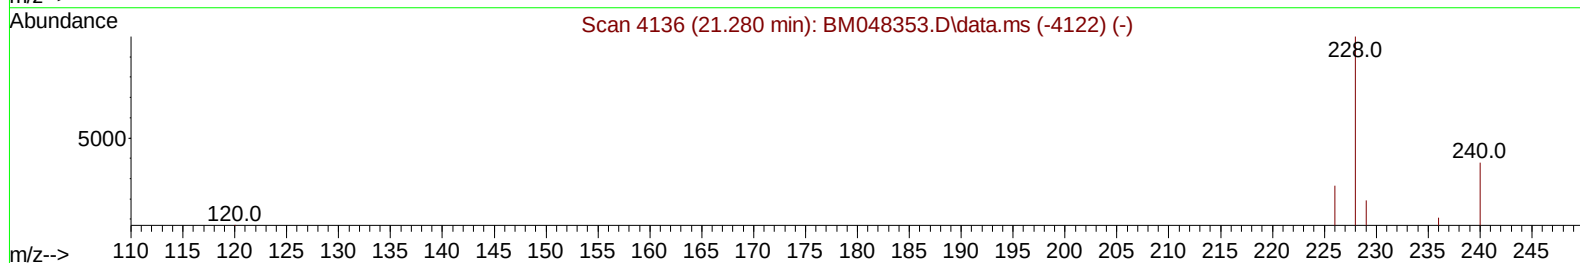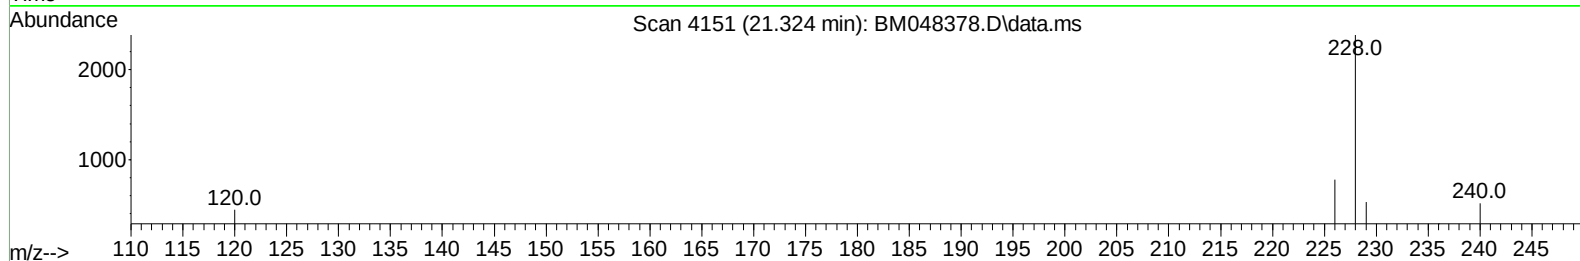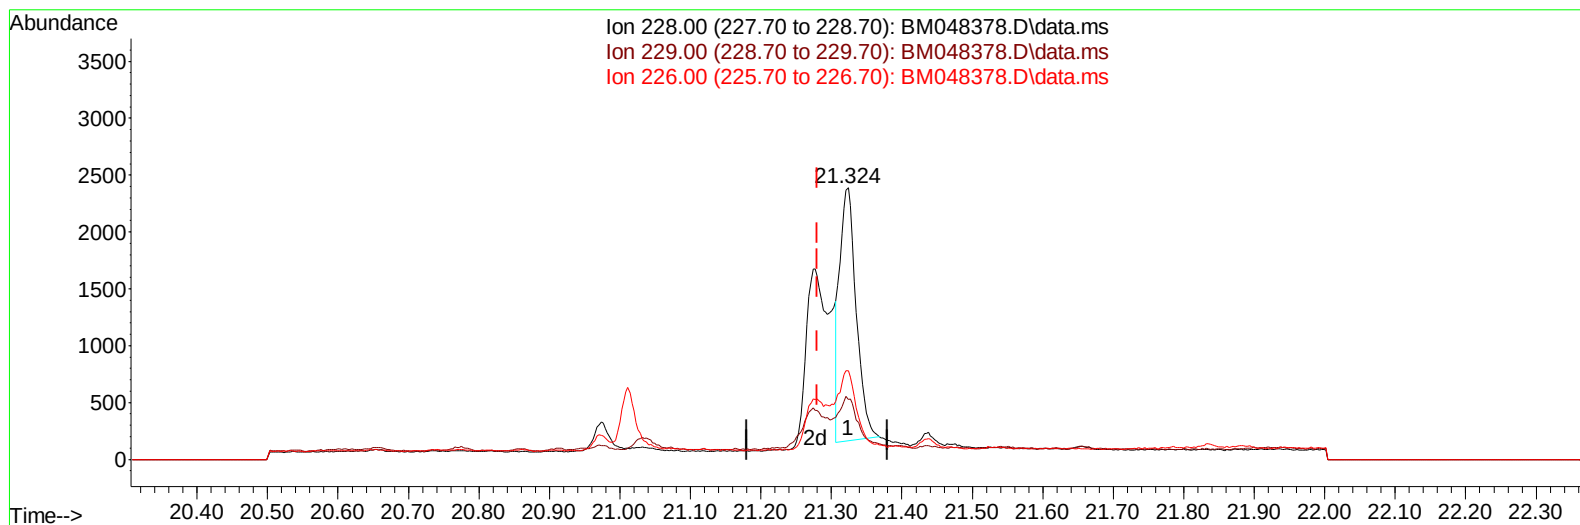

TIC: BM048378.D\data.ms

(21) Benzo(a)anthracene

21.324min (+ 0.044) 0.09 ng/u1

response 3606

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.90	22.16
226.00	27.60	32.64
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

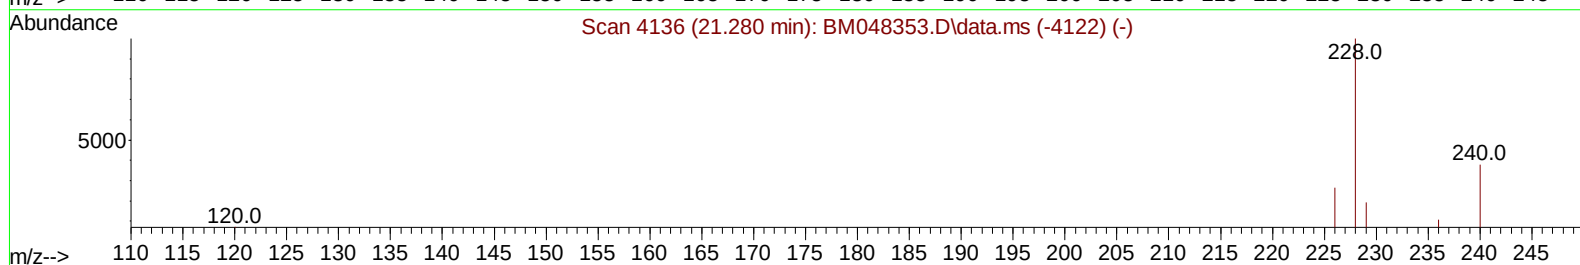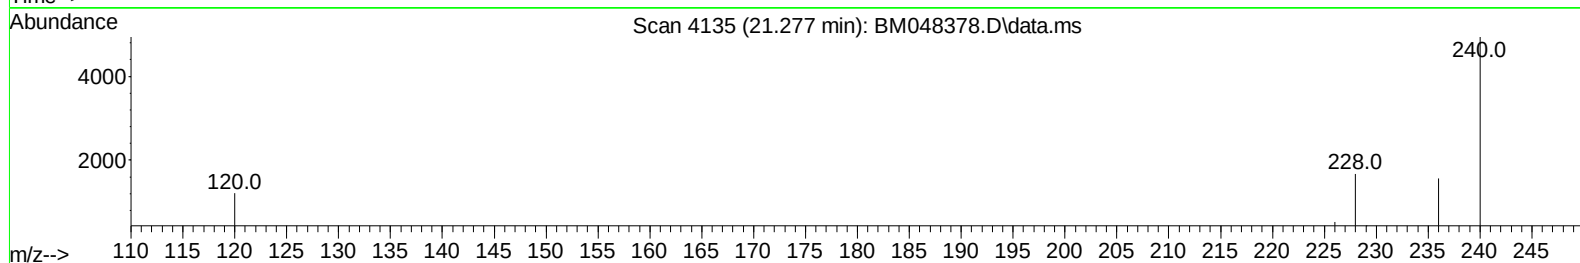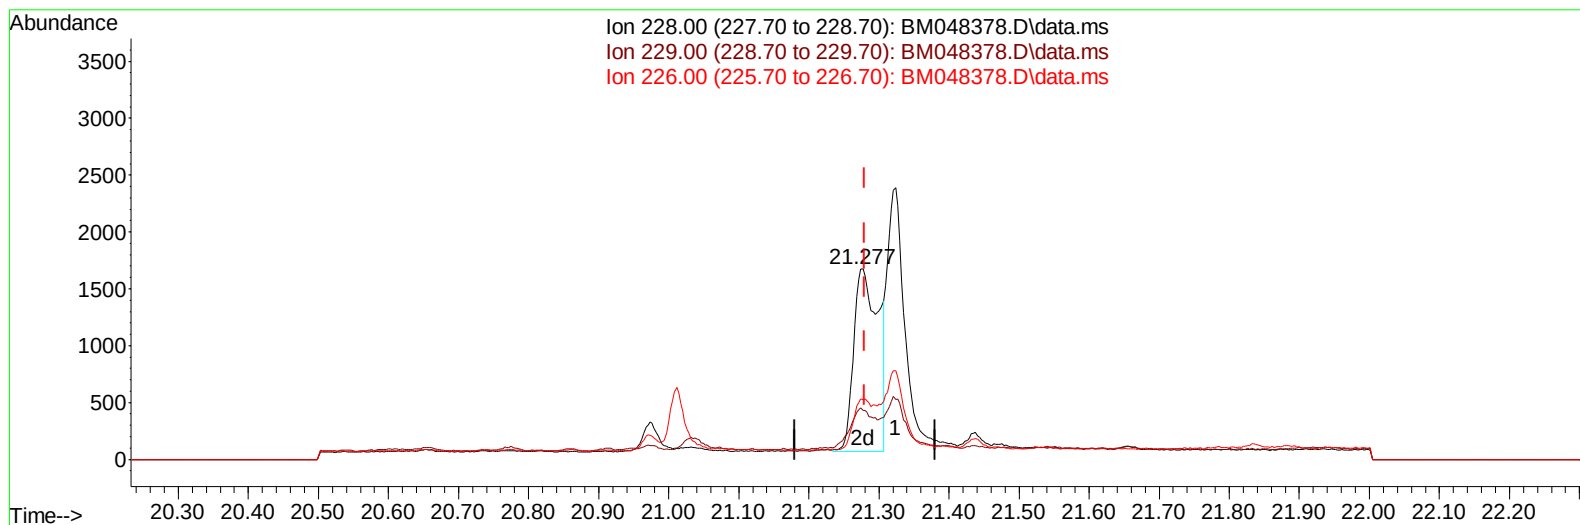

TIC: BM048378.D\data.ms

(21) Benzo(a)anthracene

21.277min (-0.003) 0.09 ng/u1 m

response 3885

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.90	25.73#
226.00	27.60	31.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

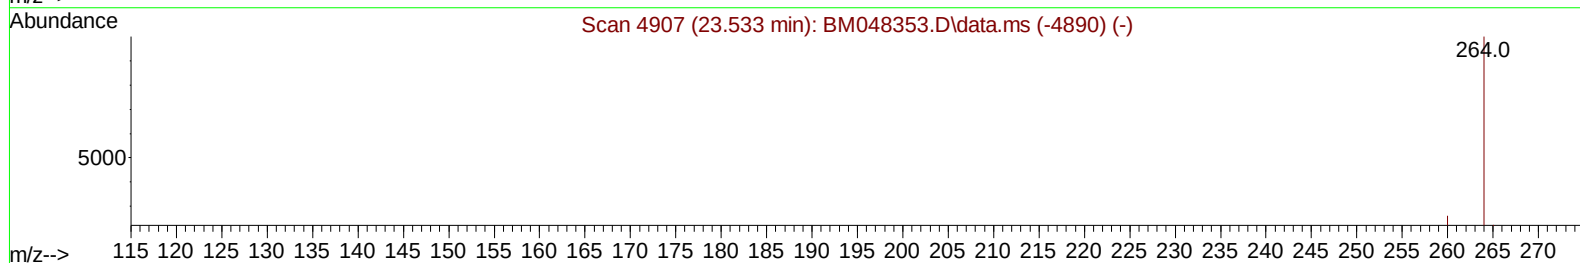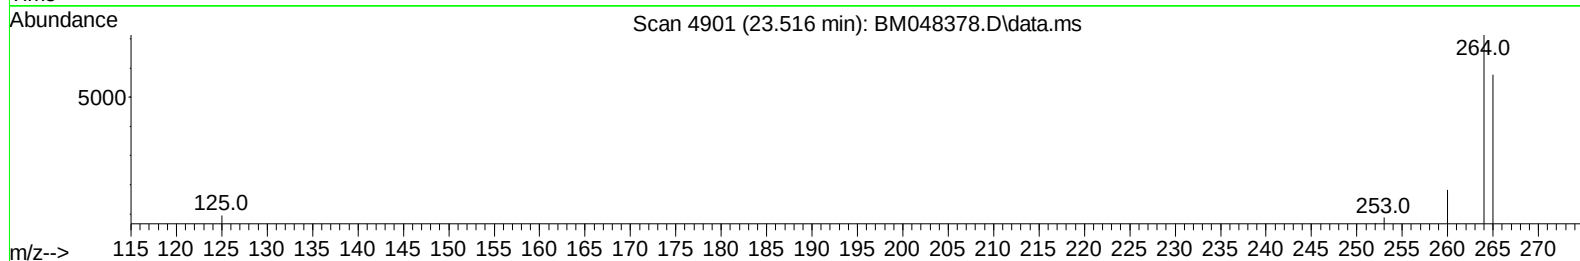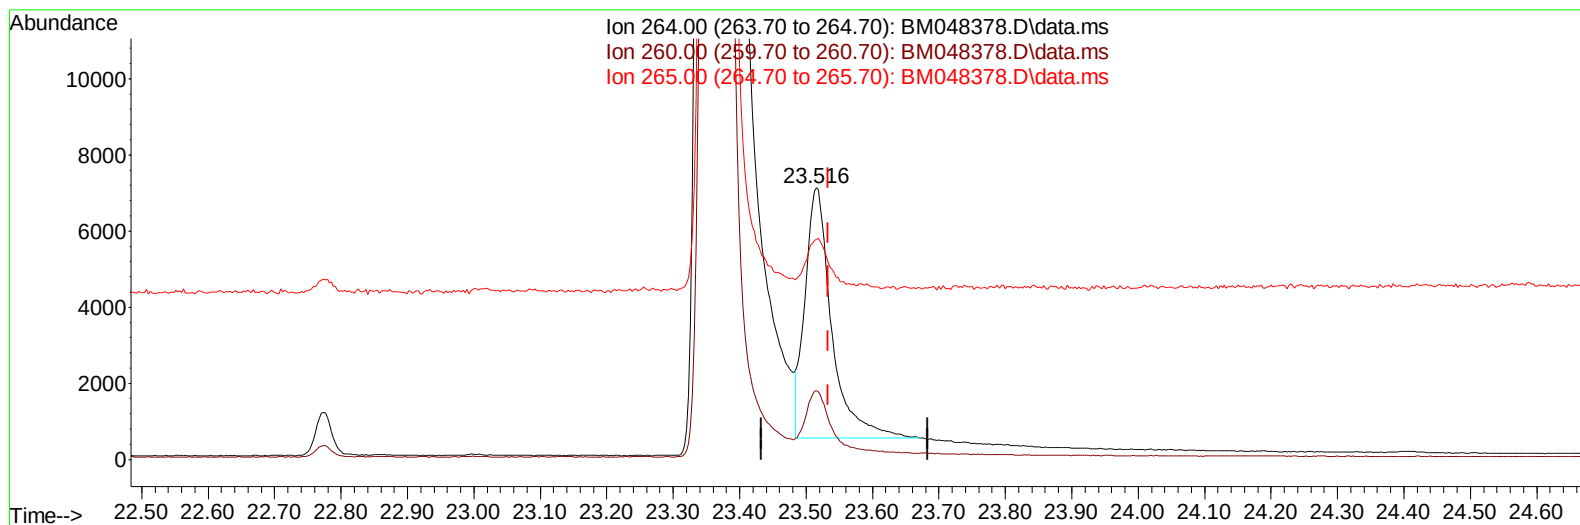

TIC: BM048378.D\data.ms

(23) Perylene-d12 (I)

23.516min (-0.018) 0.40 ng/u1

response 18527

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.43
265.00	120.80	80.96#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

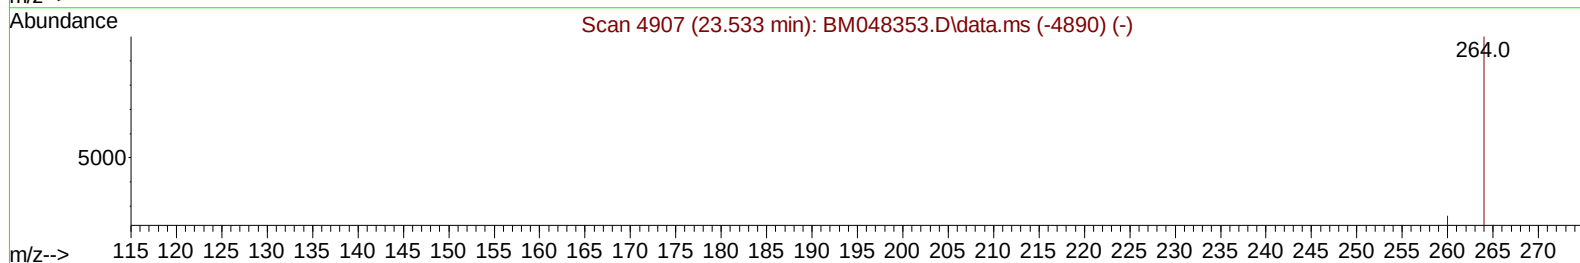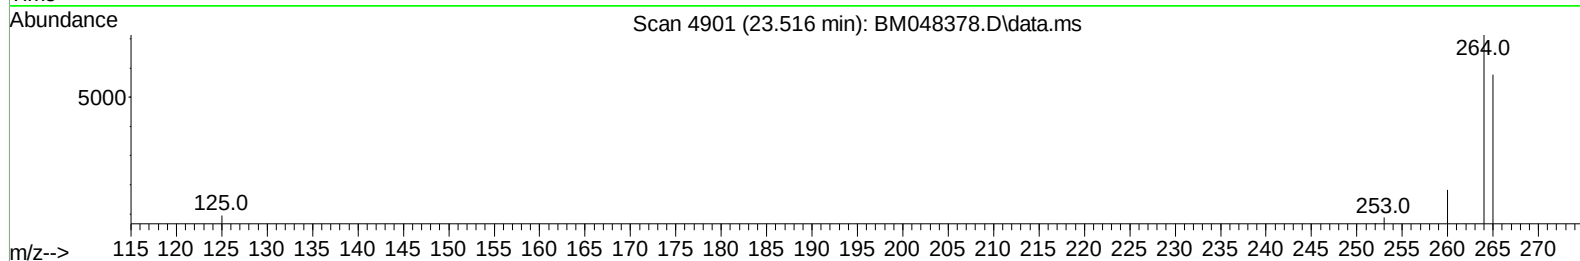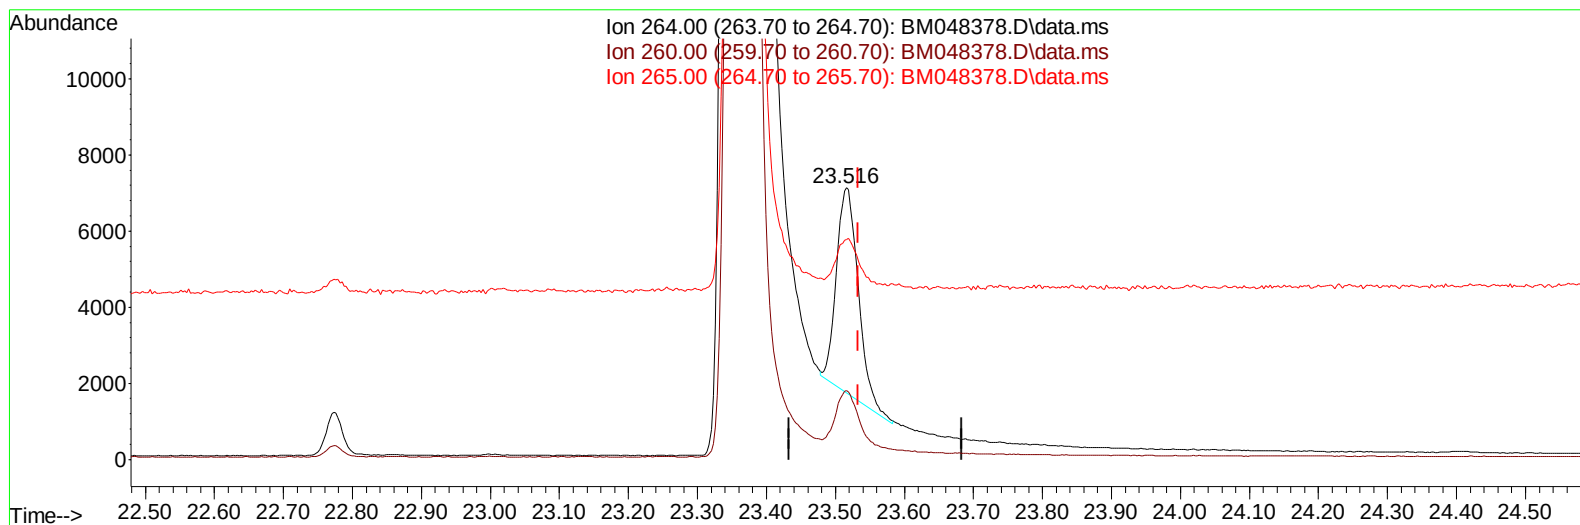

TIC: BM048378.D\data.ms

(23) Perylene-d12 (I)

23.516min (-0.018) 0.40 ng/ul m

response 11787

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.43
265.00	120.80	80.96#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

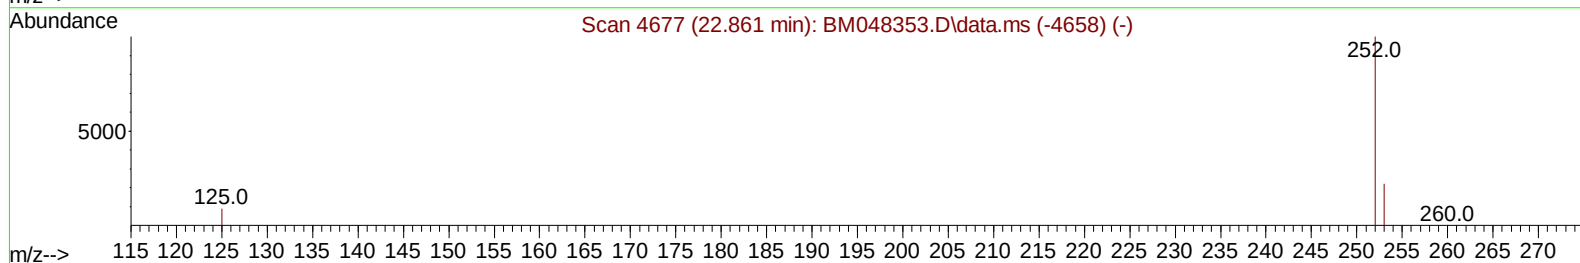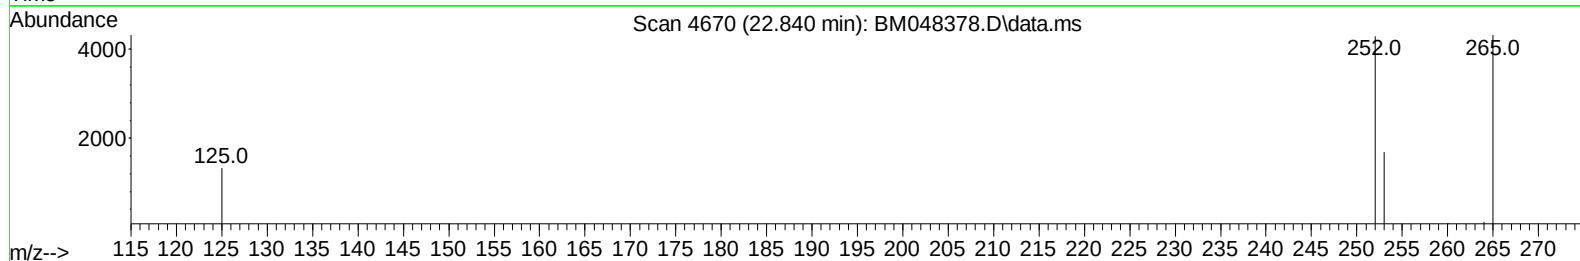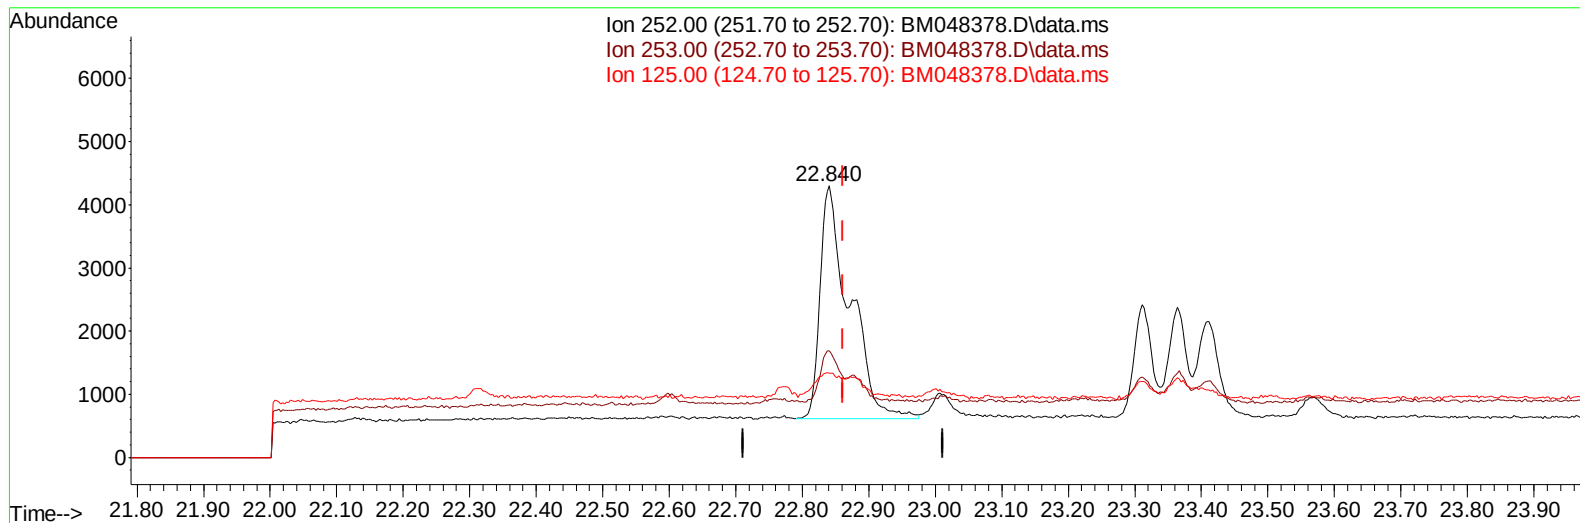

TIC: BM048378.D\data.ms

(24) Benzo(b)fluoranthene

22.840min (-0.021) 0.28 ng/u1

response 11404

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.70	39.33
125.00	19.00	31.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

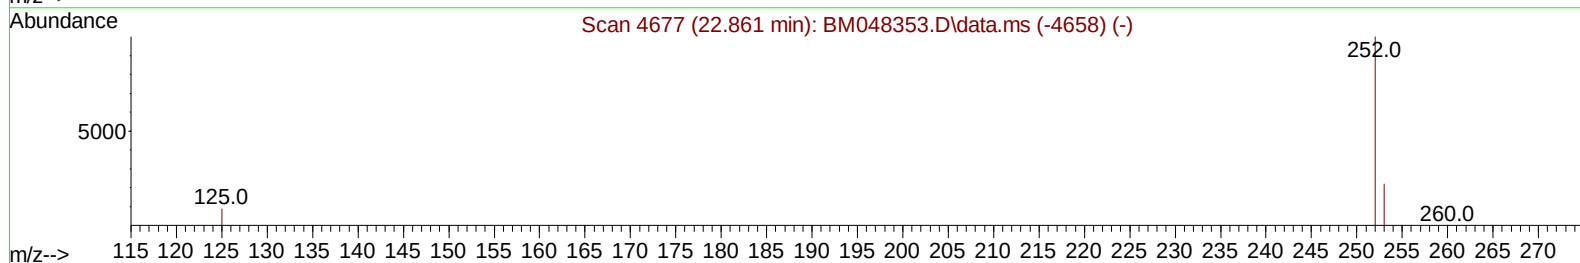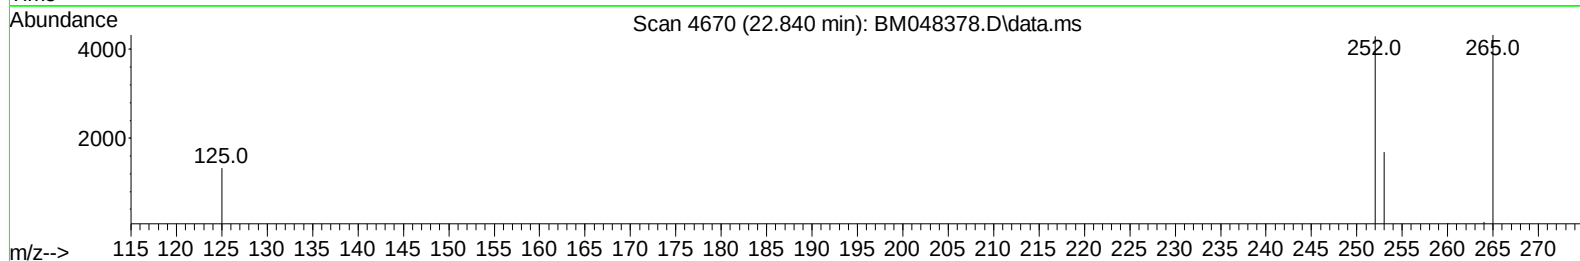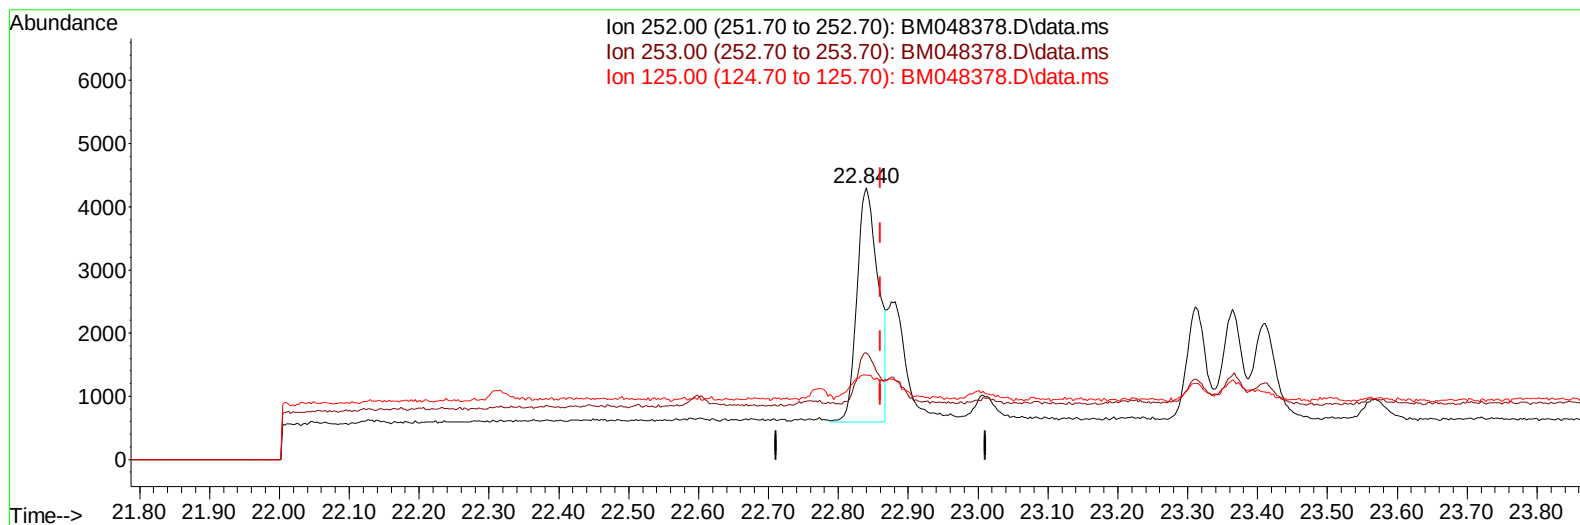

TIC: BM048378.D\data.ms

(24) Benzo(b)fluoranthene

22.840min (-0.021) 0.19 ng/ul m

response 7836

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.70	39.33
125.00	19.00	31.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

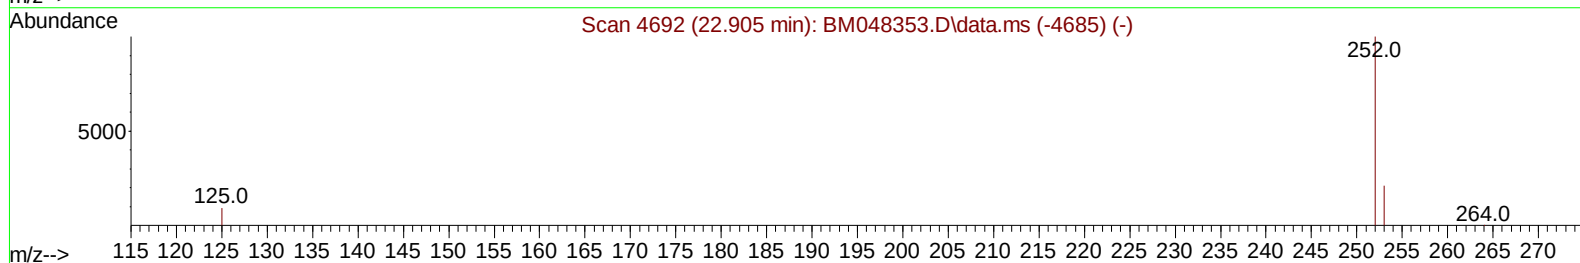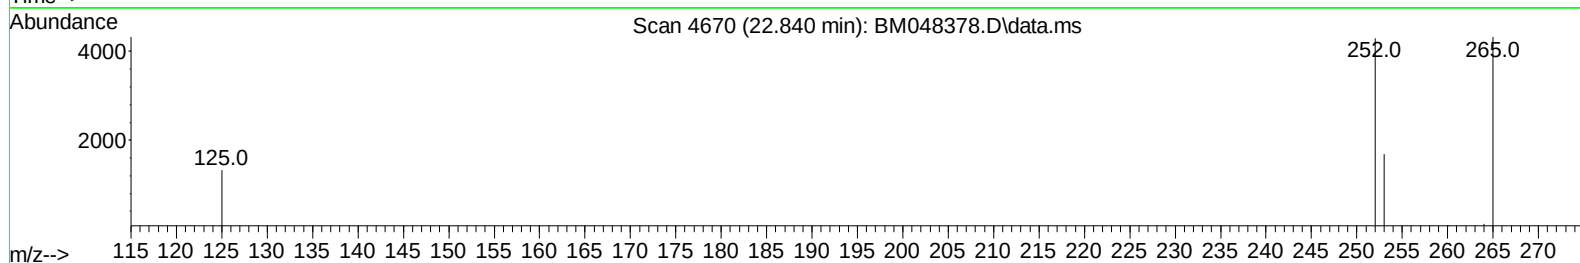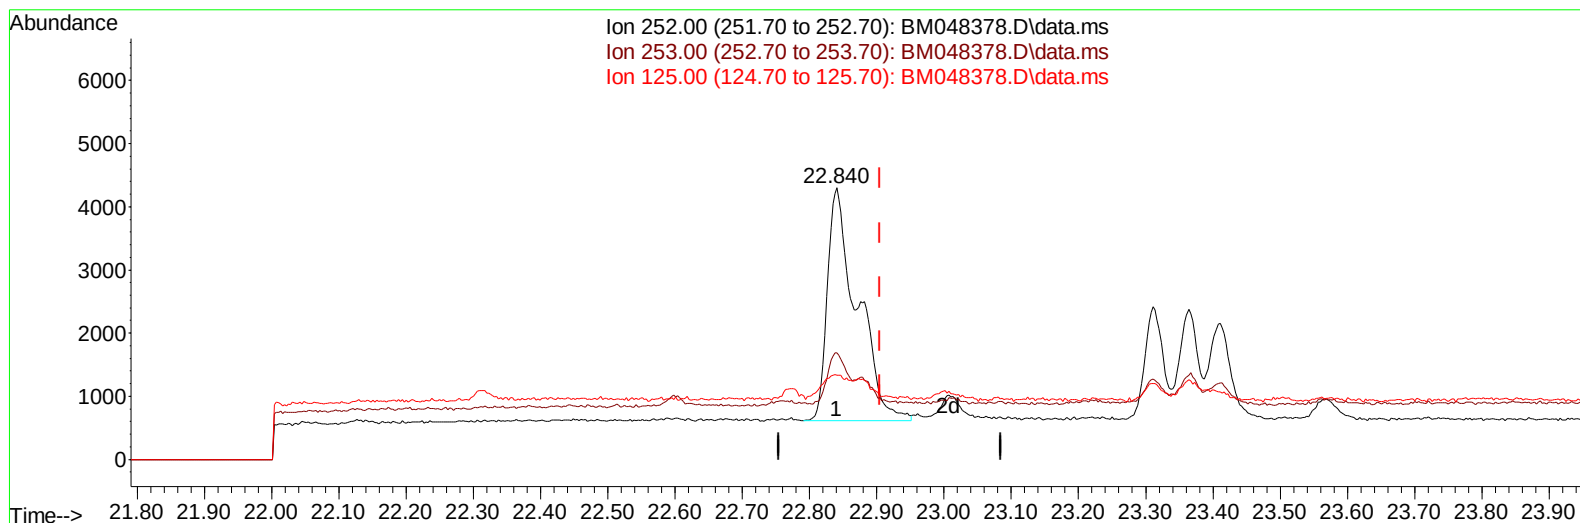

TIC: BM048378.D\data.ms

(25) Benzo(k)fluoranthene

22.840min (-0.064) 0.24 ng/u1

response 11296

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.20	39.33#
125.00	19.10	31.01#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

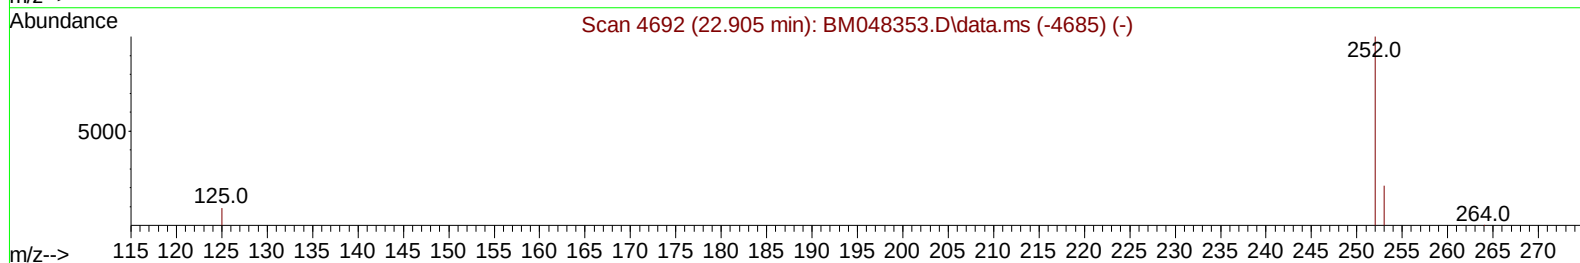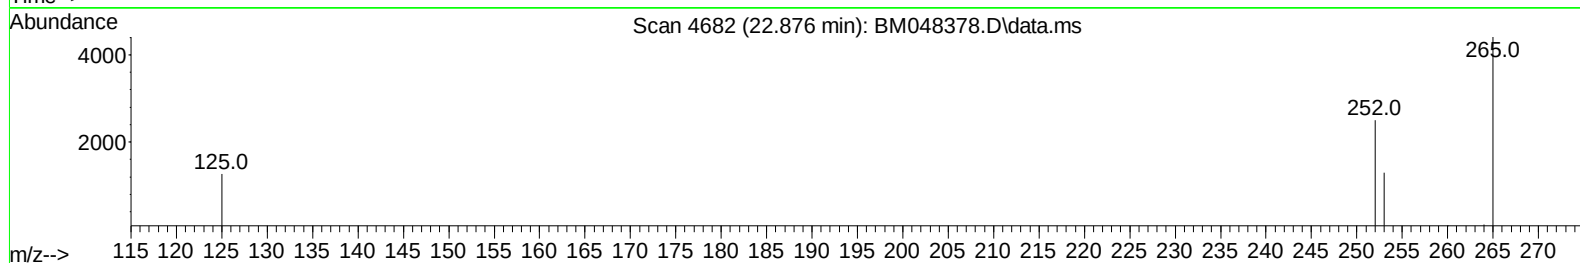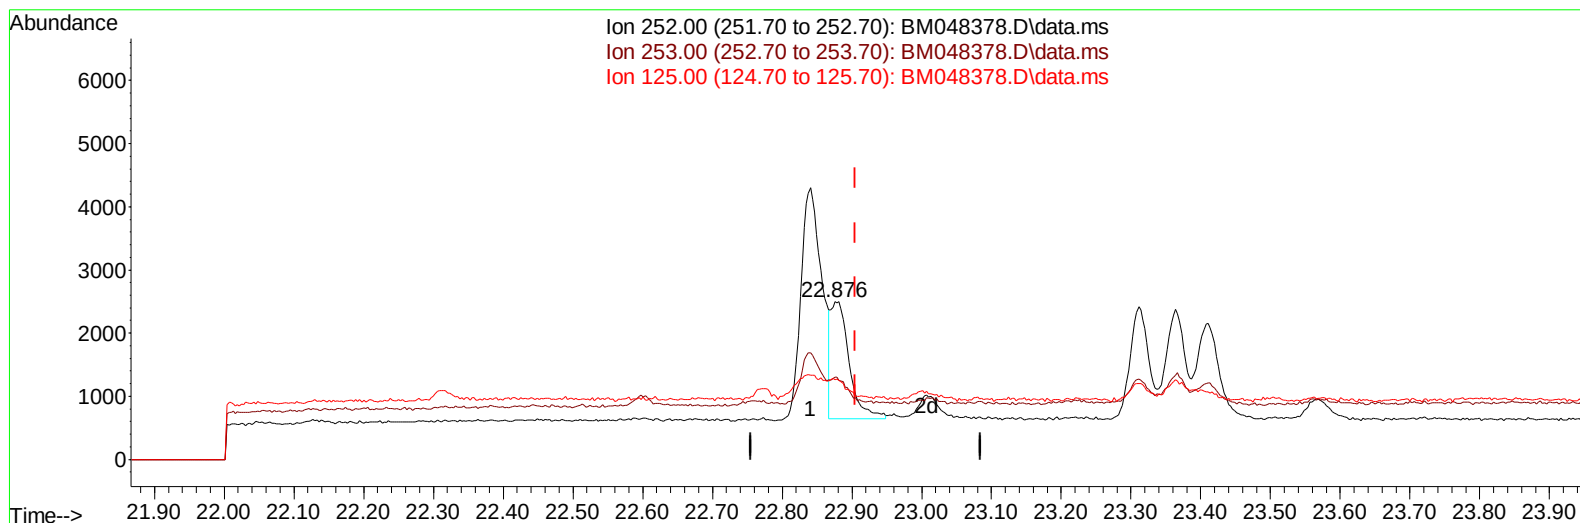

TIC: BM048378.D\data.ms

(25) Benzo(k)fluoranthene

22.876min (-0.029) 0.07 ng/ul m

response 3408

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.20	51.96#
125.00	19.10	50.48#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048378.D
 Acq On : 01 Nov 2024 04:05
 Operator : RC/JU
 Sample : P4592-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H01

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/04/2024

Quant Time: Nov 03 07:05:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.708	152		4750	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.496	136		15448	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.349	164		8395	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.095	188		16905m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.286	240		13838m	0.400	ng/ul	0.00
23) Perylene-d12	23.516	264		11787m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.164	96		22208	3.807	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.119	152		5436	0.277	ng/ul	-0.02
18) Fluoranthene-d10	19.123	212		12604	0.359	ng/ul	-0.01
Target Compounds							Qvalue
15) Phenanthrene	17.137	178		1365m	0.032	ng/ul	
19) Fluoranthene	19.155	202		5250	0.110	ng/ul#	94
20) Pyrene	19.513	202		5803m	0.113	ng/ul	
21) Benzo(a)anthracene	21.277	228		3885m	0.094	ng/ul	
22) Chrysene	21.324	228		3984	0.070	ng/ul	95
24) Benzo(b)fluoranthene	22.840	252		7836m	0.195	ng/ul	
25) Benzo(k)fluoranthene	22.876	252		3408m	0.071	ng/ul	
26) Benzo(a)pyrene	23.411	252		3267	0.086	ng/ul#	59
27) Indeno(1,2,3-cd)pyrene	25.816	276		2705	0.051	ng/ul	94
28) Dibenzo(a,h)anthracene	25.826	278		860	0.021	ng/ul#	1
29) Benzo(g,h,i)perylene	26.513	276		2385	0.053	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048378.D
Acq On : 01 Nov 2024 04:05
Operator : RC/JU
Sample : P4592-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H01

Manual IntegrationsAPPROVED

Quant Time: Nov 03 07:05:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

