



Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048393.D
Acq On : 01 Nov 2024 13:47
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Nov 03 21:49:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

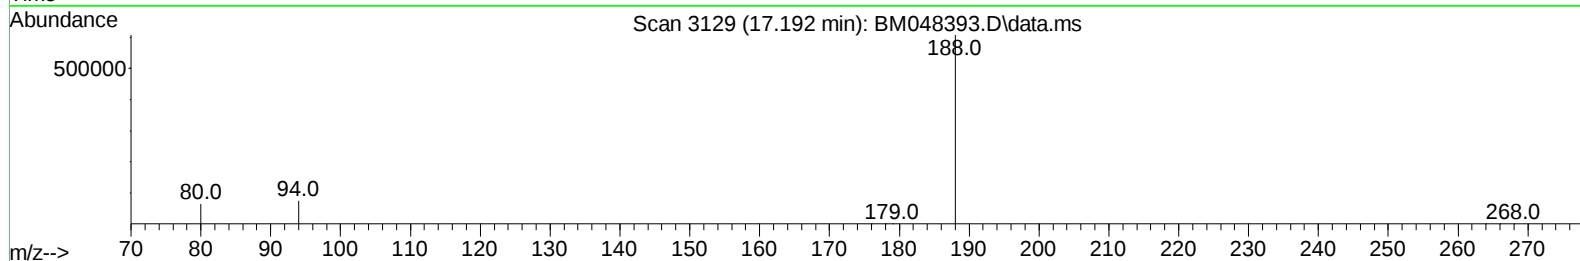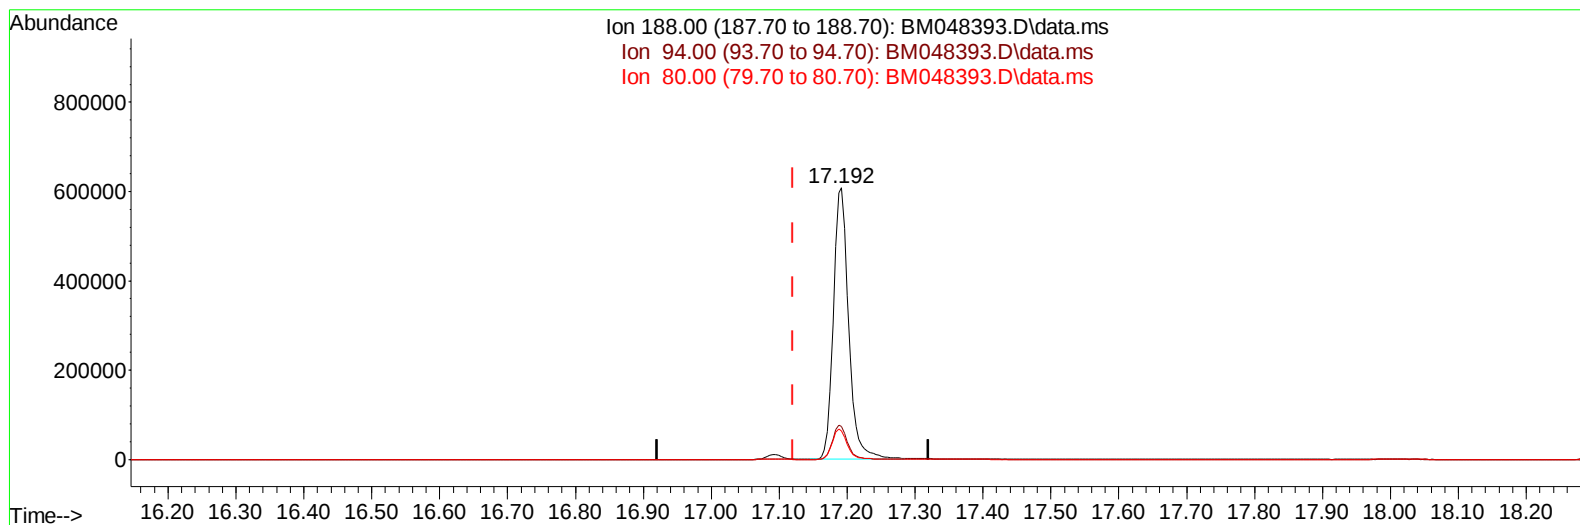

TIC: BM048393.D\data.ms

(13) Phenanthrene-d10 (I)

17.192min (+ 0.072) 0.40 ng/u1

response 948998

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.50	12.23
80.00	12.10	10.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048393.D
Acq On : 01 Nov 2024 13:47
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Nov 03 21:49:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

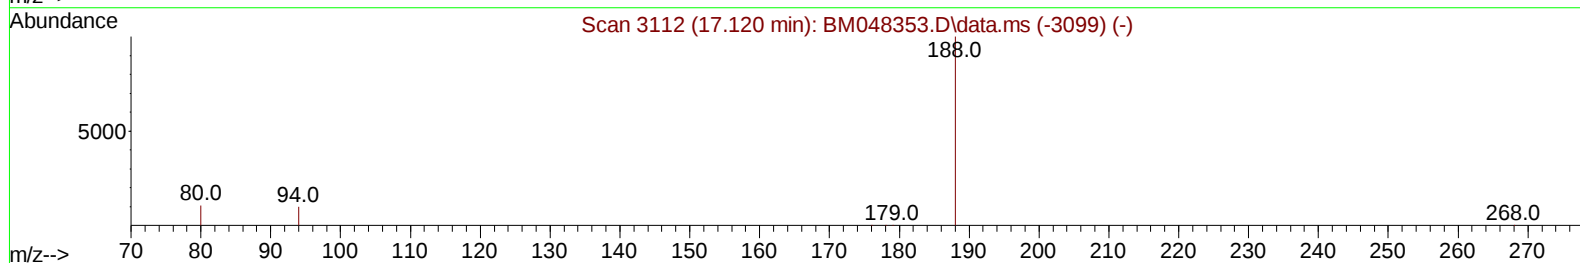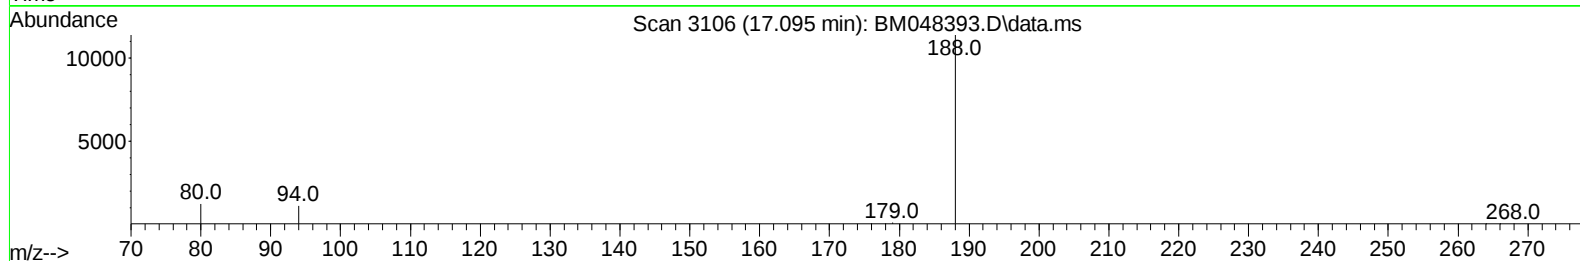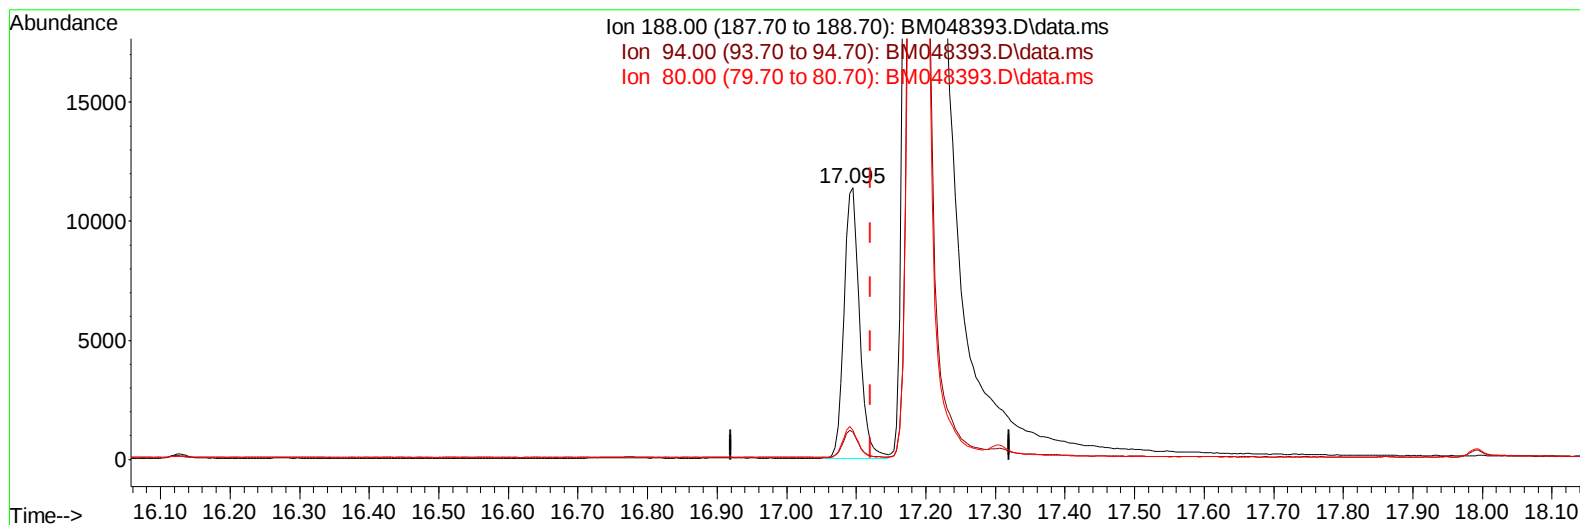

TIC: BM048393.D\data.ms

(13) Phenanthrene-d10 (I)

17.095min (-0.025) 0.40 ng/ul m

response 17570

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.50	10.03
80.00	12.10	10.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048393.D
Acq On : 01 Nov 2024 13:47
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Nov 03 21:49:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

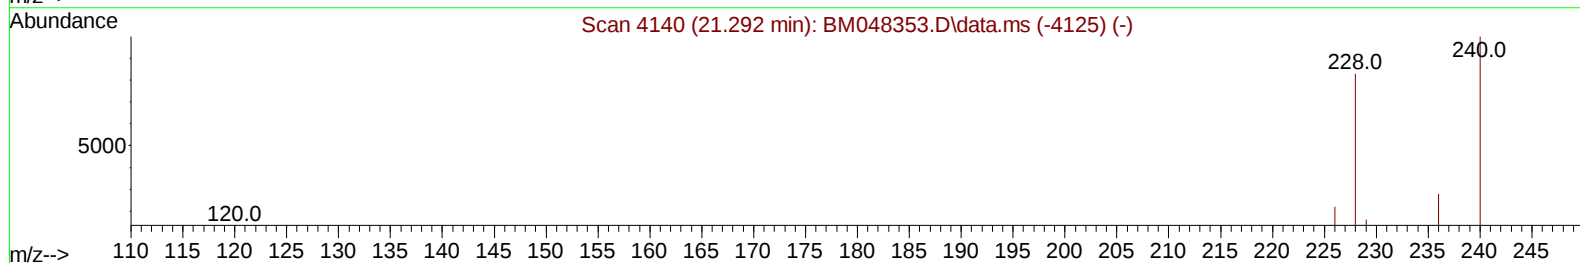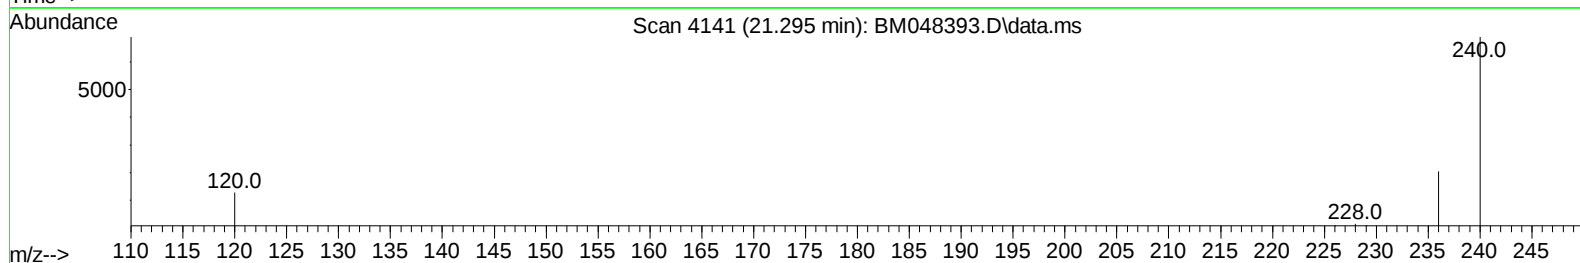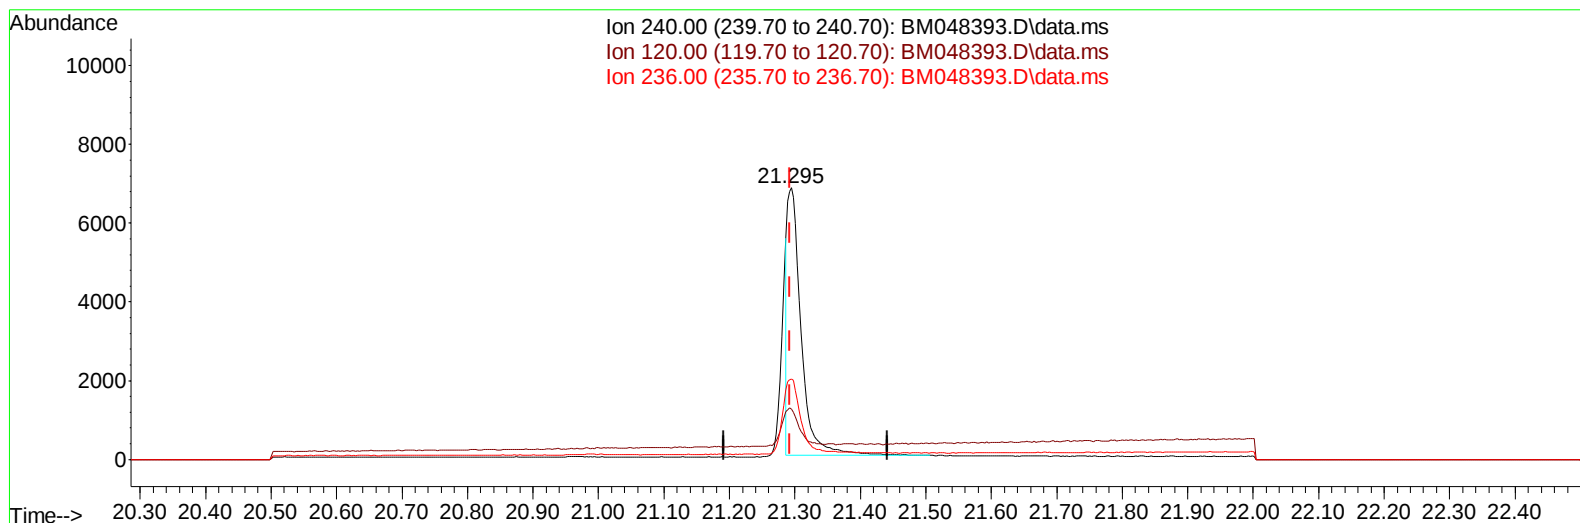

TIC: BM048393.D\data.ms

(17) Chrysene-d12

21.295min (+ 0.003) 0.40 ng/u1

response 10014

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	19.00	18.62
236.00	29.90	29.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048393.D
Acq On : 01 Nov 2024 13:47
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Nov 03 21:49:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

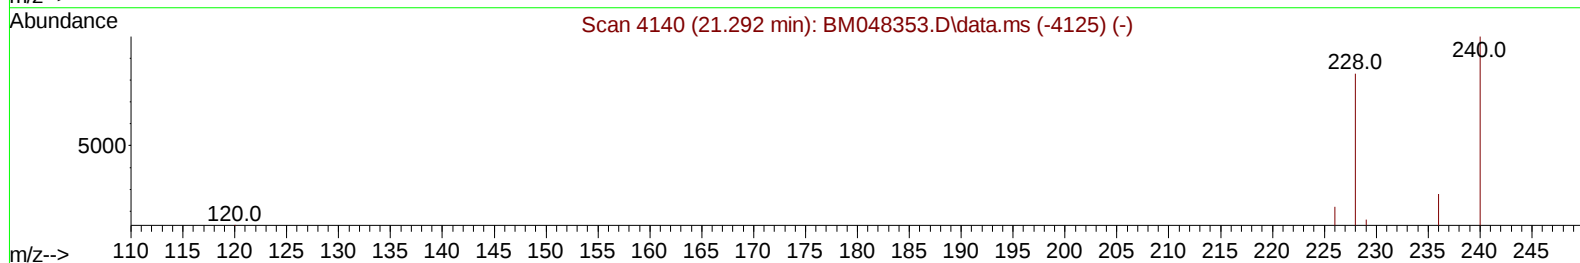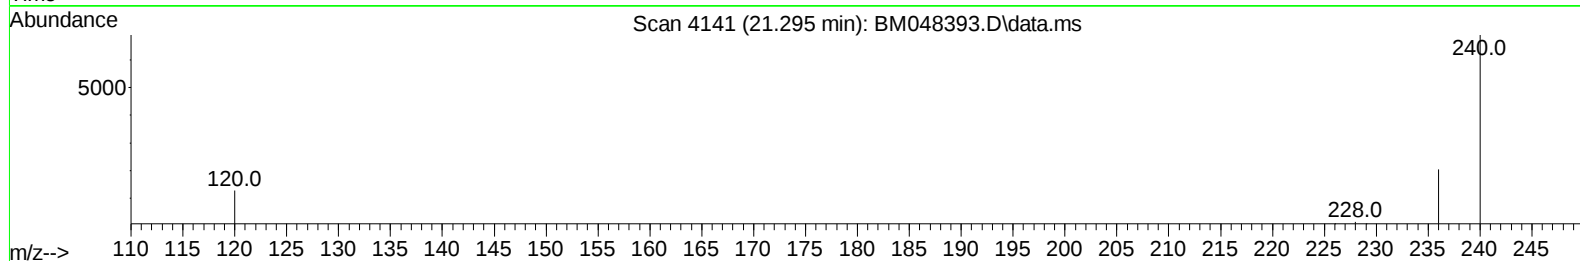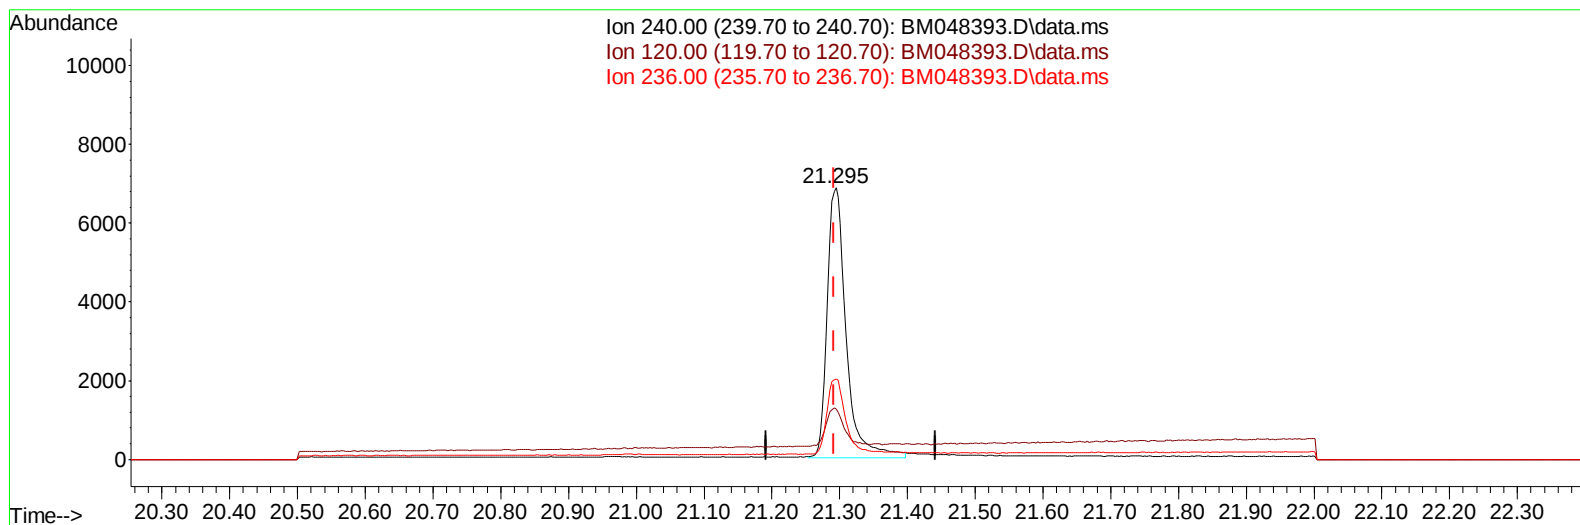

TIC: BM048393.D\data.ms

(17) Chrysene-d12

21.295min (+ 0.003) 0.40 ng/ul m

response 13311

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	19.00	18.62
236.00	29.90	29.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048393.D
Acq On : 01 Nov 2024 13:47
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Nov 03 21:49:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

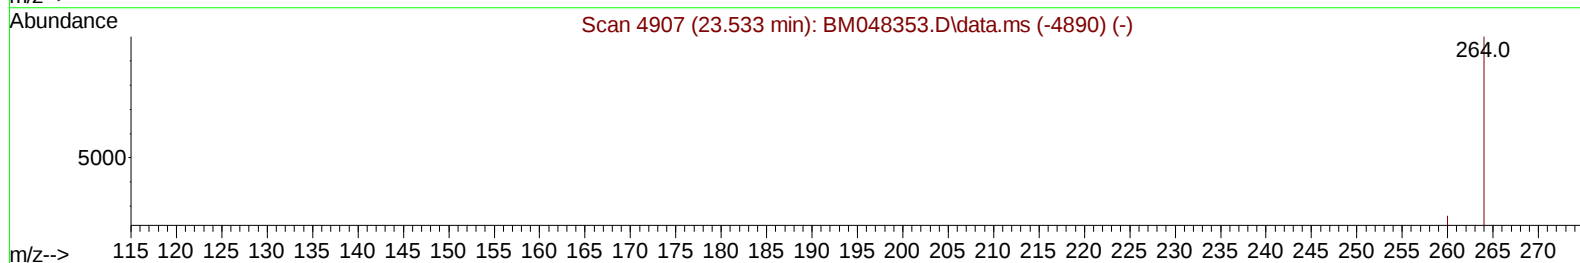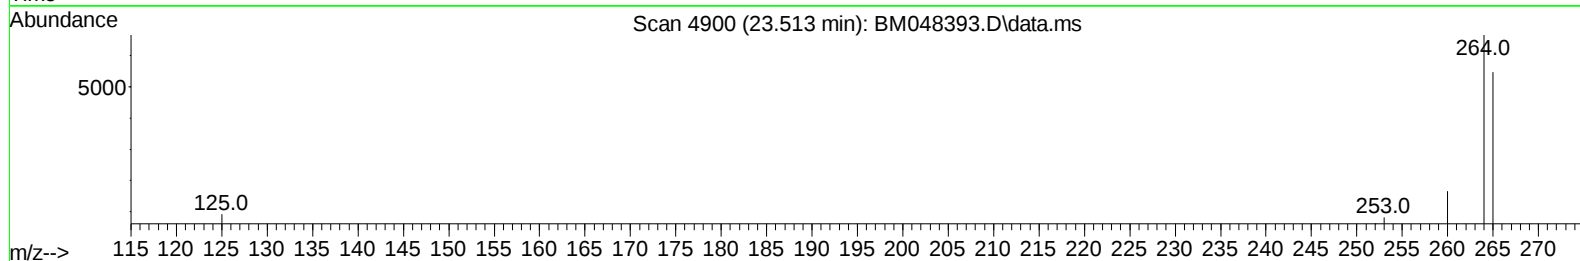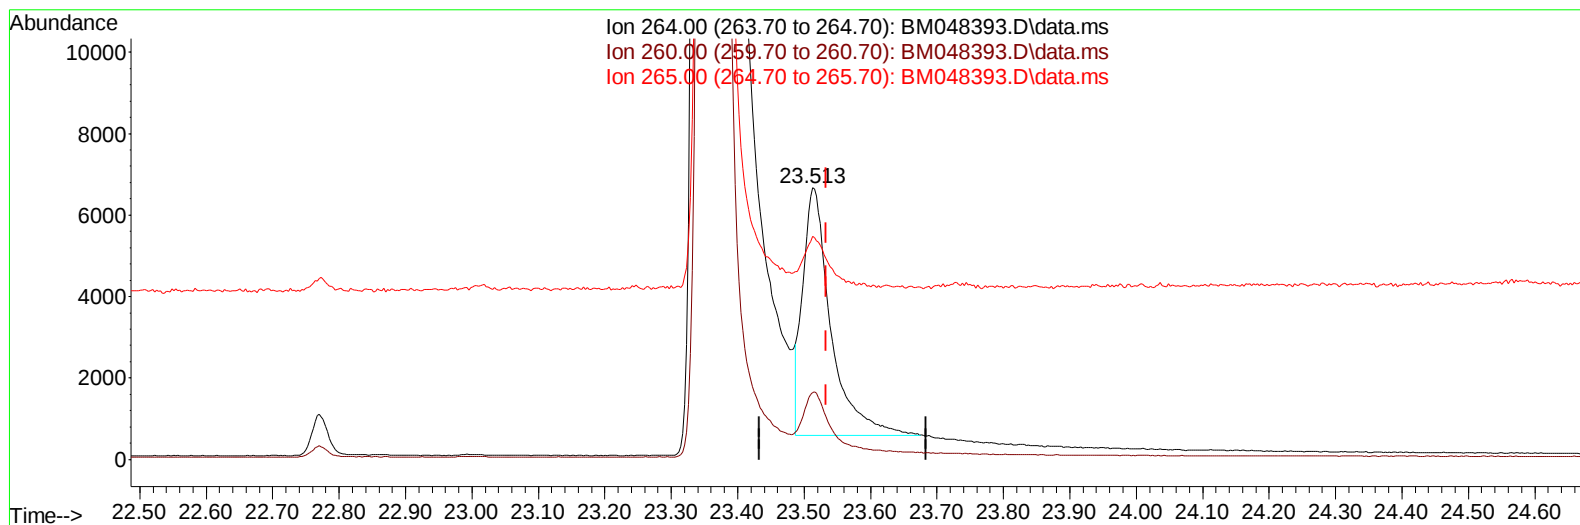

TIC: BM048393.D\data.ms

(23) Perylene-d12 (I)

23.513min (-0.020) 0.40 ng/u1

response 18075

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	24.67
265.00	120.80	82.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048393.D
Acq On : 01 Nov 2024 13:47
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Nov 03 21:49:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

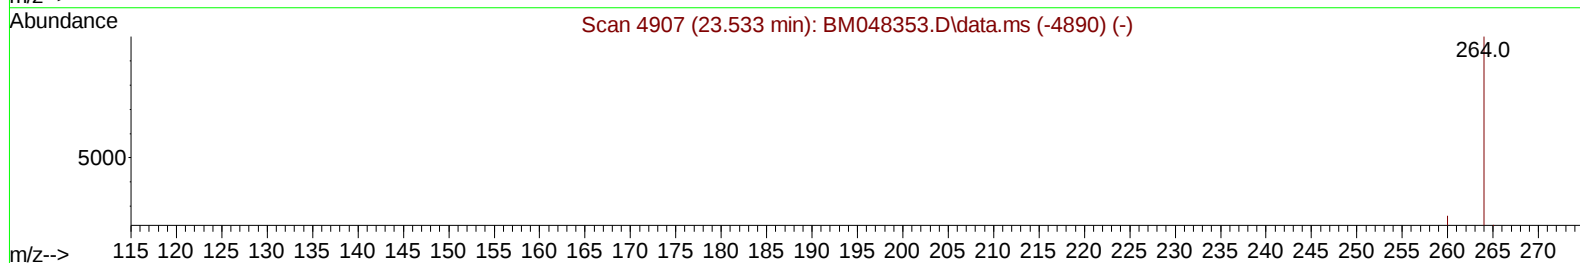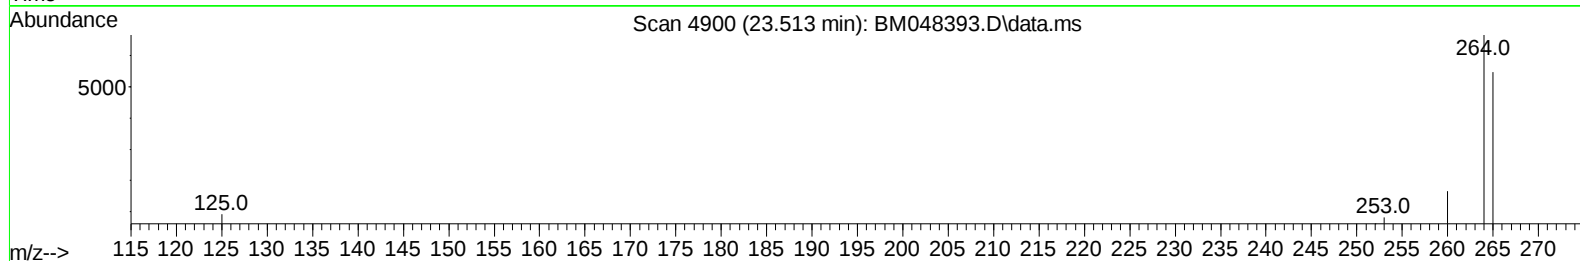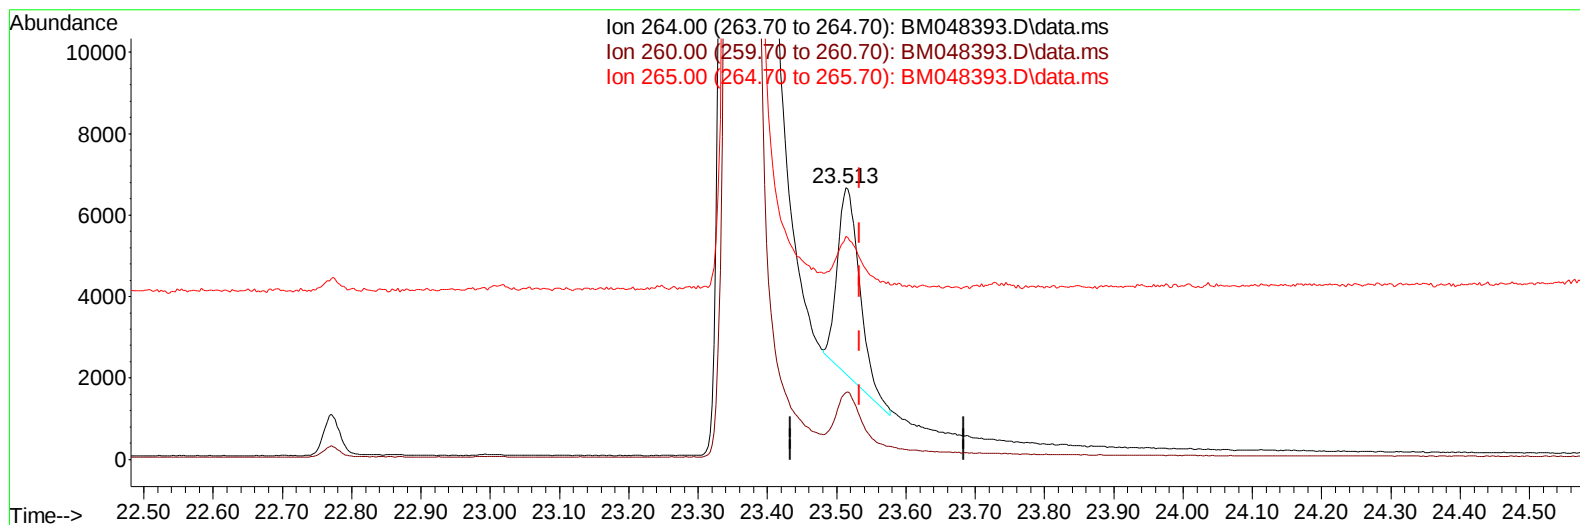

TIC: BM048393.D\data.ms

(23) Perylene-d12 (I)

23.513min (-0.020) 0.40 ng/u1 m

response 10219

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	24.67
265.00	120.80	82.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048393.D
 Acq On : 01 Nov 2024 13:47
 Operator : RC/JU
 Sample : P4592-12
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H20

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/04/2024

Quant Time: Nov 03 21:49:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4929	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.491	136	16313	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.349	164	8805	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.095	188	17570m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.295	240	13311m	0.400	ng/ul	0.00
23) Perylene-d12	23.513	264	10219m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	21467	3.546	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.119	152	5084	0.245	ng/ul	-0.02
18) Fluoranthene-d10	19.123	212	11679	0.346	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048393.D
Acq On : 01 Nov 2024 13:47
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Nov 03 21:49:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/04/2024

