

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048400.D
 Acq On : 01 Nov 2024 18:03
 Operator : RC/JU
 Sample : PB164424BS
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS424

Quant Time: Nov 03 21:50:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.788	152	2752	0.400	ng/ul	0.04
4) Naphthalene-d8	10.546	136	10408	0.400	ng/ul	0.02
9) Acenaphthene-d10	14.373	164	6068	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.133	188	12325	0.400	ng/ul	0.01
17) Chrysene-d12	21.303	240	10257	0.400	ng/ul	0.01
23) Perylene-d12	23.539	264	10389	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	3494	1.034	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.163	152	5330	0.403	ng/ul	0.02
18) Fluoranthene-d10	19.151	212	12205	0.469	ng/ul	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.197	88	9009	2.457	ng/ul#	82
5) Naphthalene	10.596	128	10028	0.369	ng/ul	97
7) 2-Methylnaphthalene	12.234	142	5667	0.350	ng/ul	99
8) 1-Methylnaphthalene	12.427	142	6688	0.388	ng/ul	97
10) Acenaphthylene	14.100	152	8735	0.372	ng/ul	98
11) Acenaphthene	14.433	153	7325	0.390	ng/ul	98
12) Fluorene	15.446	166	7780	0.372	ng/ul	99
14) Pentachlorophenol	16.799	266	1955	0.570	ng/ul	94
15) Phenanthrene	17.171	178	11147	0.364	ng/ul	98
16) Anthracene	17.293	178	9808	0.342	ng/ul	96
19) Fluoranthene	19.179	202	15121	0.428	ng/ul	99
20) Pyrene	19.537	202	16300	0.430	ng/ul	98
21) Benzo(a)anthracene	21.298	228	10288	0.335	ng/ul	100
22) Chrysene	21.338	228	18674	0.442	ng/ul	100
24) Benzo(b)fluoranthene	22.867	252	13819	0.389	ng/ul	99
25) Benzo(k)fluoranthene	22.911	252	17923	0.426	ng/ul	96
26) Benzo(a)pyrene	23.454	252	13563	0.407	ng/ul	94
27) Indeno(1,2,3-cd)pyrene	25.839	276	18192	0.390	ng/ul#	99
28) Dibenzo(a,h)anthracene	25.863	278	14009	0.385	ng/ul	96
29) Benzo(g,h,i)perylene	26.517	276	15945	0.406	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048400.D
Acq On : 01 Nov 2024 18:03
Operator : RC/JU
Sample : PB164424BS
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLCS424


Quant Time: Nov 03 21:50:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

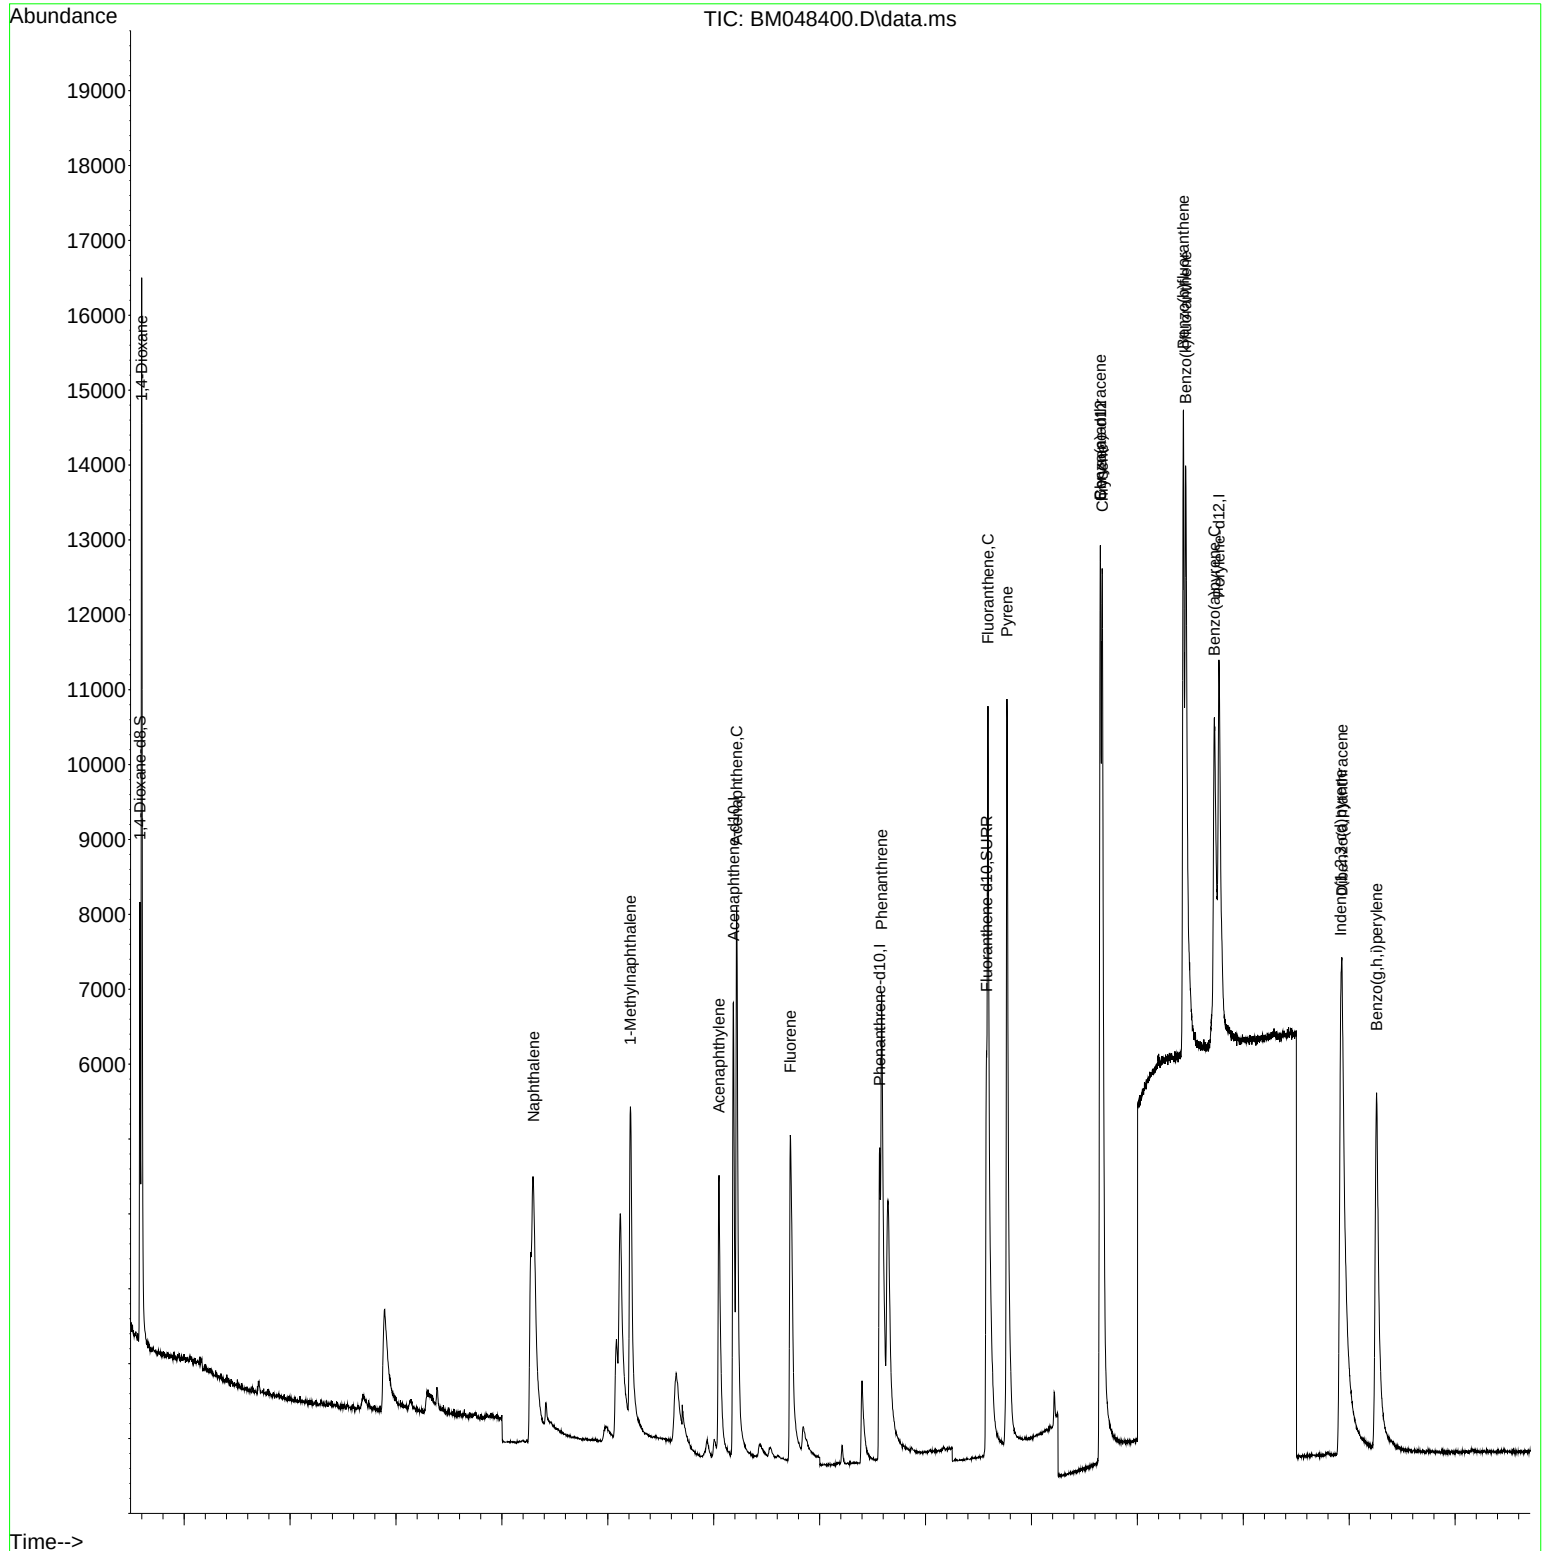



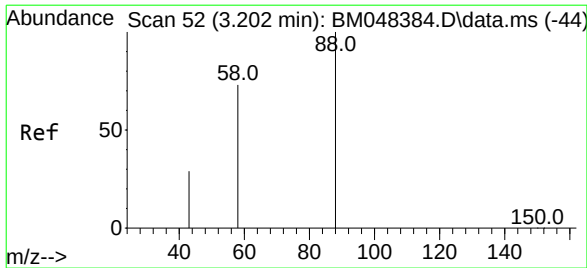


#2
1,4-Dioxane
Concen: 2.457 ng/u1
RT: 3.197 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03

Instrument :
BNA_M
ClientSampleId :
SLCS424



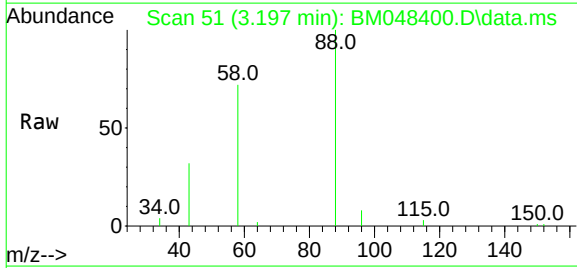



Tgt Ion: 88 Resp: 9009
Ion Ratio Lower Upper
88 100
43 32.0 36.2 54.4#
58 71.6 47.4 71.0#

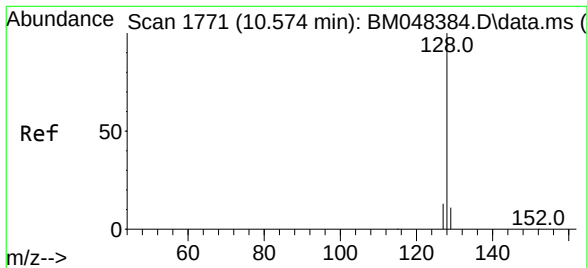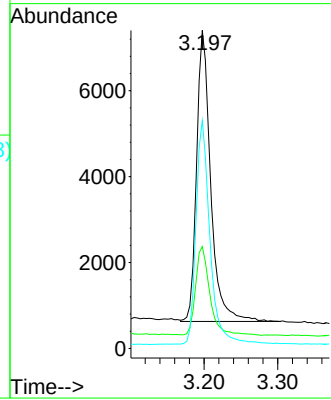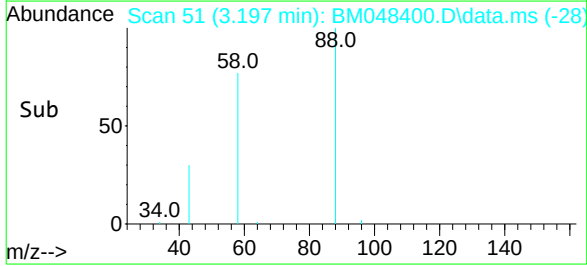

#5
Naphthalene
Concen: 0.369 ng/u1
RT: 10.596 min Scan# 1775
Delta R.T. 0.016 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03

Tgt Ion: 128 Resp: 10028
Ion Ratio Lower Upper
128 100
129 14.7 10.6 15.8
127 15.3 11.4 17.2


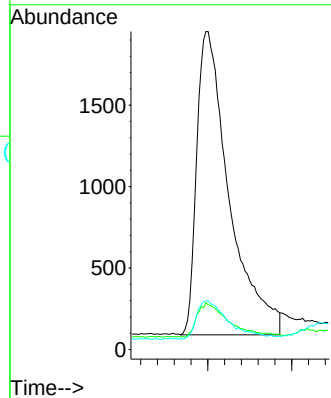
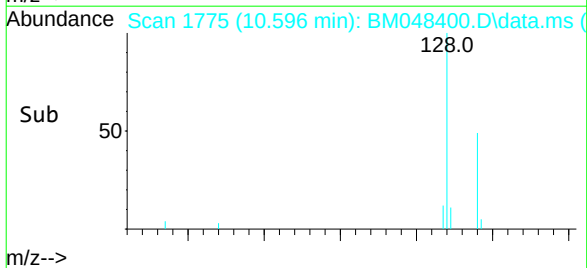
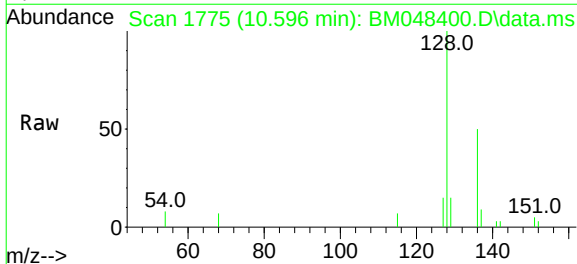


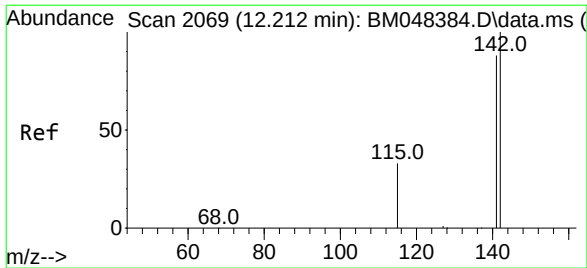

#7
2-Methylnaphthalene
Concen: 0.350 ng/ul
RT: 12.234 min Scan# 2069
Delta R.T. 0.022 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03




Instrument :
BNA_M
ClientSampleId :
SLCS424


Tgt Ion:142 Resp: 5667
Ion Ratio Lower Upper
142 100
141 91.2 72.2 108.2

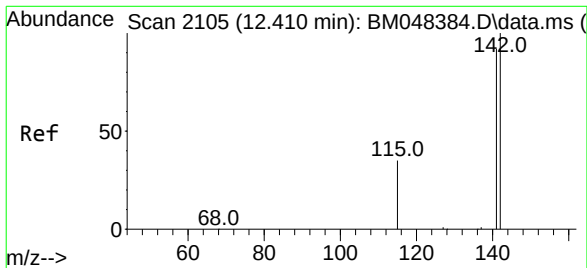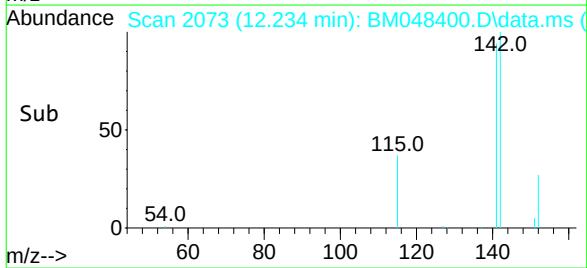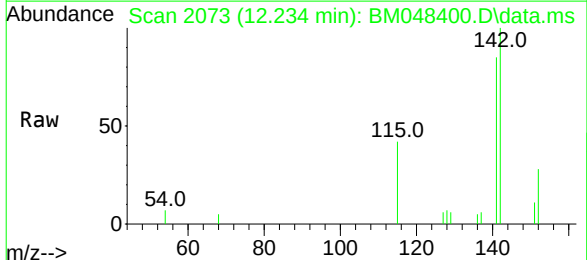

#8
1-Methylnaphthalene
Concen: 0.388 ng/ul
RT: 12.427 min Scan# 2108
Delta R.T. 0.011 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03

Tgt Ion:142 Resp: 6688
Ion Ratio Lower Upper
142 100
141 91.3 75.5 113.3


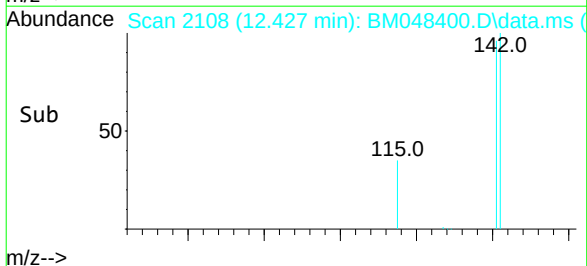
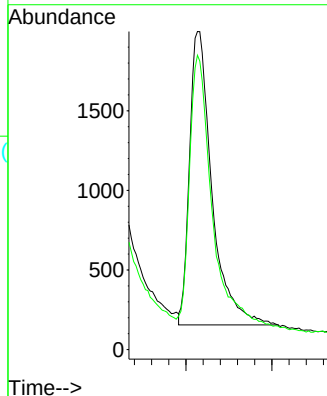
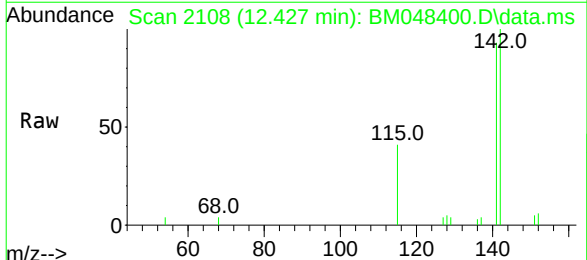


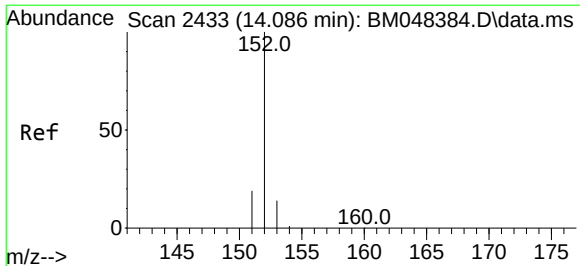

#10
 Acenaphthylene
 Concen: 0.372 ng/ul
 RT: 14.100 min Scan# 2436
 Delta R.T. 0.009 min
 Lab File: BM048400.D
 Acq: 01 Nov 2024 18:03




Instrument :
 BNA_M
 ClientSampleId :
 SLCS424


Tgt Ion:	152	Resp:	8735
Ion	Ratio	Lower	Upper
152	100		
151	22.1	16.6	24.8
153	15.1	11.8	17.6

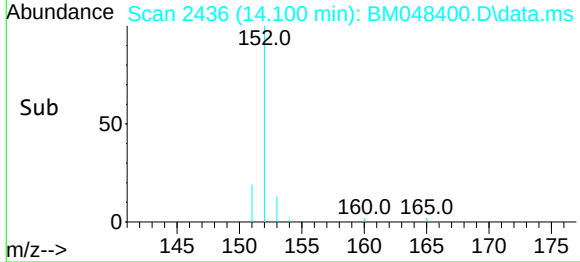

#11
 Acenaphthene
 Concen: 0.390 ng/ul
 RT: 14.433 min Scan# 2508
 Delta R.T. 0.005 min
 Lab File: BM048400.D
 Acq: 01 Nov 2024 18:03

Tgt Ion:	153	Resp:	7325
Ion	Ratio	Lower	Upper
153	100		
152	53.0	40.7	61.1
154	87.5	70.6	106.0


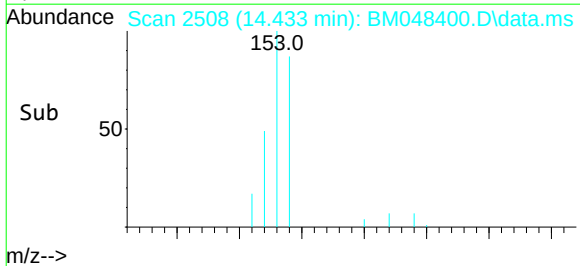

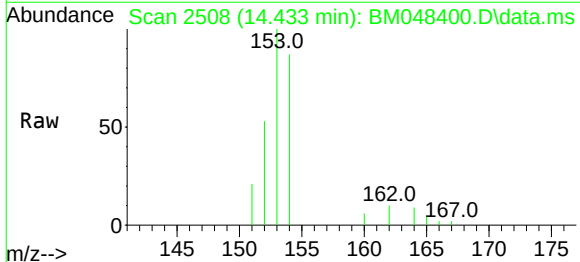


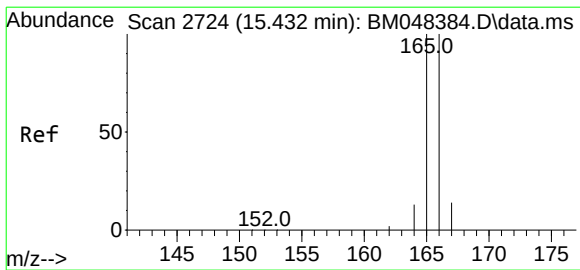

#12
 Fluorene
 Concen: 0.372 ng/u1
 RT: 15.446 min Scan# 2727
 Delta R.T. 0.014 min
 Lab File: BM048400.D
 Acq: 01 Nov 2024 18:03




Instrument :
 BNA_M
 ClientSampleId :
 SLCS424


Tgt Ion:	166	Resp:	7780
Ion	Ratio	Lower	Upper
166	100		
165	99.6	78.6	118.0
167	16.1	12.1	18.1

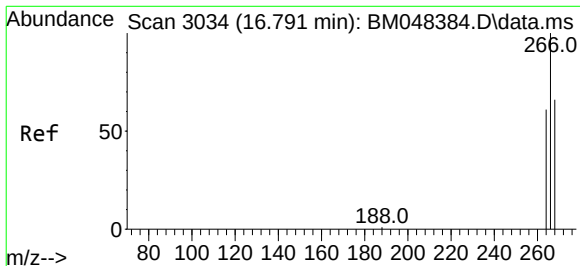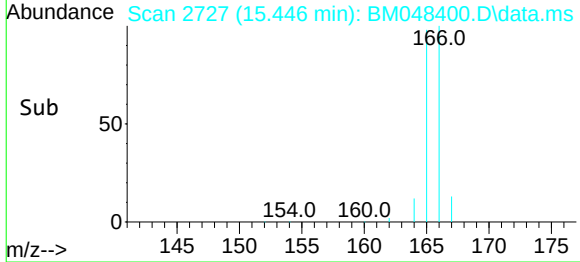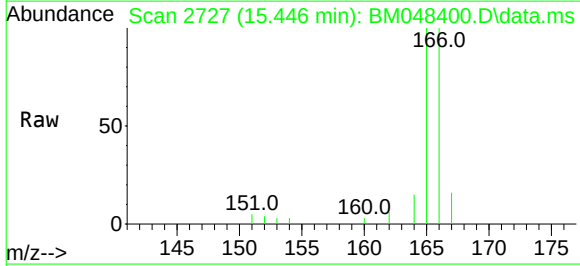

#14
 Pentachlorophenol
 Concen: 0.570 ng/u1
 RT: 16.799 min Scan# 3036
 Delta R.T. 0.013 min
 Lab File: BM048400.D
 Acq: 01 Nov 2024 18:03

Tgt Ion:	266	Resp:	1955
Ion	Ratio	Lower	Upper
266	100		
264	60.5	48.3	72.5
268	66.2	46.2	69.4


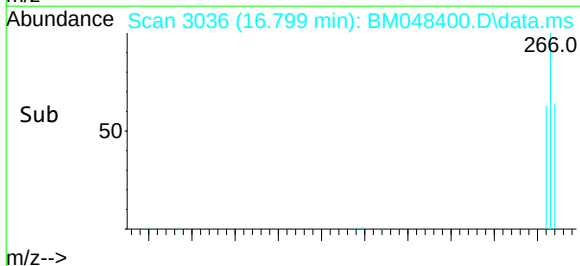

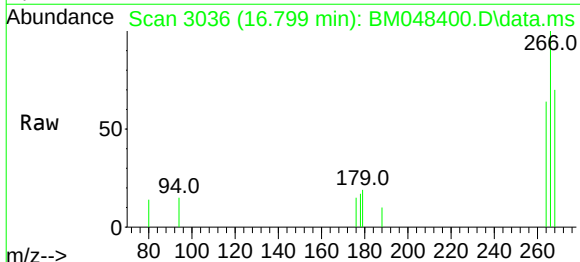




#15
 Phenanthrene
 Concen: 0.364 ng/u1
 RT: 17.171 min Scan# 3124
 Delta R.T. 0.013 min
 Lab File: BM048400.D
 Acq: 01 Nov 2024 18:03




Instrument :
 BNA_M
 ClientSampleId :
 SLCS424


Tgt Ion:	178	Resp:	11147
Ion	Ratio	Lower	Upper
178	100		
179	18.5	13.9	20.9
176	20.7	16.0	24.0

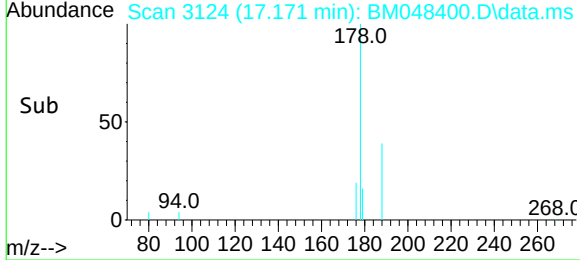

#16
 Anthracene
 Concen: 0.342 ng/u1
 RT: 17.293 min Scan# 3153
 Delta R.T. 0.034 min
 Lab File: BM048400.D
 Acq: 01 Nov 2024 18:03

Tgt Ion:	178	Resp:	9808
Ion	Ratio	Lower	Upper
178	100		
179	19.0	14.2	21.2
176	21.7	15.8	23.6


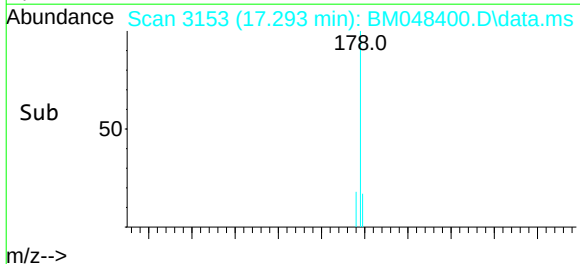
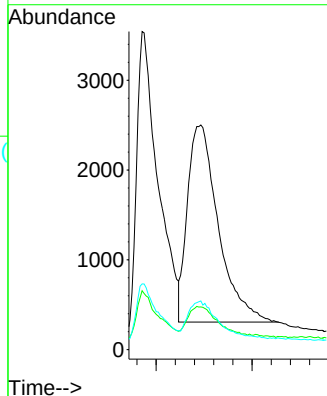
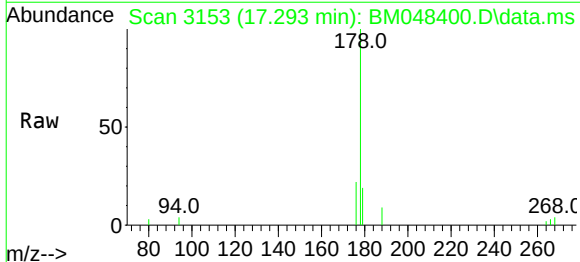




#19
 Fluoranthene
 Concen: 0.428 ng/ul
 RT: 19.179 min Scan# 3583
 Delta R.T. 0.009 min
 Lab File: BM048400.D
 Acq: 01 Nov 2024 18:03




Instrument :
 BNA_M
 ClientSampleId :
 SLCS424


Tgt Ion:	202	Resp:	15121
Ion Ratio	Lower	Upper	
202	100		
101	11.5	9.0	13.4
100	8.9	6.6	10.0

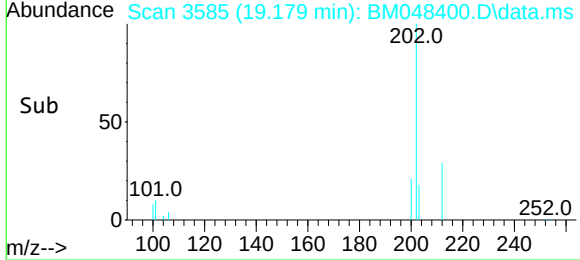

#20
 Pyrene
 Concen: 0.430 ng/ul
 RT: 19.537 min Scan# 3662
 Delta R.T. 0.005 min
 Lab File: BM048400.D
 Acq: 01 Nov 2024 18:03


Tgt Ion:	202	Resp:	16300
Ion Ratio	Lower	Upper	
202	100		
101	13.4	10.0	15.0
100	10.9	8.0	12.0

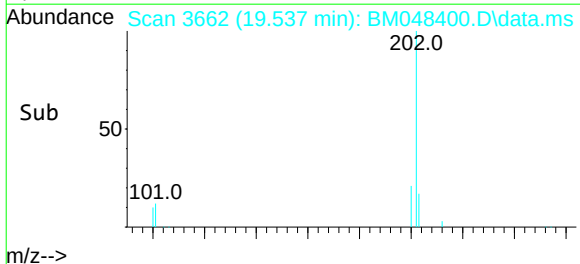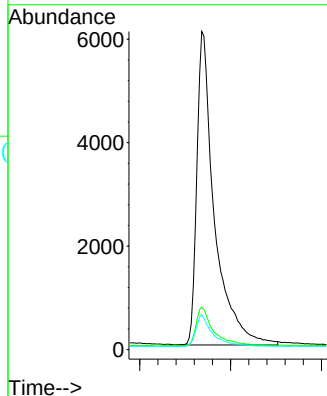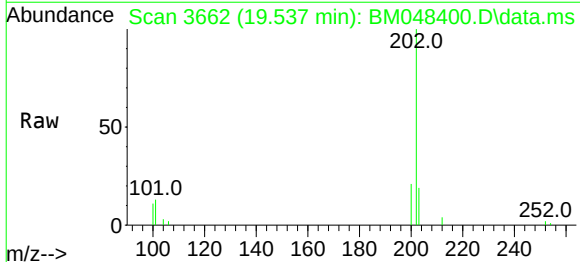






#21
Benzo(a)anthracene
Concen: 0.335 ng/u1
RT: 21.298 min Scan# 4136
Delta R.T. 0.017 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03

Instrument :
BNA_M
ClientSampleId :
SLCS424



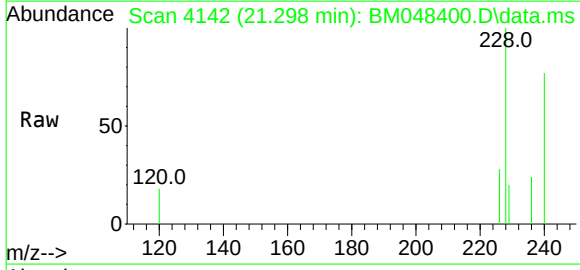



Tgt Ion:228 Resp: 10288
Ion Ratio Lower Upper
228 100
229 20.1 15.9 23.9
226 27.6 22.1 33.1

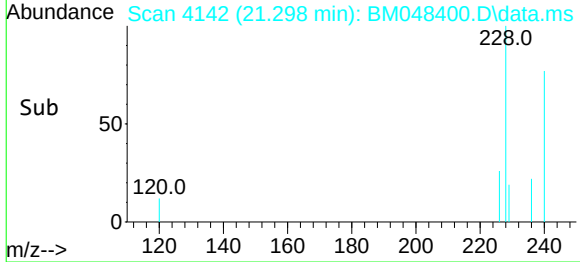

#22
Chrysene
Concen: 0.442 ng/u1
RT: 21.338 min Scan# 4156
Delta R.T. 0.012 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03


Tgt Ion:228 Resp: 18674
Ion Ratio Lower Upper
228 100
226 30.1 24.1 36.1
229 20.1 15.9 23.9

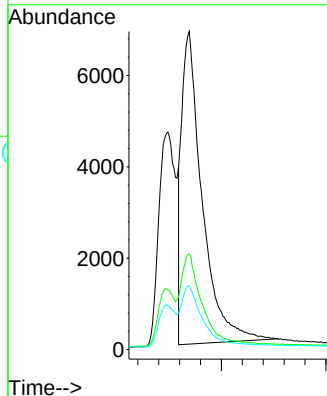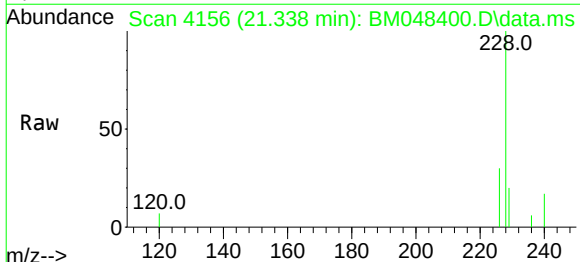






#24
Benzo(b)fluoranthene
Concen: 0.389 ng/u1
RT: 22.867 min Scan# 4675
Delta R.T. 0.006 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03

Instrument :
BNA_M
ClientSampleId :
SLCS424



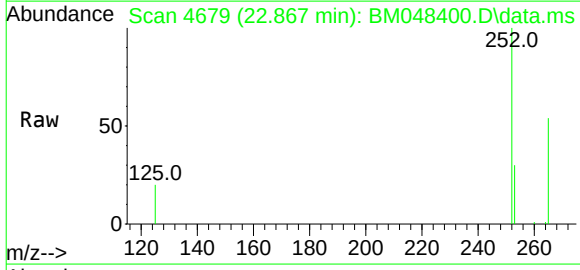



Tgt Ion:	252	Resp:	13819
Ion Ratio	Lower	Upper	
252	100		
253	29.8	0.0	59.4
125	19.8	0.0	38.0

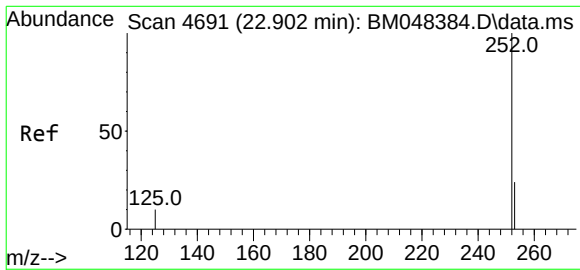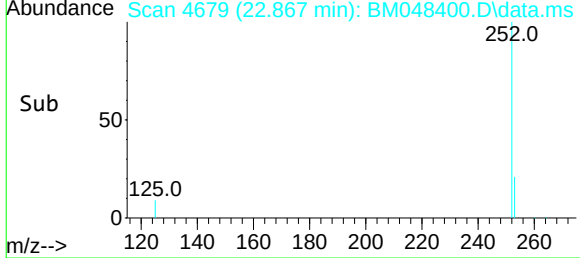

#25
Benzo(k)fluoranthene
Concen: 0.426 ng/u1
RT: 22.911 min Scan# 4694
Delta R.T. 0.006 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03

Tgt Ion:	252	Resp:	17923
Ion Ratio	Lower	Upper	
252	100		
253	30.8	23.4	35.0
125	21.4	15.3	22.9


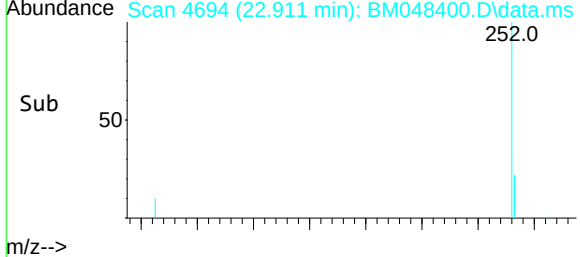

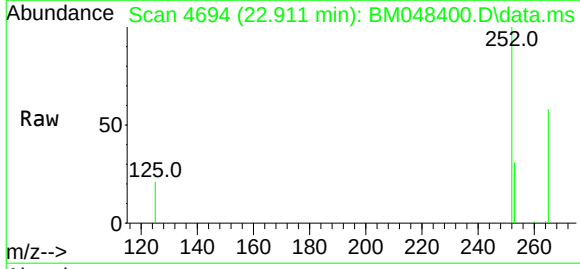


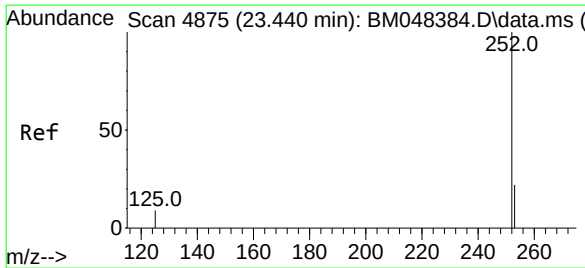

#26
Benzo(a)pyrene
Concen: 0.407 ng/ul
RT: 23.454 min Scan# 4875
Delta R.T. 0.015 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03




Instrument :
BNA_M
ClientSampleId :
SLCS424


Tgt Ion:	252	Resp:	13563
Ion Ratio	Lower	Upper	
252	100		
253	38.1	27.7	41.5
125	30.0	21.1	31.7

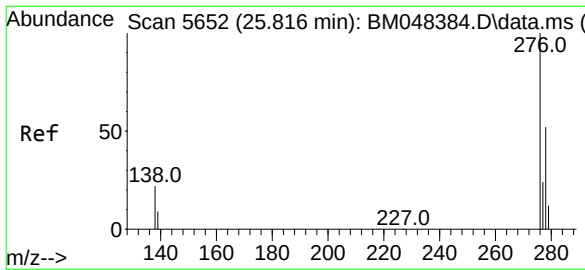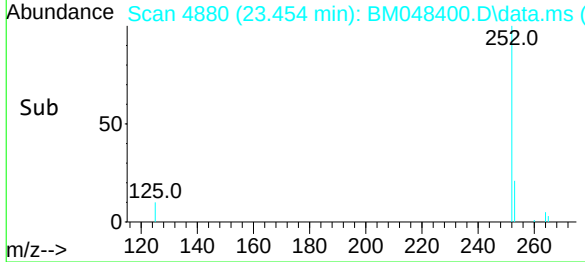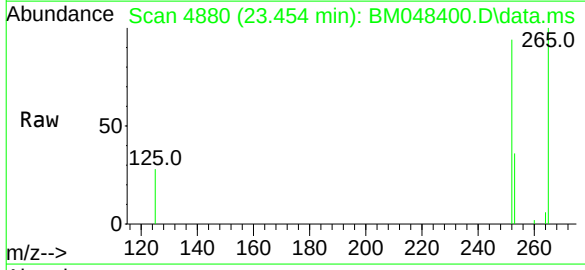

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.390 ng/ul
RT: 25.839 min Scan# 5659
Delta R.T. 0.027 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03


Tgt Ion:	276	Resp:	18192
Ion Ratio	Lower	Upper	
276	100		
138	23.8	19.6	29.4
227	0.1	0.1	0.1

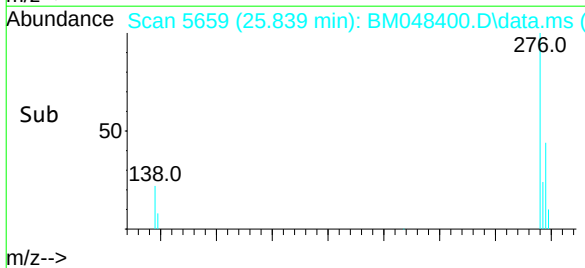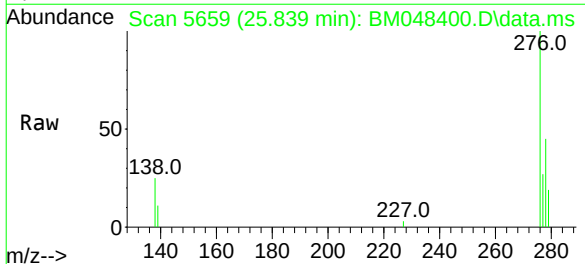



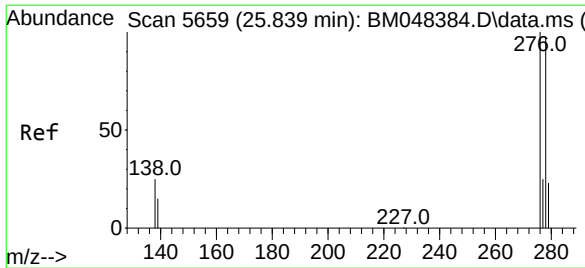


#28
Dibenzo(a,h)anthracene
Concen: 0.385 ng/ul
RT: 25.863 min Scan# 561
Delta R.T. 0.027 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03

Instrument :
BNA_M
ClientSampleId :
SLCS424

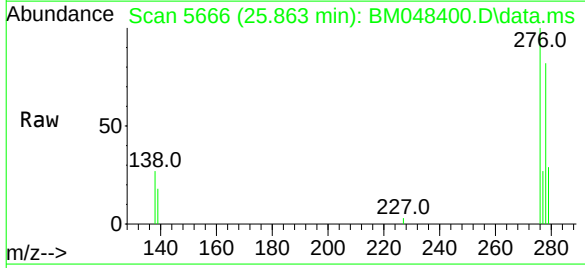

Tgt Ion:	278	Resp:	14009
Ion	Ratio	Lower	Upper
278	100		
139	21.5	15.6	23.4
279	34.8	26.4	39.6

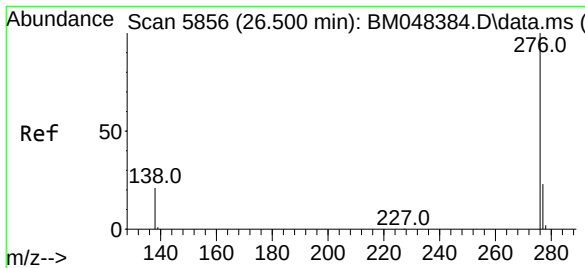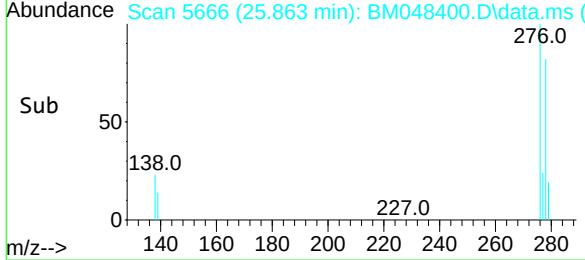

#29
Benzo(g,h,i)perylene
Concen: 0.406 ng/ul
RT: 26.517 min Scan# 5861
Delta R.T. 0.017 min
Lab File: BM048400.D
Acq: 01 Nov 2024 18:03

Tgt Ion:	276	Resp:	15945
Ion	Ratio	Lower	Upper
276	100		
138	23.5	19.0	28.6
277	26.1	20.6	31.0

