

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003028.D
 Acq On : 01 Nov 2015 14:48
 Operator : UM/IZ
 Sample : G4210-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7E8

Quant Time: Nov 02 01:24:39 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 02 01:03:38 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	131579	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	574642	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	309260	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.15	188	643045	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	652671	20.00	ng/ul	0.00
86) Perylene-d12	23.61	264	639512	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	15360	5.50	ng/uL	0.00
5) Phenol-d5	6.93	99	310677	29.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	191896	31.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	266950	30.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	257180	30.67	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	117068	33.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	122032	34.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	242680	30.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	314020	30.48	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	806698	34.67	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	987743	33.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	108987	27.79	ng/ul	0.00
58) Fluorene-d10	15.40	176	694678	34.53	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	80743	27.11	ng/ul	0.00
71) Anthracene-d10	17.25	188	1026317	36.00	ng/ul	0.00
79) Pyrene-d10	19.55	212	1103013	34.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.47	264	1121157	36.89	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.87	163	305400	12.88	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003028.D
Acq On : 01 Nov 2015 14:48
Operator : UM/IZ
Sample : G4210-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7E8

Quant Time: Nov 02 01:24:39 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 02 01:03:38 2015
Response via : Initial Calibration

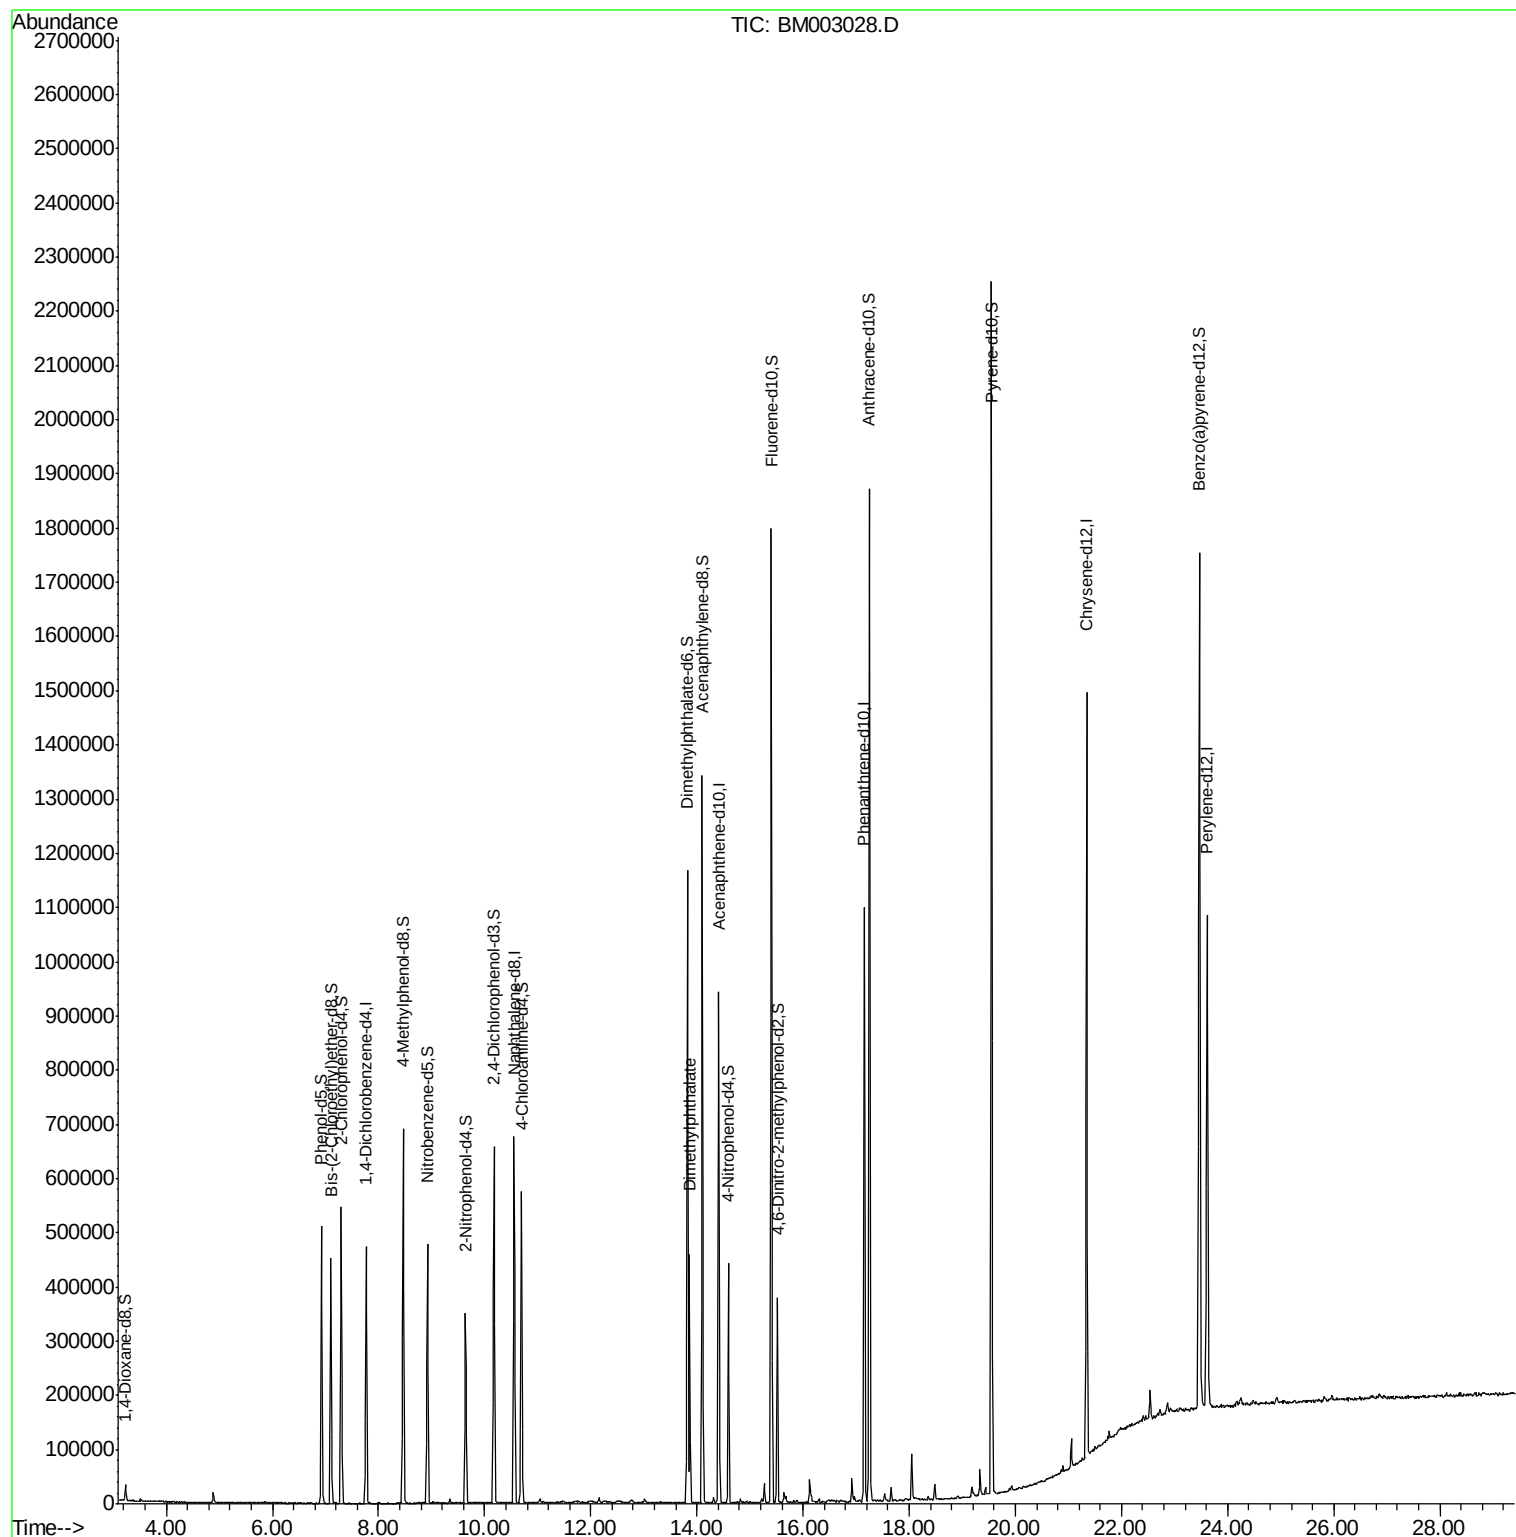

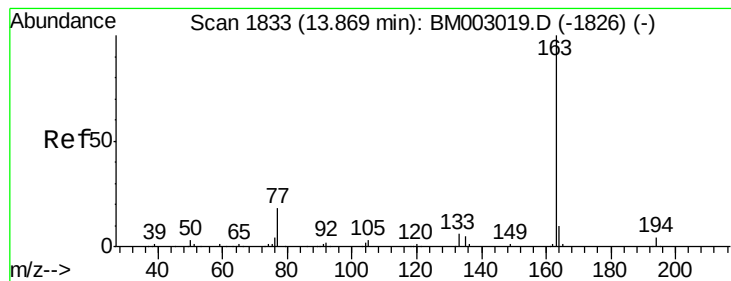

#45
 Dimethylphthalate
 Concen: 12.88 ng/ul
 RT: 13.87 min Scan# 1833
 Delta R.T. -0.00 min
 Lab File: BM003028.D
 Acq: 01 Nov 2015 14:48

Instrument :
 BNA_M
 ClientSampleId :
 BC7E8

Tgt Ion:	163	Resp:	305400
Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.2	4.8
164	9.8	7.8	11.8

