

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003022.D
 Acq On : 01 Nov 2015 11:12
 Operator : UM/IZ
 Sample : G4211-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC761

Quant Time: Nov 02 01:23:09 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 02 01:03:38 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	120223	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	530374	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	285038	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.16	188	596779	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	613302	20.00	ng/ul	0.00
86) Perylene-d12	23.62	264	606987	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	4247	1.67	ng/uL	0.00
5) Phenol-d5	6.93	99	82362	8.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	204553	36.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	240205	29.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	153641	20.05	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	126397	39.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	131050	39.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	253406	34.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	8763	0.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	831748	38.79	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	1033191	38.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	22063	6.10	ng/ul	0.00
58) Fluorene-d10	15.40	176	725204	39.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	83542	30.23	ng/ul	0.00
71) Anthracene-d10	17.25	188	1057750	39.98	ng/ul	0.00
79) Pyrene-d10	19.55	212	1149806	38.08	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.47	264	1167501	40.48	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
33) 4-Chloro-3-methylphenol	11.83	107	11446	1.44	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003022.D
Acq On : 01 Nov 2015 11:12
Operator : UM/IZ
Sample : G4211-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC761

Quant Time: Nov 02 01:23:09 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 02 01:03:38 2015
Response via : Initial Calibration

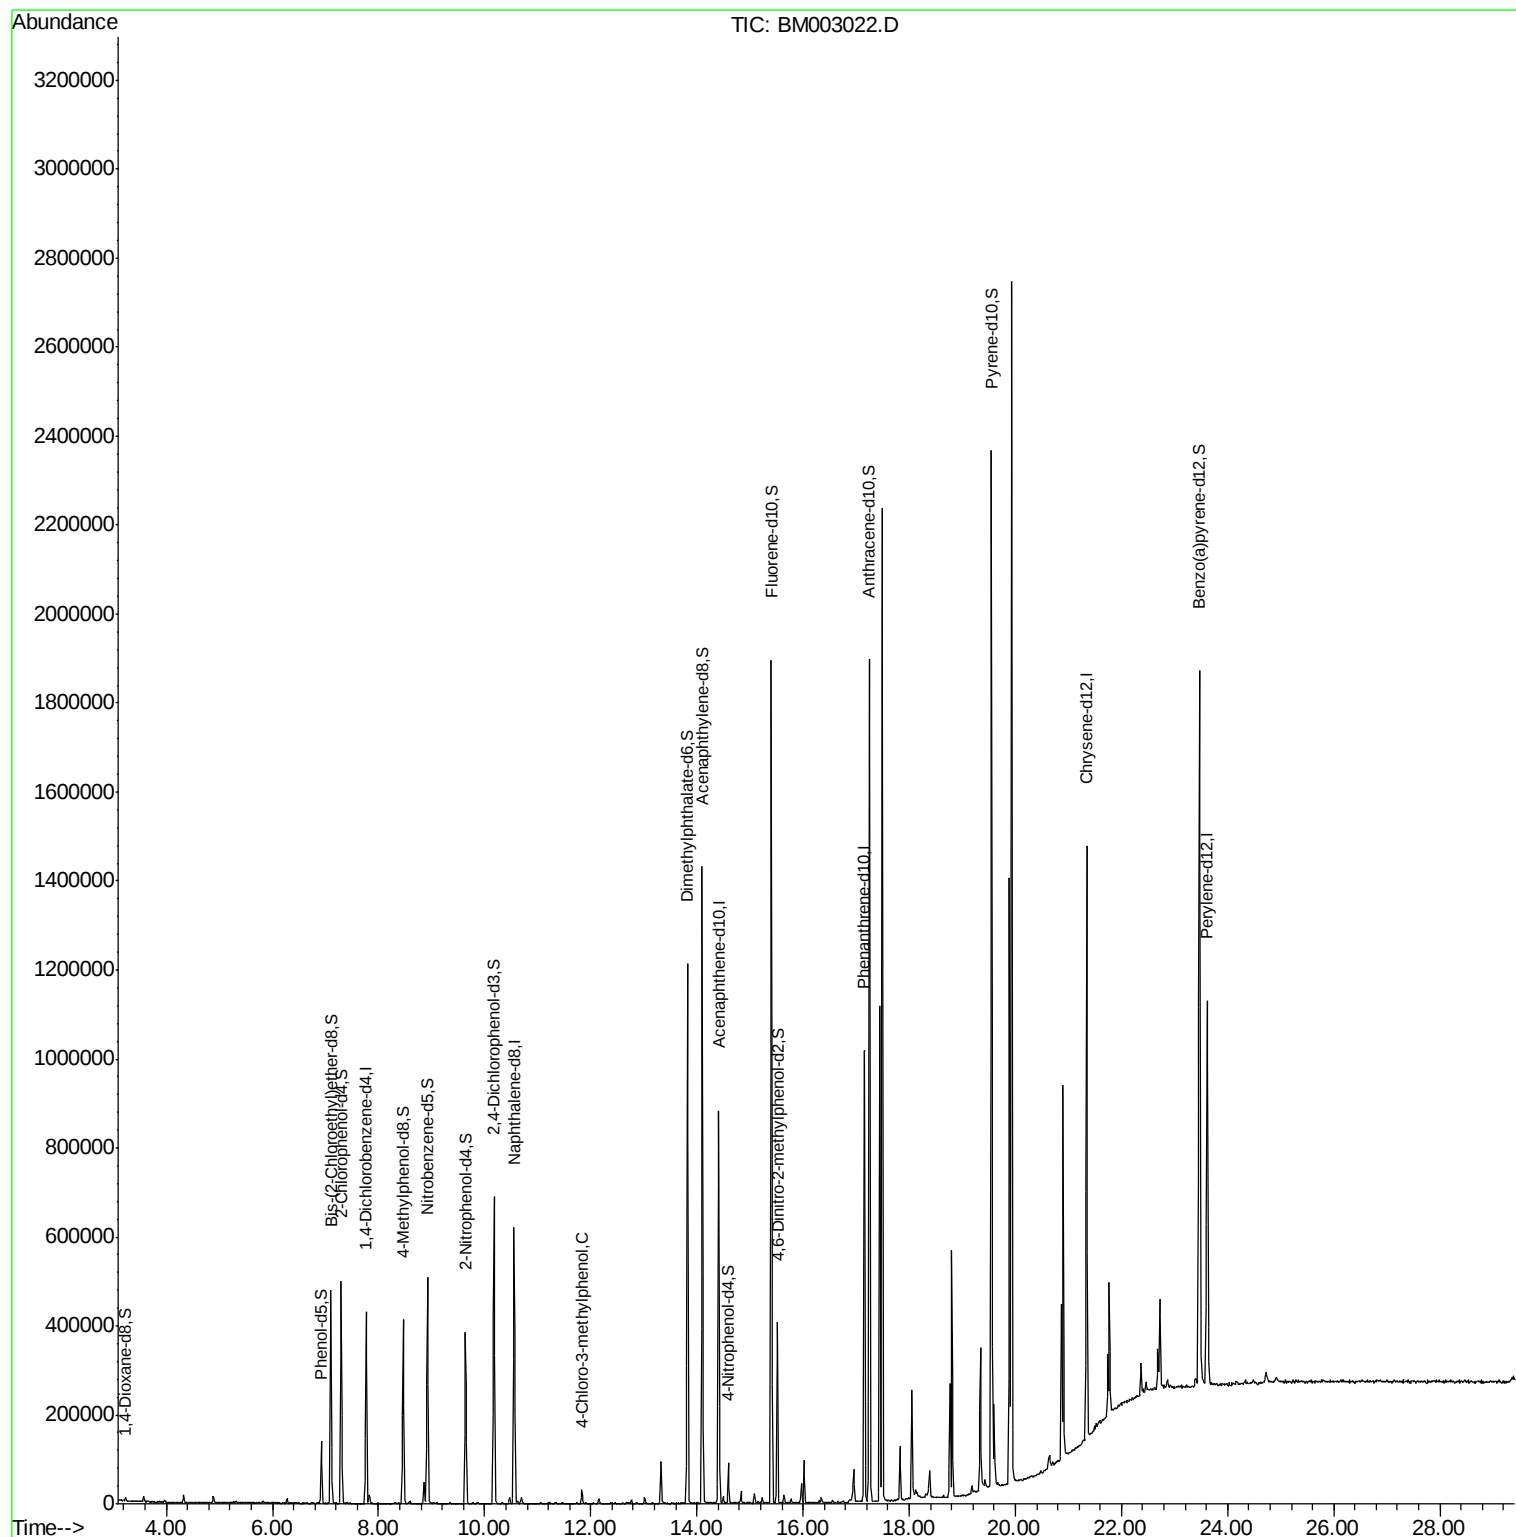


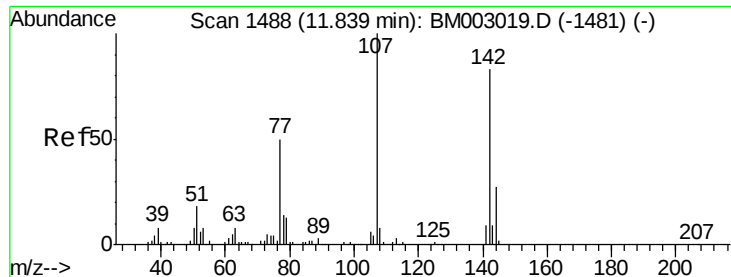

#33
 4-Chloro-3-methylphenol
 Concen: 1.44 ng/ul
 RT: 11.83 min Scan# 1487
 Delta R.T. -0.01 min
 Lab File: BM003022.D
 Acq: 01 Nov 2015 11:12

Instrument :
 BNA_M
 ClientSampleId :
 BC761

Tgt Ion	Ratio	Lower	Upper
107	100		
144	27.2	22.8	34.2
142	86.3	69.5	104.3

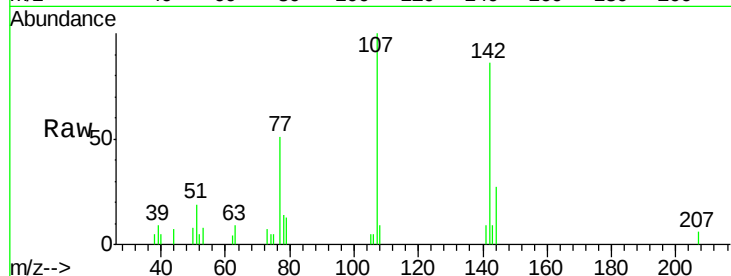

Abundance

Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E

