

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003045.D
 Acq On : 02 Nov 2015 01:37
 Operator : UM/IZ
 Sample : G4210-20
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7E0

Quant Time: Nov 02 02:54:00 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 02 02:48:24 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	255936	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	1087958	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	566657	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.15	188	1145702	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	1179513	20.00	ng/ul	0.00
86) Perylene-d12	23.61	264	1191761	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	17486	3.22	ng/uL	0.00
5) Phenol-d5	6.93	99	363747	17.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	211748	17.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	314838	18.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	300673	18.43	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	146661	22.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	156190	23.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	285895	18.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	337999	17.33	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	856288	20.09	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	1065172	19.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.60	143	124744	17.36	ng/ul	0.00
58) Fluorene-d10	15.40	176	725815	19.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	79123	14.91	ng/ul	0.00
71) Anthracene-d10	17.25	188	1051590	20.70	ng/ul	0.00
79) Pyrene-d10	19.55	212	1106390	19.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.47	264	1198703	21.17	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.86	163	402908	9.28	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003045.D
Acq On : 02 Nov 2015 01:37
Operator : UM/IZ
Sample : G4210-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7E0

Quant Time: Nov 02 02:54:00 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 02 02:48:24 2015
Response via : Initial Calibration

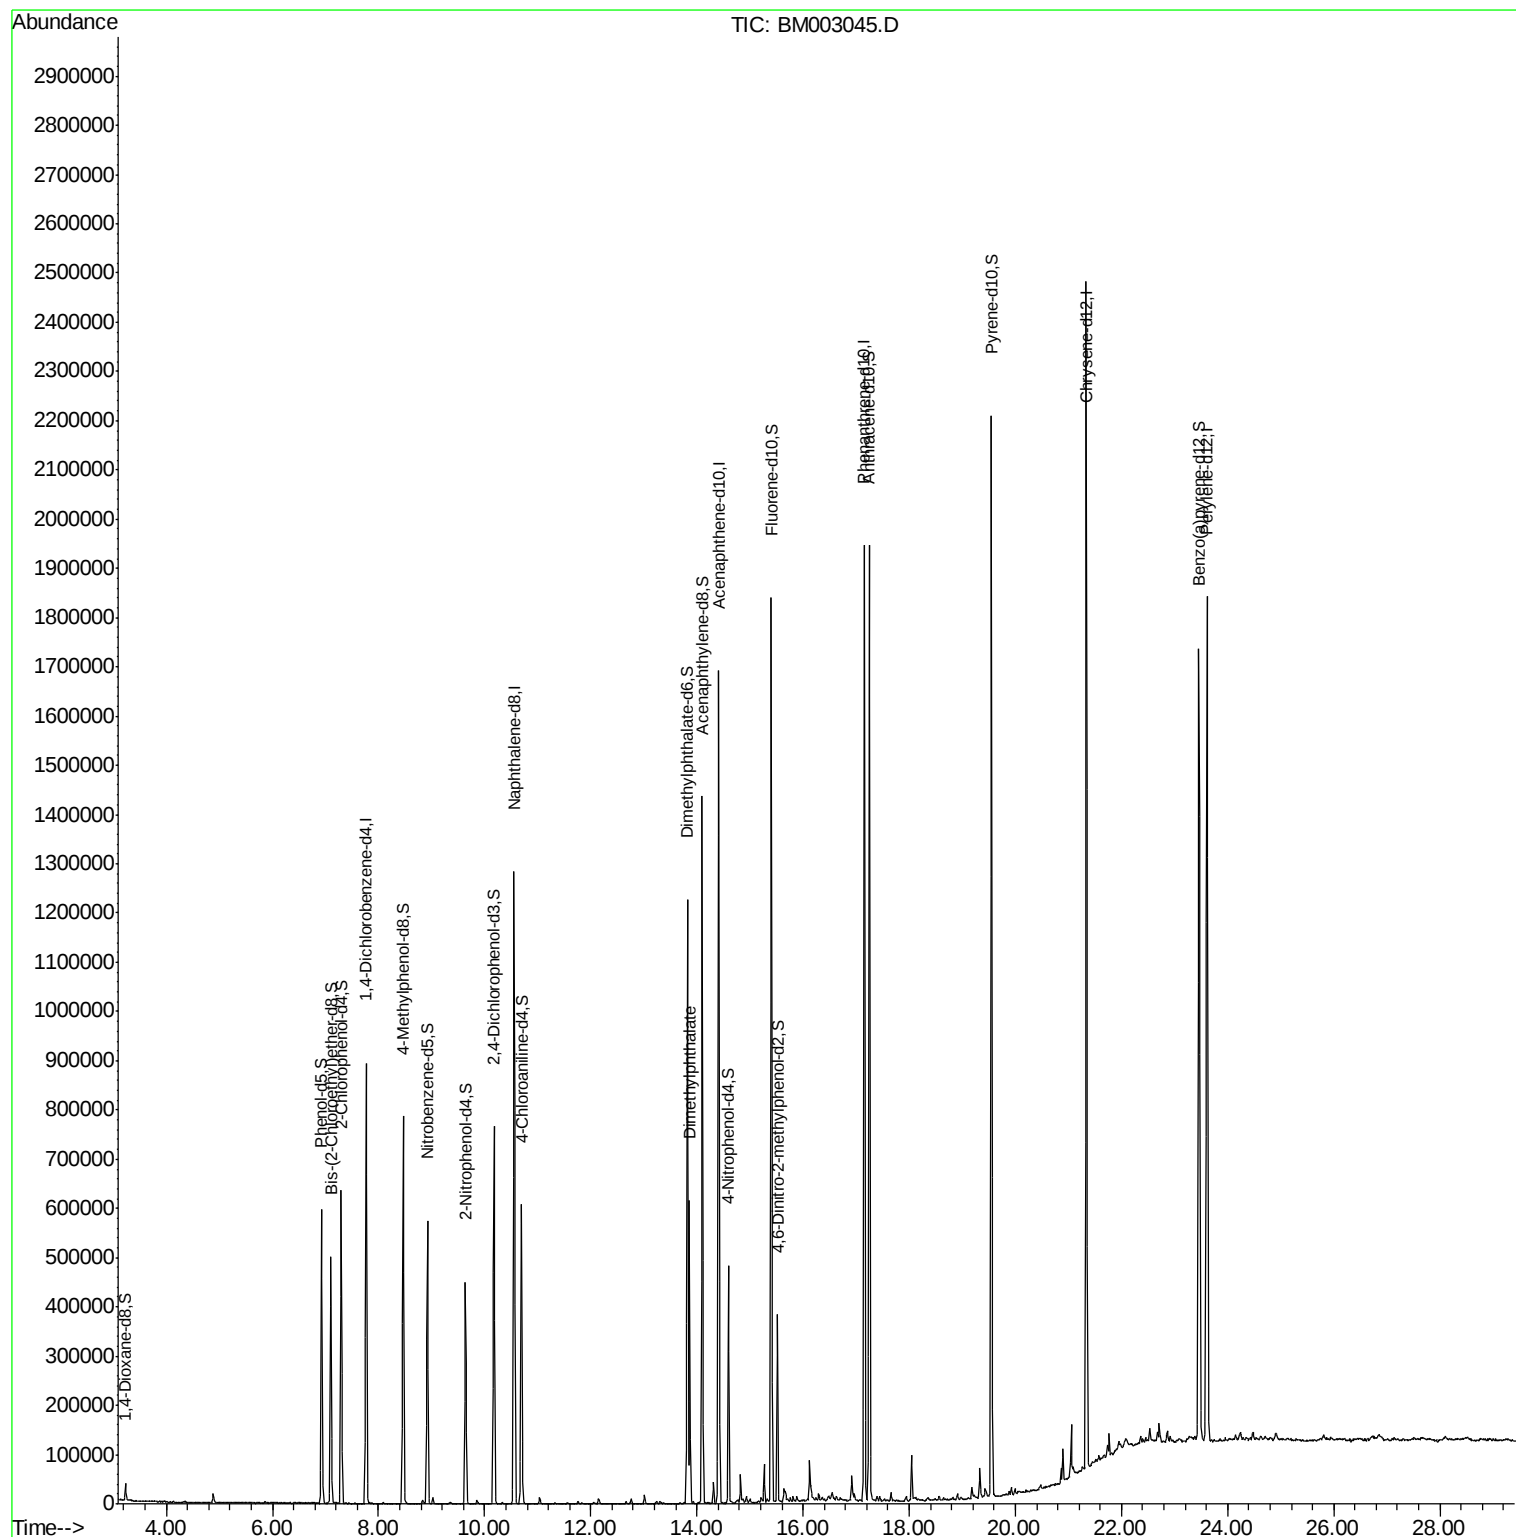

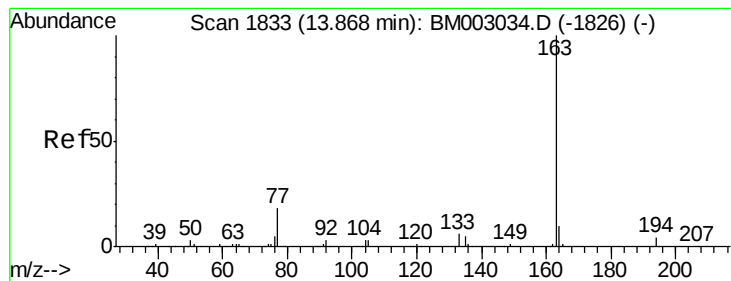

#45

Dimethylphthalate

Concen: 9.28 ng/ul

RT: 13.86 min Scan# 1832

Delta R.T. -0.01 min

Lab File: BM003045.D


Acq: 02 Nov 2015 01:37

Instrument :

BNA_M

ClientSampleId :

BC7E0

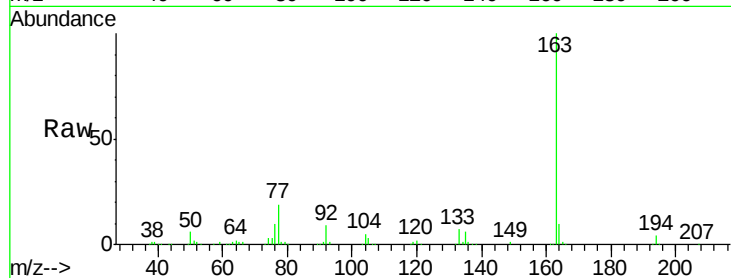

Tgt Ion:	163	Resp:	402908
Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.2	4.8
164	10.1	7.8	11.8

