

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003027.D
 Acq On : 01 Nov 2015 14:12
 Operator : UM/IZ
 Sample : G4210-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7E7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	21	rBV2	3900	4299	0.12%	0.011%
2	3.228	21	24	33	rVB	35431	45563	1.31%	0.121%
3	4.293	201	205	210	rVB	4020	5255	0.15%	0.014%
4	4.499	237	240	243	rVB2	3088	3846	0.11%	0.010%
5	4.893	302	307	310	rBV3	2759	4531	0.13%	0.012%
6	5.981	489	492	499	rVB3	2434	3985	0.11%	0.011%
7	6.928	646	653	663	rBV	579568	913484	26.26%	2.435%
8	7.098	674	682	692	rBV	518578	789148	22.69%	2.104%
9	7.298	709	716	723	rBV	635332	976083	28.06%	2.602%
10	7.769	789	796	803	rBV	515442	808108	23.23%	2.154%
11	8.463	907	914	925	rBV	771881	1197454	34.42%	3.192%
12	8.922	985	992	1000	rVB	556744	858416	24.68%	2.288%
13	9.022	1005	1009	1015	rVB	7431	9613	0.28%	0.026%
14	9.640	1107	1114	1123	rBV	409754	671221	19.30%	1.789%
15	9.857	1148	1151	1156	rBV2	3471	4756	0.14%	0.013%
16	10.175	1198	1205	1215	rBV	752656	1230785	35.38%	3.281%
17	10.557	1263	1270	1282	rBV	736533	1225901	35.24%	3.268%
18	10.692	1286	1293	1302	rBV	630697	1036318	29.79%	2.762%
19	11.039	1347	1352	1360	rBV	28590	44935	1.29%	0.120%
20	11.463	1421	1424	1436	rBV	2889	6847	0.20%	0.018%
21	12.151	1535	1541	1545	rVB	11062	17406	0.50%	0.046%
22	12.763	1641	1645	1652	rBV2	9386	12531	0.36%	0.033%
23	13.016	1684	1688	1692	rVB	16712	21435	0.62%	0.057%
24	13.822	1818	1825	1829	rBV	1414694	1977947	56.86%	5.273%
25	13.863	1829	1832	1842	rVB	689689	974217	28.01%	2.597%
26	14.104	1866	1873	1883	rVB	1581831	2356011	67.73%	6.280%
27	14.316	1904	1909	1913	rVB	28098	36008	1.04%	0.096%
28	14.410	1918	1925	1935	rVB2	1069087	1618515	46.53%	4.314%
29	14.592	1947	1956	1964	rBV	506197	711715	20.46%	1.897%
30	14.757	1978	1984	1985	rBV3	5374	7105	0.20%	0.019%
31	14.822	1991	1995	2000	rBV2	22549	29855	0.86%	0.080%
32	14.869	2000	2003	2009	rVB	5534	9319	0.27%	0.025%
33	14.927	2009	2013	2020	rVB2	10819	16691	0.48%	0.044%
34	15.004	2020	2026	2032	rBV	7244	11068	0.32%	0.030%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003027.D
 Acq On : 01 Nov 2015 14:12
 Operator : UM/IZ
 Sample : G4210-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7E7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

35	15.157	2048	2052	2054	rBV4	2469	4061	0.12%	0.011%
36	15.216	2058	2062	2066	rVV3	5721	10532	0.30%	0.028%
37	15.269	2066	2071	2076	rVV	72745	90936	2.61%	0.242%
38	15.327	2076	2081	2084	rVV2	4944	8625	0.25%	0.023%
39	15.404	2087	2094	2101	rVB	2161388	3006162	86.42%	8.013%
40	15.516	2107	2113	2119	rBV	439513	582025	16.73%	1.551%
41	15.645	2129	2135	2138	rBV2	29893	50308	1.45%	0.134%
42	15.710	2144	2146	2151	rVB4	5619	6509	0.19%	0.017%
43	15.769	2152	2156	2160	rVB2	9397	11315	0.33%	0.030%
44	15.821	2160	2165	2171	rBV2	11647	16699	0.48%	0.045%
45	15.886	2171	2176	2180	rBV2	9309	12768	0.37%	0.034%
46	16.021	2196	2199	2203	rVB3	3161	4179	0.12%	0.011%
47	16.080	2203	2209	2213	rBV4	3272	7675	0.22%	0.020%
48	16.127	2213	2217	2221	rBV	86620	120547	3.47%	0.321%
49	16.304	2243	2247	2250	rBV2	11593	13879	0.40%	0.037%
50	16.474	2271	2276	2279	rBV3	8289	14507	0.42%	0.039%
51	16.533	2283	2286	2287	rBV3	5473	6123	0.18%	0.016%
52	16.586	2292	2295	2298	rVV2	4944	6247	0.18%	0.017%
53	16.633	2299	2303	2310	rVV5	6464	9584	0.28%	0.026%
54	16.698	2311	2314	2317	rVV2	5556	6174	0.18%	0.016%
55	16.727	2317	2319	2323	rVB2	3080	3630	0.10%	0.010%
56	16.921	2346	2352	2358	rBV2	33639	52271	1.50%	0.139%
57	16.968	2358	2360	2365	rVB	8841	11373	0.33%	0.030%
58	17.151	2385	2391	2397	rBV2	1248371	1817208	52.24%	4.844%
59	17.251	2401	2408	2422	rVB2	2099817	3119698	89.69%	8.316%
60	17.439	2437	2440	2445	rBV3	3892	5983	0.17%	0.016%
61	17.492	2445	2449	2451	rVB2	4479	5304	0.15%	0.014%
62	17.657	2472	2477	2482	rBV5	4578	7970	0.23%	0.021%
63	17.951	2520	2527	2535	rBV3	9697	18900	0.54%	0.050%
64	18.045	2535	2543	2551	rVV2	110495	162929	4.68%	0.434%
65	18.121	2554	2556	2560	rVB	7904	9301	0.27%	0.025%
66	18.221	2569	2573	2577	rBV6	3419	5972	0.17%	0.016%
67	18.357	2591	2596	2600	rBV4	6046	10365	0.30%	0.028%
68	18.568	2629	2632	2637	rVB	5996	7535	0.22%	0.020%
69	18.909	2686	2690	2693	rBV2	6610	9953	0.29%	0.027%
70	19.186	2732	2737	2739	rVV	20042	29473	0.85%	0.079%
71	19.215	2739	2742	2748	rVB	12264	18748	0.54%	0.050%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003027.D
Acq On : 01 Nov 2015 14:12
Operator : UM/IZ
Sample : G4210-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7E7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Title : SVOA CALIBRATION

72	19.333	2758	2762	2771	rBV2	68005	90427	2.60%	0.241%
73	19.439	2776	2780	2783	rVV	16163	19540	0.56%	0.052%
74	19.551	2793	2799	2806	rBV	2548104	3478449	100.00%	9.272%
75	19.892	2854	2857	2860	rBV3	16261	15874	0.46%	0.042%
76	19.927	2860	2863	2867	rVB	30064	31344	0.90%	0.084%
77	20.868	3020	3023	3026	rBV4	16397	16884	0.49%	0.045%
78	20.903	3026	3029	3033	rVB2	30713	32691	0.94%	0.087%
79	21.056	3051	3055	3059	rBV2	62499	73827	2.12%	0.197%
80	21.345	3098	3104	3109	rBV	1508202	1929169	55.46%	5.142%
81	23.468	3458	3465	3478	rBV	1652641	3127678	89.92%	8.337%
82	23.615	3483	3490	3502	rVB	901136	1772531	50.96%	4.725%


Sum of corrected areas: 37514253

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003027.D
Acq On : 01 Nov 2015 14:12
Operator : UM/IZ
Sample : G4210-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7E7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

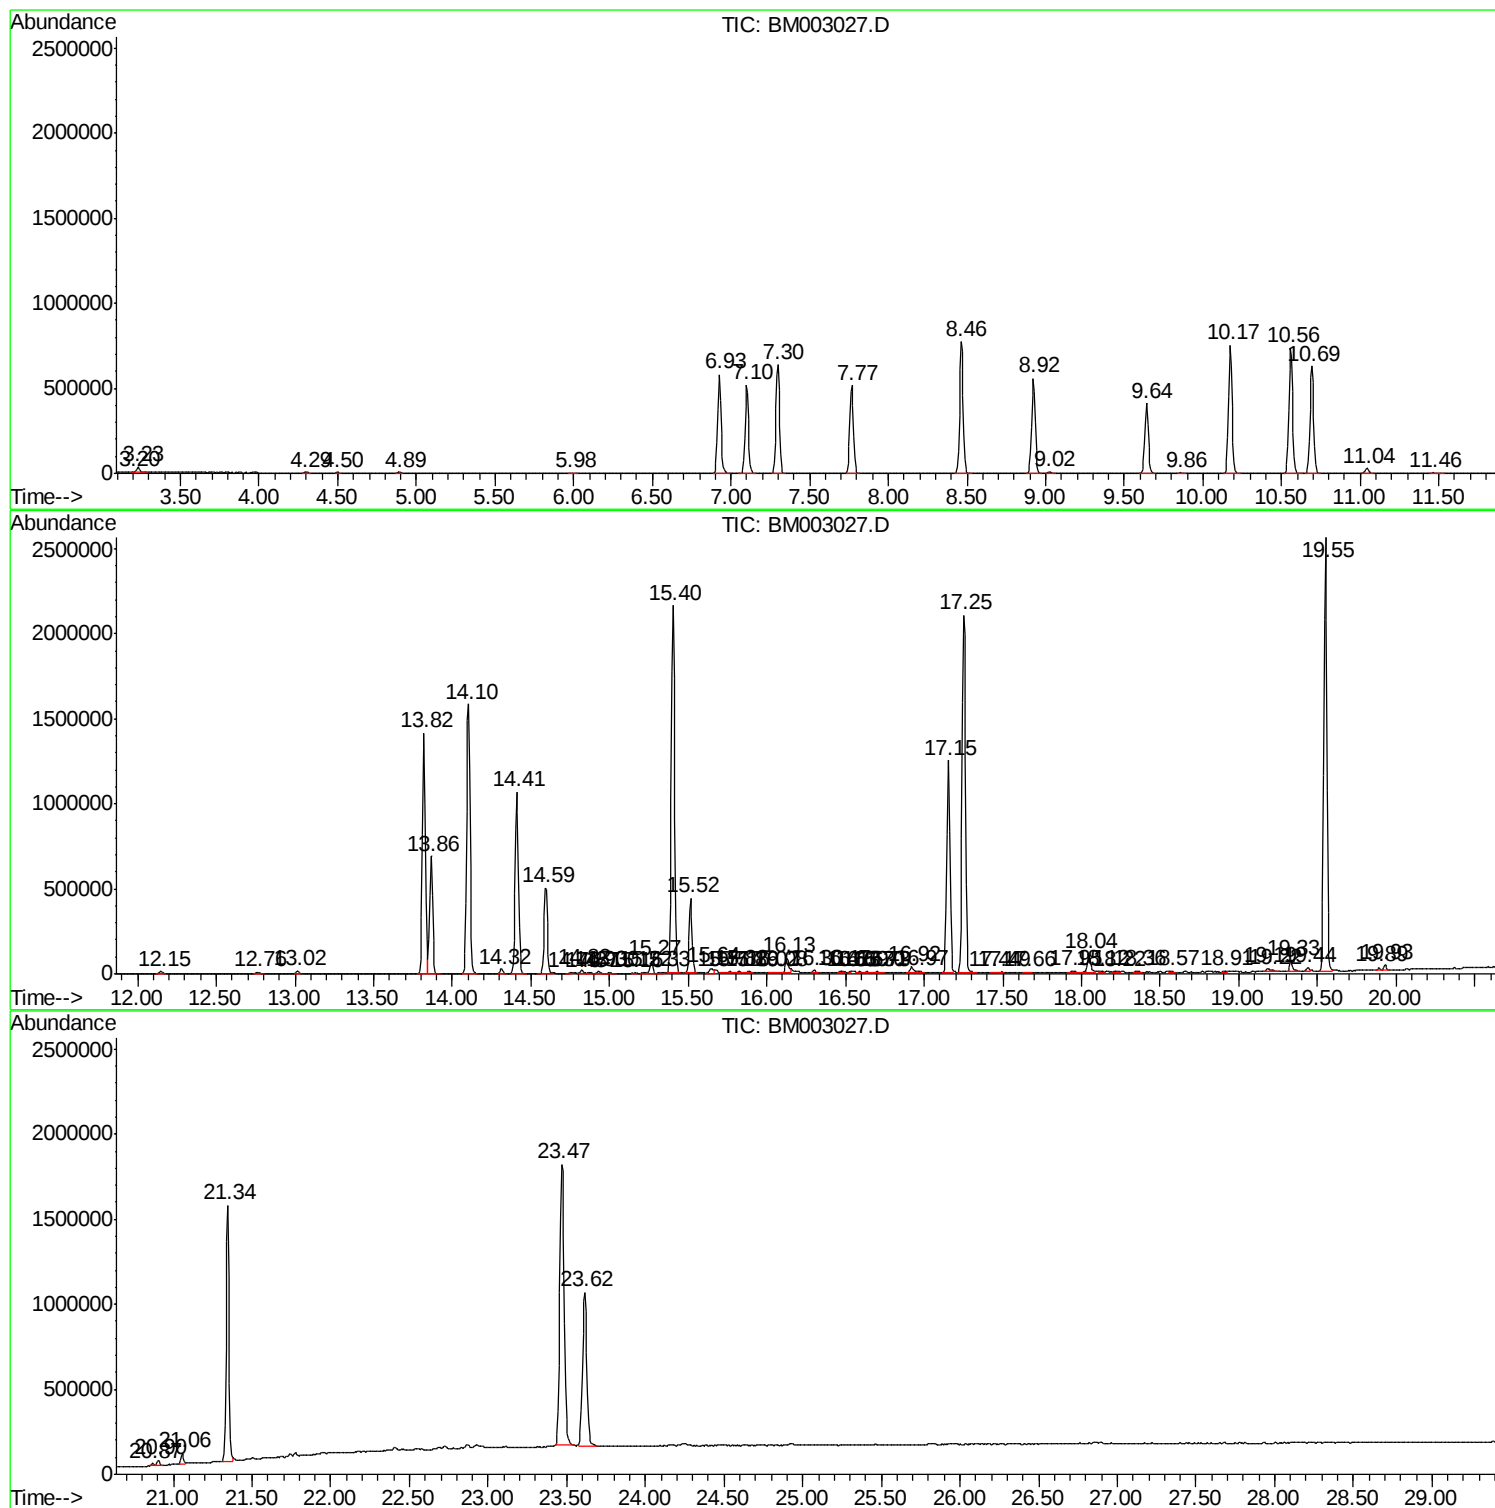

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003027.D
Acq On : 01 Nov 2015 14:12
Operator : UM/IZ
Sample : G4210-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7E7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003027.D
Acq On : 01 Nov 2015 14:12
Operator : UM/IZ
Sample : G4210-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7E7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc