

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003030.D
 Acq On : 01 Nov 2015 16:01
 Operator : UM/IZ
 Sample : G4210-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7D5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	32	rVB	36855	47570	1.20%	0.115%
2	4.893	299	307	313	rVB3	5253	10360	0.26%	0.025%
3	6.740	616	621	628	rBV	3212	5544	0.14%	0.013%
4	6.928	646	653	668	rVB	597288	989224	24.94%	2.401%
5	7.099	675	682	695	rVB	528239	809370	20.41%	1.964%
6	7.299	709	716	725	rVB	639777	1007301	25.40%	2.445%
7	7.769	789	796	803	rBV	485596	770641	19.43%	1.870%
8	8.463	907	914	926	rBV	825748	1284405	32.38%	3.117%
9	8.922	984	992	1003	rVB	570799	895102	22.57%	2.172%
10	9.034	1005	1011	1017	rBV	33079	53525	1.35%	0.130%
11	9.351	1060	1065	1069	rBV	3273	4858	0.12%	0.012%
12	9.640	1107	1114	1122	rVB	438741	705121	17.78%	1.711%
13	9.857	1147	1151	1158	rVB	4222	6362	0.16%	0.015%
14	10.175	1198	1205	1216	rVB	799340	1288888	32.50%	3.128%
15	10.557	1263	1270	1282	rVB	728133	1218933	30.73%	2.958%
16	10.693	1286	1293	1302	rBV	756627	1243032	31.34%	3.017%
17	12.145	1534	1540	1545	rBV	11896	18810	0.47%	0.046%
18	12.763	1639	1645	1649	rVB	8711	12107	0.31%	0.029%
19	13.016	1683	1688	1693	rVB	13795	19819	0.50%	0.048%
20	13.239	1720	1726	1730	rBV2	7008	9825	0.25%	0.024%
21	13.310	1734	1738	1742	rBV4	2826	5149	0.13%	0.012%
22	13.822	1818	1825	1829	rBV	1493319	2142597	54.02%	5.200%
23	13.869	1829	1833	1841	rVV	927690	1264940	31.89%	3.070%
24	13.939	1841	1845	1850	rVB	5794	7641	0.19%	0.019%
25	14.016	1854	1858	1862	rBV	4698	5563	0.14%	0.014%
26	14.104	1866	1873	1882	rVB	1679248	2537813	63.99%	6.159%
27	14.316	1902	1909	1913	rBV	60443	80104	2.02%	0.194%
28	14.410	1917	1925	1932	rBV2	1092815	1687131	42.54%	4.095%
29	14.592	1950	1956	1964	rBV	607991	853214	21.51%	2.071%
30	14.651	1964	1966	1971	rVB4	4950	6521	0.16%	0.016%
31	14.763	1979	1985	1990	rBV4	10633	24604	0.62%	0.060%
32	14.822	1990	1995	1999	rVV3	35376	49097	1.24%	0.119%
33	14.869	1999	2003	2007	rVV2	8934	14605	0.37%	0.035%
34	14.933	2009	2014	2021	rVV5	16814	27957	0.70%	0.068%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003030.D
 Acq On : 01 Nov 2015 16:01
 Operator : UM/IZ
 Sample : G4210-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7D5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

35	15.004	2021	2026	2030	rVB2	10225	13767	0.35%	0.033%
36	15.216	2057	2062	2066	rBV	21927	32883	0.83%	0.080%
37	15.263	2066	2070	2076	rVV	106253	136533	3.44%	0.331%
38	15.328	2076	2081	2084	rVV3	7959	12341	0.31%	0.030%
39	15.404	2085	2094	2101	rVB	2221386	3245368	81.83%	7.877%
40	15.516	2107	2113	2120	rBV	543024	708751	17.87%	1.720%
41	15.645	2130	2135	2137	rBV2	35305	52977	1.34%	0.129%
42	15.710	2144	2146	2152	rVB2	8827	10624	0.27%	0.026%
43	15.763	2152	2155	2160	rVB2	12172	16561	0.42%	0.040%
44	15.822	2161	2165	2170	rBV2	15803	22019	0.56%	0.053%
45	15.886	2172	2176	2180	rVB3	15503	19340	0.49%	0.047%
46	16.080	2205	2209	2212	rBV3	5575	8218	0.21%	0.020%
47	16.127	2212	2217	2220	rBV	117446	160648	4.05%	0.390%
48	16.298	2242	2246	2250	rVB	15506	21187	0.53%	0.051%
49	16.357	2250	2256	2258	rBV5	5284	8577	0.22%	0.021%
50	16.392	2260	2262	2267	rVV5	4032	6149	0.16%	0.015%
51	16.469	2271	2275	2279	rBV	16965	29403	0.74%	0.071%
52	16.533	2283	2286	2287	rVV	10973	12625	0.32%	0.031%
53	16.551	2287	2289	2292	rVV2	13727	16266	0.41%	0.039%
54	16.586	2292	2295	2298	rVV2	9660	10755	0.27%	0.026%
55	16.633	2300	2303	2311	rVV4	10571	16083	0.41%	0.039%
56	16.698	2311	2314	2317	rVV	7880	9506	0.24%	0.023%
57	16.733	2317	2320	2324	rVB2	4179	5056	0.13%	0.012%
58	16.869	2340	2343	2346	rBV4	3626	5801	0.15%	0.014%
59	16.922	2346	2352	2357	rVV2	78858	113294	2.86%	0.275%
60	16.969	2357	2360	2365	rVB2	20992	32331	0.82%	0.078%
61	17.151	2385	2391	2398	rBV2	1374362	1984432	50.04%	4.816%
62	17.251	2400	2408	2415	rBV2	2390450	3503587	88.34%	8.503%
63	17.345	2422	2424	2428	rVB4	5721	6546	0.17%	0.016%
64	17.392	2429	2432	2433	rVV	6064	6550	0.17%	0.016%
65	17.445	2437	2441	2450	rVB	15999	27256	0.69%	0.066%
66	17.527	2450	2455	2460	rBV3	5202	10496	0.26%	0.025%
67	17.657	2473	2477	2481	rVB	35270	38842	0.98%	0.094%
68	17.951	2520	2527	2534	rBV3	16333	33543	0.85%	0.081%
69	18.010	2534	2537	2539	rBV4	3573	4611	0.12%	0.011%
70	18.045	2539	2543	2550	rBV	127672	172259	4.34%	0.418%
71	18.163	2561	2563	2568	rBV6	2810	4030	0.10%	0.010%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003030.D
Acq On : 01 Nov 2015 16:01
Operator : UM/IZ
Sample : G4210-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7D5

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Title : SVOA CALIBRATION

72	18.351	2591	2595	2601	rVB4	15348	21277	0.54%	0.052%
73	18.568	2628	2632	2635	rVB2	7711	10965	0.28%	0.027%
74	18.910	2687	2690	2693	rBV	8596	9950	0.25%	0.024%
75	19.186	2732	2737	2740	rBV2	39391	55413	1.40%	0.134%
76	19.333	2758	2762	2775	rBV	118163	157965	3.98%	0.383%
77	19.439	2776	2780	2786	rVB	20649	28681	0.72%	0.070%
78	19.551	2793	2799	2806	rBV	2922800	3966061	100.00%	9.626%
79	21.057	3051	3055	3060	rBV	98933	126139	3.18%	0.306%
80	21.345	3099	3104	3112	rBV	1685034	2096527	52.86%	5.088%
81	23.474	3458	3466	3479	rBV	1716580	3281764	82.75%	7.965%
82	23.615	3483	3490	3503	rVB	959701	1820344	45.90%	4.418%


Sum of corrected areas: 41202034

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003030.D
Acq On : 01 Nov 2015 16:01
Operator : UM/IZ
Sample : G4210-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7D5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

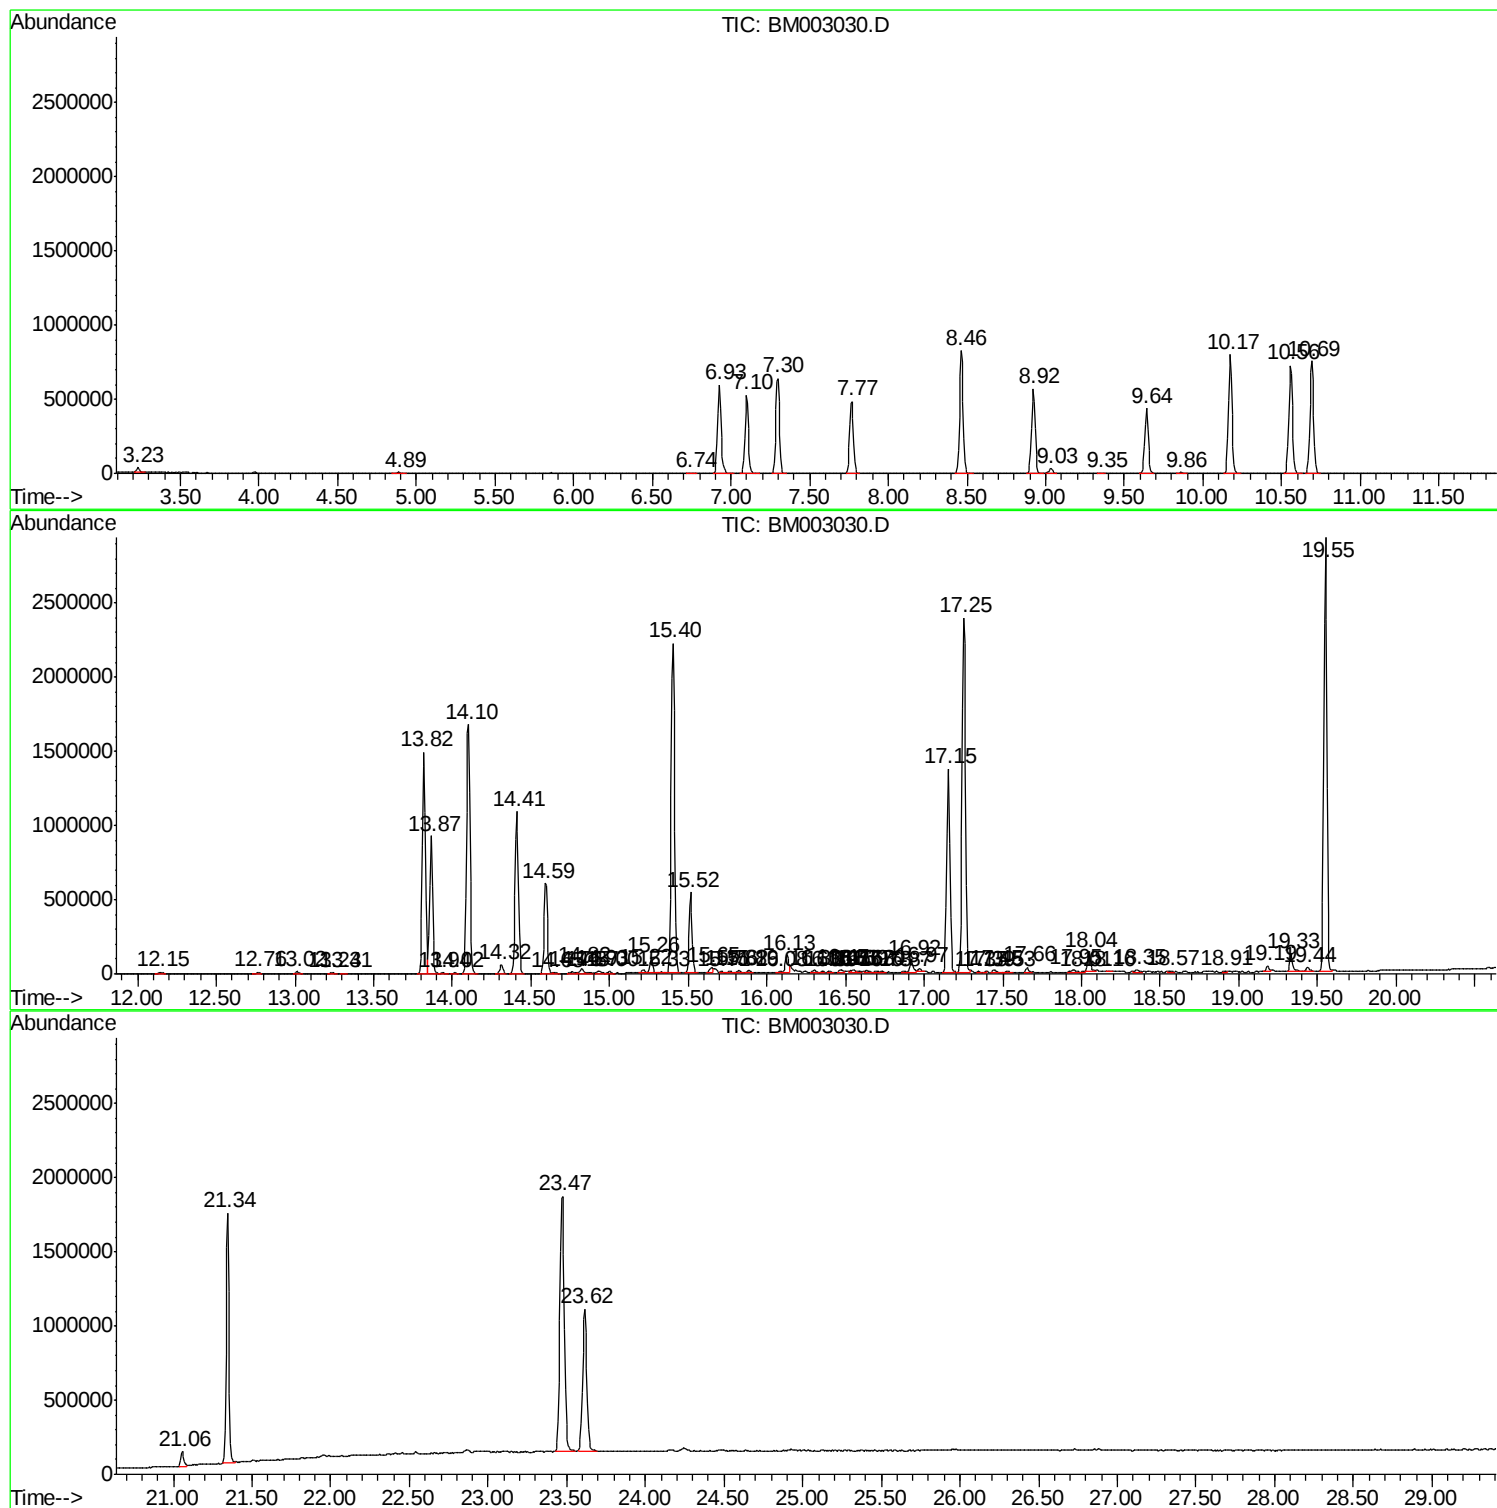

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003030.D
Acq On : 01 Nov 2015 16:01
Operator : UM/IZ
Sample : G4210-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7D5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003030.D
Acq On : 01 Nov 2015 16:01
Operator : UM/IZ
Sample : G4210-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7D5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc