

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003033.D
 Acq On : 01 Nov 2015 17:49
 Operator : UM/IZ
 Sample : G4210-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	32	rVB	33708	42160	1.29%	0.117%
2	3.969	147	150	155	rVB2	3017	4209	0.13%	0.012%
3	4.887	301	306	312	rVB2	8706	13044	0.40%	0.036%
4	5.857	468	471	476	rBV2	3342	5089	0.16%	0.014%
5	5.987	488	493	497	rVB3	2803	4332	0.13%	0.012%
6	6.928	646	653	666	rVB	555838	931628	28.40%	2.589%
7	7.098	676	682	692	rBV	494974	756175	23.05%	2.102%
8	7.298	709	716	725	rBV	603749	950160	28.97%	2.641%
9	7.769	789	796	803	rBV	475142	759149	23.14%	2.110%
10	8.075	842	848	853	rBV3	2424	5355	0.16%	0.015%
11	8.463	906	914	924	rBV	727719	1118580	34.10%	3.109%
12	8.922	984	992	1002	rVB	534174	828008	25.24%	2.301%
13	9.028	1004	1010	1018	rVB	17817	25732	0.78%	0.072%
14	9.639	1107	1114	1122	rBV	399295	648885	19.78%	1.803%
15	10.175	1197	1205	1215	rBV	728205	1167490	35.59%	3.245%
16	10.557	1263	1270	1280	rVB	706188	1152716	35.14%	3.204%
17	10.692	1285	1293	1303	rVV	607067	989092	30.15%	2.749%
18	11.045	1346	1353	1357	rBV	11939	19139	0.58%	0.053%
19	11.763	1471	1475	1480	rVB2	3758	5325	0.16%	0.015%
20	12.145	1536	1540	1545	rVB2	10149	15361	0.47%	0.043%
21	12.763	1639	1645	1649	rBV	7844	10963	0.33%	0.030%
22	13.016	1684	1688	1693	rBV	14349	19466	0.59%	0.054%
23	13.310	1734	1738	1742	rBV4	2379	3680	0.11%	0.010%
24	13.821	1818	1825	1829	rBV	1289909	1855869	56.58%	5.158%
25	13.863	1829	1832	1841	rVV	935090	1266514	38.61%	3.520%
26	13.933	1841	1844	1850	rVB3	2299	3579	0.11%	0.010%
27	14.104	1866	1873	1883	rBV	1497837	2213809	67.49%	6.153%
28	14.310	1904	1908	1913	rVB	25100	32788	1.00%	0.091%
29	14.410	1917	1925	1935	rVV2	990106	1526751	46.55%	4.243%
30	14.592	1950	1956	1965	rBV	432580	582279	17.75%	1.618%
31	14.774	1978	1987	1990	rBV3	4353	9425	0.29%	0.026%
32	14.821	1990	1995	2000	rVV	18595	26995	0.82%	0.075%
33	14.868	2000	2003	2008	rVV	5510	7852	0.24%	0.022%
34	14.933	2010	2014	2019	rVB3	8218	13024	0.40%	0.036%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
 Data File : BM003033.D
 Acq On : 01 Nov 2015 17:49
 Operator : UM/IZ
 Sample : G4210-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

35	14.998	2019	2025	2032	rBV2	5800	9535	0.29%	0.027%
36	15.216	2056	2062	2066	rBV	14998	21620	0.66%	0.060%
37	15.263	2066	2070	2076	rVB	50708	61597	1.88%	0.171%
38	15.321	2076	2080	2084	rBV4	3757	6942	0.21%	0.019%
39	15.404	2087	2094	2100	rVB	1968251	2801891	85.42%	7.787%
40	15.515	2107	2113	2119	rVB	368673	482329	14.70%	1.341%
41	15.645	2129	2135	2138	rBV3	23325	40805	1.24%	0.113%
42	15.668	2138	2139	2143	rVV2	14854	17283	0.53%	0.048%
43	15.710	2143	2146	2151	rVV4	4507	7511	0.23%	0.021%
44	15.768	2151	2156	2161	rVB2	5448	7838	0.24%	0.022%
45	15.815	2161	2164	2170	rBV3	6070	9845	0.30%	0.027%
46	15.886	2172	2176	2180	rVB3	6632	9056	0.28%	0.025%
47	16.127	2212	2217	2220	rBV	52568	70543	2.15%	0.196%
48	16.298	2243	2246	2250	rVB2	10645	14846	0.45%	0.041%
49	16.351	2254	2255	2258	rVV2	3769	4277	0.13%	0.012%
50	16.398	2259	2263	2267	rVV6	3211	5605	0.17%	0.016%
51	16.468	2270	2275	2279	rVV2	6982	13760	0.42%	0.038%
52	16.533	2282	2286	2287	rVV3	5665	7546	0.23%	0.021%
53	16.551	2287	2289	2292	rVV3	7732	9052	0.28%	0.025%
54	16.580	2292	2294	2297	rVV3	5051	5971	0.18%	0.017%
55	16.633	2299	2303	2309	rVV5	5636	11918	0.36%	0.033%
56	16.698	2309	2314	2317	rVV3	5288	8176	0.25%	0.023%
57	16.733	2317	2320	2323	rVB3	3129	3795	0.12%	0.011%
58	16.915	2346	2351	2357	rBV2	33701	50234	1.53%	0.140%
59	16.968	2357	2360	2365	rVB2	9188	13839	0.42%	0.038%
60	17.051	2371	2374	2377	rBV5	2372	3853	0.12%	0.011%
61	17.151	2385	2391	2397	rBV2	1191376	1743776	53.16%	4.847%
62	17.251	2400	2408	2420	rVV2	2017190	2924977	89.17%	8.130%
63	17.392	2429	2432	2436	rVB5	3472	4578	0.14%	0.013%
64	17.445	2437	2441	2446	rBV4	3853	6727	0.21%	0.019%
65	17.574	2461	2463	2466	rVB3	3421	3649	0.11%	0.010%
66	17.657	2472	2477	2483	rBV	14609	20656	0.63%	0.057%
67	17.951	2518	2527	2533	rBV4	7739	20771	0.63%	0.058%
68	18.045	2538	2543	2551	rBV	116330	157019	4.79%	0.436%
69	18.351	2591	2595	2598	rVB2	5478	6562	0.20%	0.018%
70	18.568	2628	2632	2635	rBV2	2679	3530	0.11%	0.010%
71	18.909	2686	2690	2692	rBV3	3873	5113	0.16%	0.014%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003033.D
Acq On : 01 Nov 2015 17:49
Operator : UM/IZ
Sample : G4210-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7D8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Title : SVOA CALIBRATION

72	19.186	2732	2737	2740	rBV2	30777	45151	1.38%	0.125%
73	19.333	2757	2762	2773	rBV	131996	178452	5.44%	0.496%
74	19.433	2776	2779	2785	rVB	16021	21200	0.65%	0.059%
75	19.486	2786	2788	2792	rVB2	7768	6337	0.19%	0.018%
76	19.551	2793	2799	2806	rBV	2322840	3280064	100.00%	9.116%
77	19.892	2853	2857	2860	rBV2	17440	19260	0.59%	0.054%
78	19.927	2860	2863	2867	rVB	39136	40751	1.24%	0.113%
79	20.897	3026	3028	3032	rBV	17774	17523	0.53%	0.049%
80	21.050	3051	3054	3059	rBV2	26680	33826	1.03%	0.094%
81	21.339	3098	3103	3109	rBV	1473909	1890452	57.63%	5.254%
82	23.468	3458	3465	3481	rVB	1590995	3044992	92.83%	8.463%
83	23.609	3483	3489	3506	rVB	960813	1789990	54.57%	4.975%


Sum of corrected areas: 35979646

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003033.D
Acq On : 01 Nov 2015 17:49
Operator : UM/IZ
Sample : G4210-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7D8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

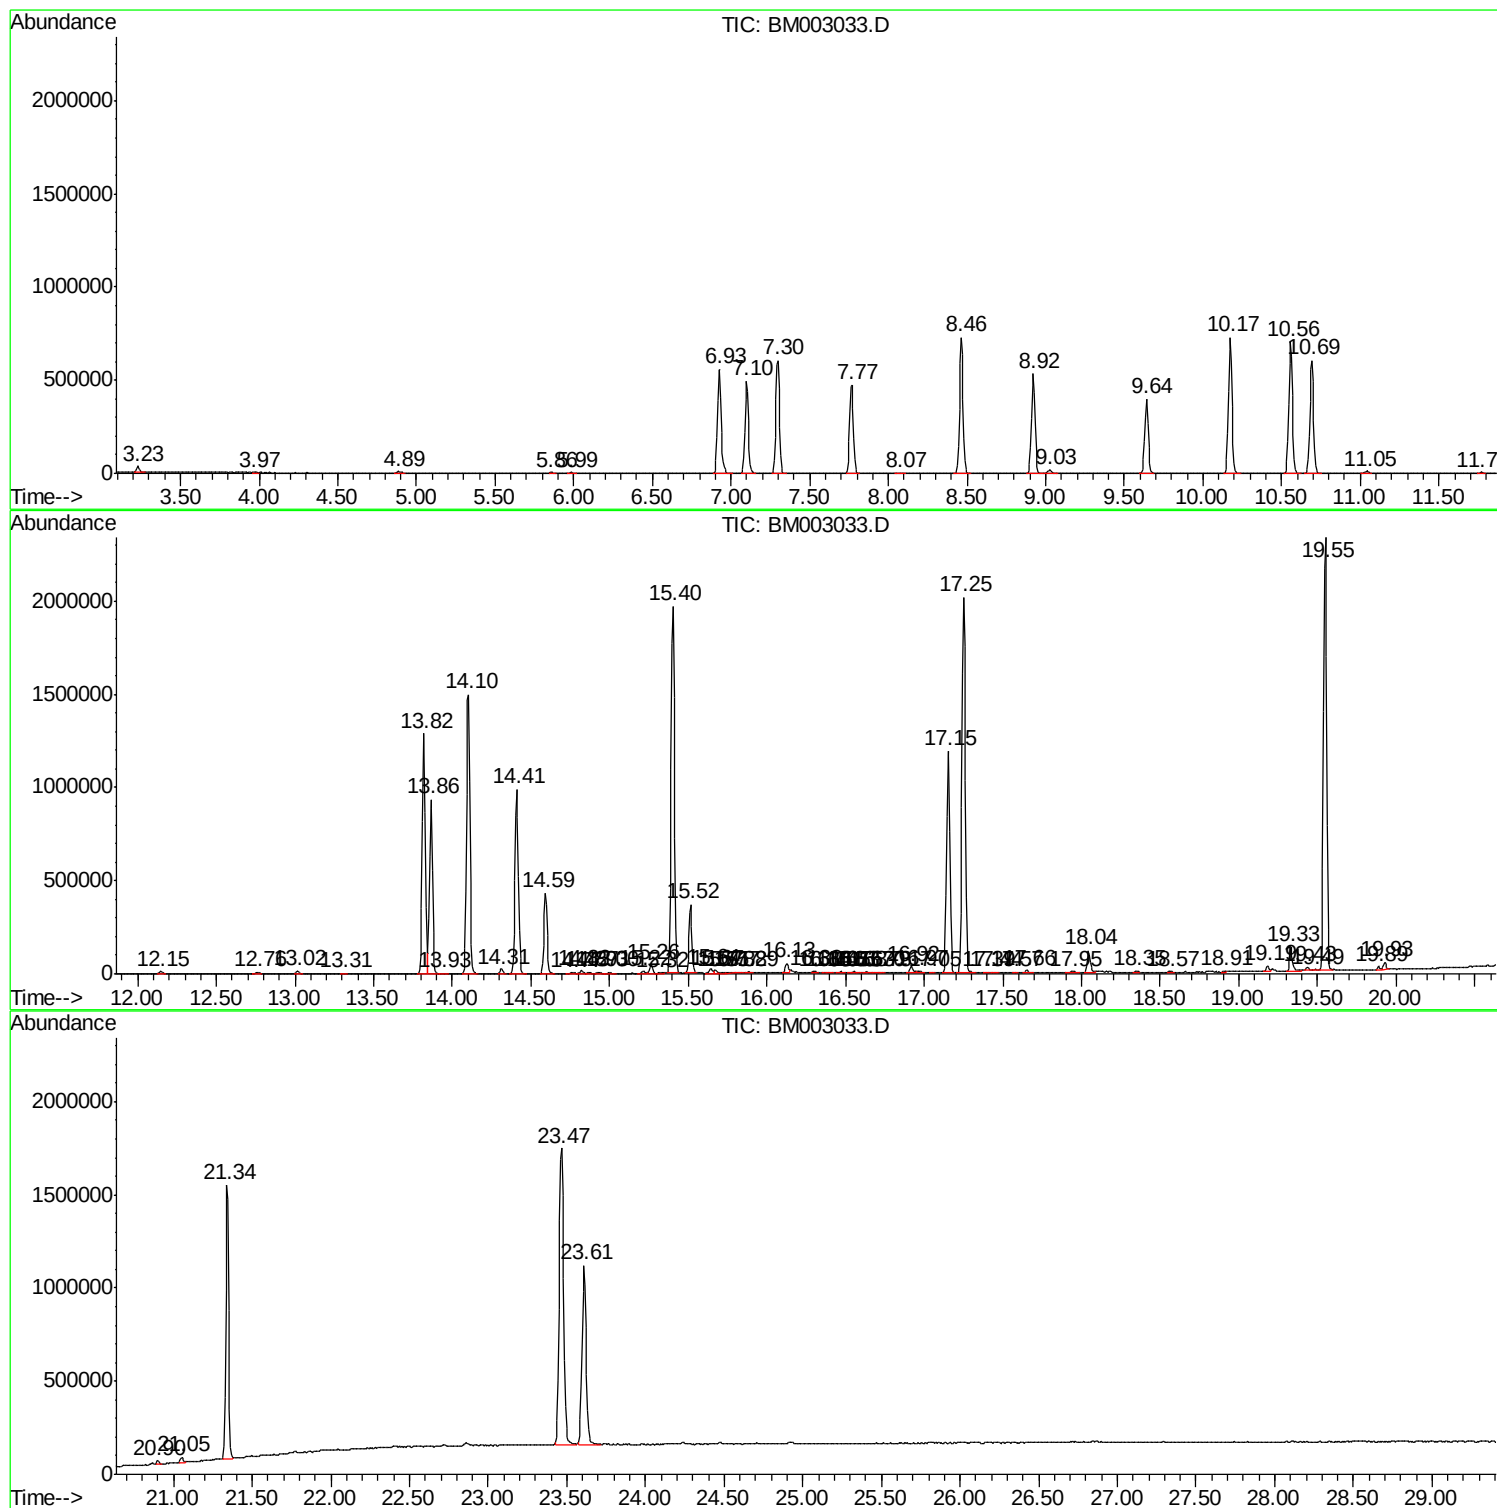

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003033.D
Acq On : 01 Nov 2015 17:49
Operator : UM/IZ
Sample : G4210-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7D8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110115\
Data File : BM003033.D
Acq On : 01 Nov 2015 17:49
Operator : UM/IZ
Sample : G4210-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7D8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc