

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110117\
 Data File : BM012660.D
 Acq On : 02 Nov 2017 05:08
 Operator : SJ/JU
 Sample : I5919-08RE
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST02081

Quant Time: Nov 02 07:13:35 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 02 04:04:31 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	478960	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	1837232	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	879119	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	2087804	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	2095896	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	2263812	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	44925	4.79	ng/uL	0.00
5) Phenol-d5	7.01	99	987841	24.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	575127	24.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	777069	25.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	540849	15.82	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	380922	33.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	419879	35.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.26	165	778406	24.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	636637	19.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	1843672	24.01	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	2365842	26.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.68	143	283826	24.86	ng/ul	0.00
57) Fluorene-d10	15.47	176	1651626	25.41	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	193736	19.17	ng/ul	0.00
70) Anthracene-d10	17.32	188	2640835	26.54	ng/ul	0.00
76) Pyrene-d10	19.61	212	2936525	30.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.54	264	2779842	25.85	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.93	163	76639	1.01 ng/ul#	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110117\
Data File : BM012660.D
Acq On : 02 Nov 2017 05:08
Operator : SJ/JU
Sample : I5919-08RE
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SSTD02081

Quant Time: Nov 02 07:13:35 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 02 04:04:31 2017
Response via : Initial Calibration

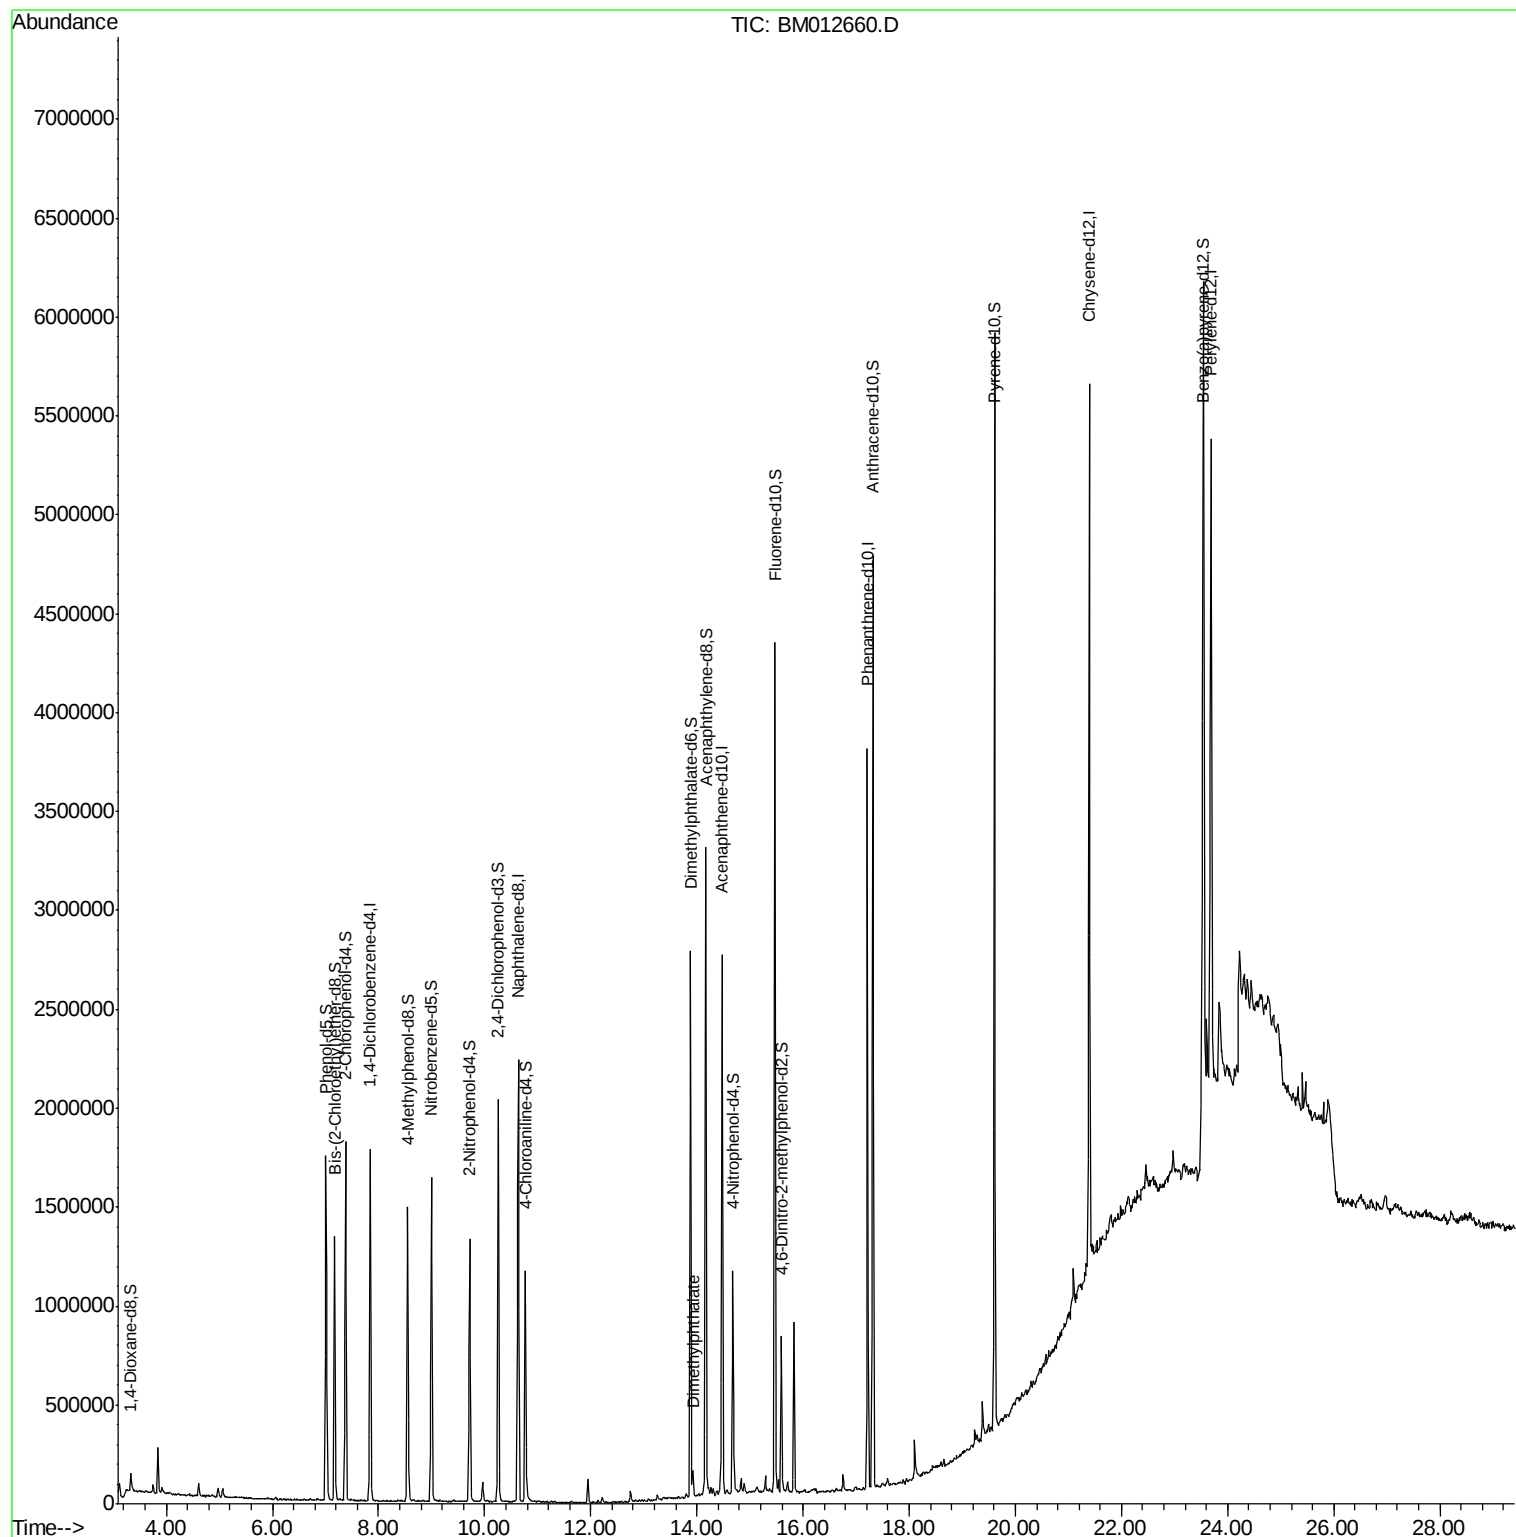

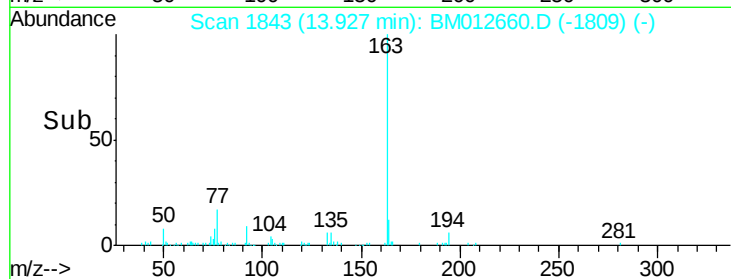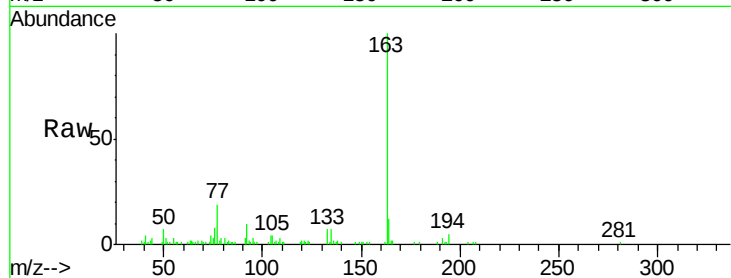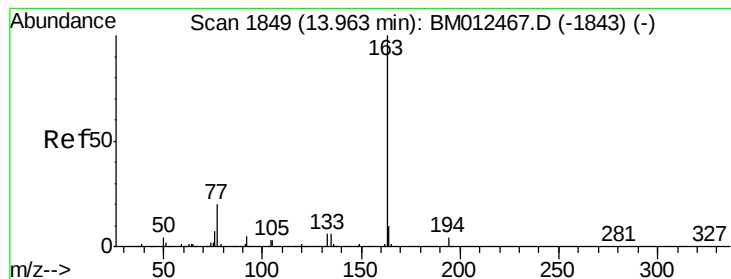

#44

Dimethylphthalate

Concen: 1.01 ng/ul

RT: 13.93 min Scan# 1843

Delta R.T. -0.00 min

Lab File: BM012660.D

Acq: 02 Nov 2017 05:08

Instrument :

BNA_M

ClientSampleId :

SSTD02081

Tot Ion:163 Resp: 76639

Ion Ratio Lower Upper

163 100

194 5.5 3.5 5.3#

164 12.0 8.2 12.4

