

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
 Data File : BM032841.D
 Acq On : 01 Nov 2021 20:15
 Operator : CG/JU
 Sample : PB140379BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB140379BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.084	377	382	396	rBV	2401270	3380173	43.68%	9.422%
2	6.701	650	657	673	rBV	2534029	3897428	50.37%	10.864%
3	7.495	786	792	804	rBV	429810	683890	8.84%	1.906%
4	8.648	981	988	1008	rBV	1600203	2527065	32.66%	7.044%
5	10.277	1258	1265	1282	rBV	608359	1010956	13.06%	2.818%
6	12.766	1681	1688	1705	rBV	3777282	5726486	74.00%	15.962%
7	14.154	1918	1924	1937	rBV	1015836	1432384	18.51%	3.993%
8	15.648	2172	2178	2194	rBV	3037534	4251352	54.94%	11.850%
9	16.889	2383	2389	2403	rBV	1235654	1714003	22.15%	4.778%
10	19.524	2831	2837	2846	rBV	6196679	7738227	100.00%	21.570%
11	21.071	3095	3100	3110	rBV	1417862	1837680	23.75%	5.122%
12	23.188	3455	3460	3471	rVB2	1016248	1675753	21.66%	4.671%




Sum of corrected areas: 35875397

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
Data File : BM032841.D
Acq On : 01 Nov 2021 20:15
Operator : CG/JU
Sample : PB140379BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140379BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

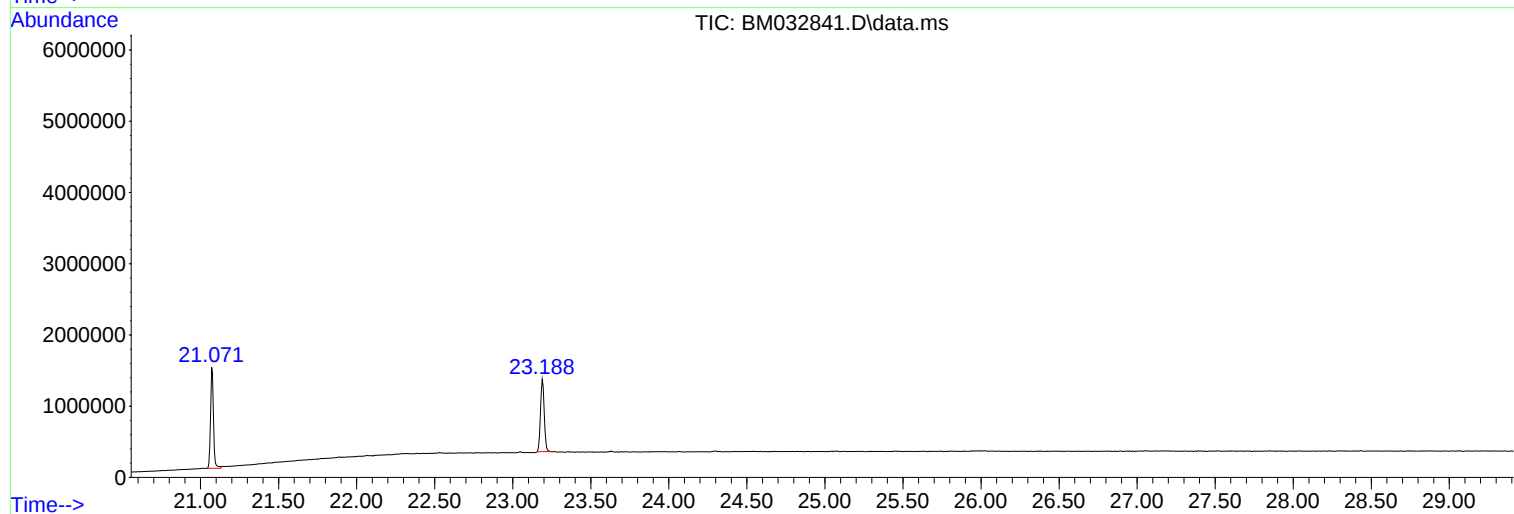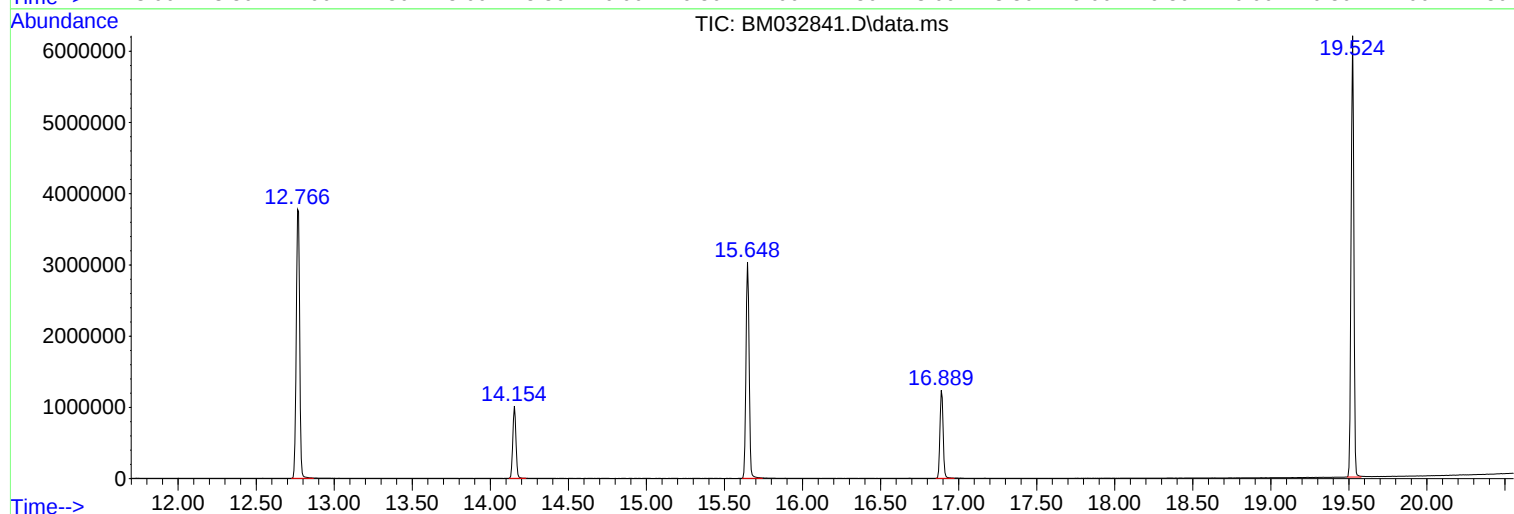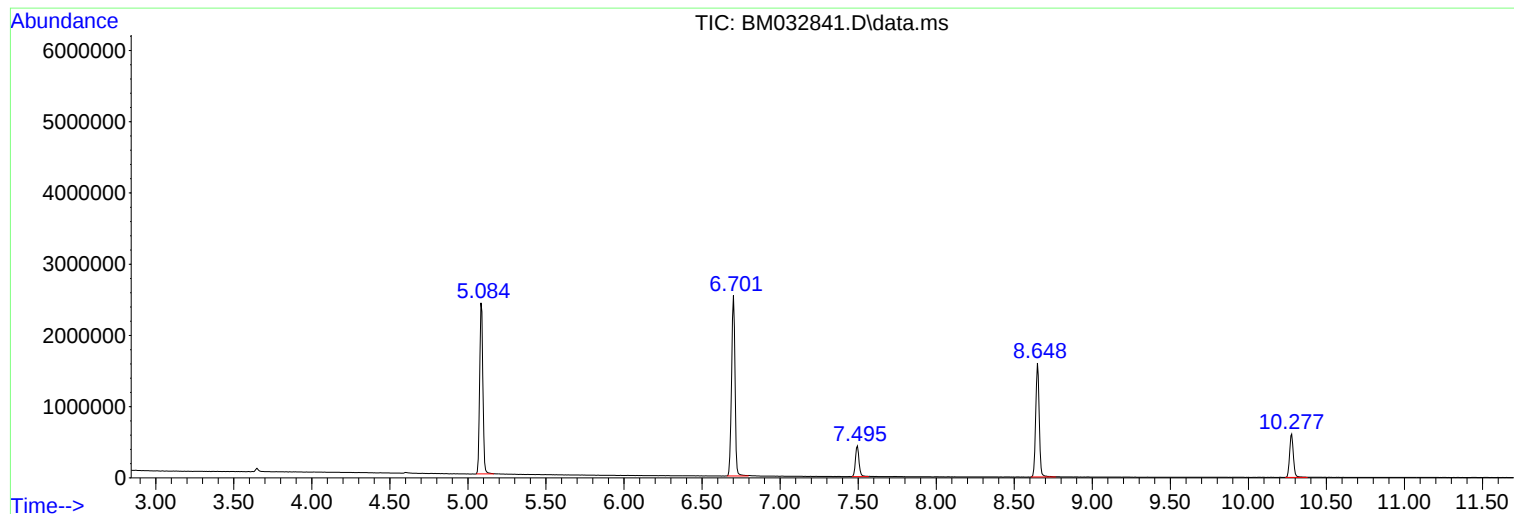

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
Data File : BM032841.D
Acq On : 01 Nov 2021 20:15
Operator : CG/JU
Sample : PB140379BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140379BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
Data File : BM032841.D
Acq On : 01 Nov 2021 20:15
Operator : CG/JU
Sample : PB140379BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140379BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------