
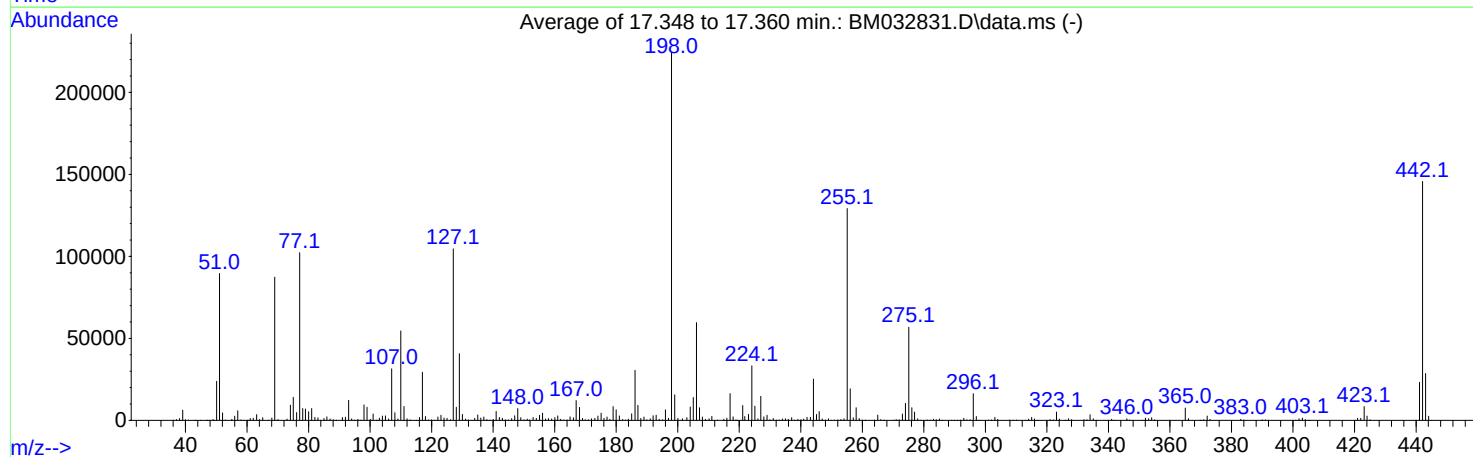


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
 Data File : BM032831.D
 Acq On : 01 Nov 2021 12:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 01 18:47:37 2021

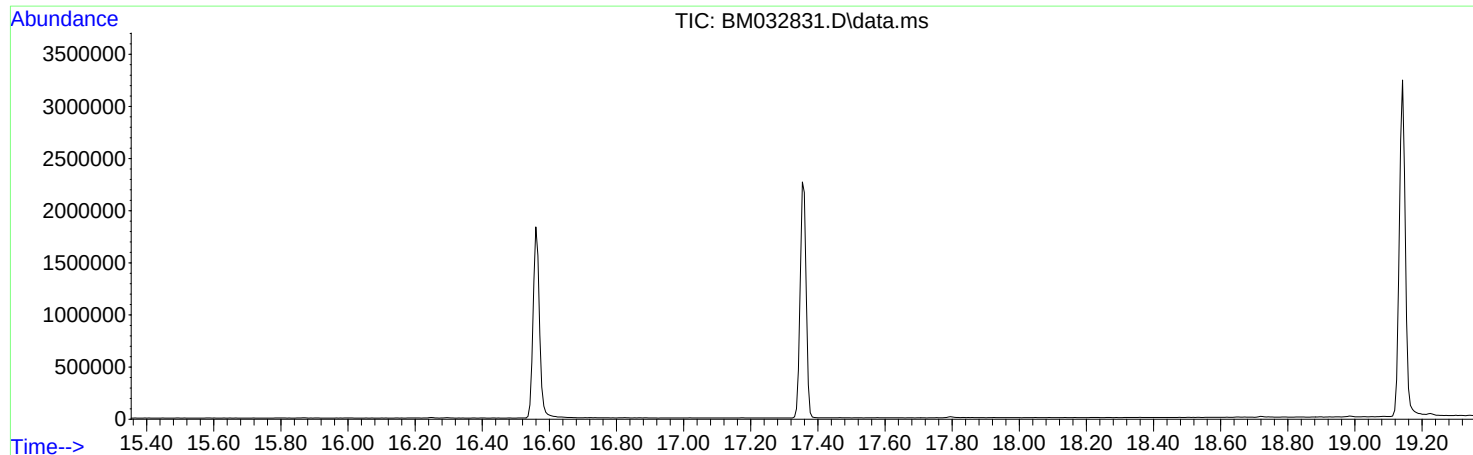




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	89585	PASS
68	69	0.00	2	1.7	1498	PASS
69	198	0.00	100	38.9	87304	PASS
70	69	0.00	2	0.5	470	PASS
127	198	10	80	46.6	104587	PASS
197	198	0.00	2	0.6	1295	PASS
198	198	100	100	100.0	224320	PASS
199	198	5	9	7.0	15611	PASS
275	198	10	60	25.3	56837	PASS
365	198	1	100	3.4	7540	PASS
441	198	0.01	100	10.3	23197	PASS
442	442	50	100	100.0	145672	PASS
443	442	15	24	19.7	28632	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
Data File : BM032831.D
Acq On : 01 Nov 2021 12:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 01 19:22:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 18:47:37 2021
Response via : Initial Calibration

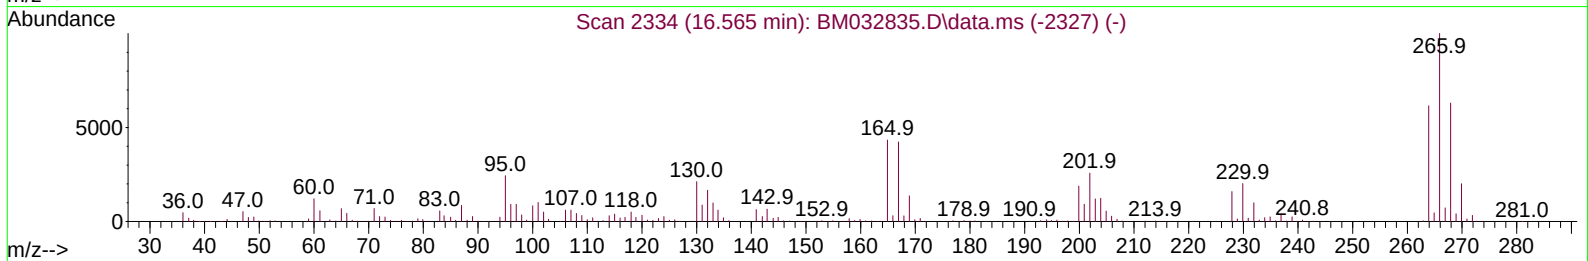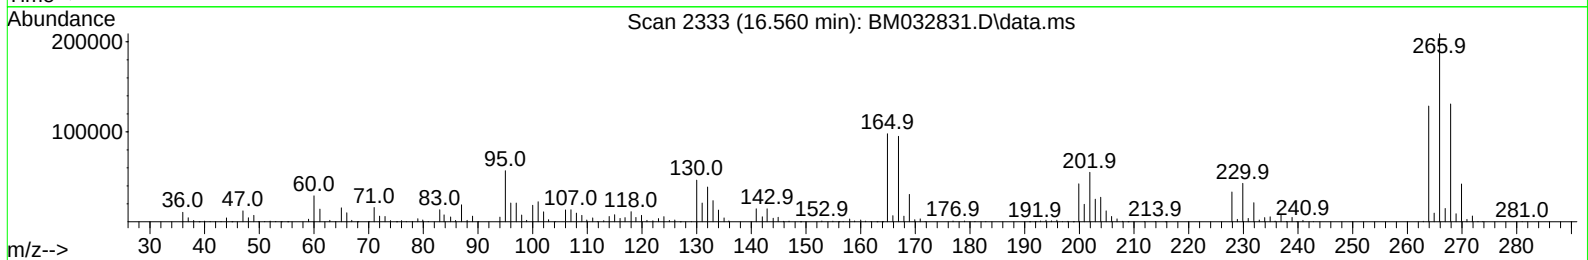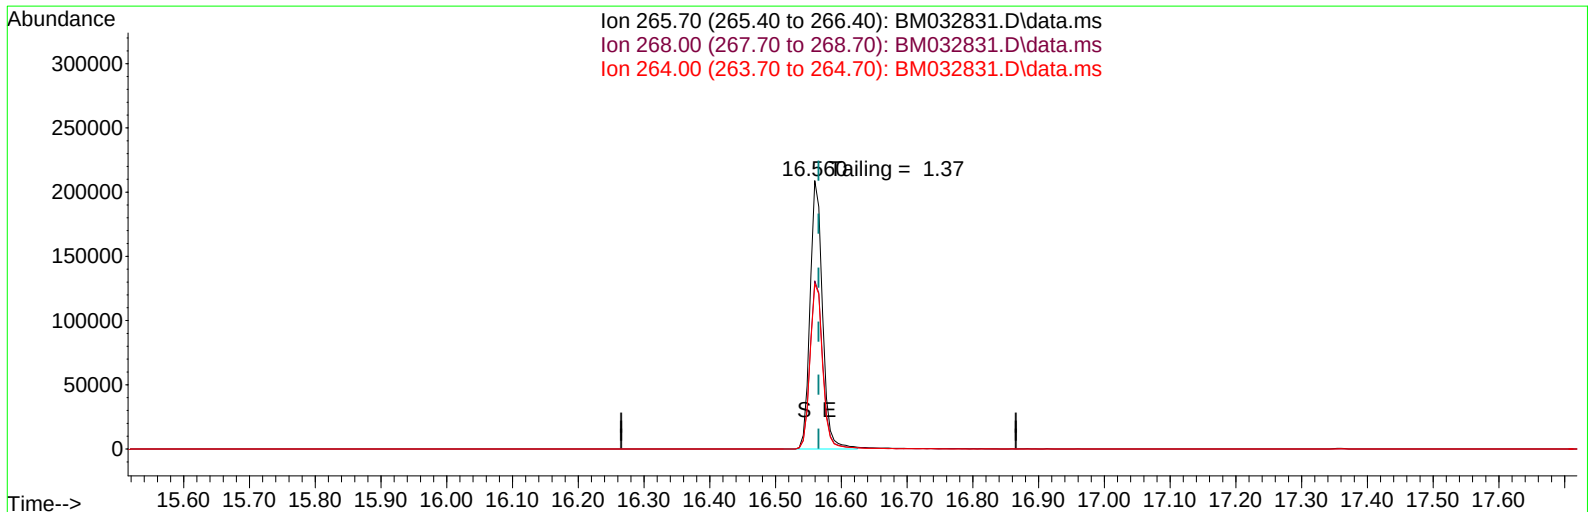

TIC: BM032831.D\data.ms

(70) Pentachlorophenol (C)

16.560min (-0.006) 0.00 ng




response 277787

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.68
264.00	65.10	61.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
 Data File : BM032831.D
 Acq On : 01 Nov 2021 12:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Nov 01 19:22:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 01 18:47:37 2021
 Response via : Initial Calibration

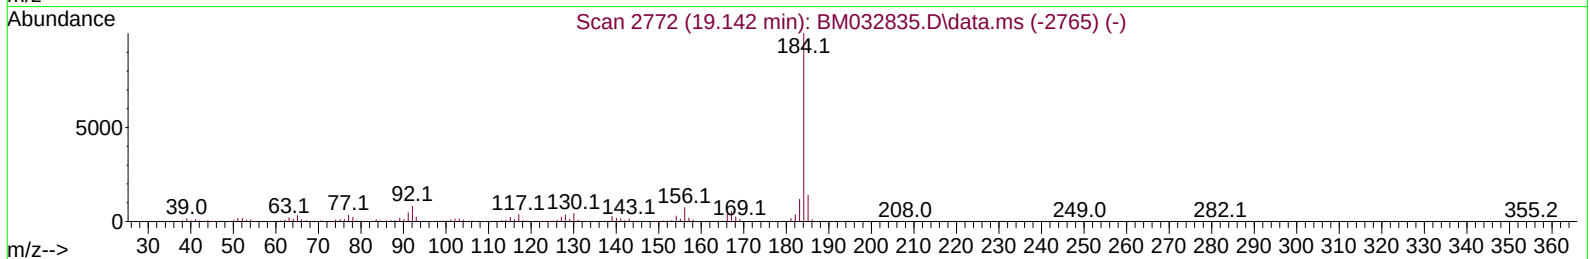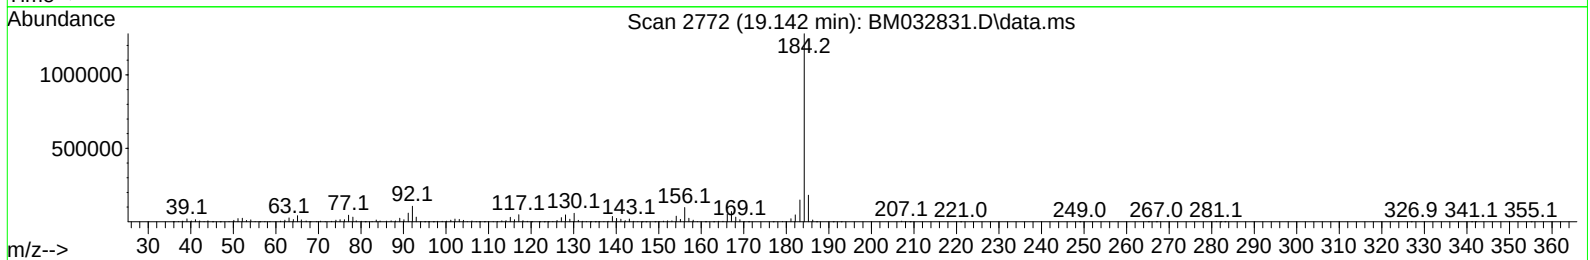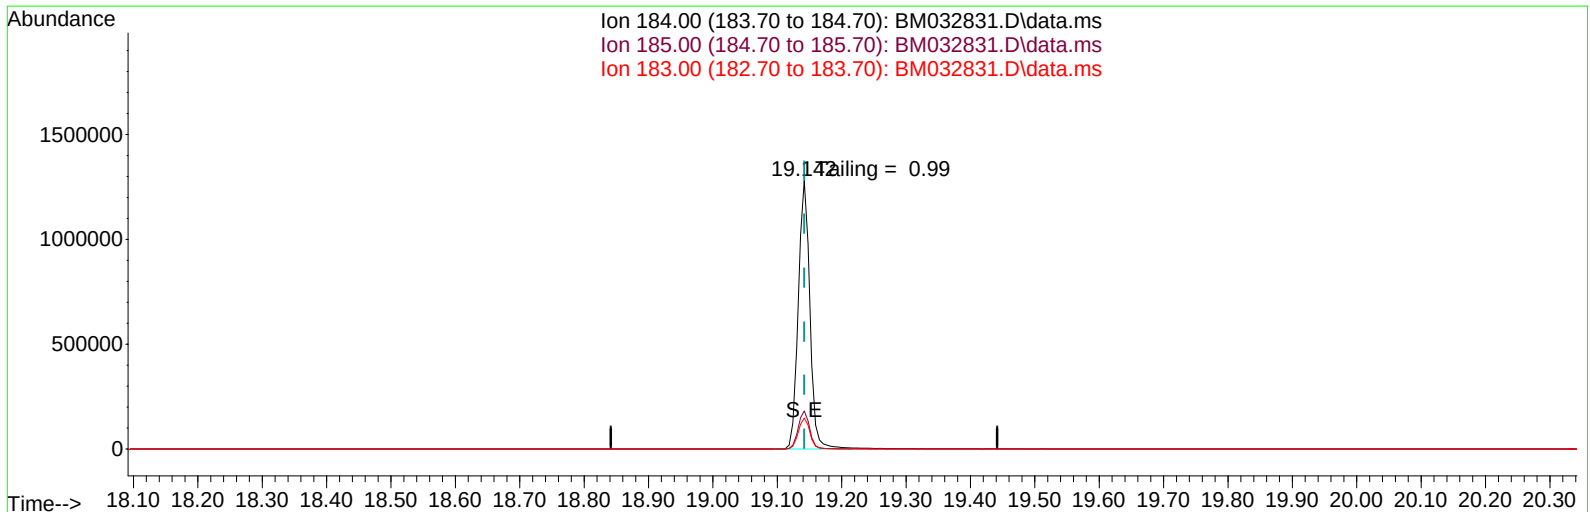

TIC: BM032831.D\data.ms

(77) Benzidine

19.142min (+ 0.000) 0.00 ng

response 1627768

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.18
183.00	11.20	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2021	BNA_M	<u>BM032831.D</u>
Compound Name	Response	Retention Time
DDT	764018	20.38
DDD	1076	19.94
DDE	1245	19.26
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2321	766339	0.30

Instrument :
BNA_M
ClientSampleId :
DFTPP