

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110217\
 Data File : BM012667.D
 Acq On : 02 Nov 2017 17:28
 Operator : SJ/JU
 Sample : PB103710BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK10

Quant Time: Nov 03 01:40:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 03 01:40:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	164415	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	1297979	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	740549	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	1651598	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1193326	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	1297292	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	34914	10.85	ng/uL	0.00
5) Phenol-d5	7.00	99	373794	27.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	210614	25.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	316194	30.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	561657	47.85	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	312708	38.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	359553	42.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	622805	28.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	891147	38.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	2179932	33.70	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	2496178	32.62	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	358639	37.29	ng/ul	0.00
57) Fluorene-d10	15.46	176	1732361	31.64	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	280750	35.12	ng/ul	0.00
70) Anthracene-d10	17.30	188	2798287	35.55	ng/ul	0.00
76) Pyrene-d10	19.60	212	1926384	35.19	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	2271461	36.86	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.53	70	15339	1.52	ng/ul#	1
45) 2,6-Dinitrotoluene	13.87	165	16707	1.64	ng/ul#	28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110217\
Data File : BM012667.D
Acq On : 02 Nov 2017 17:28
Operator : SJ/JU
Sample : PB103710BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK10

Quant Time: Nov 03 01:40:52 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 03 01:40:21 2017
Response via : Initial Calibration




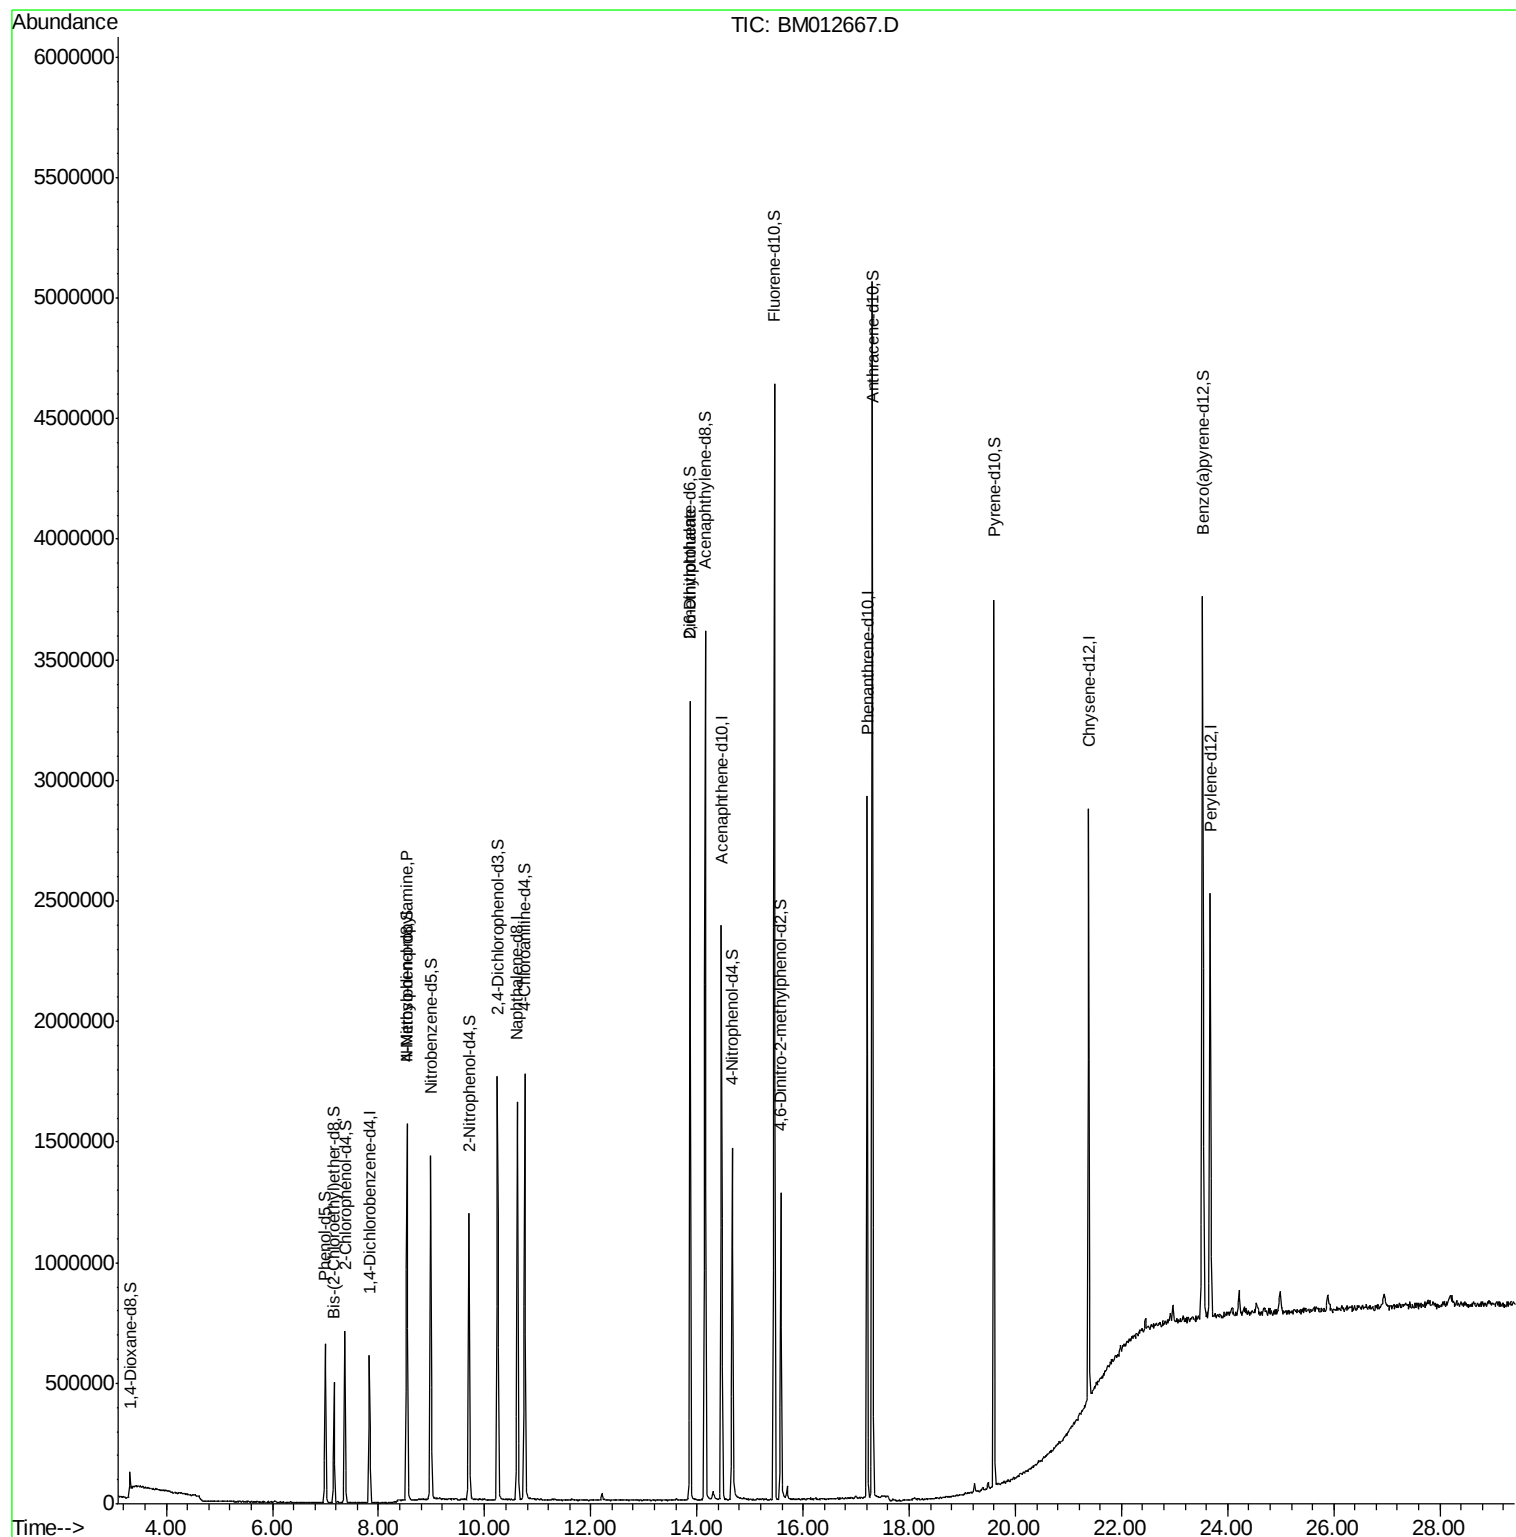


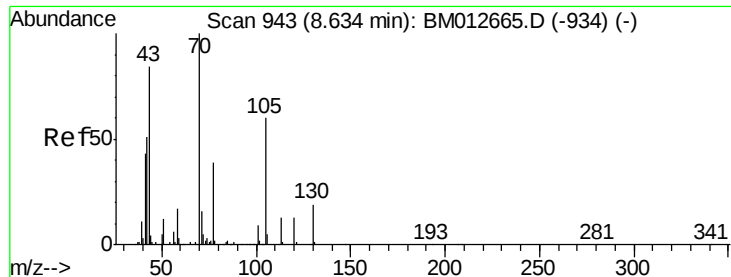

#15
N-Nitroso-di-n-propylamine
Concen: 1.52 ng/ul
RT: 8.53 min Scan# 926
Delta R.T. -0.10 min
Lab File: BM012667.D
Acq: 02 Nov 2017 17:28

Instrument :
BNA_M
ClientSampled :
SBLK10

Tot Ion	Ratio	Lower	Upper
70	100		
42	383.6	76.0	114.0#
101	0.0	6.7	10.1#
130	0.0	14.6	22.0#

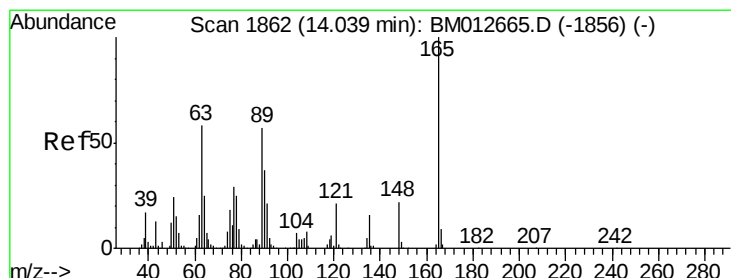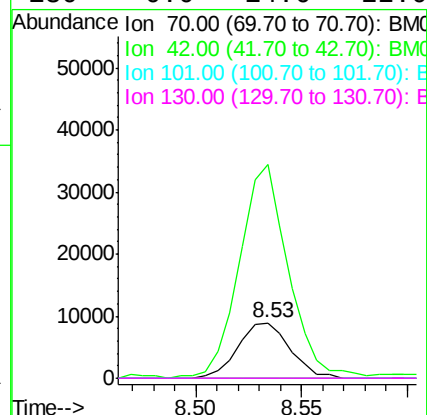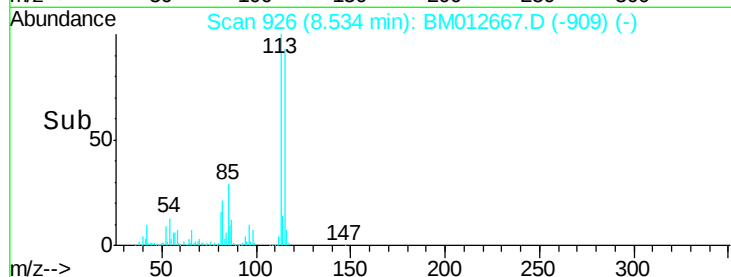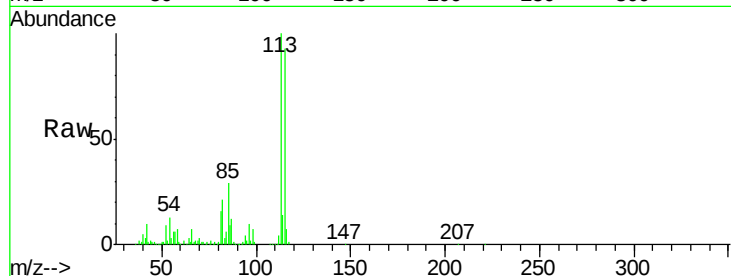

#45
2,6-Dinitrotoluene
Concen: 1.64 ng/ul
RT: 13.87 min Scan# 1834
Delta R.T. -0.16 min
Lab File: BM012667.D
Acq: 02 Nov 2017 17:28

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	52.6	79.0#
121	32.7	14.6	22.0#

