

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM110217\
 Data File : BM012684.D
 Acq On : 03 Nov 2017 03:39
 Operator : SJ/JU
 Sample : I6045-18
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0E65

Manual Integrations
 APPROVED

Sohil
 11/3/2017 1:31:13 PM

Quant Time: Nov 03 05:19:50 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 03 03:08:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	154887	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	625297	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	393047	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	992270	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1286682	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	1407955	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	2200	0.73	ng/uL	0.00
5) Phenol-d5	7.00	99	36867	2.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	21857	2.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	31655	3.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	31275	2.83	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	15869	4.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	17342	4.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	32081	3.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	40939	3.63	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	115711	3.37	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	130389	3.21	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	14525	2.85	ng/ul	0.00
57) Fluorene-d10	15.45	176	100945	3.47	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	9870m	2.06	ng/ul	0.00
70) Anthracene-d10	17.30	188	166296	3.52	ng/ul	0.00
76) Pyrene-d10	19.59	212	197728	3.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	234348	3.50	ng/ul	0.00

Target Compounds				Ovalue	
44) Dimethylphthalate	13.92	163	54386	1.601	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM110217\
Data File : BM012684.D
Acq On : 03 Nov 2017 03:39
Operator : SJ/JU
Sample : I6045-18
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
B0E65

Manual Integrations
APPROVED

Sohil
11/3/2017 1:31:13 PM

Quant Time: Nov 03 05:19:50 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 03 03:08:54 2017
Response via : Initial Calibration

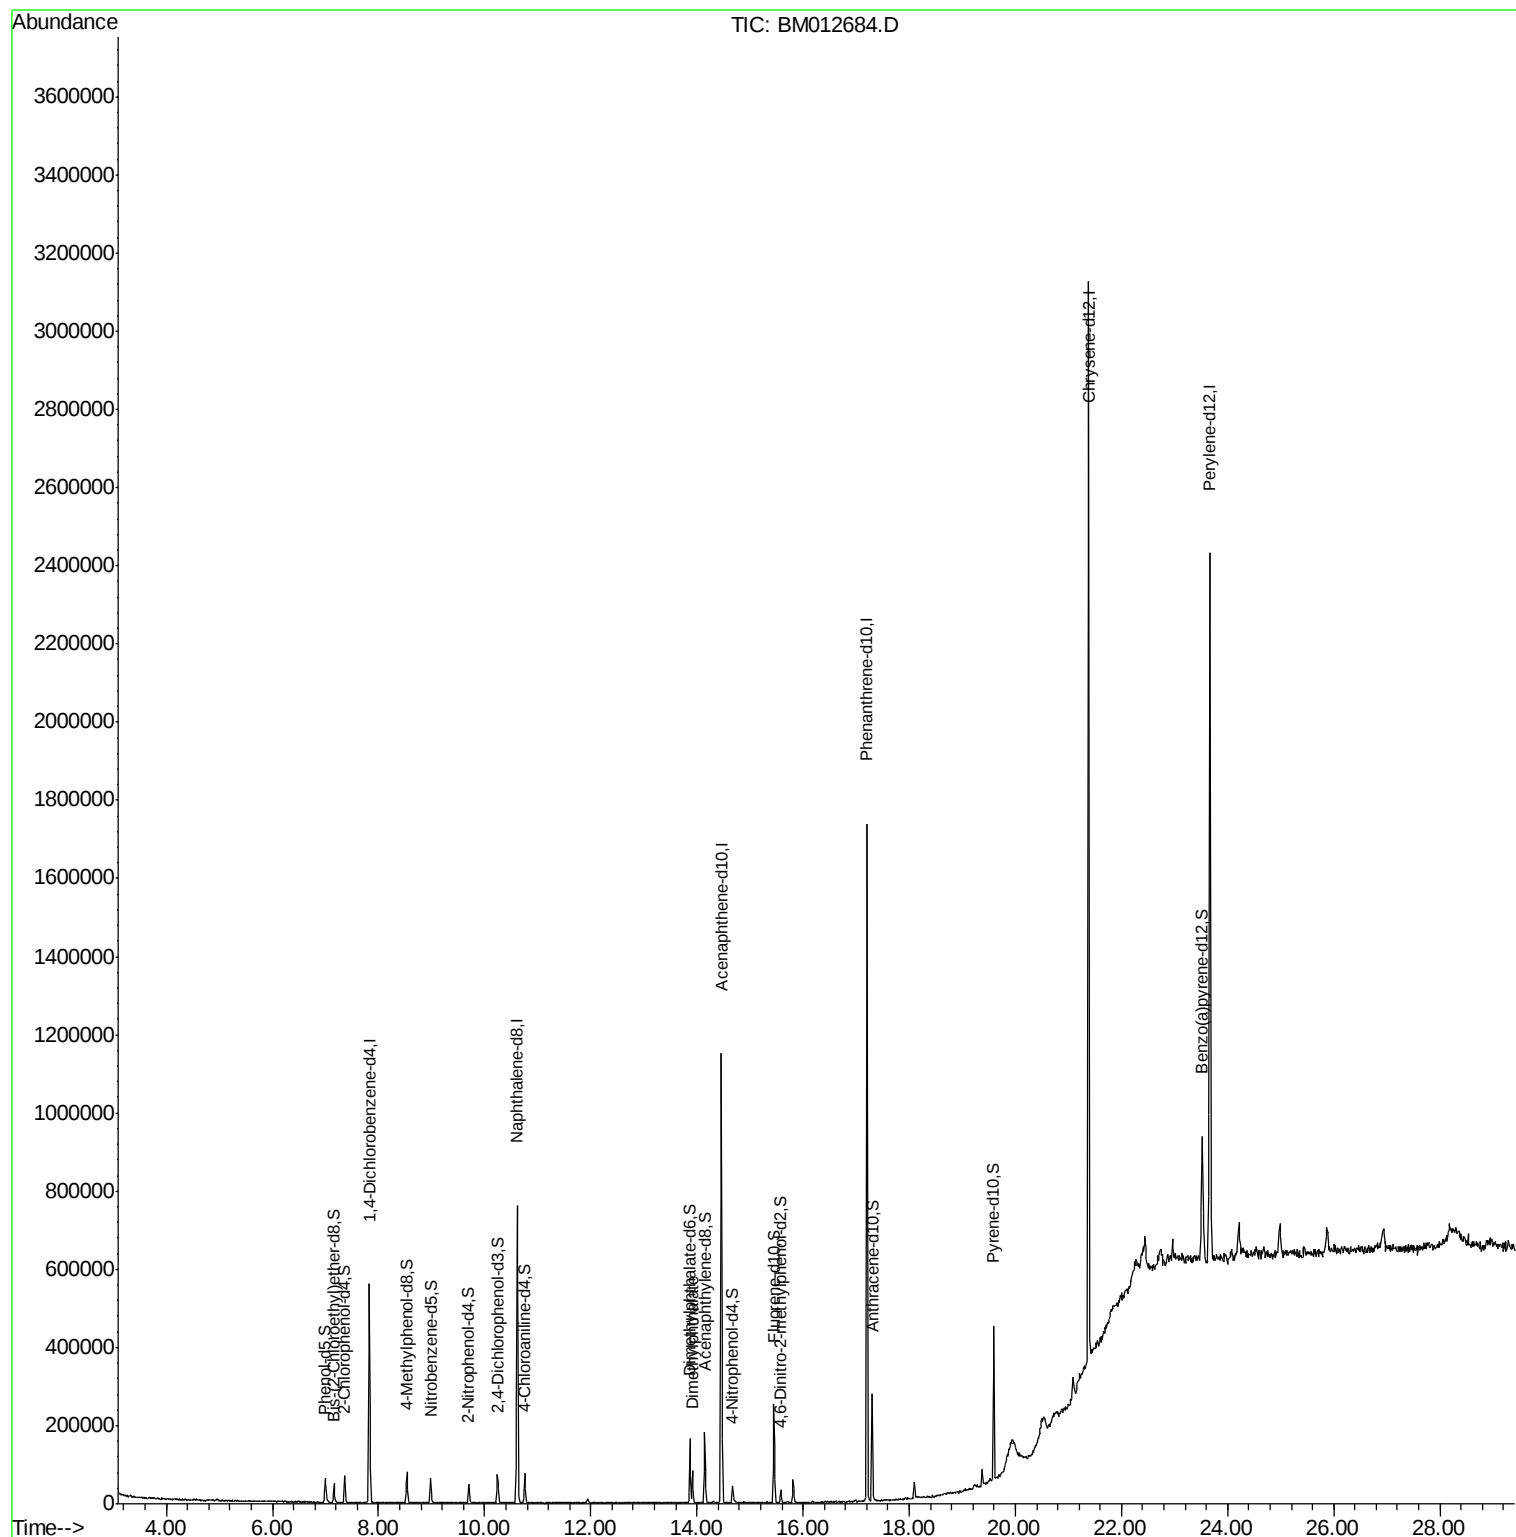

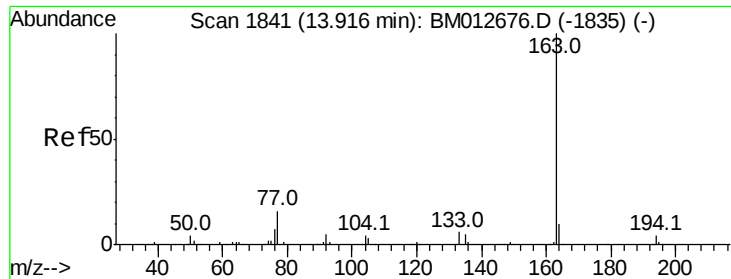

#44
 Dimethylphthalate
 Concen: 1.601 ng/ul
 RT: 13.92 min Scan# 1841
 Delta R.T. -0.00 min
 Lab File: BM012684.D
 Acq: 03 Nov 2017 03:39

Instrument :
 BNA_M
 ClientSampleId :
 B0E65

Tot Ion	Ratio	Resp	Lower	Upper
163	100	54386		
194	4.1		3.5	5.3
164	9.8		8.2	12.4

Manual Integrations
 APPROVED

Sohil
 11/3/2017 1:31:13 PM

