

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM110217\
 Data File : BM012692.D
 Acq On : 03 Nov 2017 08:26
 Operator : SJ/JU
 Sample : I6045-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0E65

Quant Time: Nov 03 08:59:54 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 03 05:31:33 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	164076	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	647046	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	397258	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	952454	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1174717	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	1262303	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	2248	0.70	ng/uL	0.00
5) Phenol-d5	6.99	99	212160	15.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	116398	14.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	180673	17.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	183669	15.68	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	88444	21.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	104053	24.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	193128	17.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	245239	21.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	605675	17.45	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	750103	18.27	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	88629	17.18	ng/ul	0.00
57) Fluorene-d10	15.45	176	530808	18.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	71378	15.49	ng/ul	0.00
70) Anthracene-d10	17.30	188	852156	18.77	ng/ul	0.00
76) Pyrene-d10	19.59	212	967548	17.95	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	1104272	18.41	ng/ul	0.00


Target Compounds				Ovalue
44) Dimethylphthalate	13.92	163	57031	1.661 ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM110217\
Data File : BM012692.D
Acq On : 03 Nov 2017 08:26
Operator : SJ/JU
Sample : I6045-18
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0E65

Quant Time: Nov 03 08:59:54 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 03 05:31:33 2017
Response via : Initial Calibration

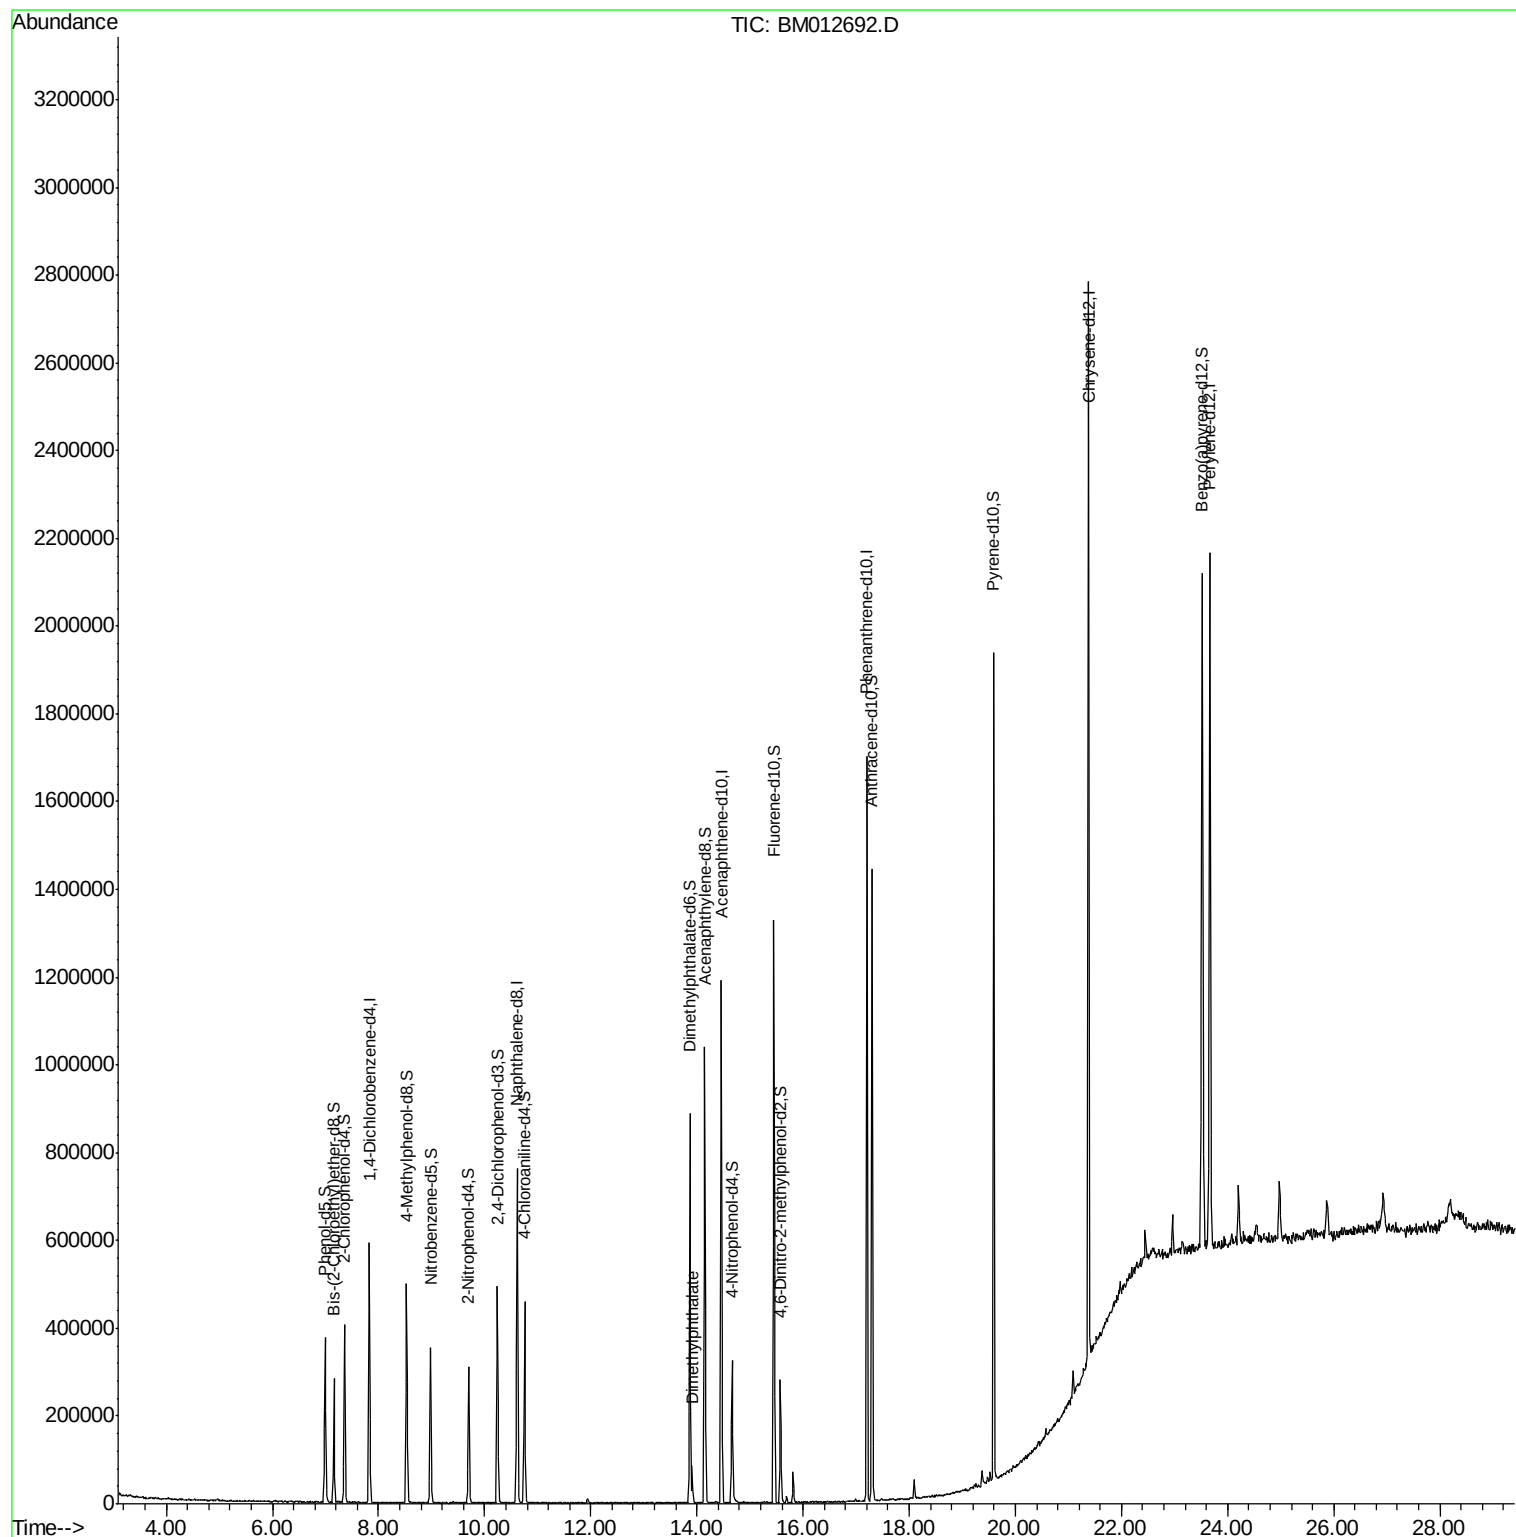

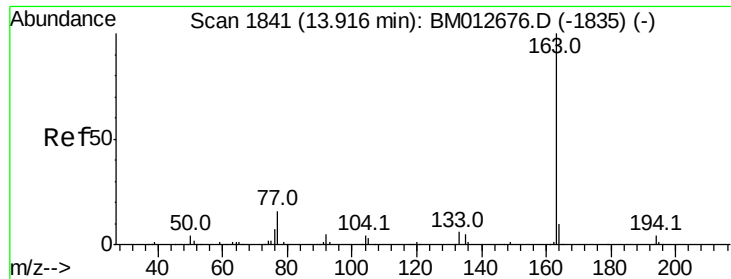

#44

Dimethylphthalate

Concen: 1.661 ng/ul

RT: 13.92 min Scan# 1841

Delta R.T. -0.00 min

Lab File: BM012692.D

Acq: 03 Nov 2017 08:26

Instrument :

BNA_M

ClientSampleId :

B0E65


Tot Ion:163 Resp: 57031

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 9.8 8.2 12.4

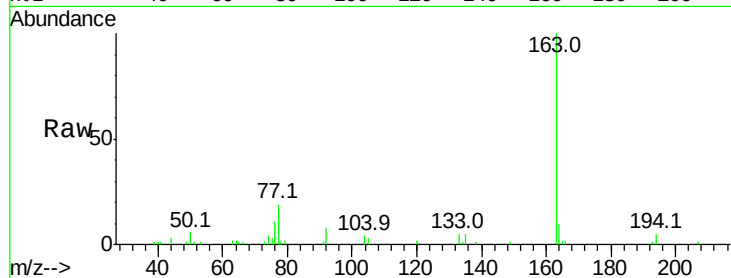

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

