
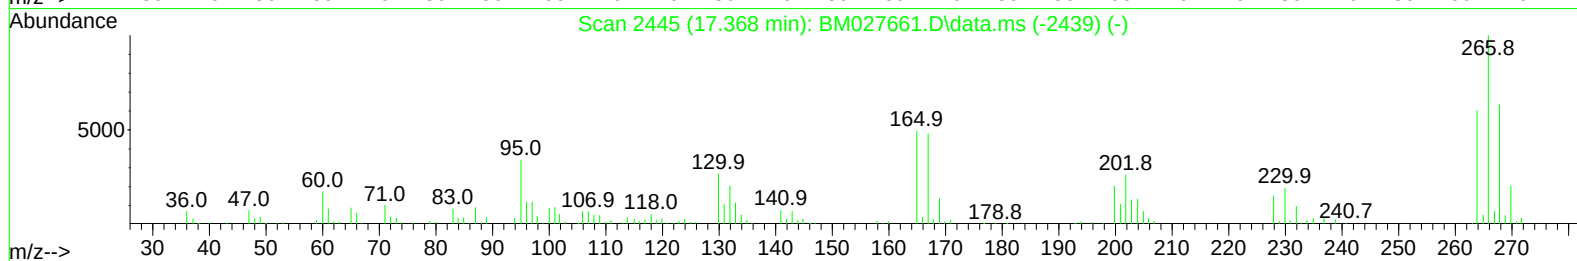
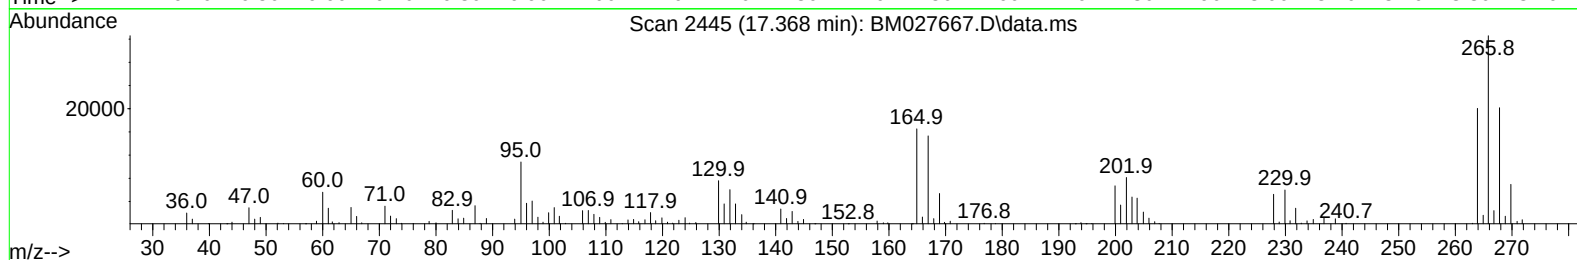


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
Data File : BM027667.D
Acq On : 02 Nov 2020 08:43
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 01:14:34 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 17:56:42 2020
Response via : Initial Calibration

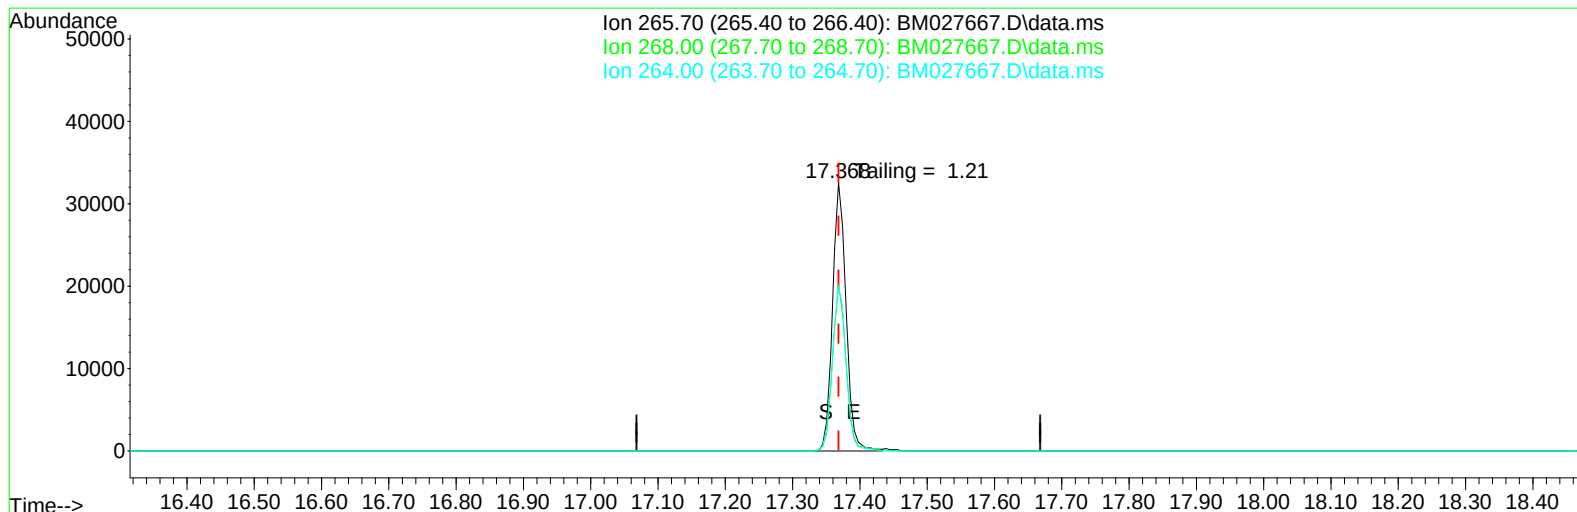

TIC: BM027667.D\data.ms

(70) Pentachlorophenol (C)




17.368min (+ 0.000) 0.00 ng

response 45712

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	61.86
264.00	63.30	61.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
Data File : BM027667.D
Acq On : 02 Nov 2020 08:43
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 01:14:34 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 17:56:42 2020
Response via : Initial Calibration

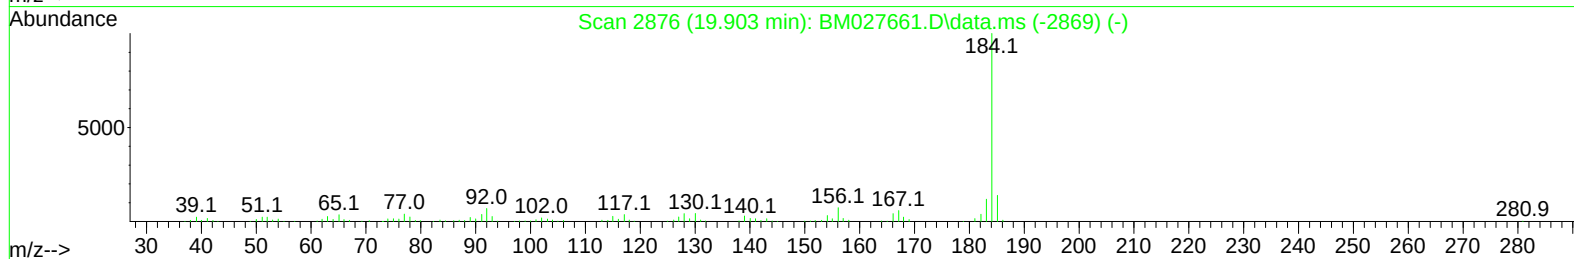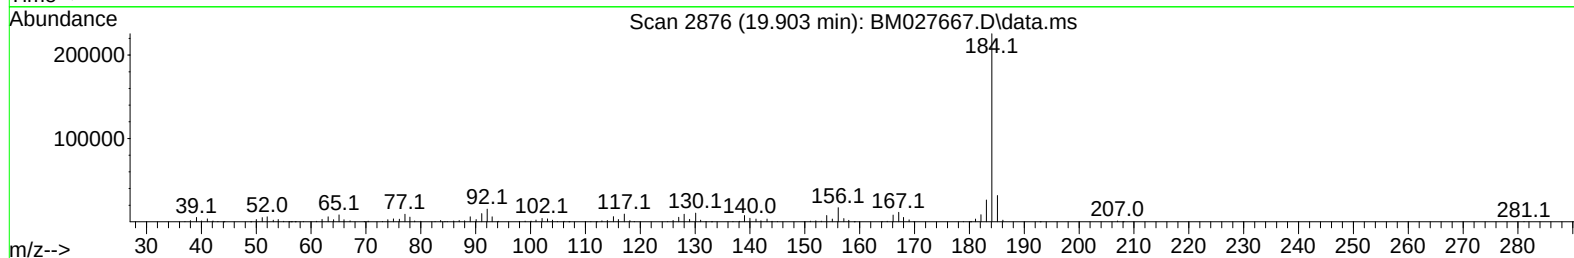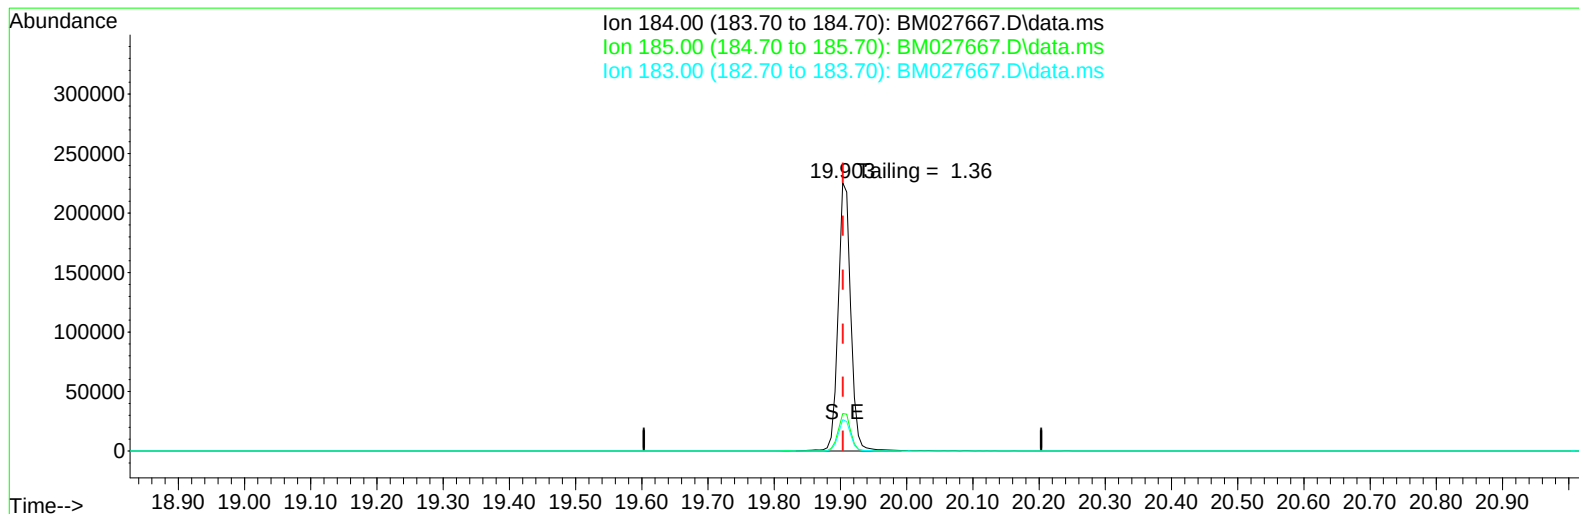

TIC: BM027667.D\data.ms

(77) Benzidine**19.903min (+ 0.000) 14571.96 ng****response 298596**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.98
183.00	12.10	11.67
0.00	0.00	0.00