

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
 Data File : BM027669.D
 Acq On : 02 Nov 2020 09:56
 Operator : JU/CG
 Sample : PB132380BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB132380BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM027669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.869	484	490	501	rBV	777165	1177357	63.41%	12.548%
2	7.522	762	771	778	rBV	767124	1221931	65.81%	13.024%
3	8.404	914	921	927	rVB	140665	227135	12.23%	2.421%
4	9.575	1113	1120	1129	rVB	494859	828213	44.61%	8.827%
5	11.245	1397	1404	1411	rVB	168661	284697	15.33%	3.034%
6	13.651	1806	1813	1819	rBV	1049422	1490829	80.30%	15.889%
7	15.010	2039	2044	2051	rVB	225701	327351	17.63%	3.489%
8	16.474	2287	2293	2305	rBV	674220	926223	49.89%	9.872%
9	17.727	2500	2506	2511	rVB	258740	354180	19.08%	3.775%
10	20.286	2935	2941	2946	rBV	1517618	1856664	100.00%	19.789%
11	21.827	3197	3203	3209	rBV	276642	354593	19.10%	3.779%
12	24.280	3611	3620	3627	rBV	163497	333327	17.95%	3.553%




Sum of corrected areas: 9382500

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
Data File : BM027669.D
Acq On : 02 Nov 2020 09:56
Operator : JU/CG
Sample : PB132380BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132380BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

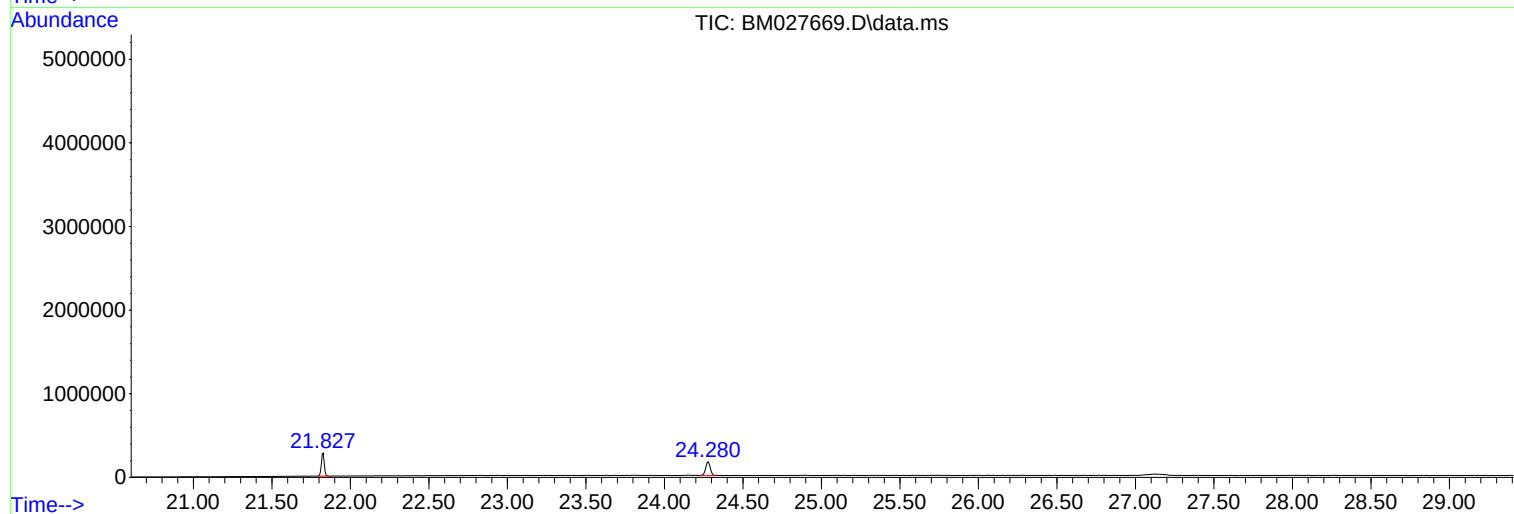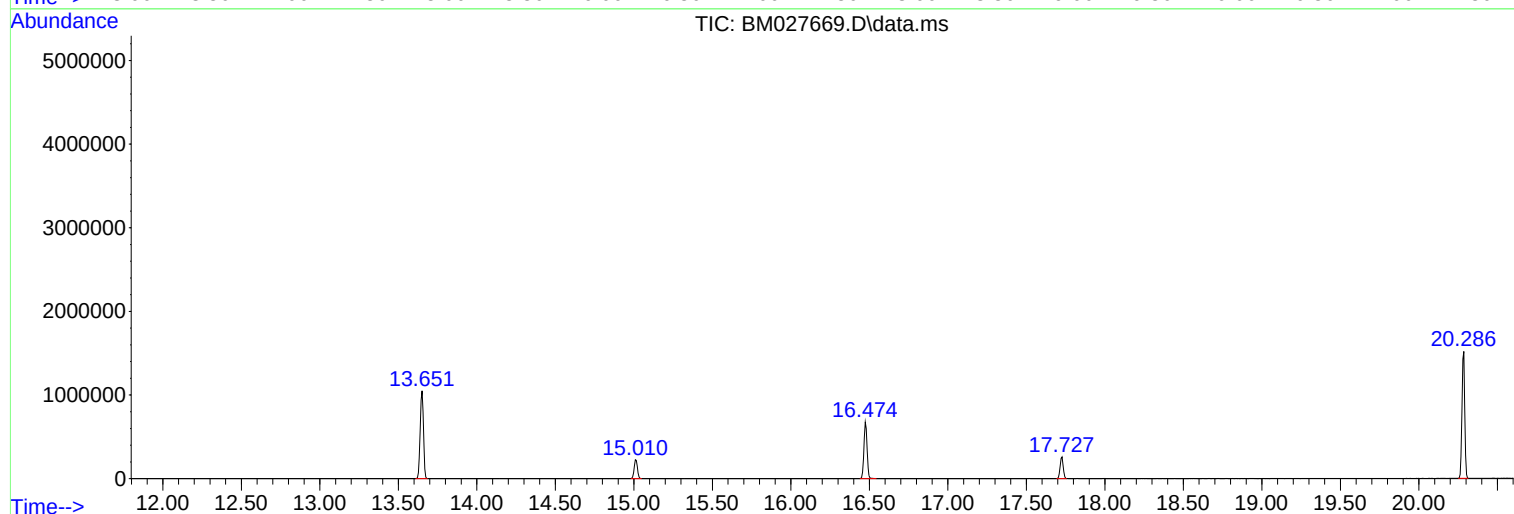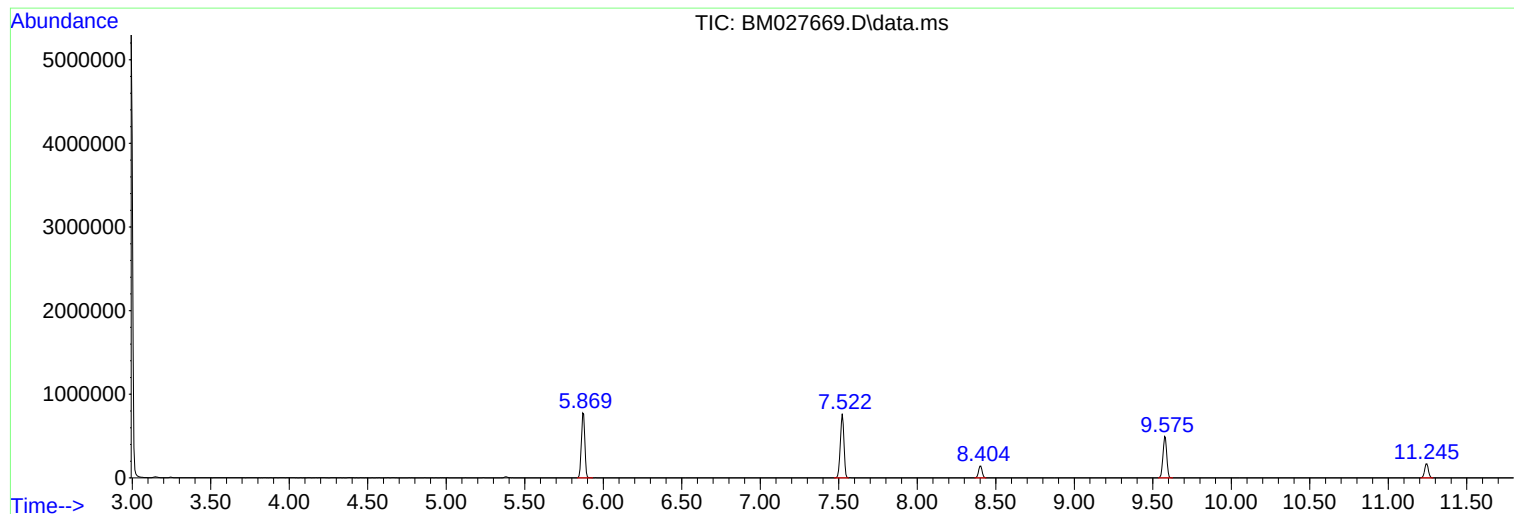

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
Data File : BM027669.D
Acq On : 02 Nov 2020 09:56
Operator : JU/CG
Sample : PB132380BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132380BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
Data File : BM027669.D
Acq On : 02 Nov 2020 09:56
Operator : JU/CG
Sample : PB132380BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132380BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------