

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
 Data File : BM027670.D
 Acq On : 02 Nov 2020 10:32
 Operator : JU/CG
 Sample : PB132384BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB132384BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM027670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.870	484	490	497	rBV	618977	904720	57.81%	12.196%
2	7.522	763	771	778	rBV	606344	951895	60.82%	12.832%
3	8.399	914	920	927	rVB	108035	169515	10.83%	2.285%
4	9.575	1112	1120	1129	rVB	384253	634655	40.55%	8.555%
5	11.246	1397	1404	1410	rVB	122509	210142	13.43%	2.833%
6	13.651	1806	1813	1819	rBV	789270	1138294	72.73%	15.344%
7	15.010	2038	2044	2051	rBV	173183	245533	15.69%	3.310%
8	16.475	2287	2293	2304	rBV	554324	758075	48.44%	10.219%
9	17.728	2499	2506	2511	rBV	199339	280477	17.92%	3.781%
10	20.280	2935	2940	2946	rVB	1260067	1565073	100.00%	21.097%
11	21.822	3197	3202	3211	rBV	232736	291764	18.64%	3.933%
12	24.280	3612	3620	3628	rVB2	134541	268218	17.14%	3.616%




Sum of corrected areas: 7418361

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
Data File : BM027670.D
Acq On : 02 Nov 2020 10:32
Operator : JU/CG
Sample : PB132384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132384BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

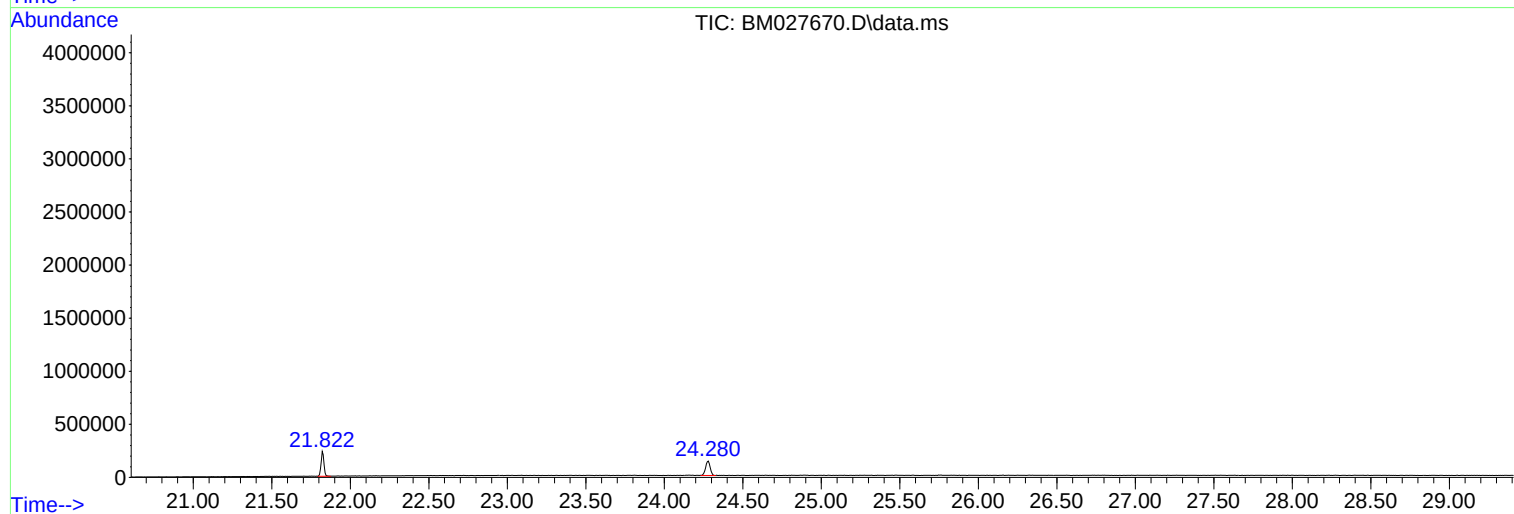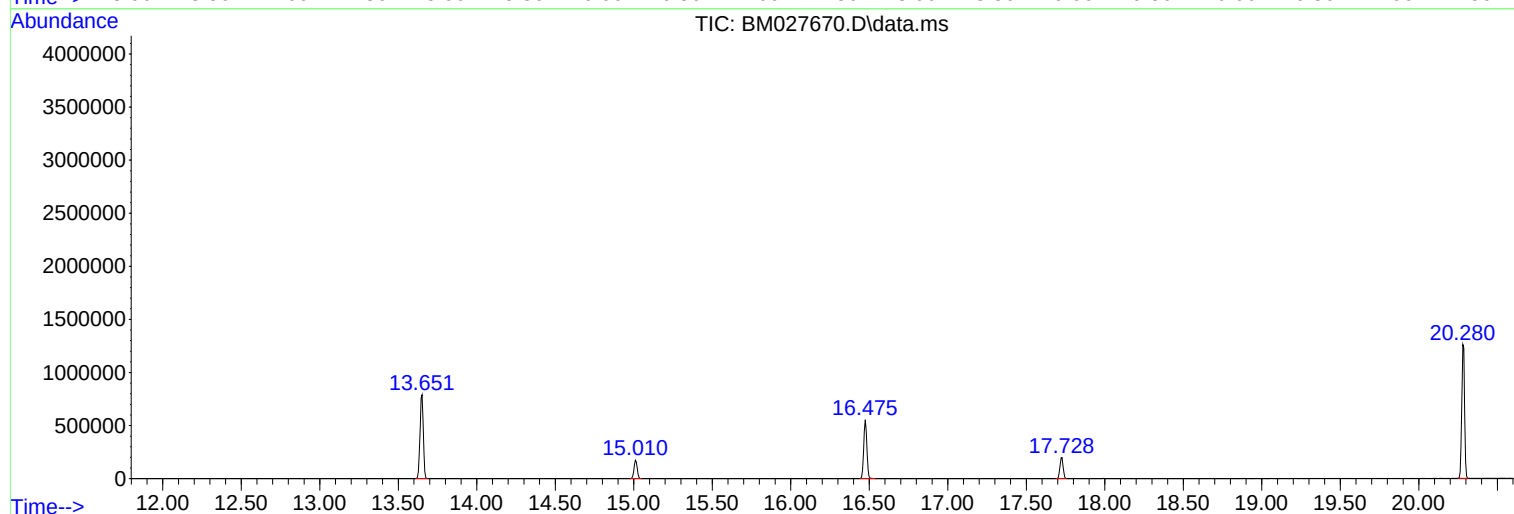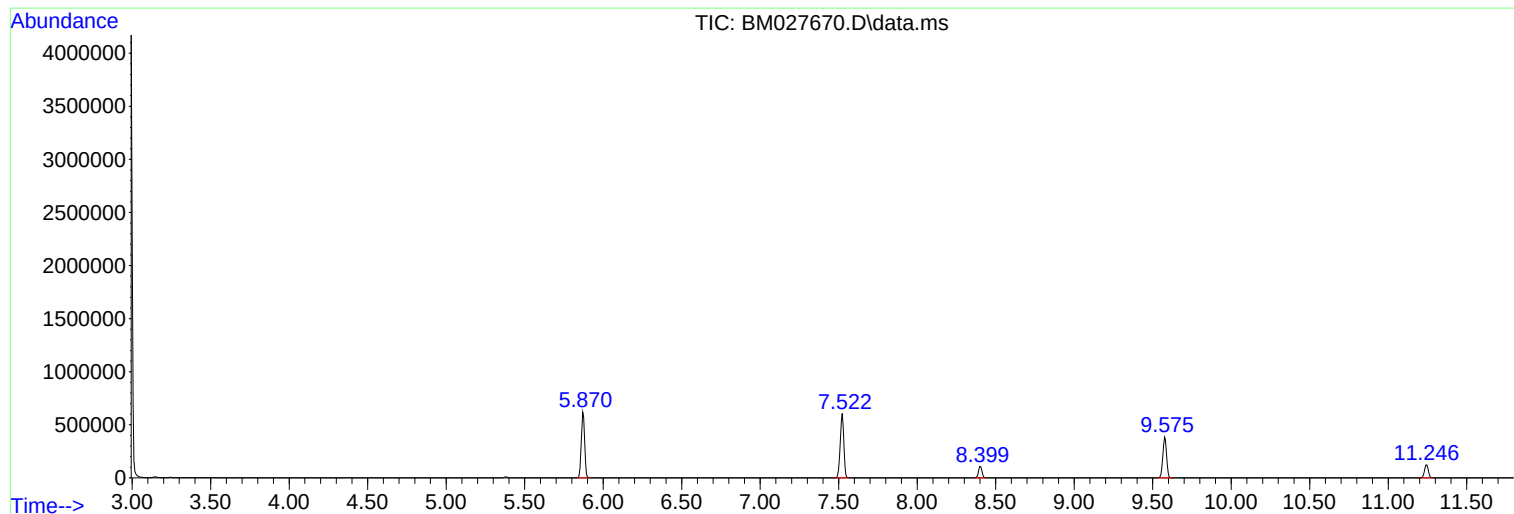

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
Data File : BM027670.D
Acq On : 02 Nov 2020 10:32
Operator : JU/CG
Sample : PB132384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132384BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110220\
Data File : BM027670.D
Acq On : 02 Nov 2020 10:32
Operator : JU/CG
Sample : PB132384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132384BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------