
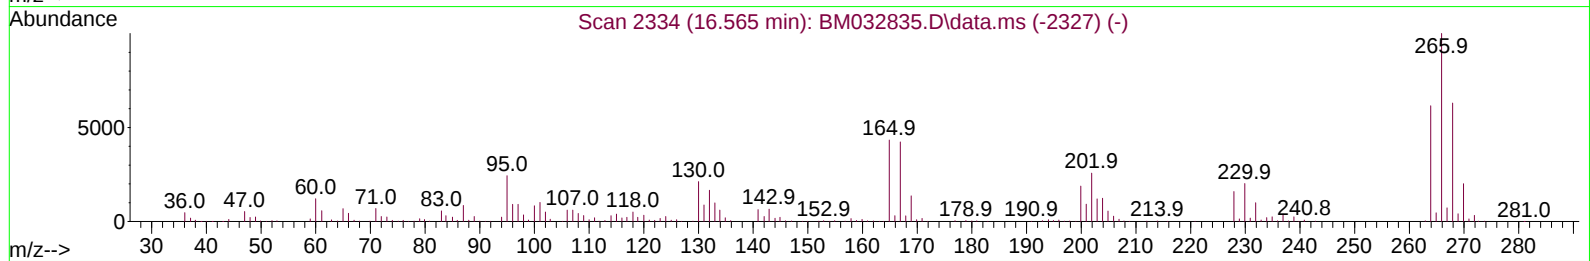
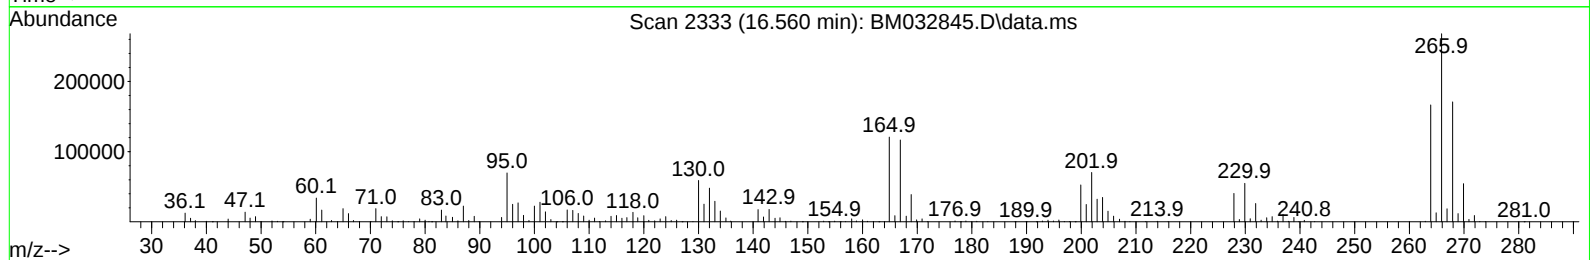


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110221\
Data File : BM032845.D
Acq On : 02 Nov 2021 08:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 11:33:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 18:47:37 2021
Response via : Initial Calibration

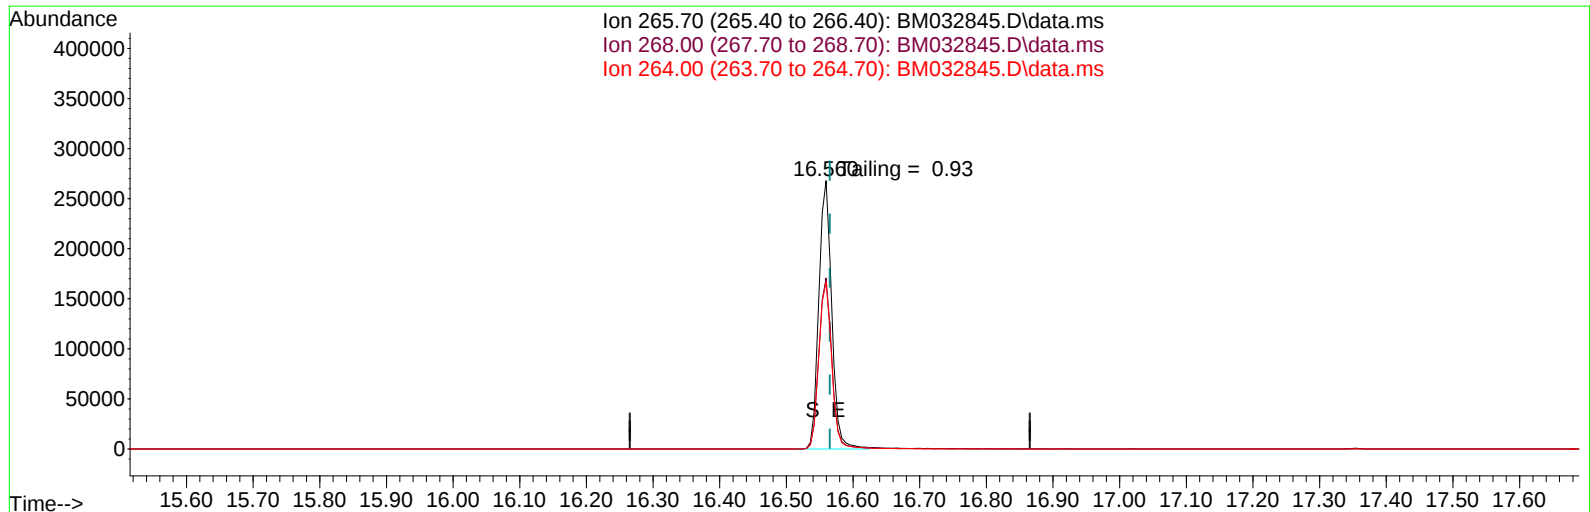

TIC: BM032845.D\data.ms

(70) Pentachlorophenol (C)




16.560min (-0.006) 689098.76 ng

response 363012

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.75
264.00	65.10	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110221\
Data File : BM032845.D
Acq On : 02 Nov 2021 08:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 11:33:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 18:47:37 2021
Response via : Initial Calibration

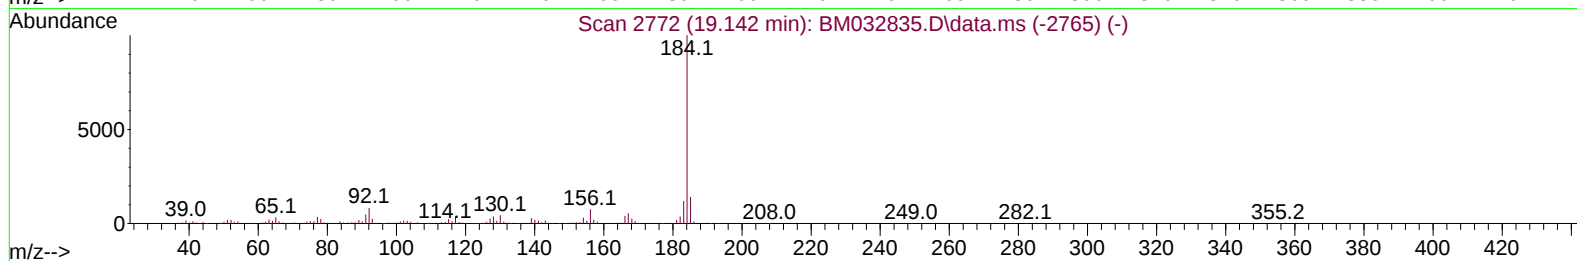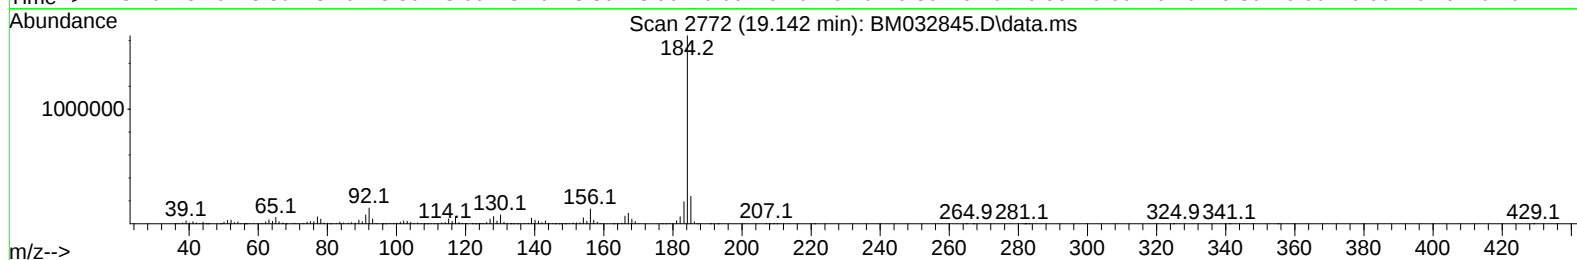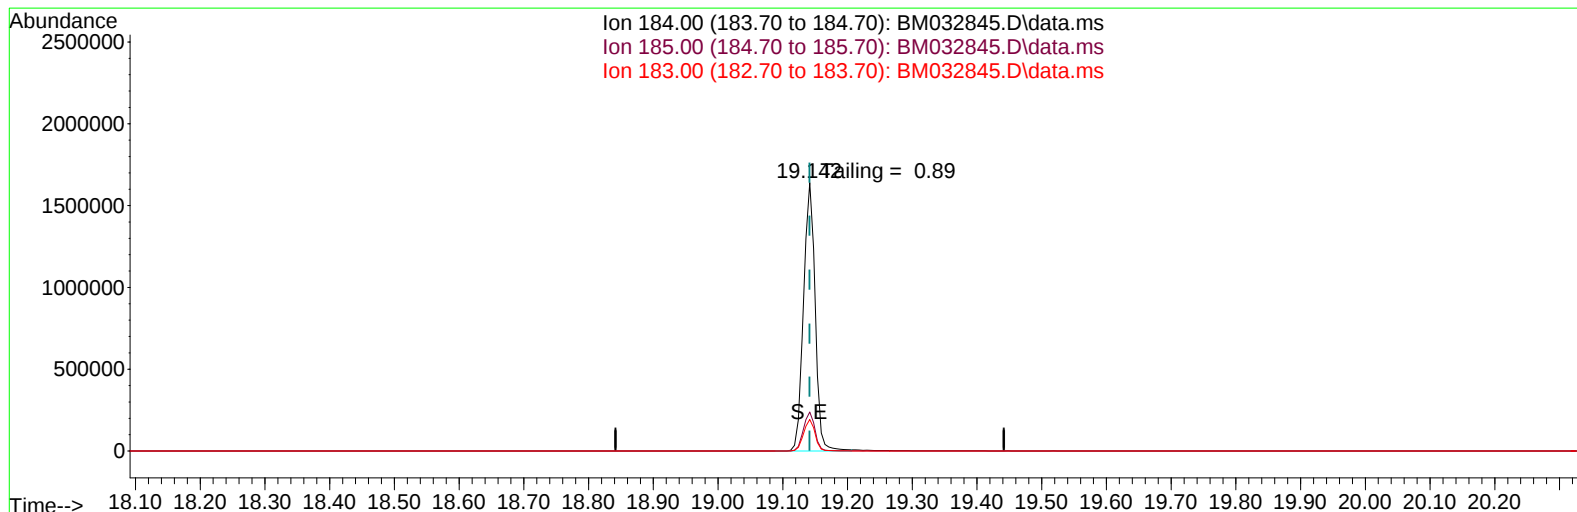

TIC: BM032845.D\data.ms

(77) Benzidine

19.142min (+ 0.000) 37334.67 ng

response 2067981

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.56
183.00	11.20	11.76
0.00	0.00	0.00