

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110221\
Data File : BM032855.D
Acq On : 02 Nov 2021 17:19
Operator : CG/JU
Sample : PB140166BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140166BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.084	375	382	402	rBV	2805966	4108964	44.11%	9.886%
2	6.695	649	656	682	rBV	2764487	4409403	47.33%	10.609%
3	7.489	783	791	804	rBV	435153	699172	7.50%	1.682%
4	8.648	980	988	1012	rBV	1697317	2803840	30.10%	6.746%
5	10.272	1257	1264	1283	rBV	634279	1038880	11.15%	2.500%
6	12.766	1681	1688	1704	rBV	4408194	6667165	71.57%	16.042%
7	14.154	1917	1924	1938	rBV	1079887	1555780	16.70%	3.743%
8	15.648	2171	2178	2196	rBV	3595770	5126335	55.03%	12.334%
9	16.889	2383	2389	2403	rBV	1409772	1940743	20.83%	4.670%
10	19.524	2831	2837	2842	rBV	7154737	9316230	100.00%	22.415%
11	21.071	3095	3100	3108	rBV	1642304	2037799	21.87%	4.903%
12	23.188	3454	3460	3470	rBV	1102260	1857583	19.94%	4.469%




Sum of corrected areas: 41561894

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110221\
Data File : BM032855.D
Acq On : 02 Nov 2021 17:19
Operator : CG/JU
Sample : PB140166BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140166BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

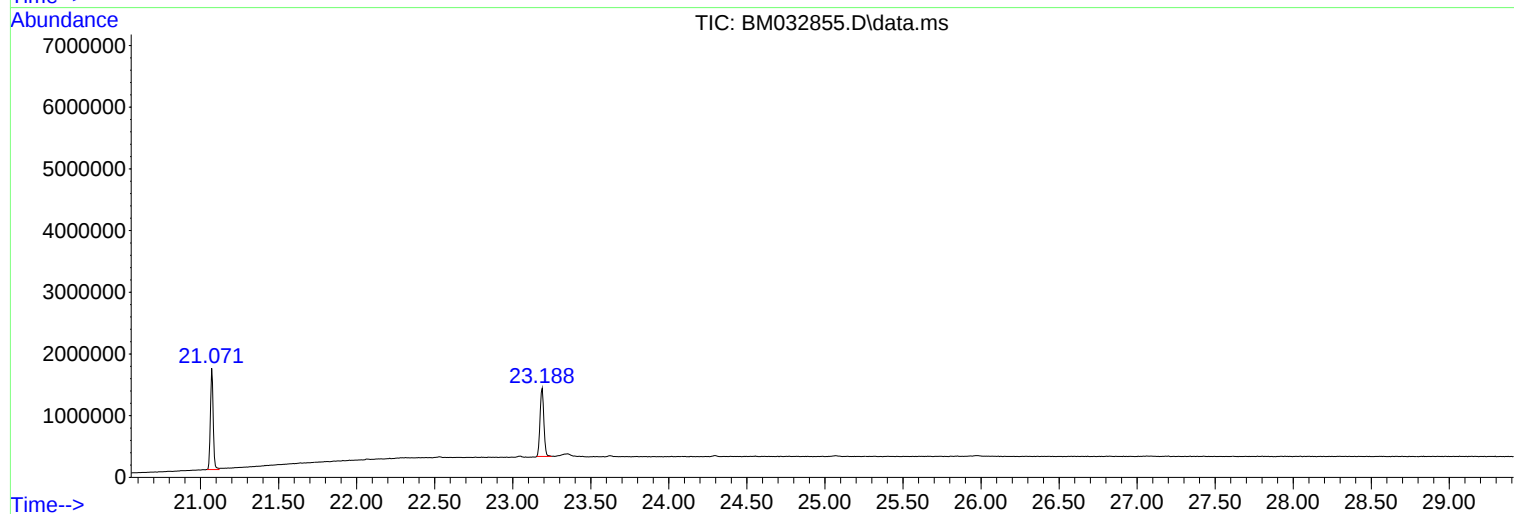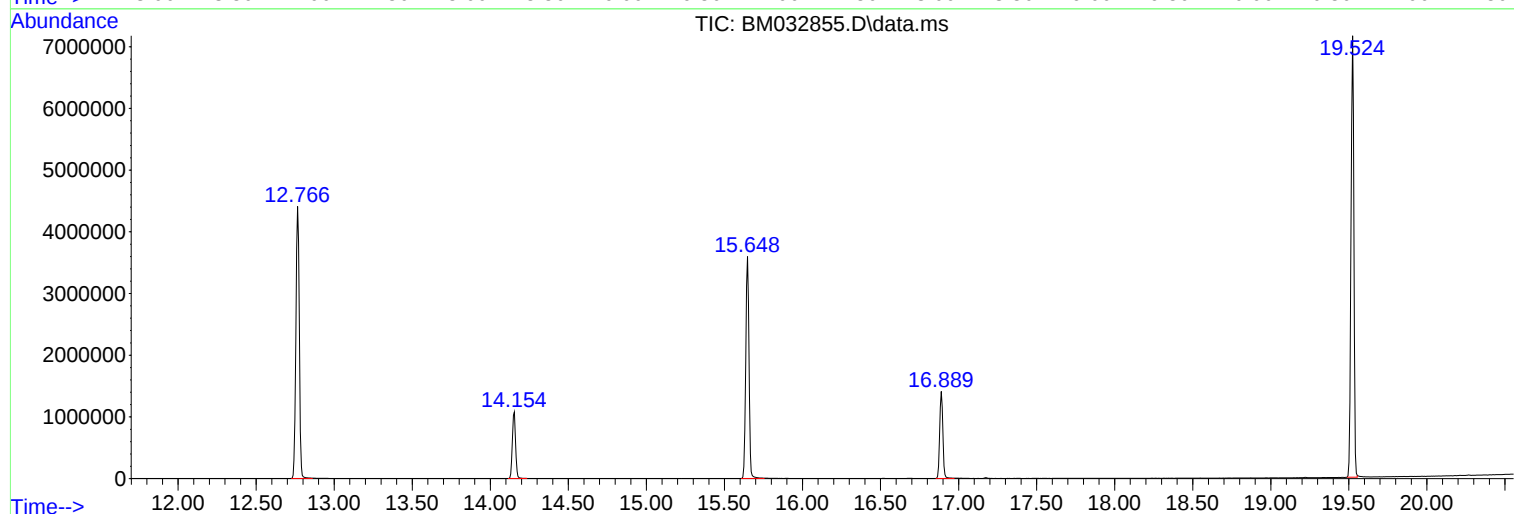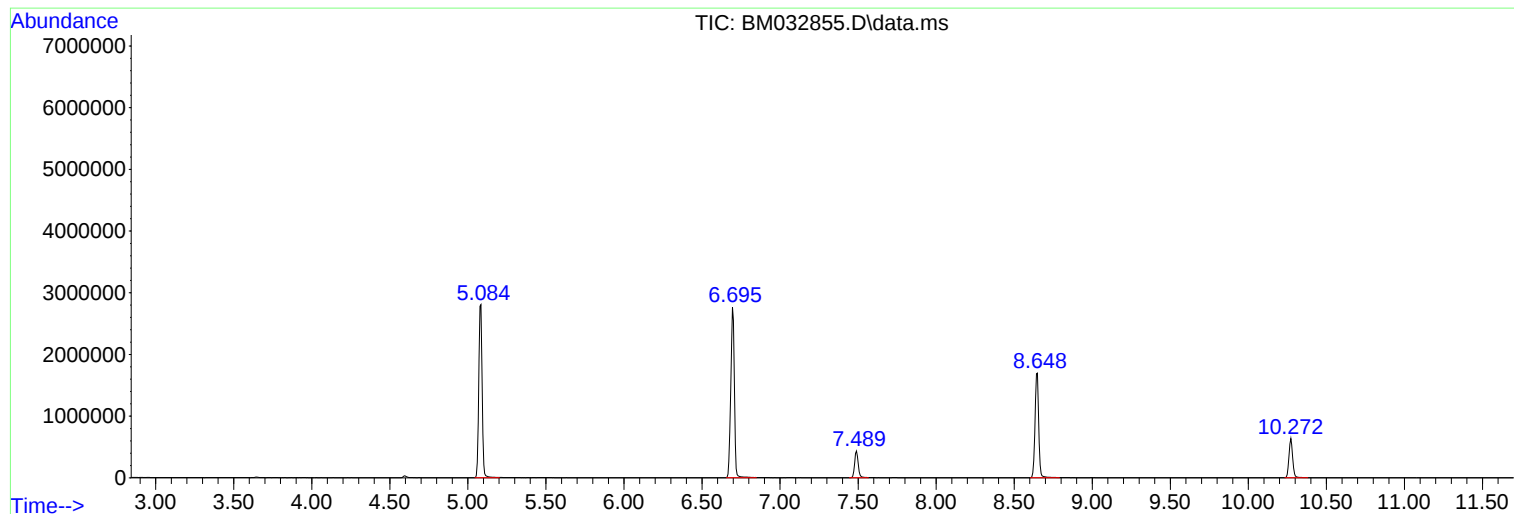

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110221\
Data File : BM032855.D
Acq On : 02 Nov 2021 17:19
Operator : CG/JU
Sample : PB140166BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140166BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110221\
Data File : BM032855.D
Acq On : 02 Nov 2021 17:19
Operator : CG/JU
Sample : PB140166BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140166BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------