
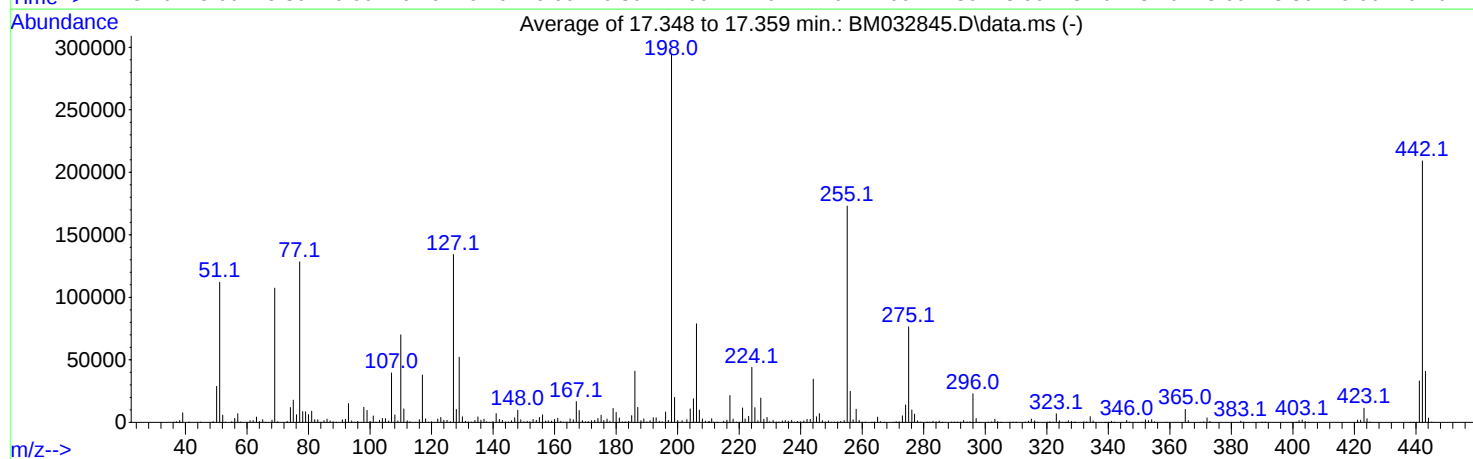


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM110221\  
 Data File : BM032845.D  
 Acq On : 02 Nov 2021 08:45  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM110221.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Nov 02 16:07:18 2021

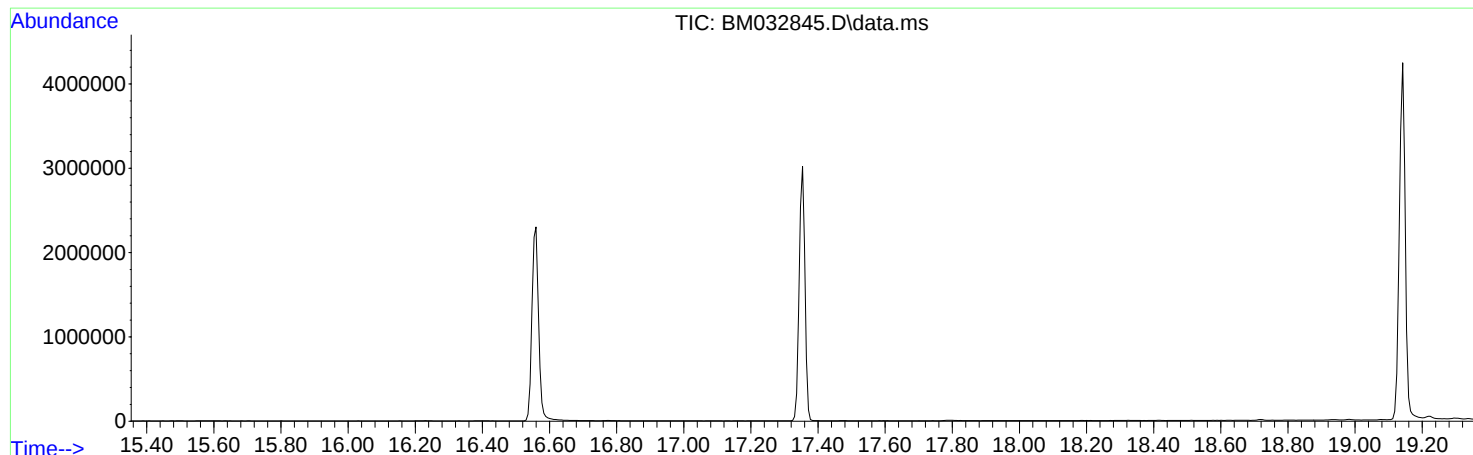




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 38.1      | 111984  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 1864    | PASS             |
| 69          | 198          | 0.00         | 100          | 36.5      | 107365  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 579     | PASS             |
| 127         | 198          | 10           | 80           | 45.6      | 134259  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 1640    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 294208  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 19979   | PASS             |
| 275         | 198          | 10           | 60           | 26.0      | 76413   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 10397   | PASS             |
| 441         | 198          | 0.01         | 100          | 11.3      | 33109   | PASS             |
| 442         | 442          | 50           | 100          | 100.0     | 209152  | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 40816   | PASS             |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM110221\  
 Data File : BM032845.D  
 Acq On : 02 Nov 2021 08:45  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Nov 02 11:33:04 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM110121.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Nov 01 18:47:37 2021  
 Response via : Initial Calibration

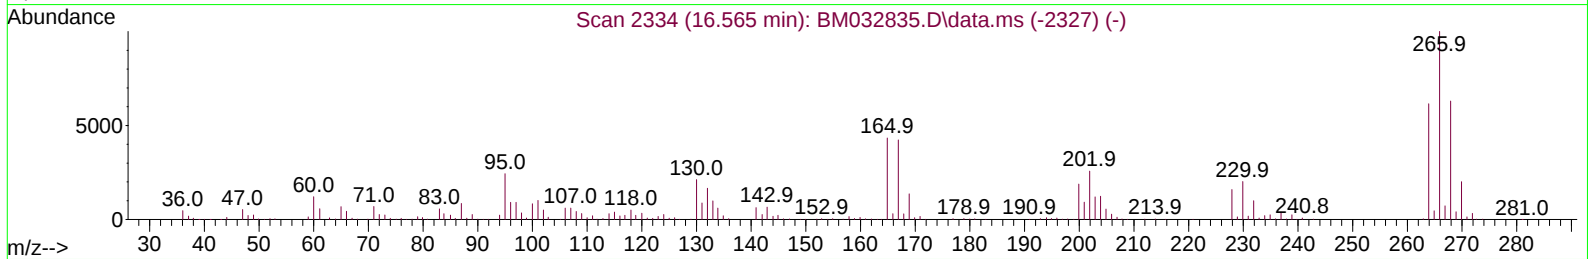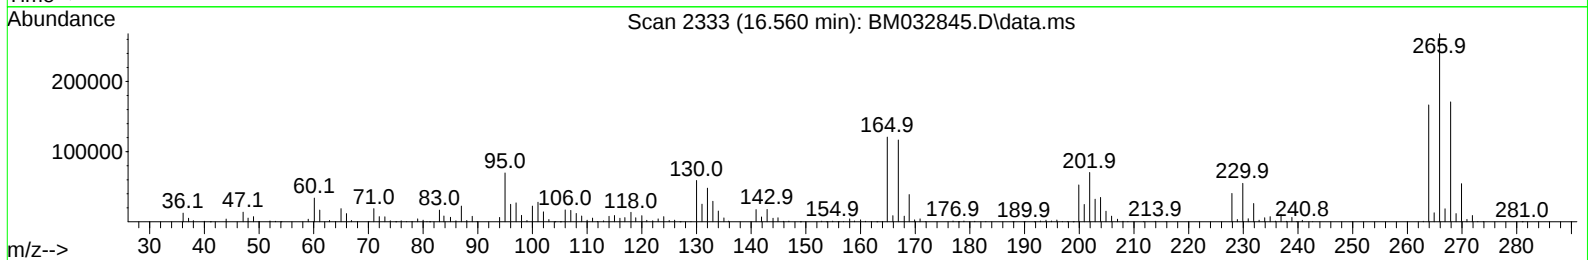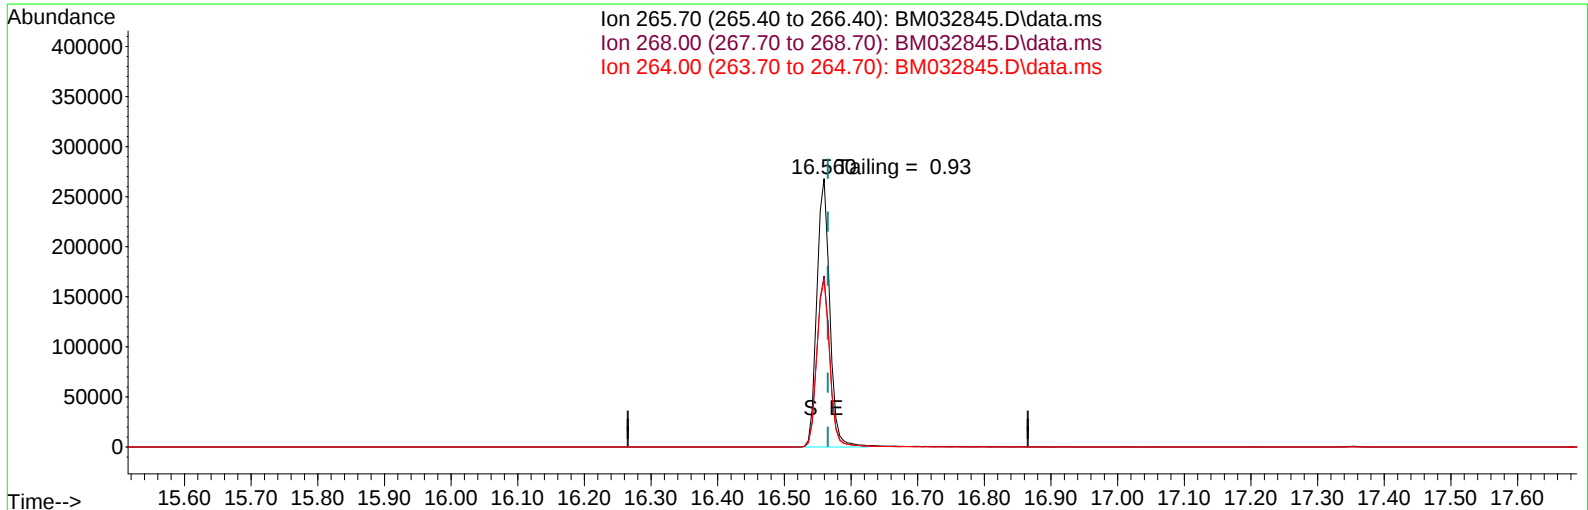

TIC: BM032845.D\data.ms

**(70) Pentachlorophenol (C)**

16.560min (-0.006) 689098.76 ng




response 363012

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.90  | 63.75  |
| 264.00 | 65.10  | 62.15  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM110221\  
Data File : BM032845.D  
Acq On : 02 Nov 2021 08:45  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Nov 02 11:33:04 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM110121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 01 18:47:37 2021  
Response via : Initial Calibration

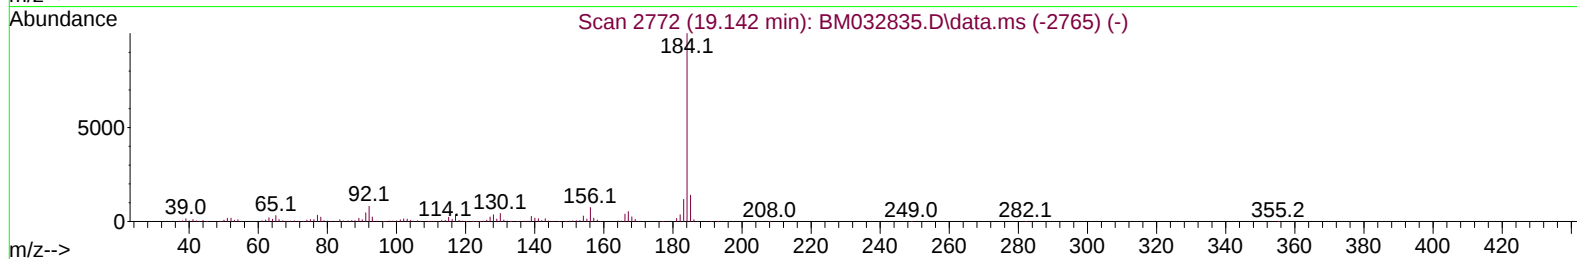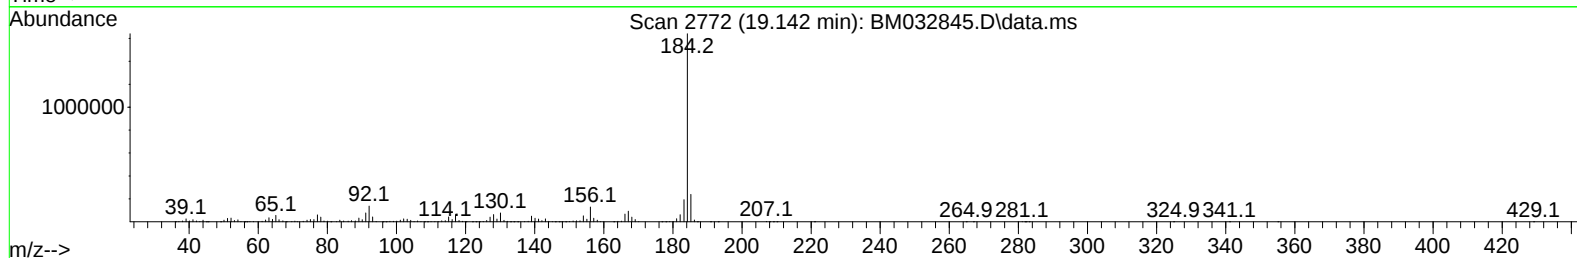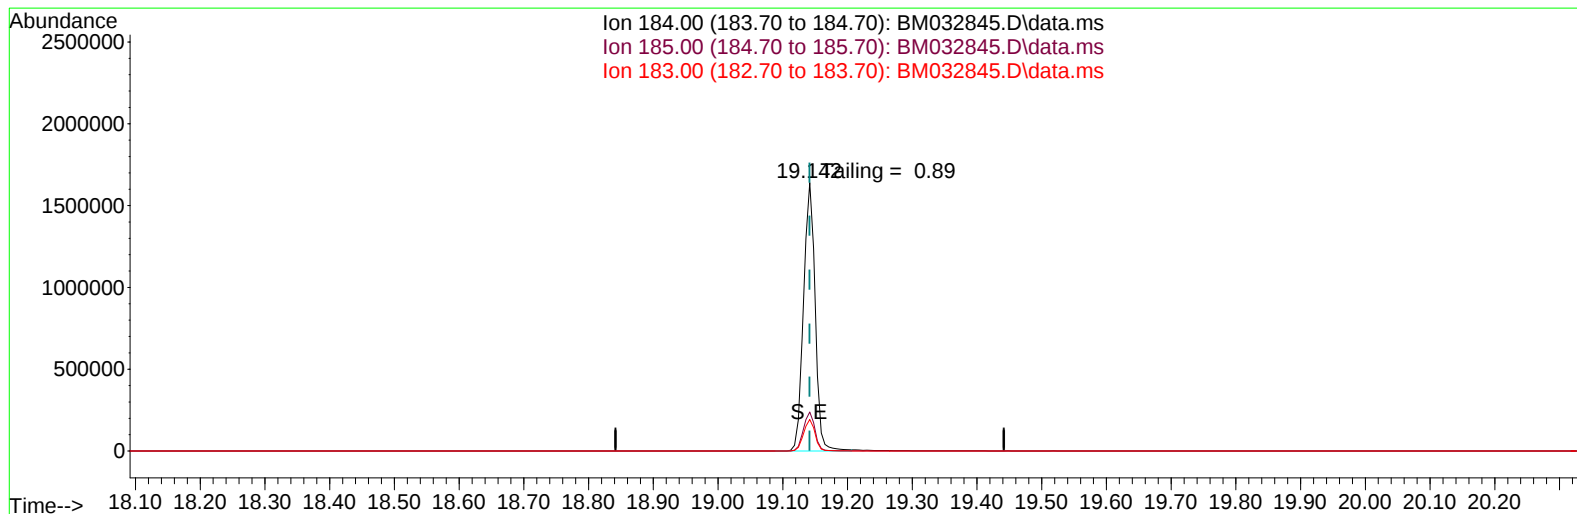

TIC: BM032845.D\data.ms

**(77) Benzidine**

19.142min (+ 0.000) 37334.67 ng

response 2067981

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.30  | 14.56  |
| 183.00 | 11.20  | 11.76  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/2/2021     | BNA_M            | <u>BM032845.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 973491           | 20.38              |
| DDD           | 3216             | 19.94              |
| DDE           | 637              | 19.43              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3853          | 977344           | 0.39               |
|               |                  |                    |