
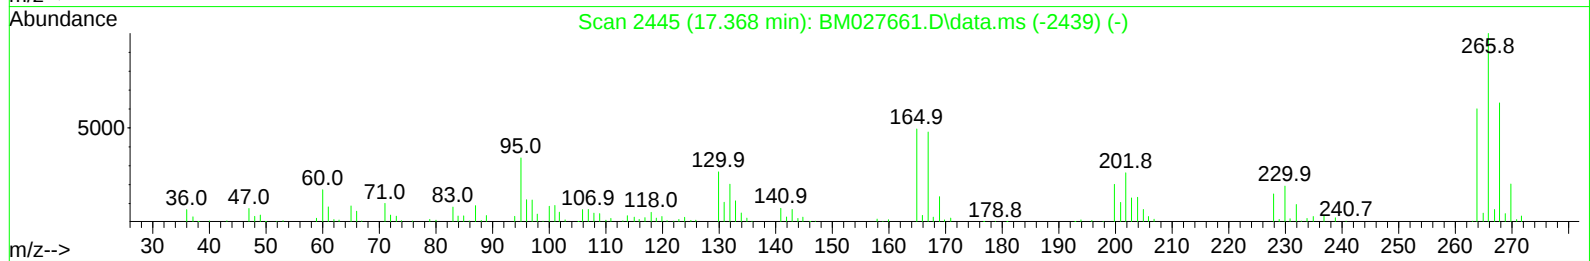
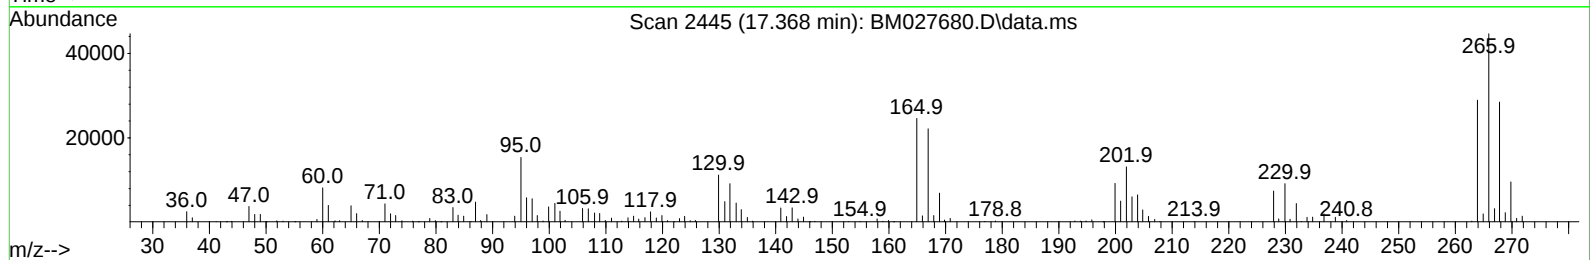


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110320\
Data File : BM027680.D
Acq On : 03 Nov 2020 08:21
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 05:25:25 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 17:56:42 2020
Response via : Initial Calibration

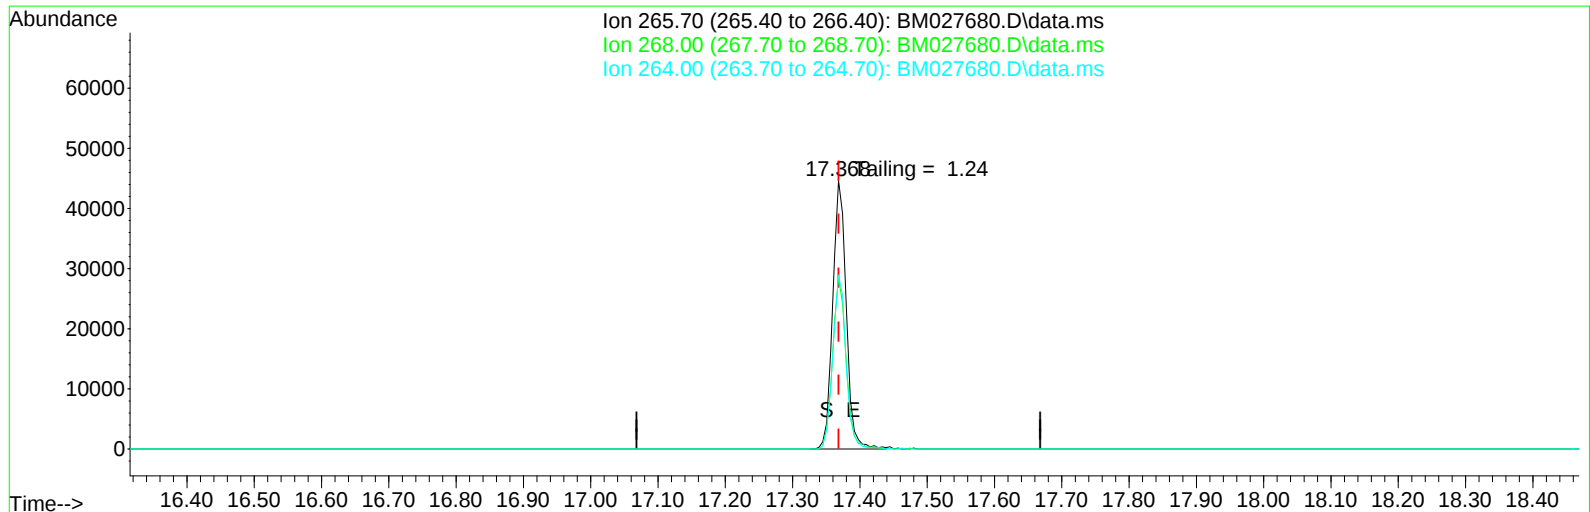

TIC: BM027680.D\data.ms

(70) Pentachlorophenol (C)




17.368min (+ 0.000) 166528.16 ng

response 62684

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.75
264.00	63.30	64.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110320\
Data File : BM027680.D
Acq On : 03 Nov 2020 08:21
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 05:25:25 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 17:56:42 2020
Response via : Initial Calibration

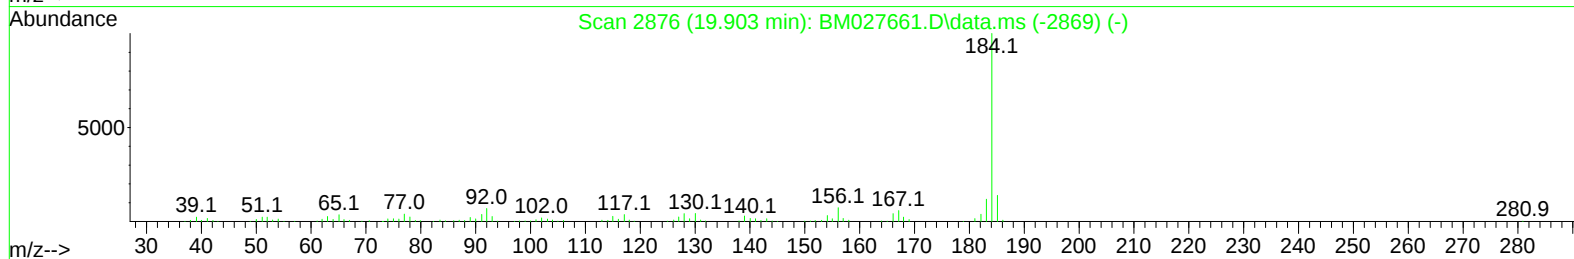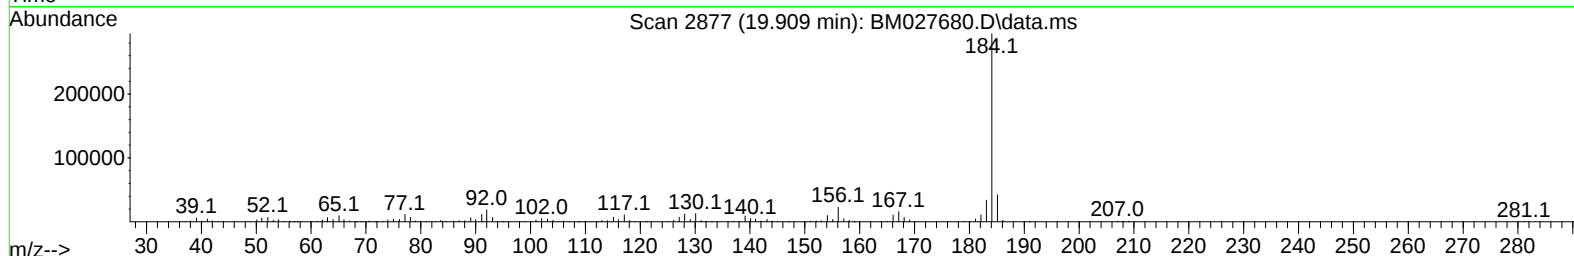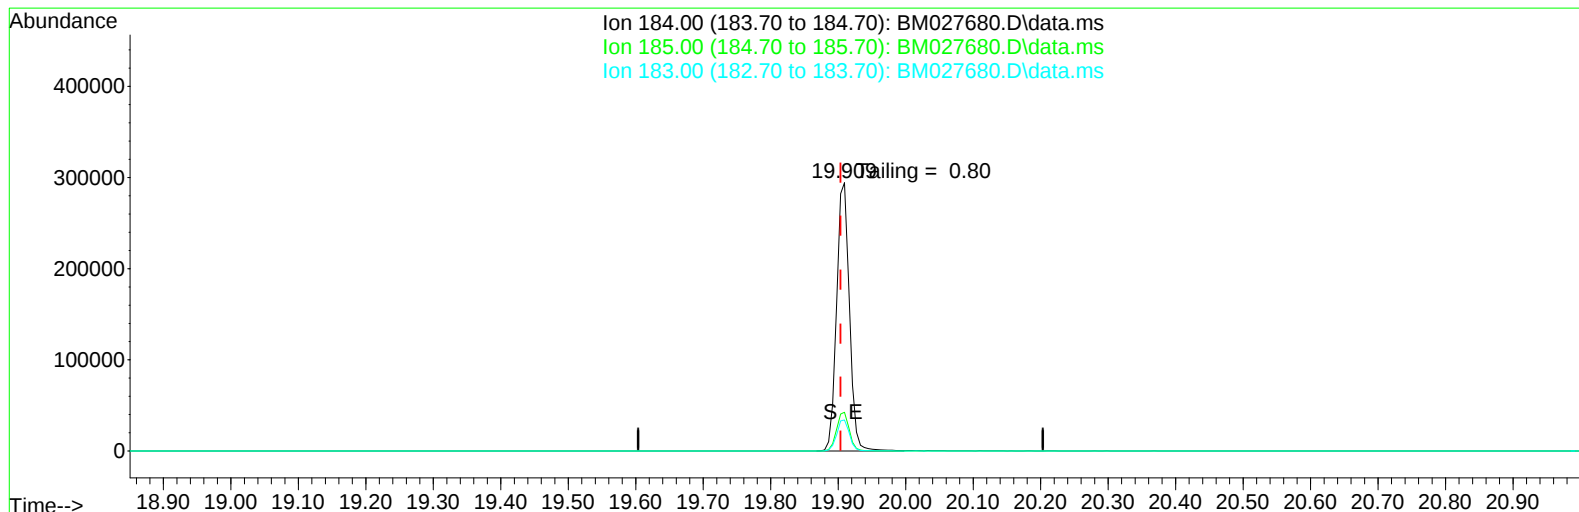

TIC: BM027680.D\data.ms

(77) Benzidine**19.909min (+ 0.006) 33281.69 ng****response 390244**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.44
183.00	12.10	11.56
0.00	0.00	0.00