

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110320\
 Data File : BM027682.D
 Acq On : 03 Nov 2020 10:08
 Operator : JU/CG
 Sample : PB132413BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB132413BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM027682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.869	483	490	498	rBV	1016015	1523025	59.52%	12.304%
2	7.522	762	771	779	rBV	1005786	1598460	62.46%	12.913%
3	8.398	914	920	927	rVB	157518	249269	9.74%	2.014%
4	9.575	1112	1120	1129	rVB	634409	1045588	40.86%	8.447%
5	11.239	1396	1403	1410	rBV	187567	322169	12.59%	2.603%
6	13.645	1806	1812	1819	rVB	1362618	2000646	78.18%	16.162%
7	15.010	2038	2044	2051	rVB	274637	390219	15.25%	3.152%
8	16.474	2287	2293	2307	rBV	1058043	1453278	56.79%	11.740%
9	17.727	2500	2506	2512	rVB	306157	434427	16.98%	3.510%
10	20.286	2935	2941	2946	rBV	2053097	2559038	100.00%	20.673%
11	21.821	3197	3202	3208	rBV2	328387	421905	16.49%	3.408%
12	24.274	3612	3619	3627	rVB	188375	380484	14.87%	3.074%




Sum of corrected areas: 12378508

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110320\
Data File : BM027682.D
Acq On : 03 Nov 2020 10:08
Operator : JU/CG
Sample : PB132413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132413BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

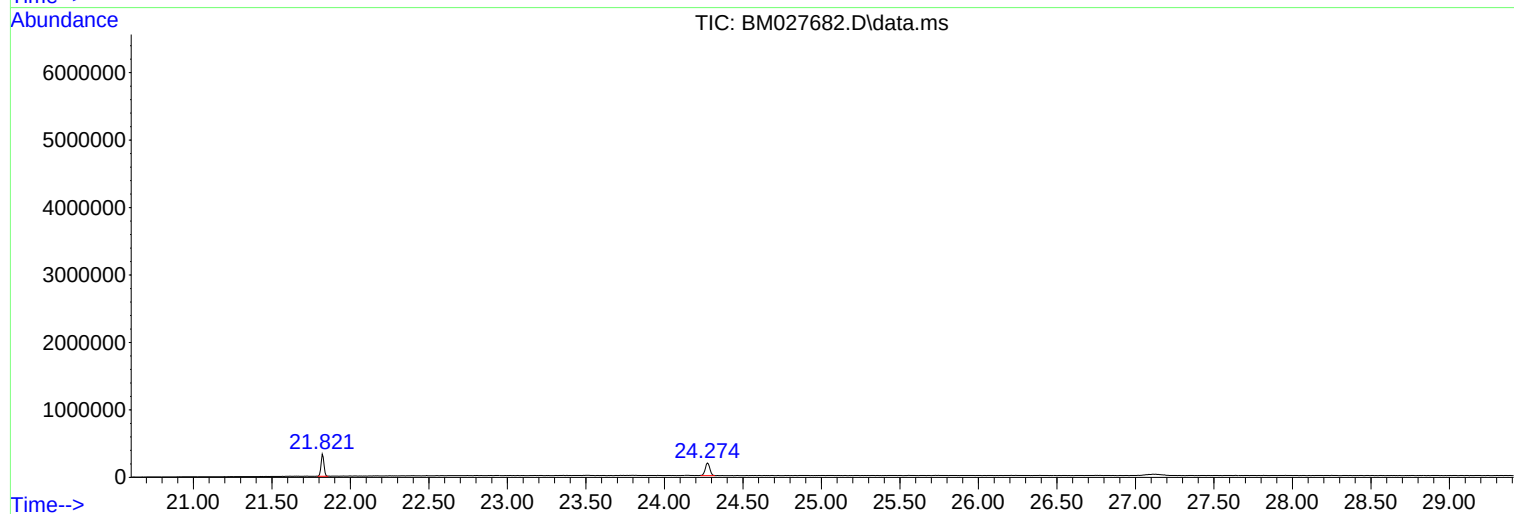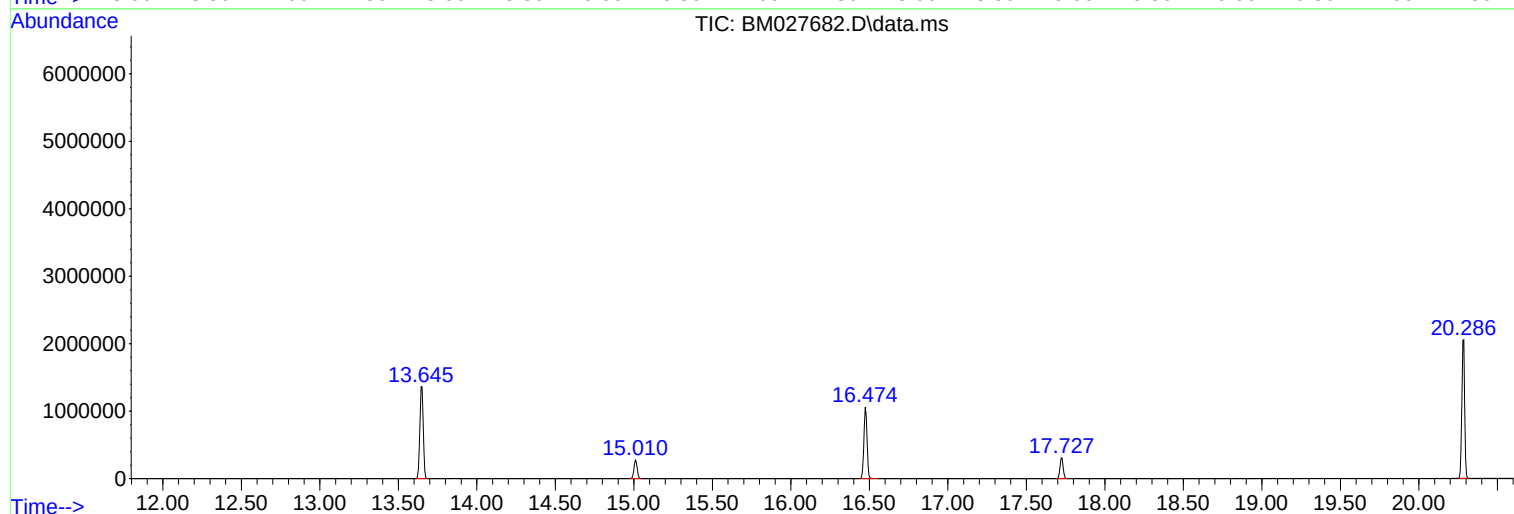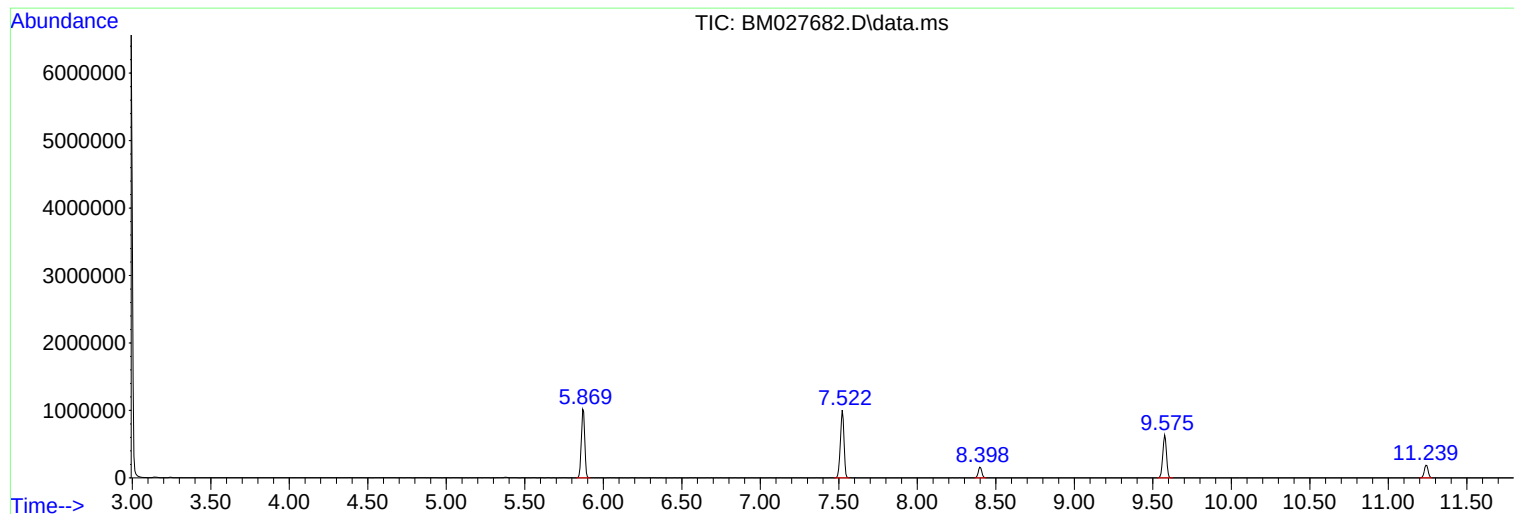

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110320\
Data File : BM027682.D
Acq On : 03 Nov 2020 10:08
Operator : JU/CG
Sample : PB132413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132413BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110320\
Data File : BM027682.D
Acq On : 03 Nov 2020 10:08
Operator : JU/CG
Sample : PB132413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB132413BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------