
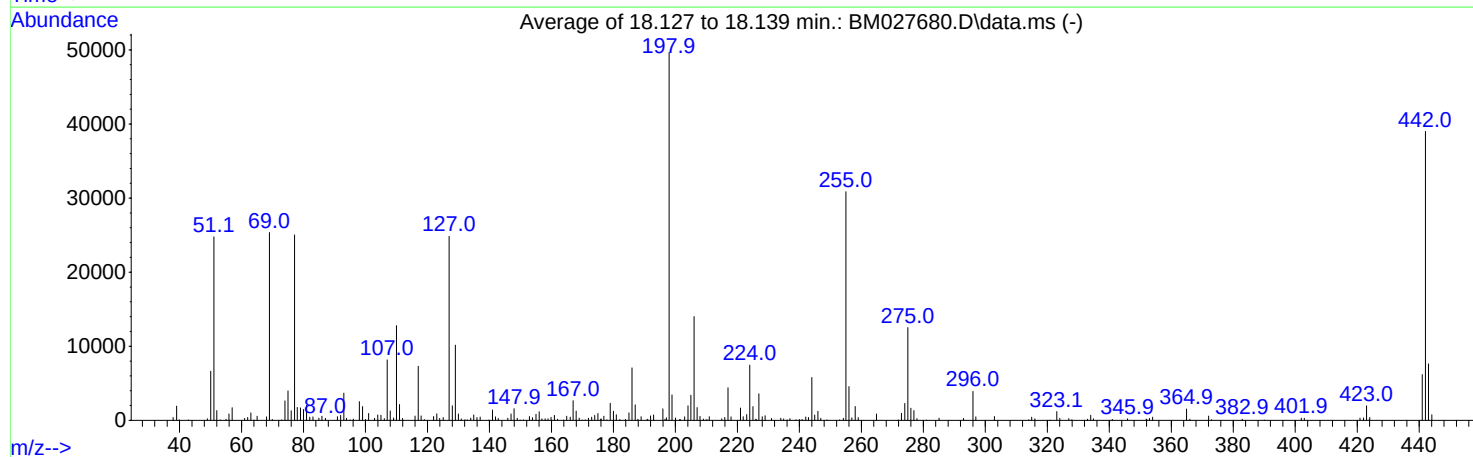


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110320\
 Data File : BM027680.D
 Acq On : 03 Nov 2020 08:21
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 17:56:42 2020

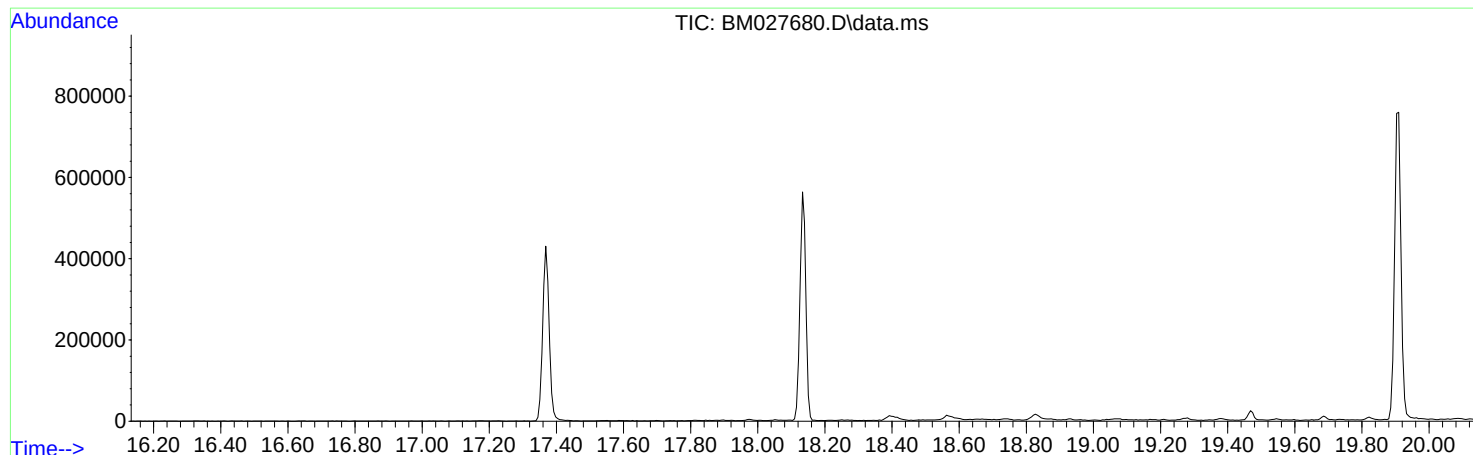

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	24763	PASS
68	69	0.00	2	1.9	481	PASS
69	198	0.00	100	51.1	25357	PASS
70	69	0.00	2	0.6	140	PASS
127	198	10	80	50.0	24843	PASS
197	198	0.00	2	0.7	338	PASS
198	198	100	100	100.0	49651	PASS
199	198	5	9	6.9	3427	PASS
275	198	10	60	25.2	12524	PASS
365	198	1	100	3.1	1531	PASS
441	198	0.01	100	12.4	6174	PASS
442	198	50	100	78.6	39003	PASS
443	442	15	24	19.5	7616	PASS