

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110321\
 Data File : BM032859.D
 Acq On : 03 Nov 2021 11:19
 Operator : CG/JU
 Sample : PB140340BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB140340BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.084	375	382	397	rBV	2116466	3092864	36.86%	8.934%
2	6.695	649	656	670	rBV	2134519	3288112	39.19%	9.498%
3	7.490	785	791	803	rBV	353750	552661	6.59%	1.596%
4	8.642	980	987	1006	rBV	1304186	2091378	24.93%	6.041%
5	10.272	1257	1264	1276	rBV	507866	821540	9.79%	2.373%
6	12.766	1681	1688	1702	rBV	3553546	5229806	62.34%	15.106%
7	14.148	1917	1923	1939	rBV	881150	1283440	15.30%	3.707%
8	15.648	2171	2178	2196	rBV	2939626	4332701	51.64%	12.515%
9	16.889	2383	2389	2402	rBV	1139758	1651767	19.69%	4.771%
10	19.518	2830	2836	2841	rBV	6220321	8389711	100.00%	24.233%
11	21.071	3095	3100	3108	rBV	1564593	1930882	23.01%	5.577%
12	23.183	3453	3459	3470	rVB2	1131548	1955794	23.31%	5.649%




Sum of corrected areas: 34620656

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110321\
Data File : BM032859.D
Acq On : 03 Nov 2021 11:19
Operator : CG/JU
Sample : PB140340BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140340BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

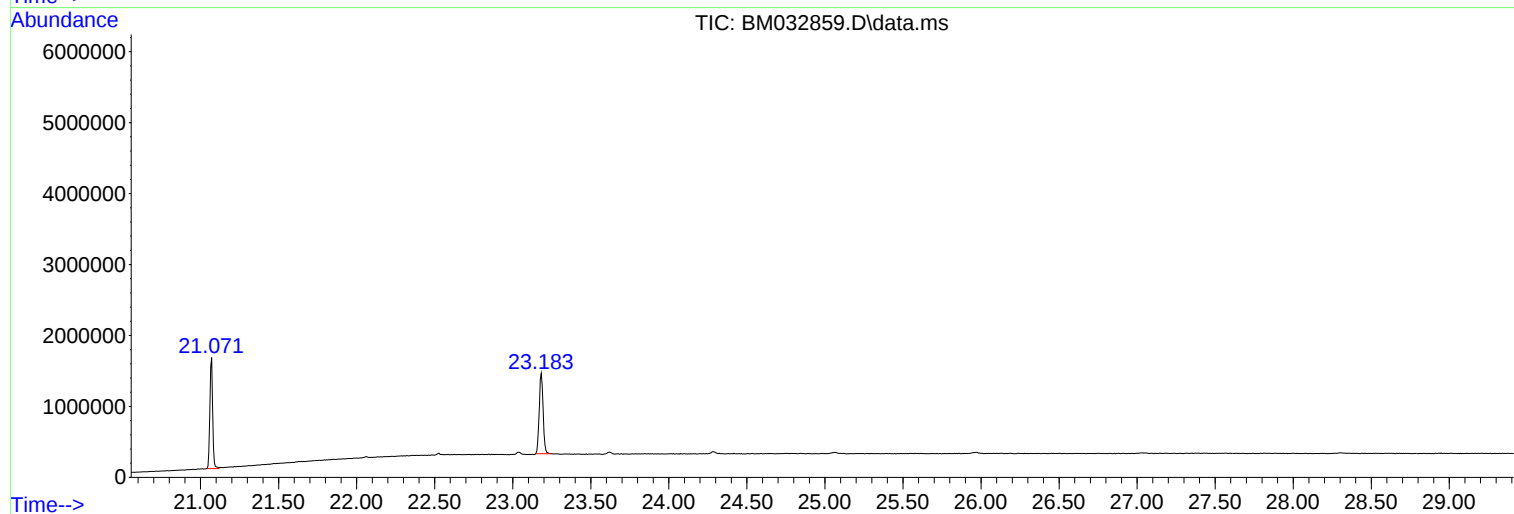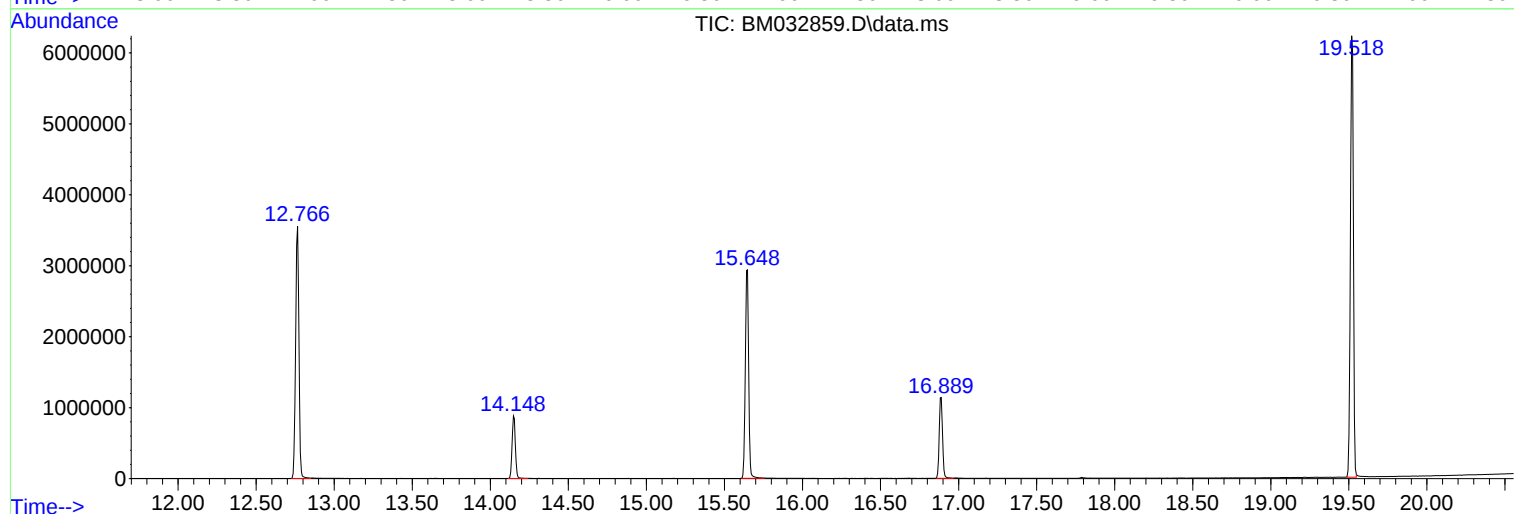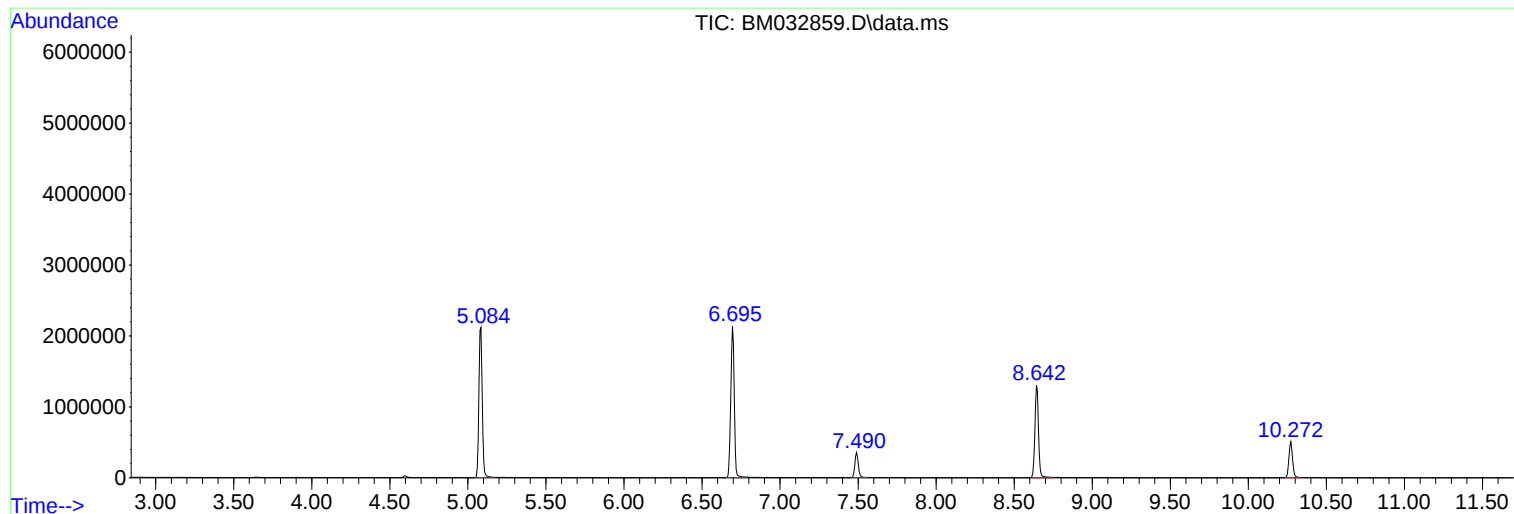

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110321\
Data File : BM032859.D
Acq On : 03 Nov 2021 11:19
Operator : CG/JU
Sample : PB140340BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140340BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110321\
Data File : BM032859.D
Acq On : 03 Nov 2021 11:19
Operator : CG/JU
Sample : PB140340BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140340BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------