
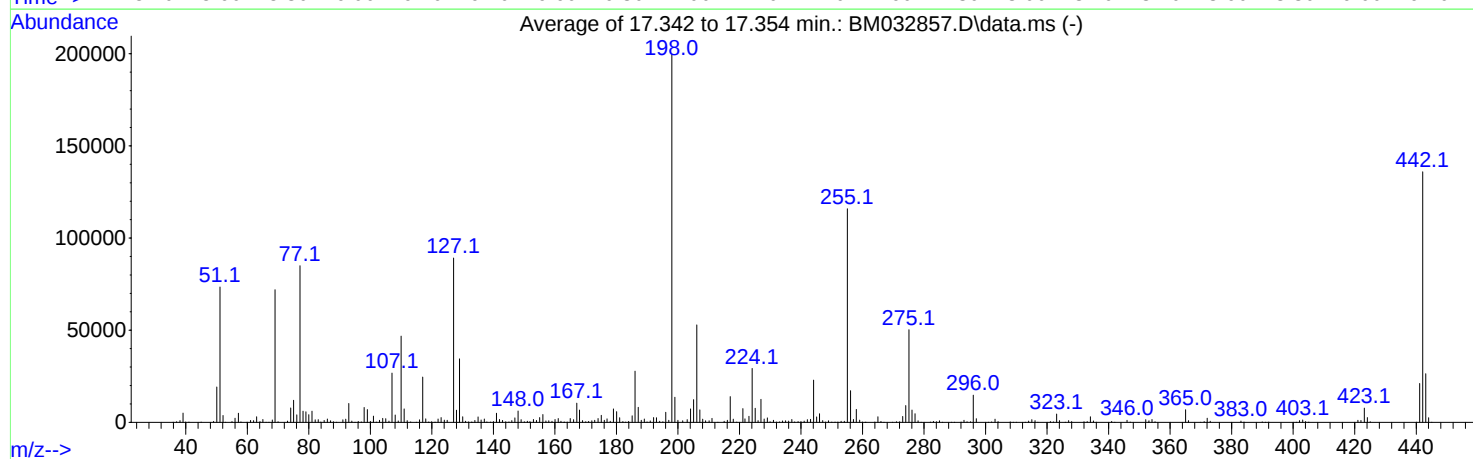


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110321\
 Data File : BM032857.D
 Acq On : 03 Nov 2021 09:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 02 16:07:18 2021

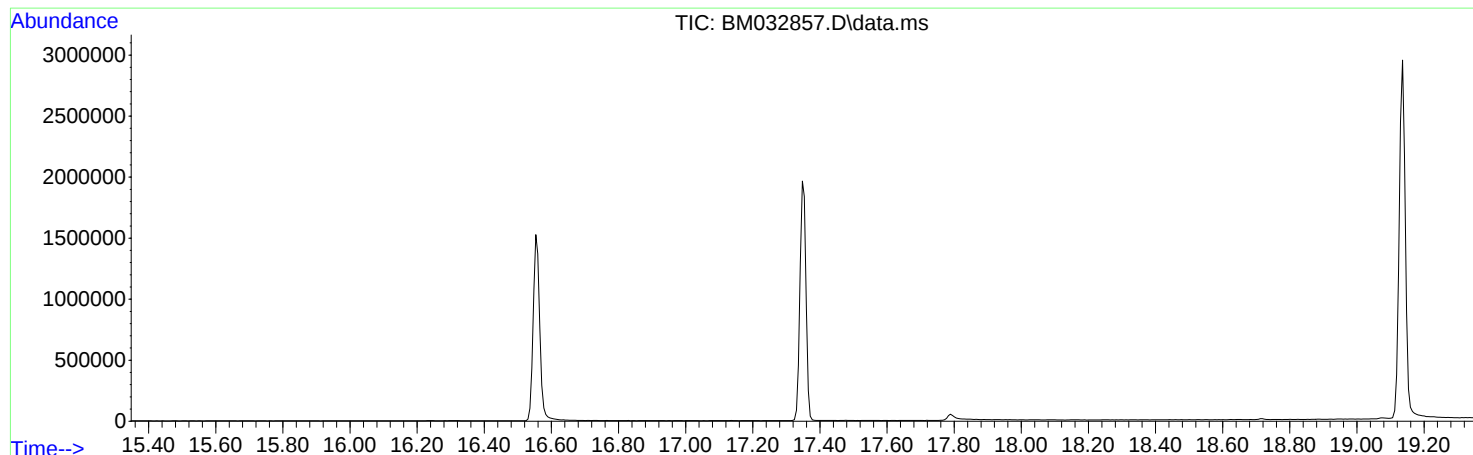




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	73451	PASS
68	69	0.00	2	1.8	1324	PASS
69	198	0.00	100	36.1	71968	PASS
70	69	0.00	2	0.5	360	PASS
127	198	10	80	44.7	89160	PASS
197	198	0.00	2	0.6	1140	PASS
198	198	100	100	100.0	199595	PASS
199	198	5	9	6.8	13671	PASS
275	198	10	60	25.2	50280	PASS
365	198	1	100	3.4	6831	PASS
441	198	0.01	100	10.6	21087	PASS
442	442	50	100	100.0	135933	PASS
443	442	15	24	19.4	26357	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110321\
 Data File : BM032857.D
 Acq On : 03 Nov 2021 09:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Nov 03 11:13:47 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 02 16:07:18 2021
 Response via : Initial Calibration

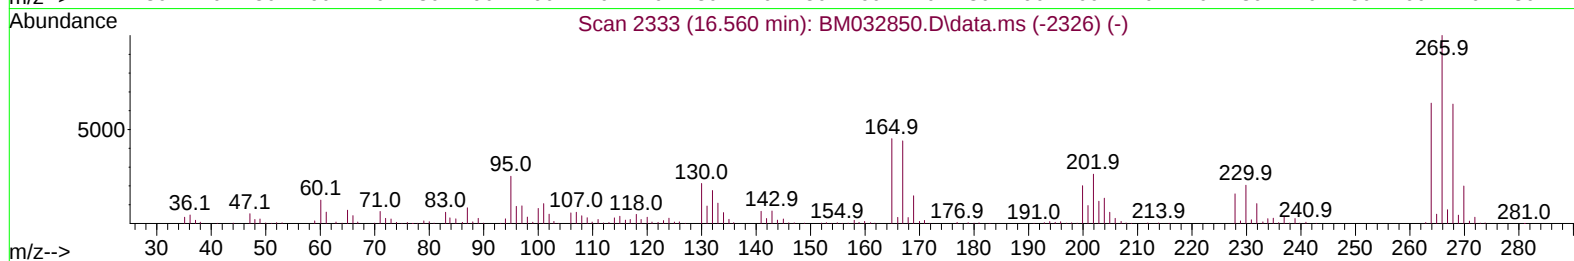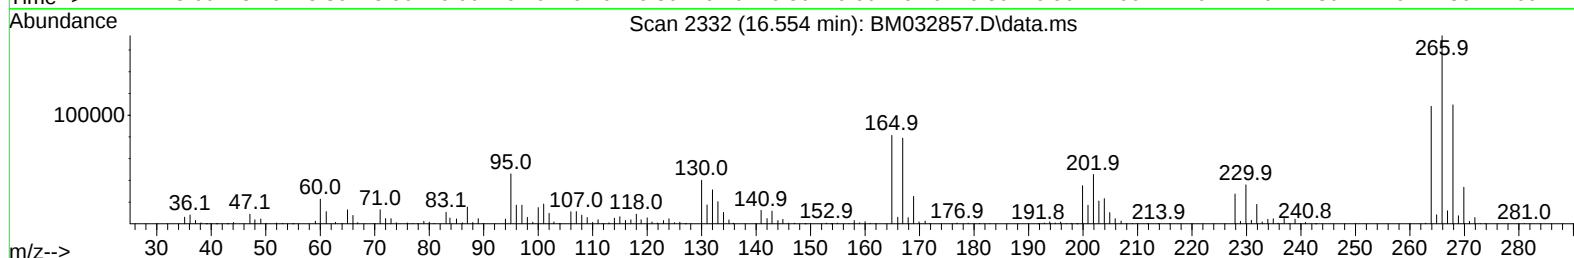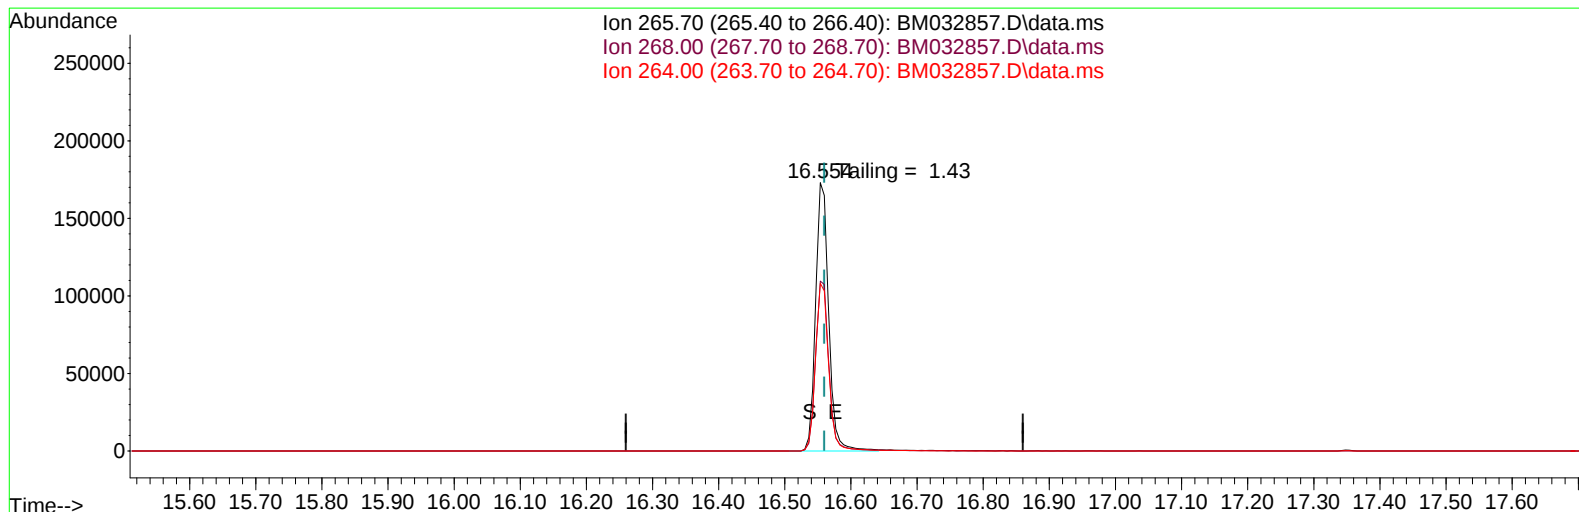

TIC: BM032857.D\data.ms

(70) Pentachlorophenol (C)

16.554min (-0.006) 0.00 ng




response 239860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.30
264.00	65.10	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110321\
Data File : BM032857.D
Acq On : 03 Nov 2021 09:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 03 11:13:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 16:07:18 2021
Response via : Initial Calibration

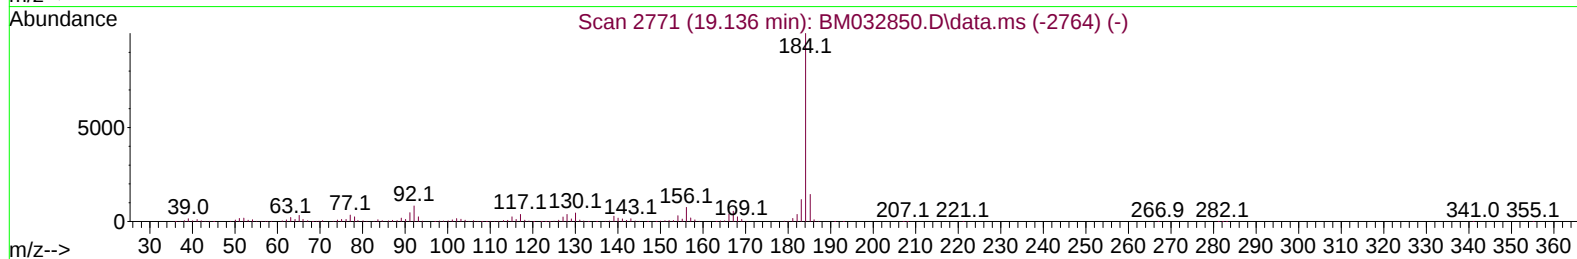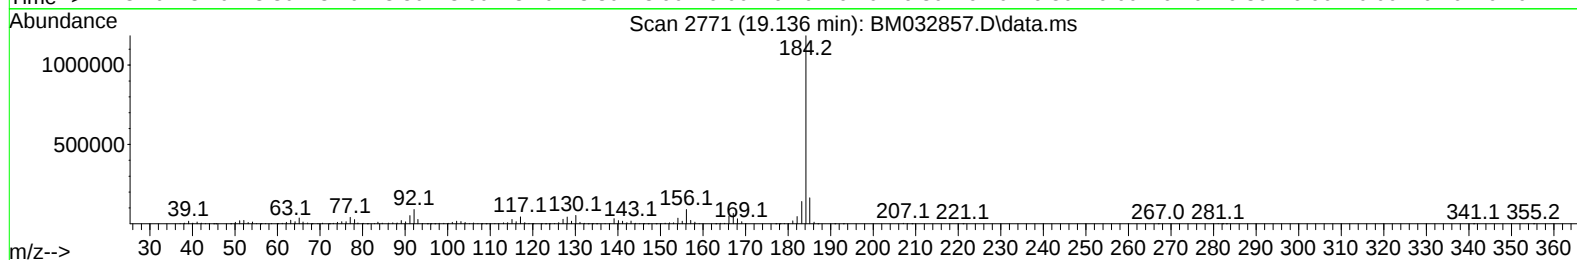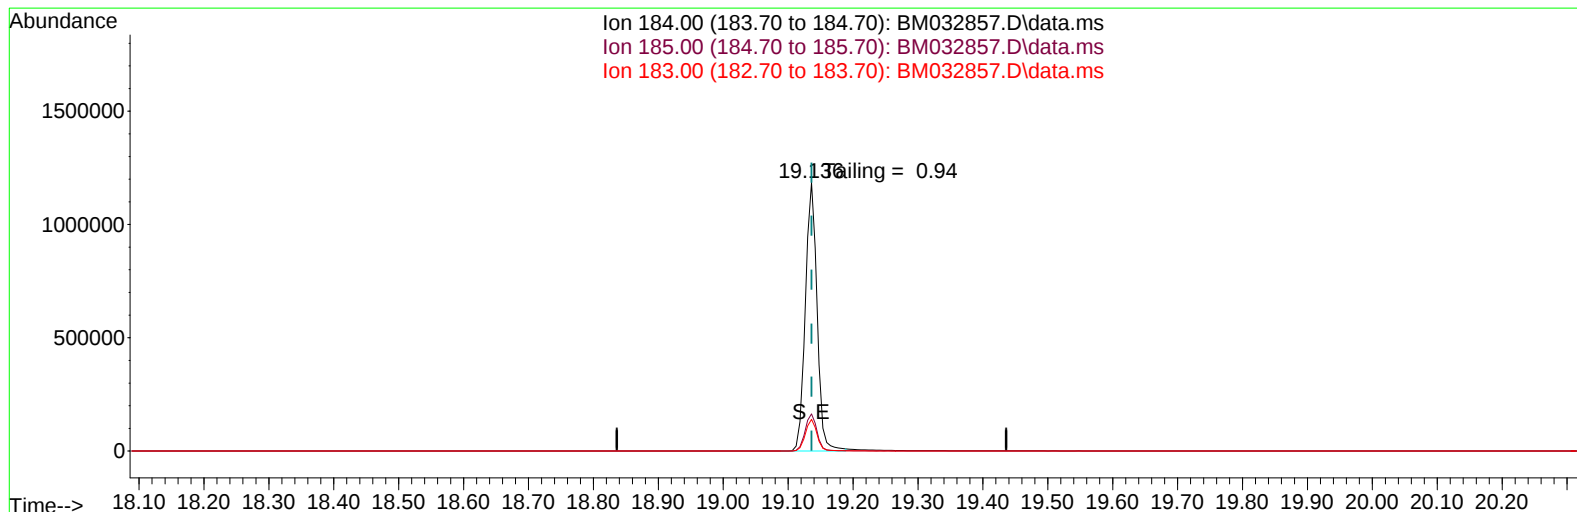

TIC: BM032857.D\data.ms

(77) Benzidine

19.136min (-0.000) 481713.15 ng

response 1518164

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.83
183.00	11.20	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2021	BNA_M	<u>BM032857.D</u>
Compound Name	Response	Retention Time
DDT	703401	20.37
DDD	5617	19.93
DDE	504	19.43
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6121	709522	0.86

Instrument :
BNA_M
ClientSampleId :
DFTPP