

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037348.D
 Acq On : 03 Nov 2022 16:01
 Operator : CG/JU
 Sample : N5276-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X4

Quant Time: Nov 04 01:03:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 02 03:33:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	336008	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136	1581714	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.486	164	1037934	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	2165435	20.000	ng/ul	0.00
79) Chrysene-d12	21.397	240	2043308	20.000	ng/ul	0.00
88) Perylene-d12	23.744	264	1722646	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	34598	4.539	ng/uL	0.00
4) Pyridine-d5	3.710	84	1558	0.068	ng/ul	0.01
7) Phenol-d5	7.028	99	198811	6.799	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.186	67	529030	29.482	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	528395	23.650	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	363656	15.229	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	344449	29.153	ng/ul	0.00
24) 2-Nitrophenol-d4	9.739	143	357351	27.766	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.280	165	608451	25.643	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	21358	0.589	ng/ul	0.01
46) Dimethylphthalate-d6	13.910	166	2308357	32.166	ng/ul	0.00
49) Acenaphthylene-d8	14.180	160	2666950	30.911	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	86682	6.043	ng/ul	0.00
60) Fluorene-d10	15.480	176	2105134	32.894	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	355015	25.884	ng/ul	0.00
73) Anthracene-d10	17.327	188	3401657	34.109	ng/ul	0.00
81) Pyrene-d10	19.615	212	3796080	35.552	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.597	264	3085197	34.793	ng/ul	0.00


Target Compounds					Qvalue
35) 4-Chloro-3-methylphenol	12.021	107	7889195	311.482 ng/ul#	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037348.D
Acq On : 03 Nov 2022 16:01
Operator : CG/JU
Sample : N5276-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X4

Quant Time: Nov 04 01:03:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 02 03:33:37 2022
Response via : Initial Calibration

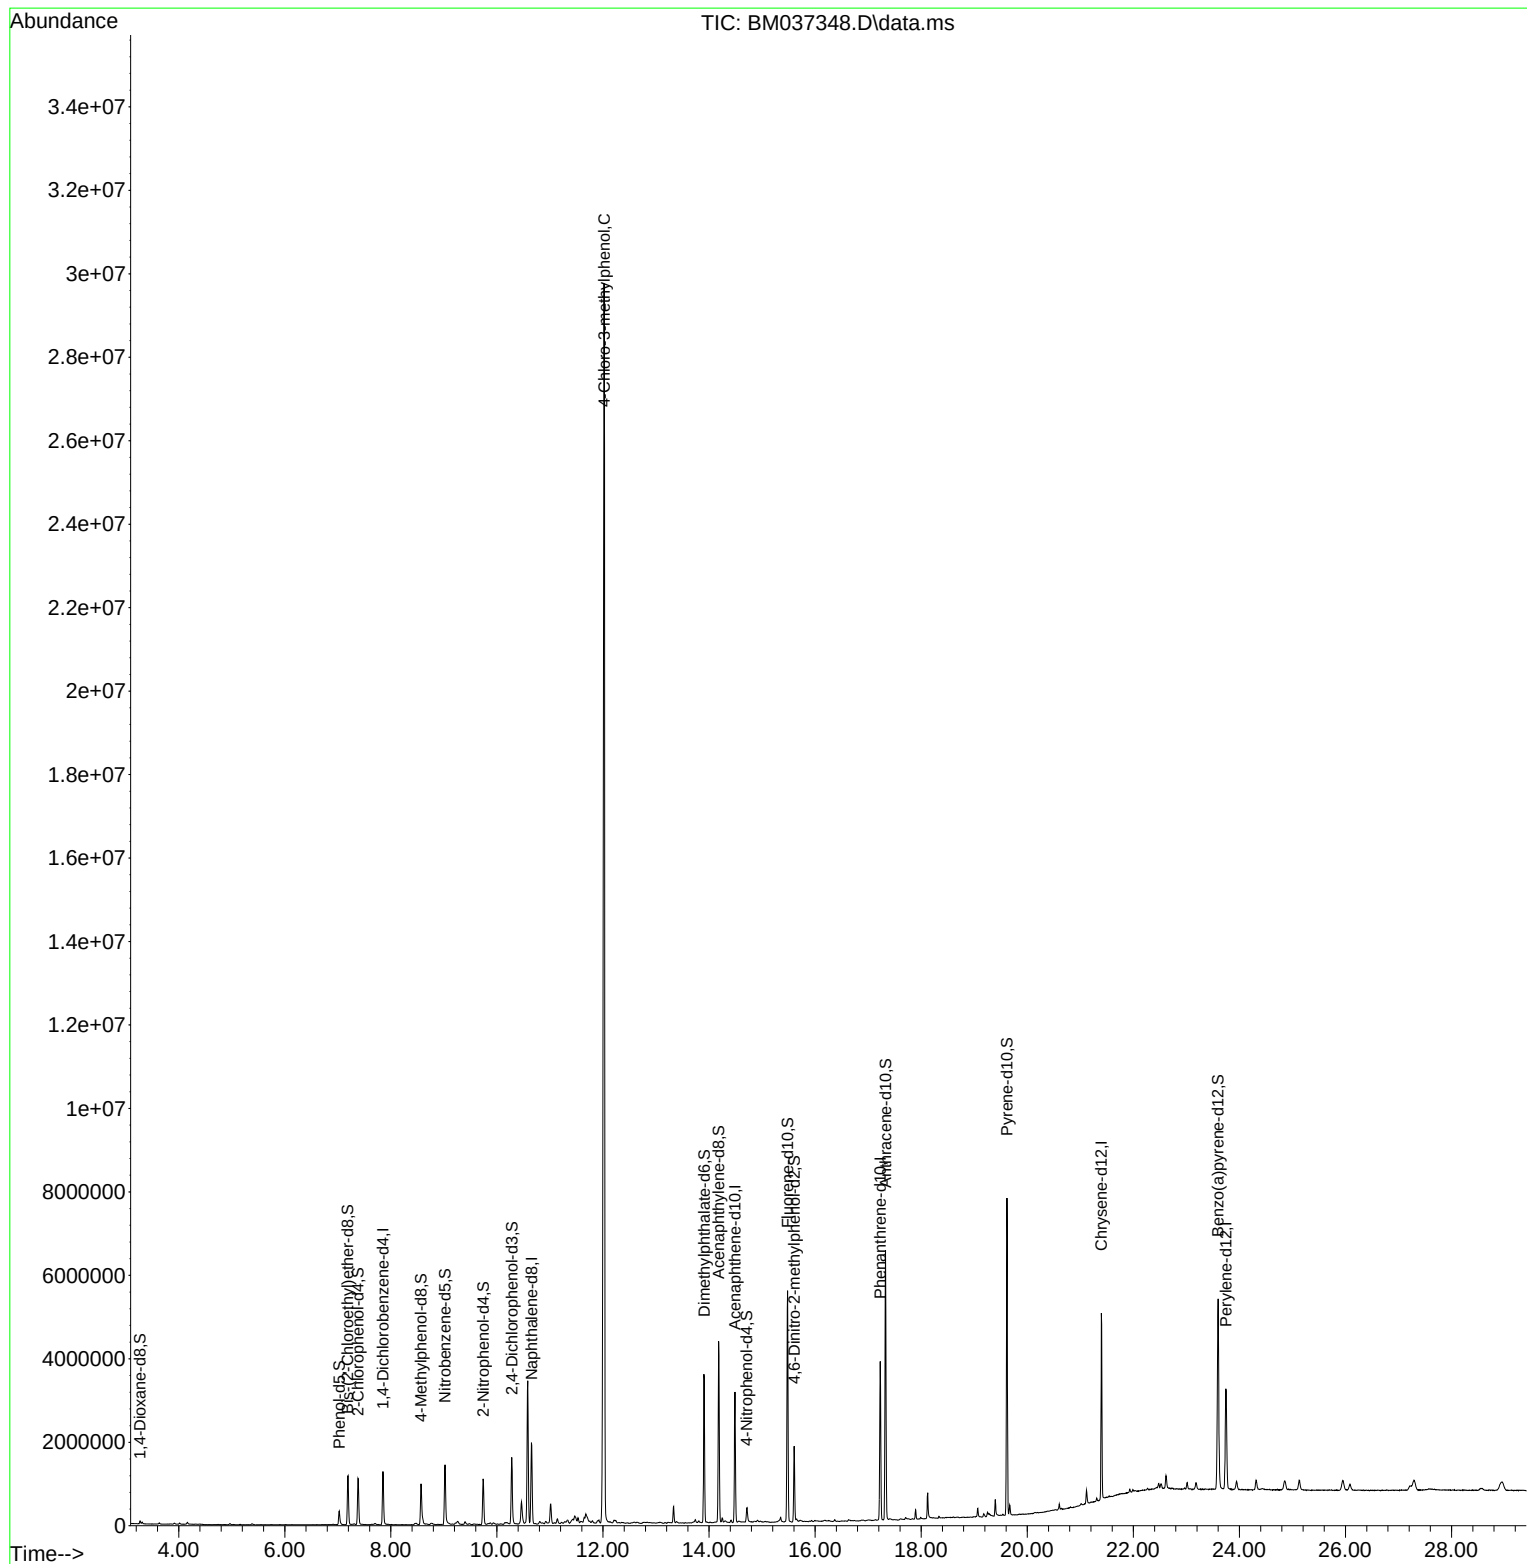

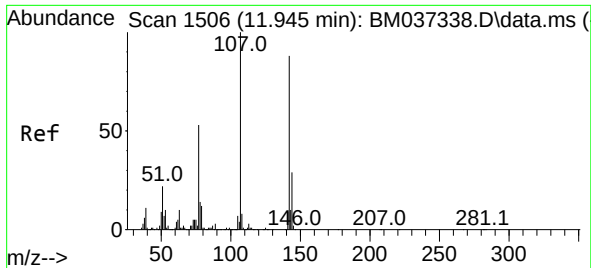

#35
 4-Chloro-3-methylphenol
 Concen: 311.482 ng/ul
 RT: 12.021 min Scan# 11
 Delta R.T. 0.065 min
 Lab File: BM037348.D
 Acq: 03 Nov 2022 16:01

Instrument :
 BNA_M
 ClientSampleId :
 EW4X4

Tgt Ion:107 Resp: 7889195
 Ion Ratio Lower Upper
 107 100
 144 0.0 23.3 34.9#
 142 0.0 69.4 104.2#

