

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037350.D
 Acq On : 03 Nov 2022 17:16
 Operator : CG/JU
 Sample : N5276-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X2

Quant Time: Nov 04 01:04:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 02 03:33:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	297790	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136	1331733	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.486	164	870423	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	1830800	20.000	ng/ul	0.00
79) Chrysene-d12	21.403	240	1738749	20.000	ng/ul	0.00
88) Perylene-d12	23.744	264	1532035	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	26484	3.920	ng/uL	0.00
4) Pyridine-d5	3.699	84	796	0.039	ng/ul	0.00
7) Phenol-d5	7.028	99	161855	6.245	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.186	67	493982	31.062	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	481400	24.312	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	312526	14.768	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	316340	31.800	ng/ul	0.00
24) 2-Nitrophenol-d4	9.739	143	325183	30.009	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.280	165	544748	27.267	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	7719	0.253	ng/ul	0.02
46) Dimethylphthalate-d6	13.904	166	2026498	33.672	ng/ul	0.00
49) Acenaphthylene-d8	14.180	160	2370846	32.767	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	53911	4.481	ng/ul	0.00
60) Fluorene-d10	15.480	176	1941414	36.174	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	313271	27.016	ng/ul	0.00
73) Anthracene-d10	17.327	188	3327682	39.466	ng/ul	0.00
81) Pyrene-d10	19.615	212	3718006	40.920	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.597	264	3111683	39.457	ng/ul	0.00
Target Compounds					Qvalue	
48) 2,6-Dinitrotoluene	14.015	165	13958	1.112	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037350.D
Acq On : 03 Nov 2022 17:16
Operator : CG/JU
Sample : N5276-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X2

Quant Time: Nov 04 01:04:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 02 03:33:37 2022
Response via : Initial Calibration

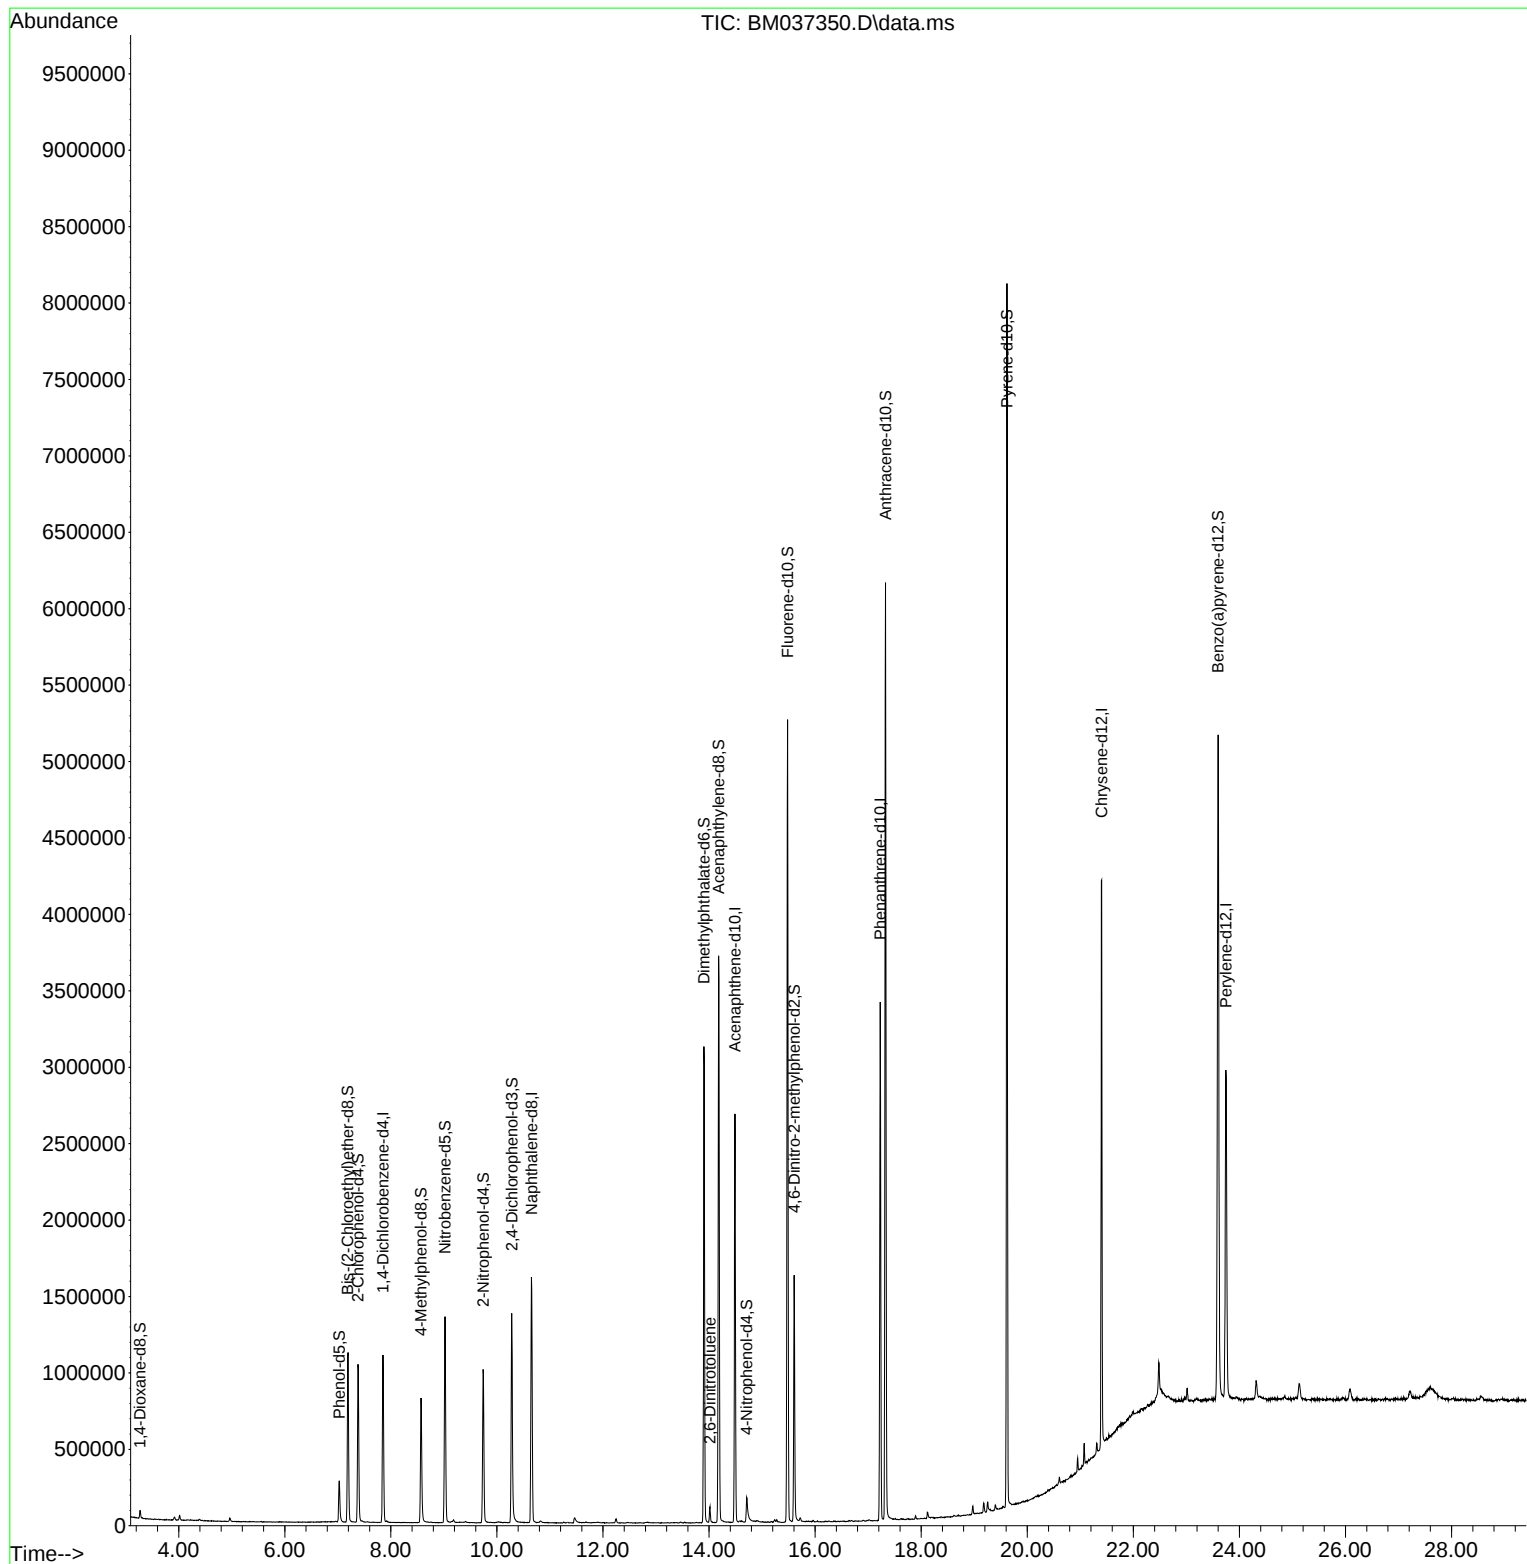

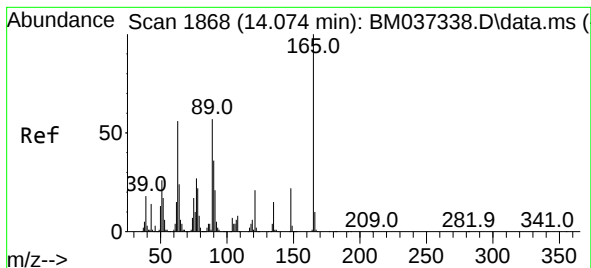

#48

2,6-Dinitrotoluene

Concen: 1.112 ng/ul

RT: 14.015 min Scan# 11

Delta R.T. -0.065 min

Lab File: BM037350.D


Acq: 03 Nov 2022 17:16

Instrument :

BNA_M

ClientSampleId :

EW4X2

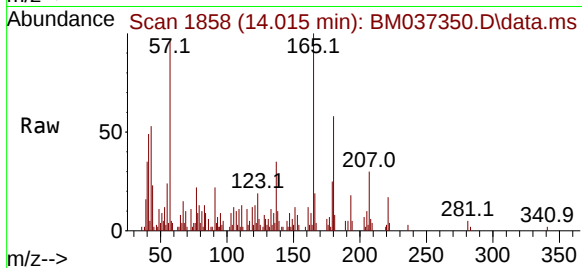

Tgt Ion:165 Resp: 13958

Ion Ratio Lower Upper

165 100

89 2.3 45.4 68.0#

121 12.6 17.0 25.6#

