

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037340.D
 Acq On : 03 Nov 2022 11:13
 Operator : CG/JU
 Sample : N5276-21
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	34	rBV	84297	106272	1.16%	0.124%
2	3.305	34	37	49	rVB	57133	85966	0.94%	0.100%
3	3.687	99	102	123	rBV	1033221	1587718	17.39%	1.848%
4	3.916	138	141	145	rVB2	14294	19007	0.21%	0.022%
5	3.952	145	147	152	rVB6	7707	10042	0.11%	0.012%
6	4.010	154	157	164	rVB	22691	32592	0.36%	0.038%
7	7.022	662	669	681	rBV	1343608	2143104	23.47%	2.494%
8	7.187	690	697	711	rBV	1165114	1780619	19.50%	2.072%
9	7.375	722	729	740	rBV	1345650	2156109	23.61%	2.510%
10	7.845	801	809	818	rBV	909513	1448269	15.86%	1.686%
11	8.563	925	931	949	rBV	1733005	2816351	30.84%	3.278%
12	9.016	1000	1008	1021	rBV	1346556	2164395	23.70%	2.519%
13	9.734	1122	1130	1146	rBV	1078639	1840534	20.16%	2.142%
14	10.275	1213	1222	1237	rBV	1697563	2832953	31.02%	3.297%
15	10.651	1276	1286	1294	rBV	1371608	2270885	24.87%	2.643%
16	10.798	1303	1311	1332	rBV	1573881	2947137	32.27%	3.430%
17	12.239	1551	1556	1565	rBV	23711	44926	0.49%	0.052%
18	12.822	1648	1655	1658	rBV6	5413	12751	0.14%	0.015%
19	13.904	1828	1839	1848	rBV	3348260	4447501	48.71%	5.176%
20	14.180	1879	1886	1898	rBV	3985886	5533209	60.60%	6.440%
21	14.486	1930	1938	1947	rBV	2160960	3202704	35.07%	3.728%
22	14.698	1968	1974	1996	rBV	1244489	2079581	22.77%	2.420%
23	14.910	2003	2010	2022	rVB6	34461	75444	0.83%	0.088%
24	15.474	2099	2106	2113	rBV	5350604	7224783	79.12%	8.409%
25	15.604	2122	2128	2142	rBV	1488992	2045852	22.40%	2.381%
26	15.715	2142	2147	2159	rVB2	25371	47770	0.52%	0.056%
27	16.680	2307	2311	2316	rBV7	8556	13278	0.15%	0.015%
28	17.221	2397	2403	2414	rBV	2642672	3727601	40.82%	4.339%
29	17.321	2414	2420	2435	rVV	5881484	7998888	87.60%	9.310%
30	19.180	2731	2736	2743	rBV2	66518	96754	1.06%	0.113%
31	19.251	2744	2748	2752	rVV	54789	73257	0.80%	0.085%
32	19.615	2804	2810	2820	rBV	6918714	9131343	100.00%	10.628%
33	21.397	3108	3113	3121	rBV	3166770	4020561	44.03%	4.680%
34	23.591	3479	3486	3499	rVB	4428222	8284159	90.72%	9.642%
35	23.744	3506	3512	3524	rVB2	1817020	3614944	39.59%	4.207%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037340.D
Acq On : 03 Nov 2022 11:13
Operator : CG/JU
Sample : N5276-21
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Title : SVOA CALIBRATION




Sum of corrected areas: 85917259

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037340.D
Acq On : 03 Nov 2022 11:13
Operator : CG/JU
Sample : N5276-21
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

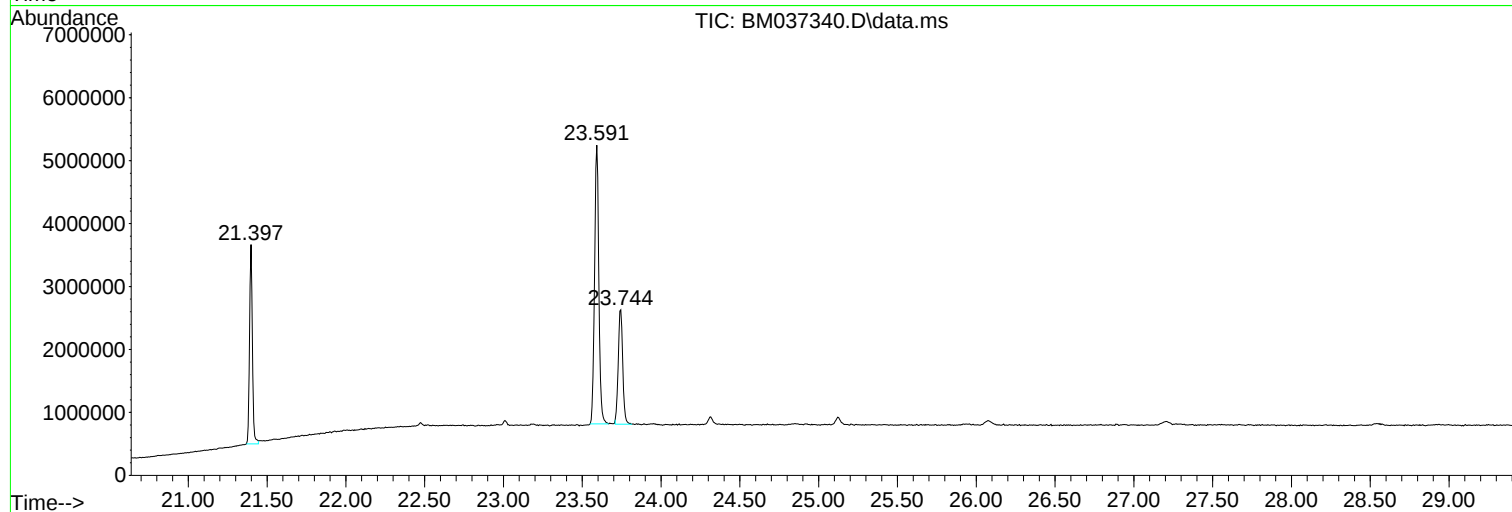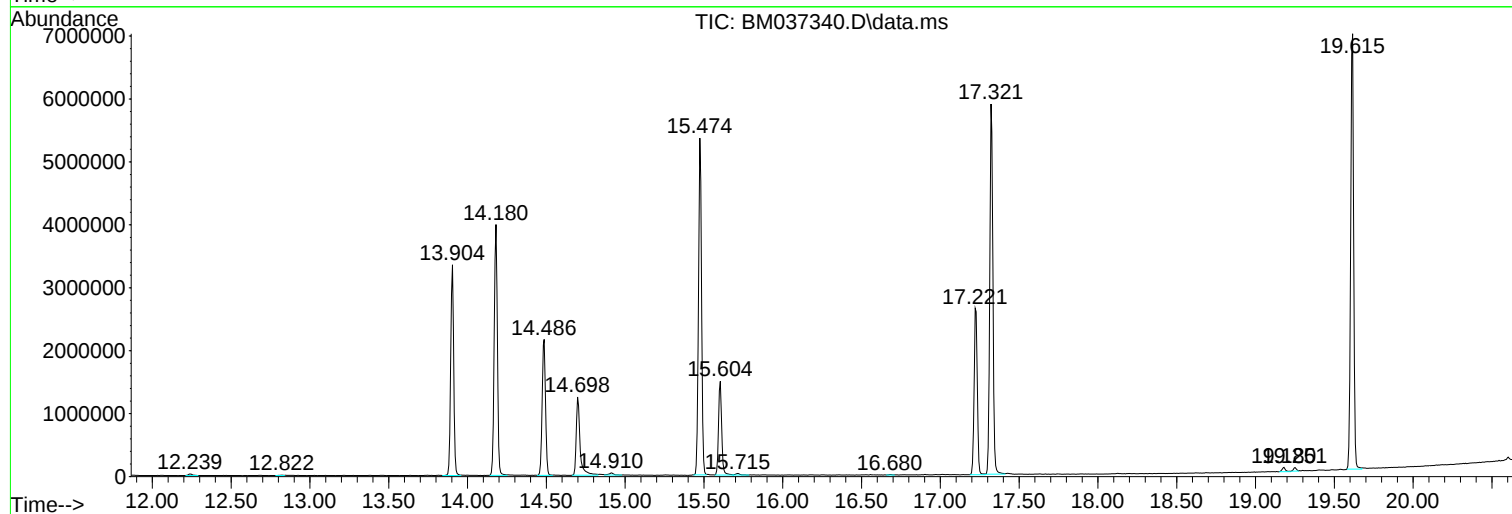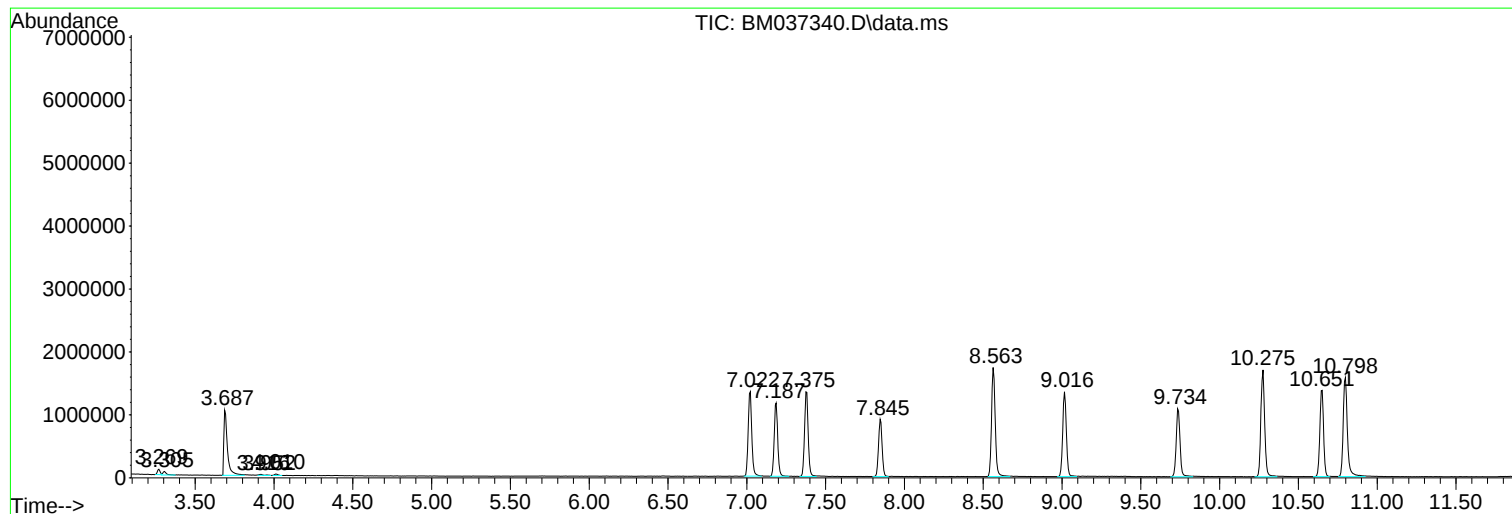

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037340.D
Acq On : 03 Nov 2022 11:13
Operator : CG/JU
Sample : N5276-21
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037340.D
Acq On : 03 Nov 2022 11:13
Operator : CG/JU
Sample : N5276-21
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc