

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037341.D
 Acq On : 03 Nov 2022 11:48
 Operator : CG/JU
 Sample : N5276-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	39	rVB	62071	88064	0.82%	0.098%
2	3.704	103	105	116	rBV	149933	258989	2.42%	0.290%
3	3.916	137	141	147	rVB	23287	35009	0.33%	0.039%
4	4.016	154	158	163	rVB2	20142	26689	0.25%	0.030%
5	4.963	314	319	325	rVB	15909	26021	0.24%	0.029%
6	5.904	473	479	483	rBV4	8241	14210	0.13%	0.016%
7	7.022	663	669	685	rVB	342083	585523	5.46%	0.655%
8	7.187	689	697	708	rBV	1349867	2110254	19.69%	2.360%
9	7.381	723	730	741	rBV	1257186	1977354	18.45%	2.211%
10	7.851	803	810	818	rBV	952294	1496173	13.96%	1.673%
11	7.910	818	820	827	rVB5	7427	12403	0.12%	0.014%
12	8.569	925	932	948	rBV	1024016	1686918	15.74%	1.887%
13	9.022	1001	1009	1025	rBV	1567938	2595759	24.22%	2.903%
14	9.145	1025	1030	1040	rVV2	15793	35764	0.33%	0.040%
15	9.404	1069	1074	1081	rVB2	15815	28846	0.27%	0.032%
16	9.739	1122	1131	1143	rBV	1219655	1985500	18.52%	2.220%
17	10.275	1215	1222	1237	rBV	1759444	2995652	27.95%	3.350%
18	10.439	1243	1250	1267	rBV	97956	243562	2.27%	0.272%
19	10.651	1278	1286	1294	rVB	1395948	2306156	21.51%	2.579%
20	10.798	1304	1311	1325	rBV	1428968	2426915	22.64%	2.714%
21	11.469	1420	1425	1437	rBV6	18428	53984	0.50%	0.060%
22	11.898	1492	1498	1504	rVB6	7941	16452	0.15%	0.018%
23	12.239	1550	1556	1564	rVB2	31489	56232	0.52%	0.063%
24	13.098	1697	1702	1708	rVB7	8042	12869	0.12%	0.014%
25	13.304	1729	1737	1743	rBV8	8653	15619	0.15%	0.017%
26	13.380	1746	1750	1755	rVV5	9822	14486	0.14%	0.016%
27	13.457	1759	1763	1767	rBV4	8276	13144	0.12%	0.015%
28	13.904	1829	1839	1853	rBV	3695031	5022175	46.85%	5.616%
29	14.051	1861	1864	1867	rBV4	9306	13181	0.12%	0.015%
30	14.180	1879	1886	1904	rBV	4685354	6481324	60.47%	7.248%
31	14.486	1927	1938	1947	rBV	2305616	3264505	30.46%	3.651%
32	14.704	1970	1975	1990	rBV	195782	449599	4.19%	0.503%
33	14.910	2005	2010	2017	rVB9	14279	38253	0.36%	0.043%
34	15.063	2029	2036	2049	rBV4	15425	52327	0.49%	0.059%
35	15.274	2067	2072	2075	rBV2	17165	28291	0.26%	0.032%
36	15.321	2075	2080	2084	rVB4	11173	21246	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037341.D
 Acq On : 03 Nov 2022 11:48
 Operator : CG/JU
 Sample : N5276-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	15.474	2095	2106	2118	rBV	6063135	8495279	79.25%	9.501%
38	15.604	2122	2128	2140	rVV	1740957	2357282	21.99%	2.636%
39	15.715	2142	2147	2152	rVB	27067	47176	0.44%	0.053%
40	15.933	2179	2184	2190	rVB9	10790	19188	0.18%	0.021%
41	16.180	2223	2226	2233	rVV4	11813	16949	0.16%	0.019%
42	16.251	2235	2238	2245	rVB3	15216	22987	0.21%	0.026%
43	16.974	2357	2361	2365	rBV2	28754	37663	0.35%	0.042%
44	17.021	2365	2369	2376	rVB8	12011	28810	0.27%	0.032%
45	17.139	2386	2389	2393	rVB5	13347	15792	0.15%	0.018%
46	17.227	2397	2404	2414	rBV	2654164	3741501	34.91%	4.184%
47	17.327	2414	2421	2432	rBV	6358181	9236425	86.17%	10.329%
48	17.715	2483	2487	2490	rBV	30184	36353	0.34%	0.041%
49	17.892	2513	2517	2522	rVB	56936	66423	0.62%	0.074%
50	18.115	2551	2555	2565	rBV	167946	278903	2.60%	0.312%
51	18.403	2601	2604	2610	rBV	36625	44456	0.41%	0.050%
52	19.180	2732	2736	2742	rBV2	75948	121564	1.13%	0.136%
53	19.250	2744	2748	2754	rBV	74524	117968	1.10%	0.132%
54	19.392	2768	2772	2780	rBV	132876	213710	1.99%	0.239%
55	19.615	2804	2810	2822	rBV	8402883	10718936	100.00%	11.987%
56	21.115	3061	3065	3071	rBV2	199451	344261	3.21%	0.385%
57	21.397	3108	3113	3123	rBV	3346669	4032988	37.62%	4.510%
58	23.591	3479	3486	3500	rVB2	5065940	9334752	87.09%	10.439%
59	23.744	3506	3512	3523	rVB2	1925469	3600185	33.59%	4.026%




Sum of corrected areas: 89418999

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037341.D
Acq On : 03 Nov 2022 11:48
Operator : CG/JU
Sample : N5276-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Y0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

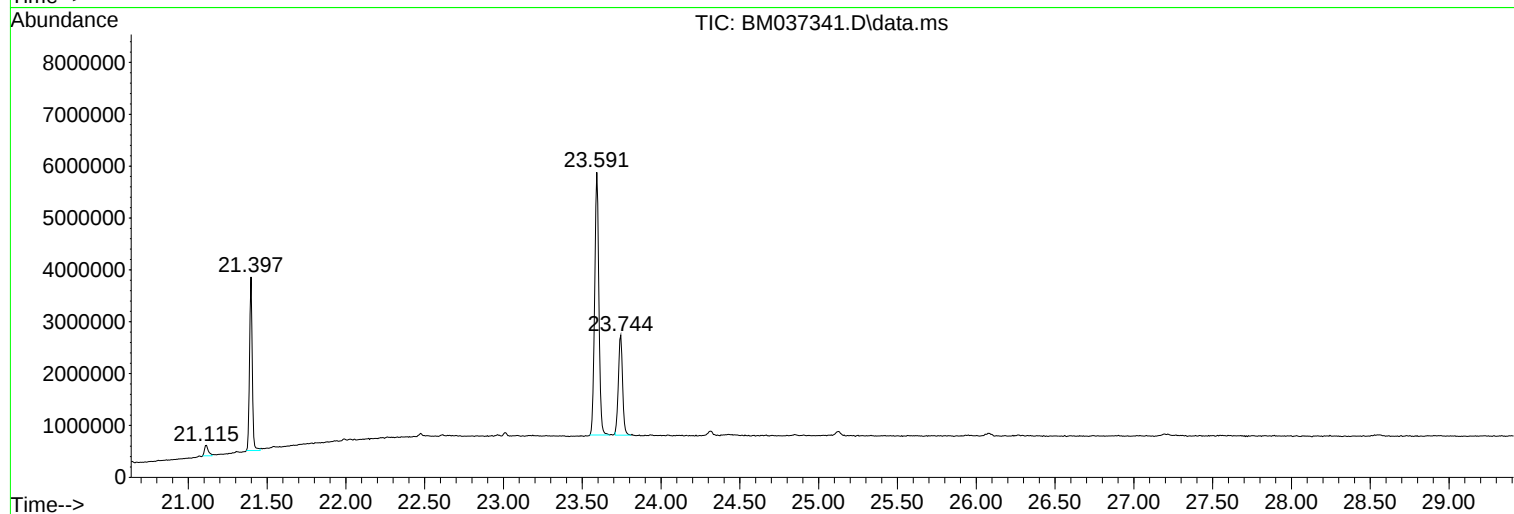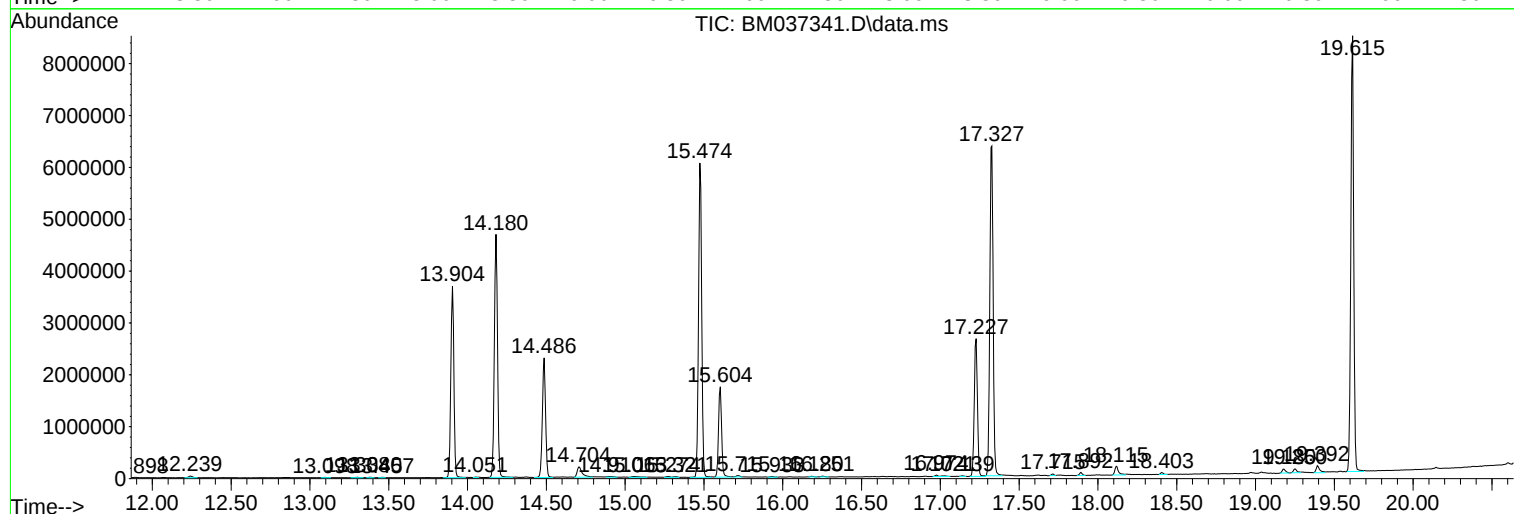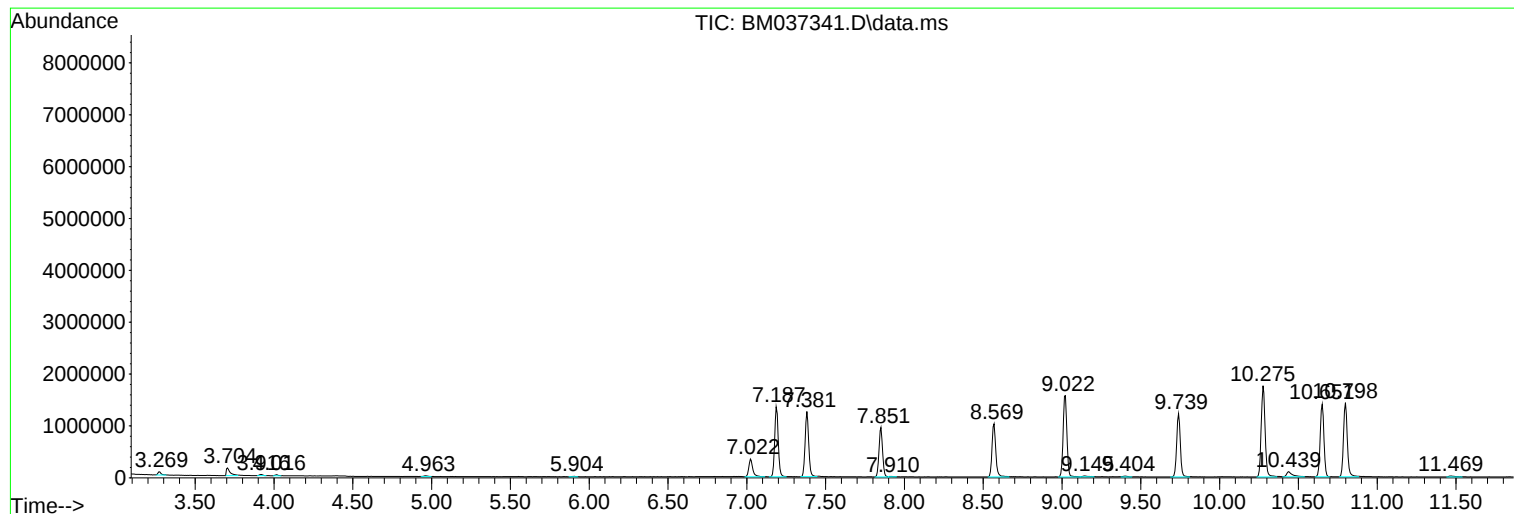

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037341.D
Acq On : 03 Nov 2022 11:48
Operator : CG/JU
Sample : N5276-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Y0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.439	2.11 ng/ul	243562	Naphthalene-d8	10.651

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	64
5			Di-sec-Butyl ether	130	C8H18O	006863-58-7	50

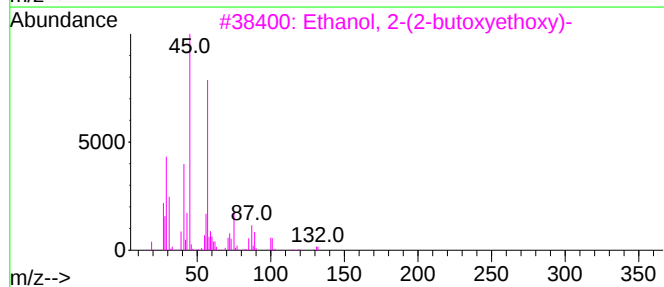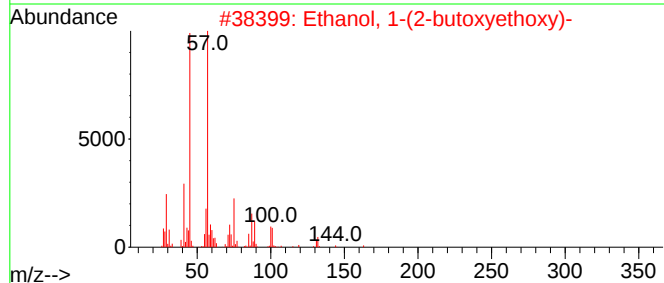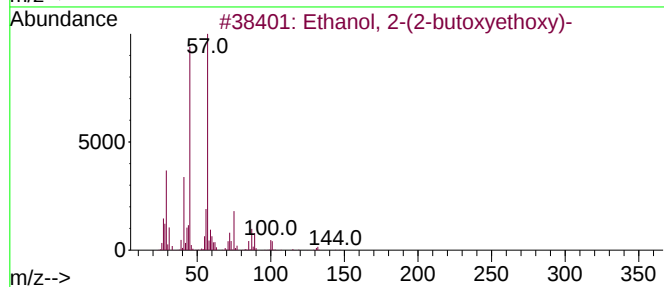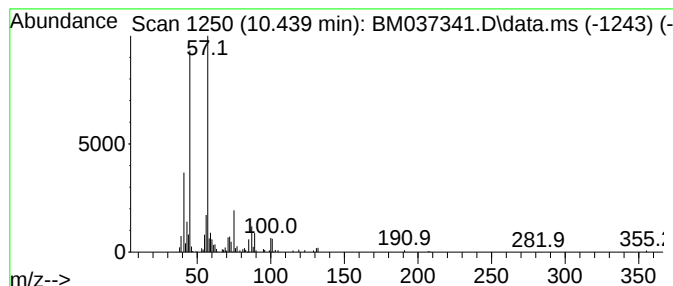

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037341.D
Acq On : 03 Nov 2022 11:48
Operator : CG/JU
Sample : N5276-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Y0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.439	2.1	ng/u1	243562	2	10.651	2306160	20.0