

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037346.D
 Acq On : 03 Nov 2022 14:49
 Operator : CG/JU
 Sample : PB148645BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK645

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	40	rVB	101989	131256	1.48%	0.144%
2	3.693	99	103	125	rBV	1182055	1767297	19.94%	1.945%
3	4.016	154	158	164	rVB	20160	26445	0.30%	0.029%
4	7.022	662	669	685	rBV	1393345	2261036	25.51%	2.489%
5	7.187	691	697	710	rBV	1197307	1864143	21.04%	2.052%
6	7.381	723	730	744	rBV	1472699	2312939	26.10%	2.546%
7	7.851	803	810	821	rBV	1267912	1967476	22.20%	2.166%
8	8.569	925	932	944	rBV	1803824	2885752	32.56%	3.176%
9	9.022	1000	1009	1022	rBV	1420122	2302347	25.98%	2.534%
10	9.739	1122	1131	1148	rBV	1156735	1911695	21.57%	2.104%
11	10.281	1214	1223	1249	rBV	1698766	2992438	33.77%	3.294%
12	10.651	1278	1286	1297	rBV	1871149	3077952	34.73%	3.388%
13	10.798	1304	1311	1332	rBV	1755803	3077191	34.72%	3.387%
14	12.245	1552	1557	1568	rVB2	24303	52630	0.59%	0.058%
15	13.463	1758	1764	1770	rVB6	7523	13436	0.15%	0.015%
16	13.904	1833	1839	1852	rBV	3163641	4336876	48.94%	4.774%
17	14.180	1878	1886	1897	rBV	3937666	5634298	63.58%	6.202%
18	14.486	1931	1938	1947	rBV	3028559	4332341	48.89%	4.769%
19	14.704	1968	1975	1996	rBV	1175569	2095918	23.65%	2.307%
20	14.898	2005	2008	2015	rVB9	9083	15738	0.18%	0.017%
21	15.480	2100	2107	2122	rBV	5150393	7194576	81.19%	7.919%
22	15.604	2122	2128	2142	rVV	1467852	1996344	22.53%	2.197%
23	15.715	2142	2147	2154	rVB2	27667	45519	0.51%	0.050%
24	16.515	2278	2283	2286	rBV6	4412	9382	0.11%	0.010%
25	16.909	2346	2350	2354	rBV7	5892	10478	0.12%	0.012%
26	17.227	2398	2404	2414	rBV	3719155	5013303	56.57%	5.518%
27	17.327	2414	2421	2440	rVV	5798235	7868551	88.79%	8.661%
28	19.180	2732	2736	2742	rBV2	62865	87126	0.98%	0.096%
29	19.251	2744	2748	2754	rVV	51196	77795	0.88%	0.086%
30	19.615	2804	2810	2819	rBV	6726112	8861708	100.00%	9.754%
31	21.397	3108	3113	3121	rBV	4181110	5216459	58.87%	5.742%
32	23.597	3480	3487	3497	rVB2	3619280	6990997	78.89%	7.695%
33	23.750	3506	3513	3528	rVB2	2212814	4421508	49.89%	4.867%




Sum of corrected areas: 90852950

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037346.D
Acq On : 03 Nov 2022 14:49
Operator : CG/JU
Sample : PB148645BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK645

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

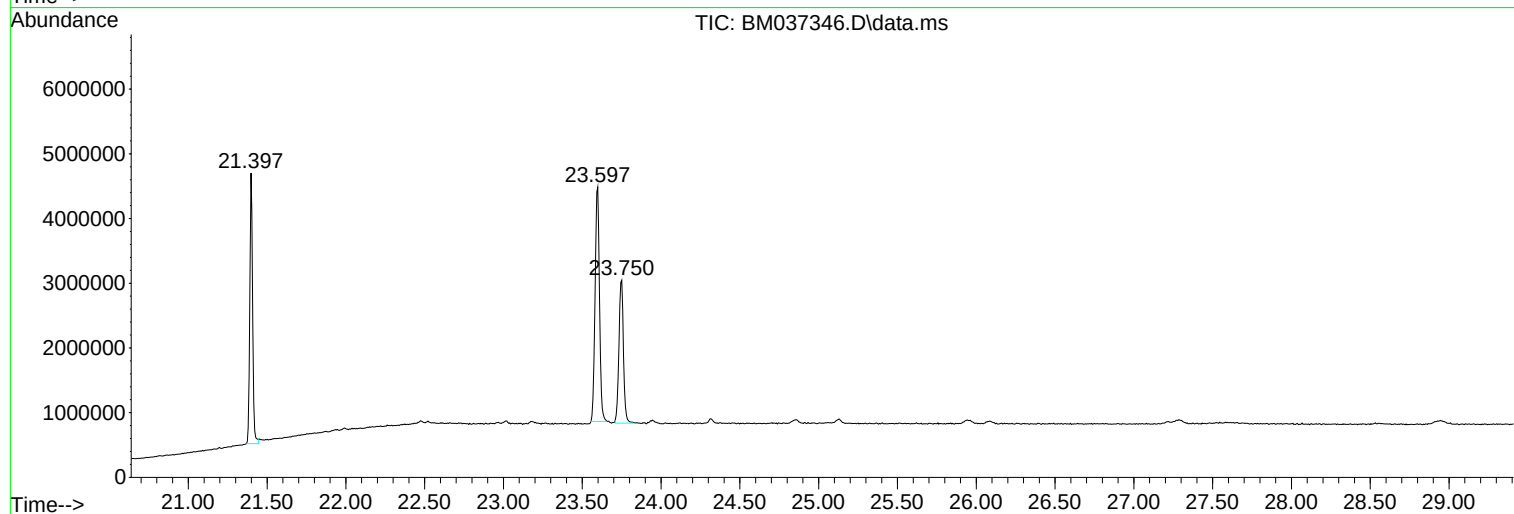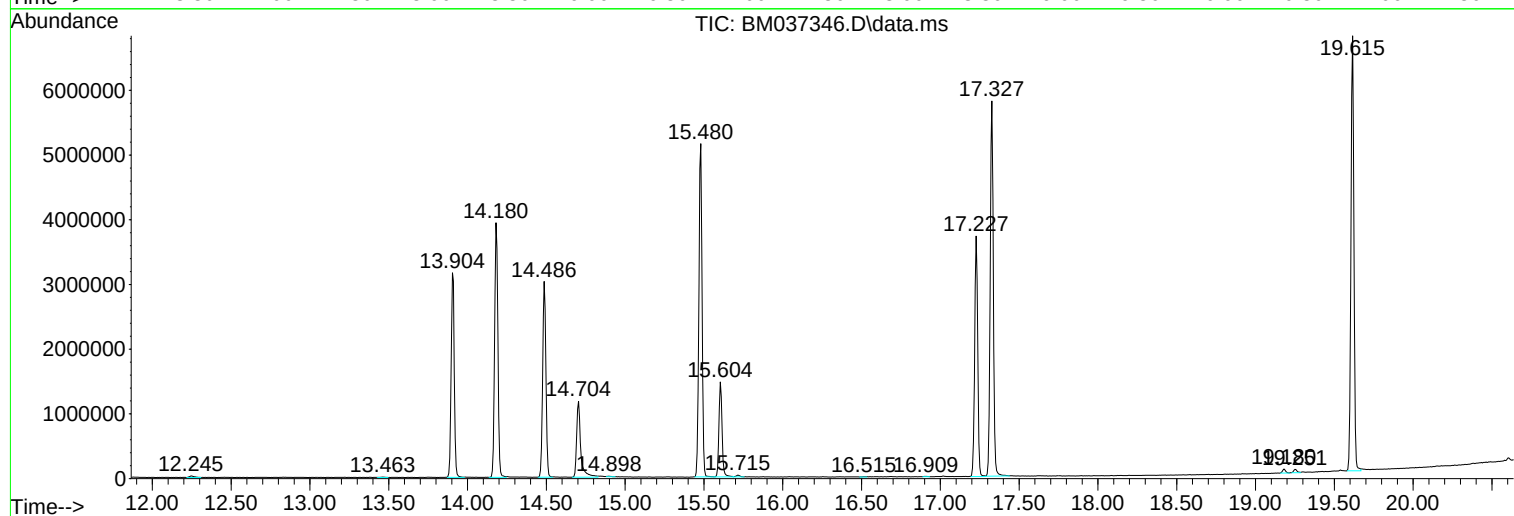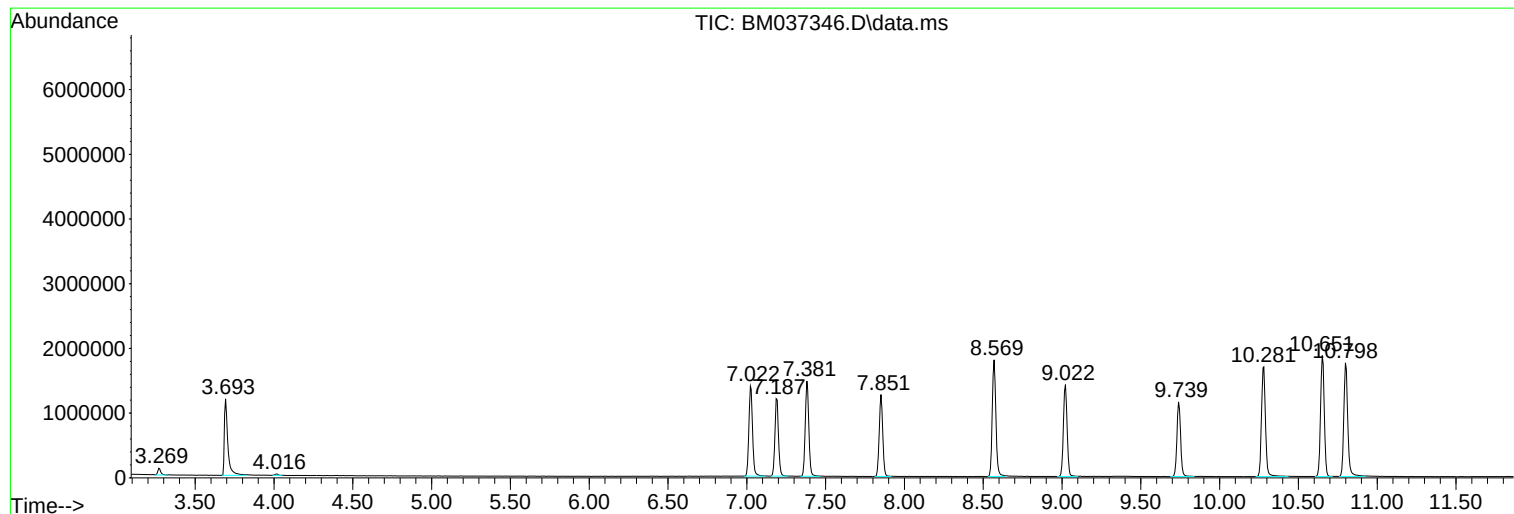

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037346.D
Acq On : 03 Nov 2022 14:49
Operator : CG/JU
Sample : PB148645BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK645

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037346.D
Acq On : 03 Nov 2022 14:49
Operator : CG/JU
Sample : PB148645BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK645

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc