

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037347.D
 Acq On : 03 Nov 2022 15:25
 Operator : CG/JU
 Sample : PB148651BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	43	rVB	98606	142482	1.60%	0.161%
2	3.693	99	103	123	rBV	1145550	1735810	19.54%	1.962%
3	4.016	154	158	163	rVB	19685	26417	0.30%	0.030%
4	7.022	663	669	686	rBV	1359671	2198501	24.75%	2.485%
5	7.193	691	698	710	rVB	1164027	1825506	20.55%	2.063%
6	7.381	721	730	741	rBV	1432175	2255162	25.39%	2.549%
7	7.851	804	810	820	rBV	1128917	1741847	19.61%	1.969%
8	8.569	925	932	948	rBV	1706021	2778521	31.29%	3.140%
9	9.022	1000	1009	1024	rBV	1395309	2222996	25.03%	2.513%
10	9.739	1124	1131	1141	rBV	1105914	1810595	20.39%	2.046%
11	10.281	1214	1223	1238	rBV	1641183	2825293	31.81%	3.193%
12	10.651	1279	1286	1295	rBV	1616841	2698575	30.39%	3.050%
13	10.798	1305	1311	1329	rBV	1636366	2958016	33.31%	3.343%
14	12.251	1551	1558	1568	rBV3	21403	44879	0.51%	0.051%
15	12.839	1651	1658	1662	rBV10	3938	9286	0.10%	0.010%
16	13.904	1832	1839	1852	rBV	3078676	4135745	46.57%	4.674%
17	14.180	1878	1886	1902	rBV	3650797	5364495	60.40%	6.063%
18	14.486	1931	1938	1949	rBV	2738107	3805553	42.85%	4.301%
19	14.704	1968	1975	1999	rBV	1188589	2095234	23.59%	2.368%
20	15.480	2094	2107	2120	rBV	4945788	6906153	77.76%	7.806%
21	15.604	2122	2128	2143	rVV	1417978	1968010	22.16%	2.224%
22	15.716	2143	2147	2153	rVB3	23261	37948	0.43%	0.043%
23	16.257	2234	2239	2243	rBV7	7075	13092	0.15%	0.015%
24	16.910	2344	2350	2352	rBV6	7351	11473	0.13%	0.013%
25	17.010	2364	2367	2373	rBV6	7116	14146	0.16%	0.016%
26	17.227	2397	2404	2414	rBV	3289469	4473886	50.37%	5.057%
27	17.327	2414	2421	2435	rVV	5535208	7595988	85.53%	8.585%
28	19.180	2732	2736	2743	rBV	66770	91641	1.03%	0.104%
29	19.251	2744	2748	2754	rBV	53228	80439	0.91%	0.091%
30	19.615	2804	2810	2819	rBV	7083255	8881184	100.00%	10.038%
31	21.398	3108	3113	3123	rBV	4006992	5009612	56.41%	5.662%
32	23.597	3480	3487	3501	rVB2	4196732	8179821	92.10%	9.245%
33	23.744	3506	3512	3523	rVB2	2295592	4536318	51.08%	5.127%




Sum of corrected areas: 88474624

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037347.D
Acq On : 03 Nov 2022 15:25
Operator : CG/JU
Sample : PB148651BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

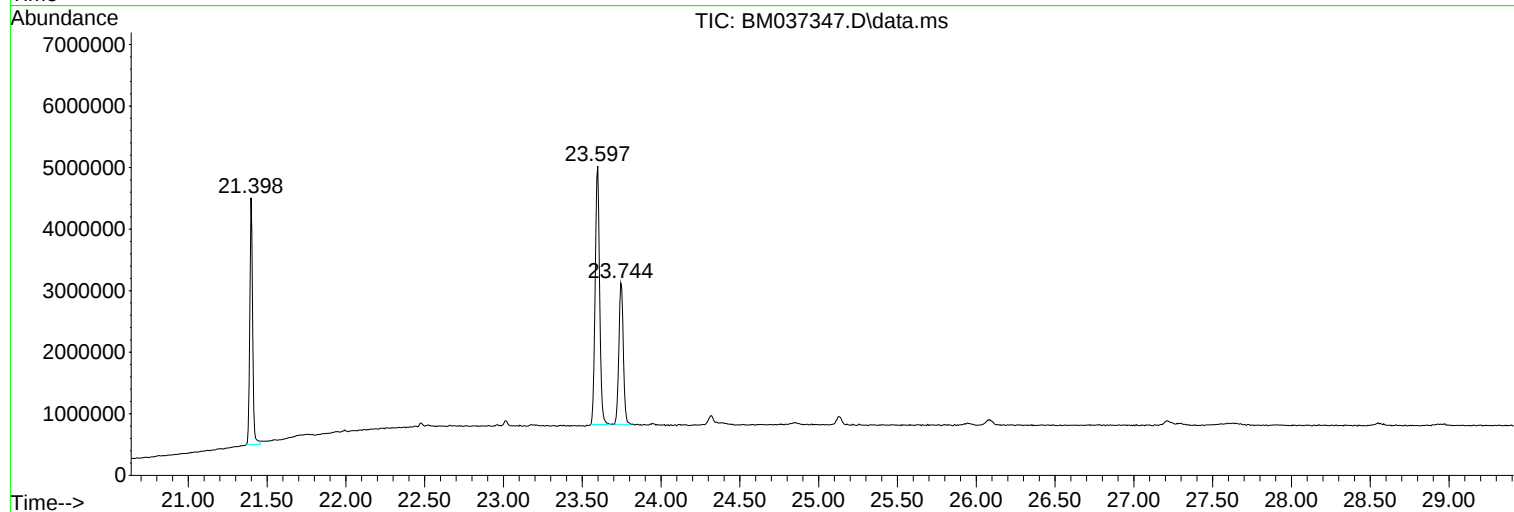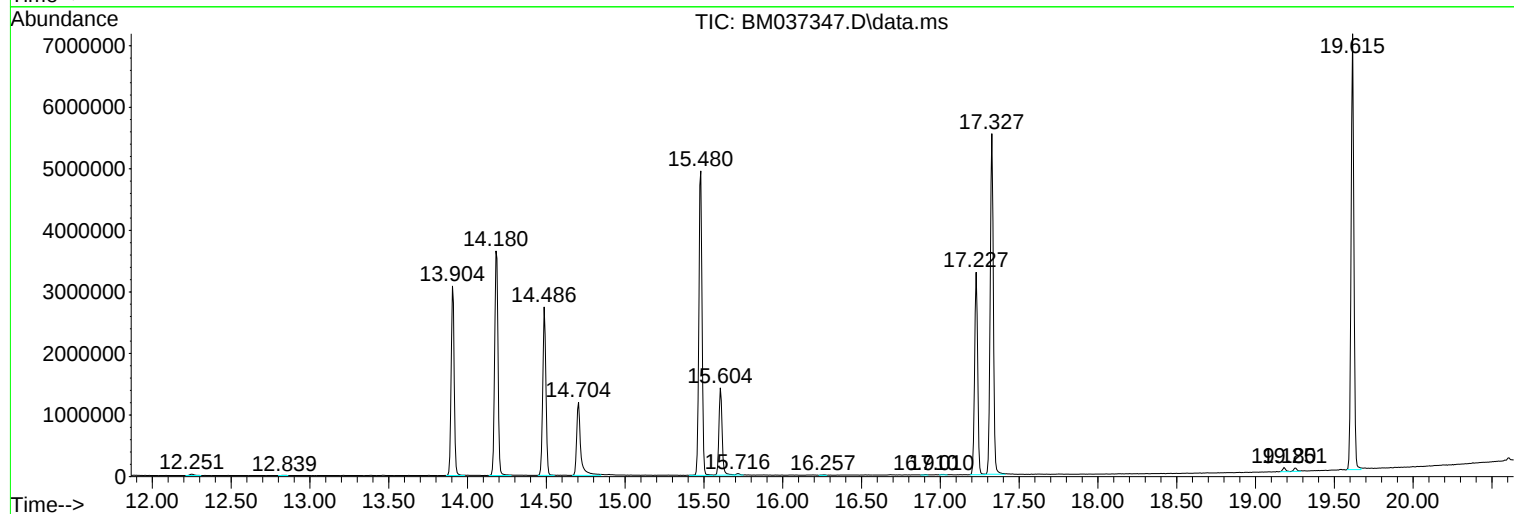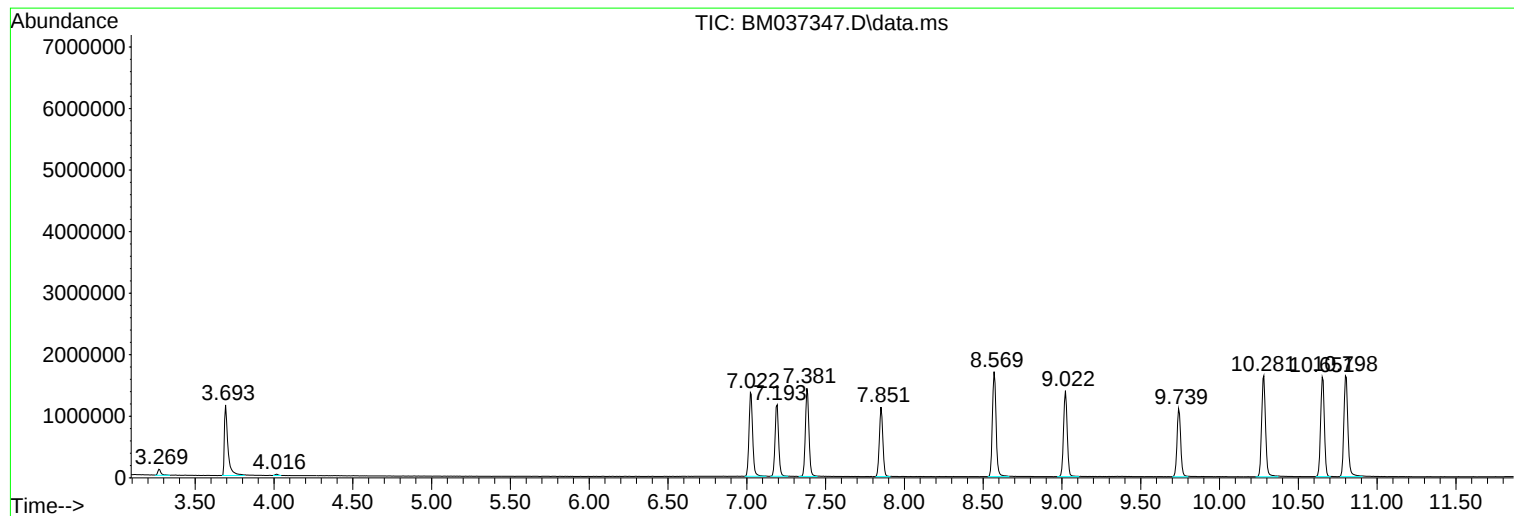

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037347.D
Acq On : 03 Nov 2022 15:25
Operator : CG/JU
Sample : PB148651BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037347.D
Acq On : 03 Nov 2022 15:25
Operator : CG/JU
Sample : PB148651BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc