

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037349.D
 Acq On : 03 Nov 2022 16:39
 Operator : CG/JU
 Sample : N5276-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rBV	56947	69987	0.74%	0.088%
2	3.563	77	81	87	rBV	45963	74868	0.79%	0.095%
3	3.922	138	142	147	rVB	22174	33799	0.36%	0.043%
4	4.016	154	158	165	rVB	35450	46856	0.50%	0.059%
5	4.428	227	228	237	rVB4	7340	12026	0.13%	0.015%
6	4.963	316	319	325	rVB	15952	25896	0.27%	0.033%
7	7.028	664	670	686	rVB	280895	480301	5.08%	0.607%
8	7.192	691	698	707	rBV	1127257	1757383	18.60%	2.221%
9	7.387	723	731	741	rBV	1033661	1695232	17.94%	2.142%
10	7.851	803	810	819	rBV	1136408	1695760	17.95%	2.143%
11	8.569	925	932	948	rBV	860245	1431041	15.15%	1.808%
12	9.022	1001	1009	1020	rBV	1350382	2193780	23.22%	2.772%
13	9.739	1124	1131	1147	rBV	1023399	1720253	18.21%	2.174%
14	10.280	1214	1223	1246	rBV	1467055	2605449	27.58%	3.293%
15	10.651	1277	1286	1301	rBV	1637636	2699155	28.57%	3.411%
16	10.816	1306	1314	1323	rBV	50021	117228	1.24%	0.148%
17	11.892	1491	1497	1504	rVB9	5882	13811	0.15%	0.017%
18	12.245	1551	1557	1565	rBV2	23240	48151	0.51%	0.061%
19	12.839	1653	1658	1664	rBV8	8230	17093	0.18%	0.022%
20	13.098	1698	1702	1712	rVB8	9778	16727	0.18%	0.021%
21	13.457	1757	1763	1770	rVV5	6982	14208	0.15%	0.018%
22	13.904	1831	1839	1852	rBV	3110347	4417715	46.76%	5.583%
23	14.186	1878	1887	1901	rBV	3721883	5482253	58.03%	6.928%
24	14.486	1931	1938	1949	rBV	2642868	3774205	39.95%	4.770%
25	14.715	1970	1977	1996	rBV	163024	396808	4.20%	0.501%
26	14.904	2003	2009	2012	rBV8	11274	18923	0.20%	0.024%
27	15.057	2029	2035	2041	rBV6	8640	25238	0.27%	0.032%
28	15.274	2068	2072	2076	rBV3	9951	13120	0.14%	0.017%
29	15.480	2097	2107	2116	rBV	5349339	7306978	77.35%	9.234%
30	15.604	2122	2128	2141	rBV	1644408	2184231	23.12%	2.760%
31	15.715	2143	2147	2153	rVB2	24470	38814	0.41%	0.049%
32	16.186	2225	2227	2233	rVB6	8859	11141	0.12%	0.014%
33	16.257	2235	2239	2245	rBV8	8972	15401	0.16%	0.019%
34	16.680	2309	2311	2317	rVB4	7403	9495	0.10%	0.012%
35	16.739	2317	2321	2331	rBV4	12382	34538	0.37%	0.044%
36	17.009	2365	2367	2373	rVB4	8392	13847	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037349.D
 Acq On : 03 Nov 2022 16:39
 Operator : CG/JU
 Sample : N5276-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	17.227	2398	2404	2414	rBV	3194310	4392690	46.50%	5.551%
38	17.327	2414	2421	2441	rVV	6199193	8327052	88.15%	10.523%
39	17.898	2514	2518	2523	rBV3	22423	35980	0.38%	0.045%
40	18.121	2551	2556	2565	rBV	188103	310798	3.29%	0.393%
41	19.180	2732	2736	2741	rVB2	66712	94132	1.00%	0.119%
42	19.250	2744	2748	2752	rBV	80901	118893	1.26%	0.150%
43	19.392	2769	2772	2780	rBV	127523	203457	2.15%	0.257%
44	19.615	2804	2810	2820	rBV	7312298	9446825	100.00%	11.938%
45	21.115	3062	3065	3073	rBV4	143397	228260	2.42%	0.288%
46	21.397	3109	3113	3121	rBV	3419757	4377272	46.34%	5.532%
47	23.597	3480	3487	3500	rVB2	3939199	7362598	77.94%	9.304%
48	23.750	3507	3513	3527	rVB2	1905628	3722016	39.40%	4.704%




Sum of corrected areas: 79131684

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037349.D
Acq On : 03 Nov 2022 16:39
Operator : CG/JU
Sample : N5276-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

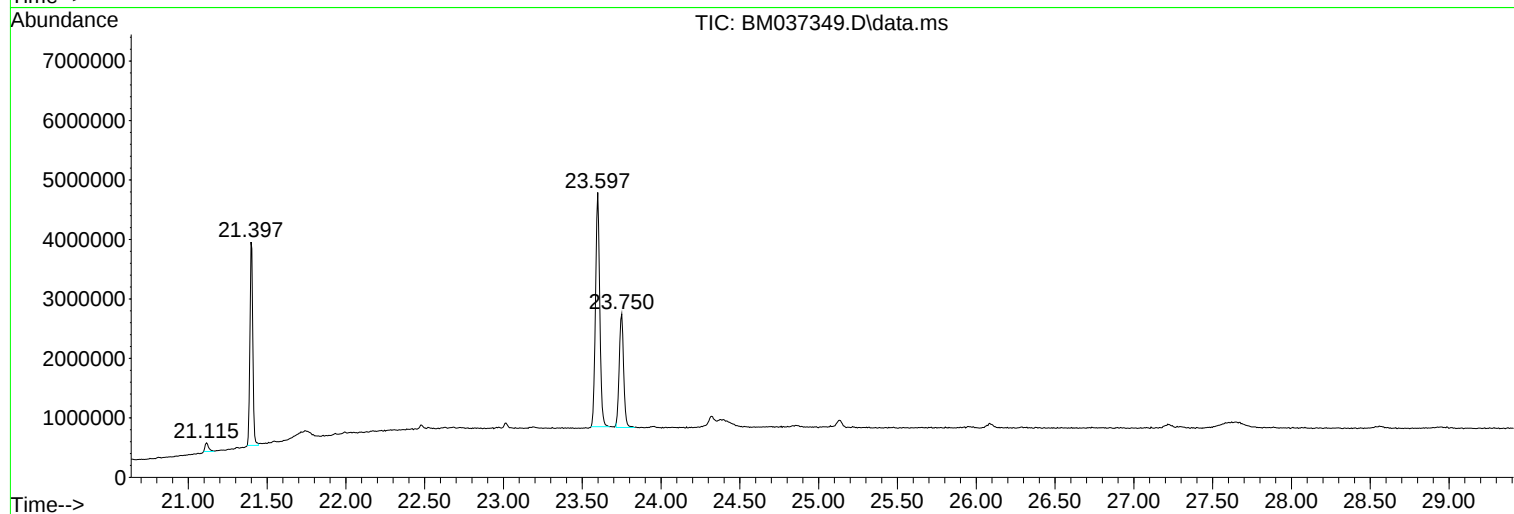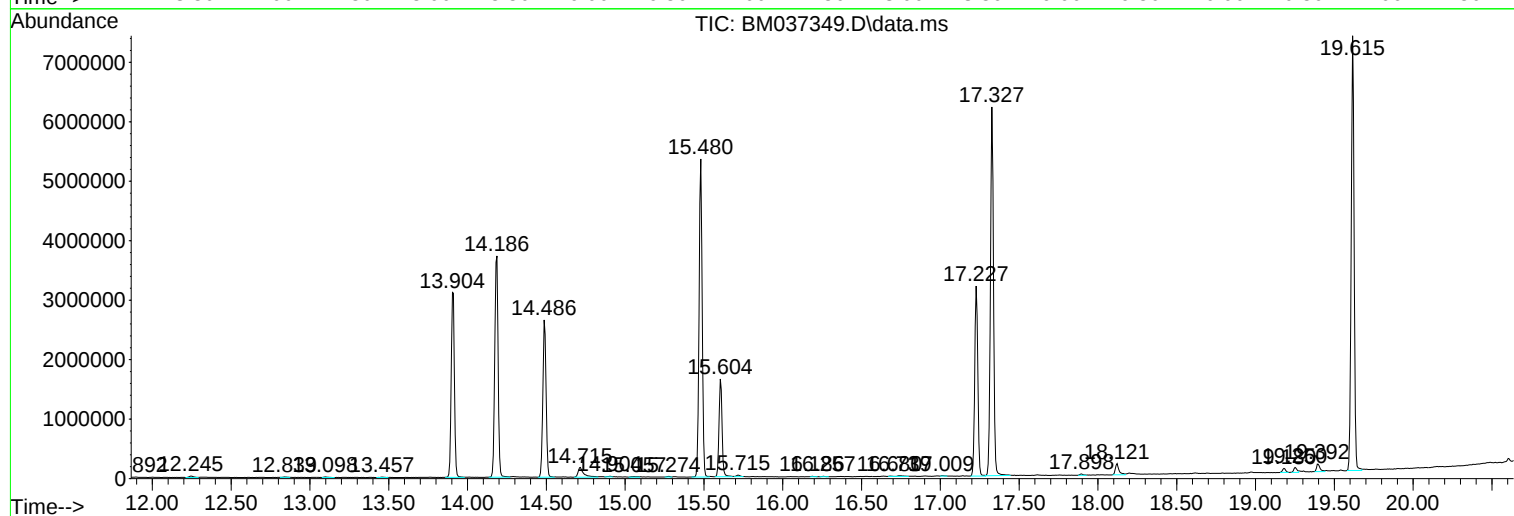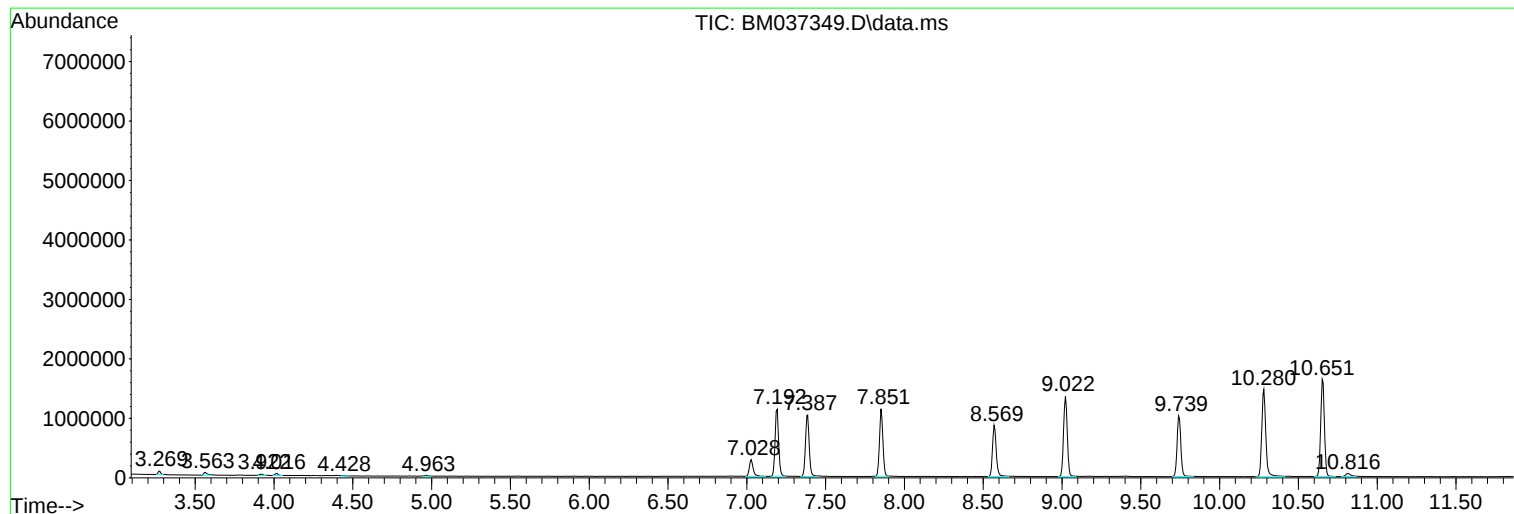

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037349.D
Acq On : 03 Nov 2022 16:39
Operator : CG/JU
Sample : N5276-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037349.D
Acq On : 03 Nov 2022 16:39
Operator : CG/JU
Sample : N5276-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc