

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037350.D
 Acq On : 03 Nov 2022 17:16
 Operator : CG/JU
 Sample : N5276-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rBV	48698	62496	0.63%	0.077%
2	3.916	136	141	148	rVB	19550	33596	0.34%	0.041%
3	4.016	154	158	166	rVB	30739	46157	0.47%	0.057%
4	4.963	315	319	327	rVB	22455	34869	0.35%	0.043%
5	7.028	664	670	680	rBV	268214	450873	4.56%	0.556%
6	7.192	691	698	709	rBV	1108807	1741735	17.62%	2.150%
7	7.381	724	730	741	rBV	1032268	1646468	16.65%	2.032%
8	7.851	802	810	818	rBV	1096021	1729838	17.50%	2.135%
9	7.922	818	822	832	rVB5	11214	25967	0.26%	0.032%
10	8.569	926	932	950	rBV	813456	1359596	13.75%	1.678%
11	9.022	1001	1009	1024	rBV	1349769	2166657	21.91%	2.674%
12	9.151	1026	1031	1033	rVV6	5520	11095	0.11%	0.014%
13	9.181	1033	1036	1041	rVB6	15116	21496	0.22%	0.027%
14	9.404	1070	1074	1079	rVB6	7419	13279	0.13%	0.016%
15	9.739	1124	1131	1146	rBV	1004039	1672707	16.92%	2.065%
16	10.022	1174	1179	1184	rBV9	4509	11873	0.12%	0.015%
17	10.280	1215	1223	1243	rBV	1369366	2469087	24.97%	3.047%
18	10.651	1275	1286	1302	rBV	1607079	2719582	27.51%	3.357%
19	10.822	1311	1315	1323	rVB5	10062	22378	0.23%	0.028%
20	11.257	1385	1389	1393	rBV6	7521	12013	0.12%	0.015%
21	11.463	1420	1424	1437	rBV2	33308	93786	0.95%	0.116%
22	12.245	1551	1557	1565	rVB	27214	48996	0.50%	0.060%
23	13.468	1759	1765	1771	rBV7	7220	13710	0.14%	0.017%
24	13.904	1831	1839	1851	rBV	3117486	4292413	43.41%	5.298%
25	14.015	1853	1858	1868	rVB2	104658	150246	1.52%	0.185%
26	14.180	1876	1886	1904	rBV	3708601	5433107	54.95%	6.706%
27	14.486	1931	1938	1949	rBV	2671180	3830712	38.74%	4.728%
28	14.615	1957	1960	1967	rVB8	8994	14856	0.15%	0.018%
29	14.710	1970	1976	1994	rBV	163380	397469	4.02%	0.491%
30	14.904	2005	2009	2011	rBV5	6850	10961	0.11%	0.014%
31	15.239	2062	2066	2069	rVV2	16431	24744	0.25%	0.031%
32	15.274	2069	2072	2077	rVB	16103	20966	0.21%	0.026%
33	15.480	2100	2107	2115	rBV	5245967	7249126	73.32%	8.947%
34	15.604	2122	2128	2142	rBV	1611193	2139852	21.64%	2.641%
35	15.715	2143	2147	2153	rVB	22954	39361	0.40%	0.049%
36	15.962	2186	2189	2193	rVB6	9302	11923	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037350.D
 Acq On : 03 Nov 2022 17:16
 Operator : CG/JU
 Sample : N5276-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	16.256	2236	2239	2246	rVB8	6185	10050	0.10%	0.012%
38	16.686	2309	2312	2318	rVB6	6564	12296	0.12%	0.015%
39	16.904	2345	2349	2355	rVB9	6072	11641	0.12%	0.014%
40	17.015	2365	2368	2373	rVB6	6029	10191	0.10%	0.013%
41	17.227	2398	2404	2412	rBV	3392067	4458348	45.09%	5.503%
42	17.327	2414	2421	2437	rVV	6129168	8536071	86.33%	10.536%
43	17.621	2467	2471	2473	rBV5	6918	10103	0.10%	0.012%
44	17.892	2514	2517	2523	rVB6	22766	29786	0.30%	0.037%
45	18.115	2552	2555	2561	rBV4	41053	66918	0.68%	0.083%
46	18.974	2697	2701	2706	rBV2	50736	64333	0.65%	0.079%
47	19.180	2732	2736	2742	rBV	62109	90204	0.91%	0.111%
48	19.250	2744	2748	2754	rBV	65414	115722	1.17%	0.143%
49	19.397	2770	2773	2779	rBV6	32797	52441	0.53%	0.065%
50	19.615	2804	2810	2825	rBV	8007136	9887166	100.00%	12.203%
51	20.950	3034	3037	3041	rBV	89948	105184	1.06%	0.130%
52	21.074	3055	3058	3061	rBV	141661	145885	1.48%	0.180%
53	21.403	3109	3114	3123	rBV	3696580	4746087	48.00%	5.858%
54	23.597	3480	3487	3500	rVB2	4321061	8421533	85.18%	10.394%
55	23.744	3506	3512	3524	rVB2	2138173	4222250	42.70%	5.211%




Sum of corrected areas: 81020199

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037350.D
Acq On : 03 Nov 2022 17:16
Operator : CG/JU
Sample : N5276-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

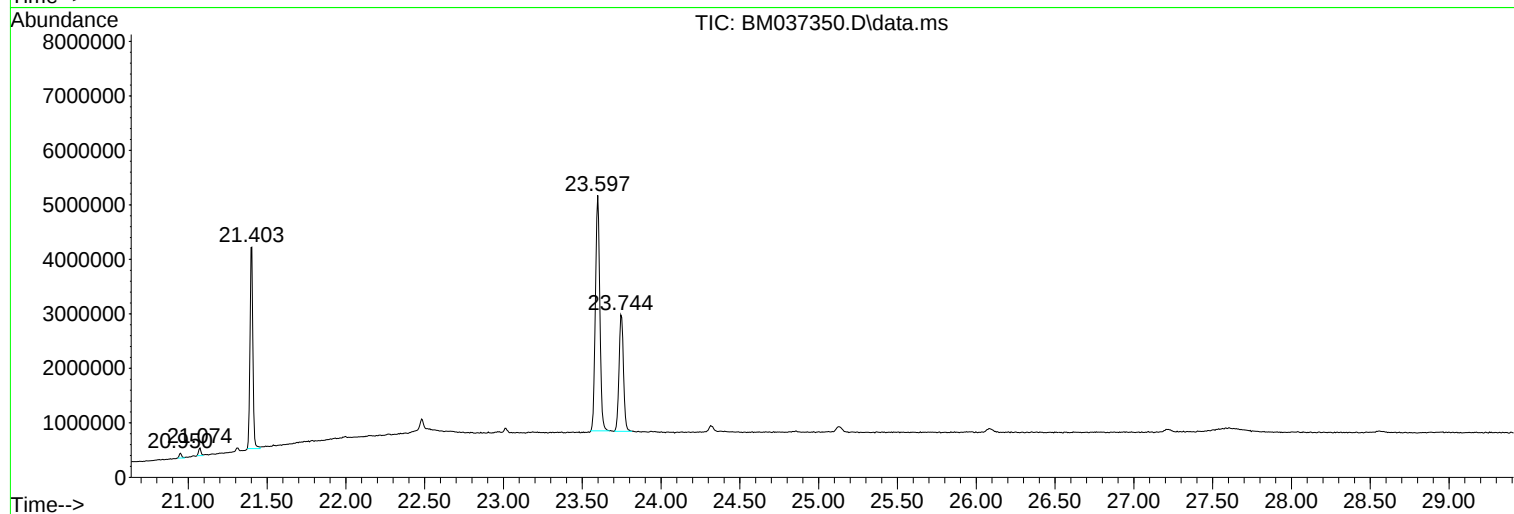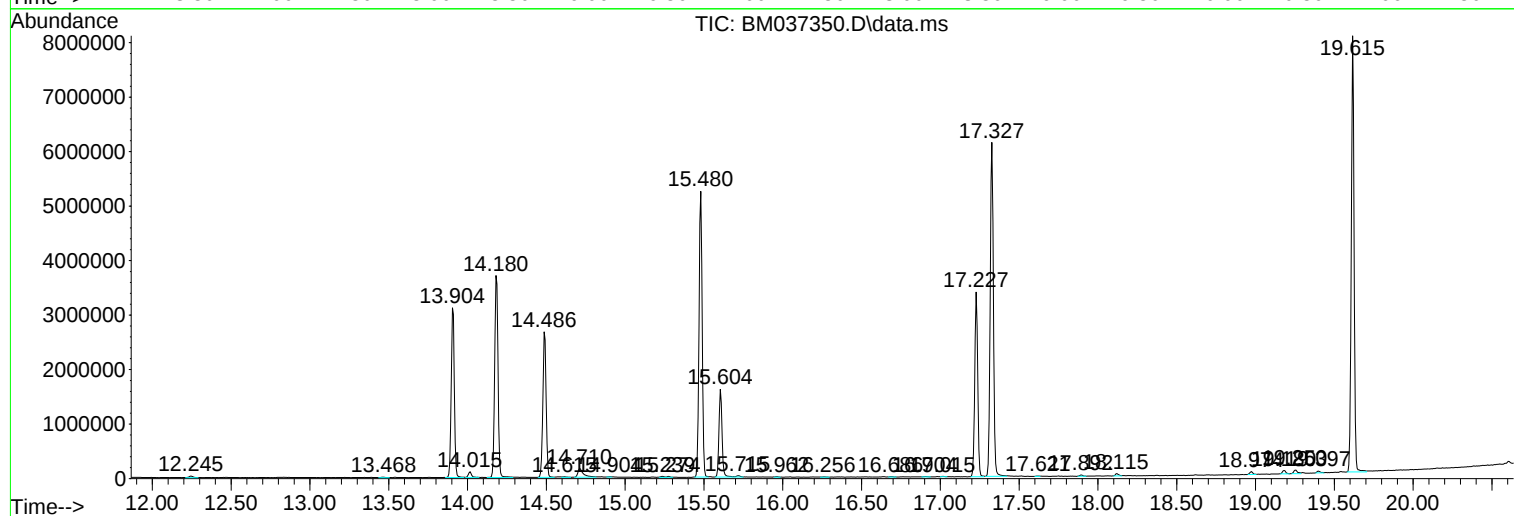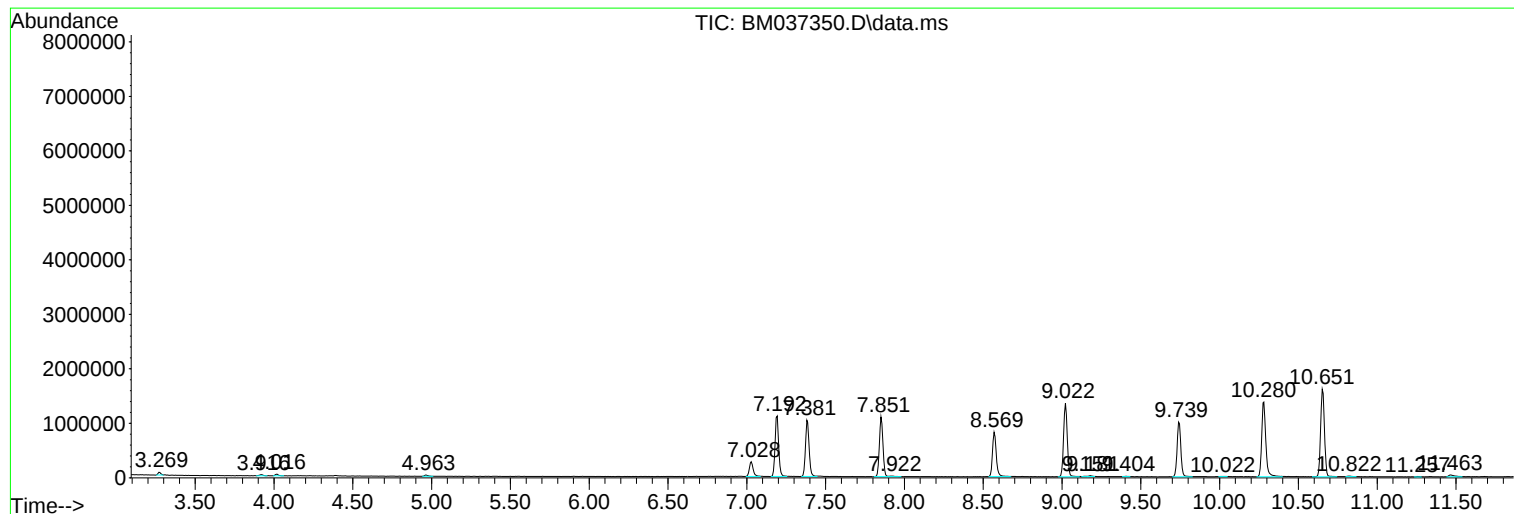

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037350.D
Acq On : 03 Nov 2022 17:16
Operator : CG/JU
Sample : N5276-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037350.D
Acq On : 03 Nov 2022 17:16
Operator : CG/JU
Sample : N5276-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc