

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037351.D
 Acq On : 03 Nov 2022 17:52
 Operator : CG/JU
 Sample : N5276-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	41	rVB	72468	101277	0.98%	0.116%
2	3.916	137	141	146	rVB	24784	36143	0.35%	0.041%
3	4.016	154	158	164	rBV	38496	57000	0.55%	0.065%
4	4.963	314	319	326	rBV	56772	82974	0.81%	0.095%
5	7.028	663	670	684	rVB	332005	558998	5.43%	0.641%
6	7.187	691	697	710	rBV	1209901	1947928	18.91%	2.234%
7	7.381	723	730	741	rBV	1189248	1874462	18.19%	2.150%
8	7.851	803	810	819	rBV	1179572	1834744	17.81%	2.105%
9	7.922	819	822	826	rVB4	8899	14562	0.14%	0.017%
10	8.410	900	905	913	rVB9	7657	13101	0.13%	0.015%
11	8.569	923	932	944	rBV	965791	1589192	15.43%	1.823%
12	9.022	1001	1009	1023	rBV	1498219	2403428	23.33%	2.757%
13	9.404	1070	1074	1082	rVB4	15690	23042	0.22%	0.026%
14	9.739	1123	1131	1145	rBV	1122694	1849615	17.95%	2.122%
15	10.280	1215	1223	1242	rBV	1555143	2777153	26.96%	3.186%
16	10.651	1279	1286	1295	rBV	1740689	2869669	27.85%	3.292%
17	10.810	1305	1313	1325	rBV	58677	135521	1.32%	0.155%
18	11.898	1490	1498	1502	rVB7	8350	17713	0.17%	0.020%
19	12.245	1552	1557	1566	rBV2	25051	46825	0.45%	0.054%
20	13.386	1747	1751	1757	rVB5	8829	12698	0.12%	0.015%
21	13.904	1831	1839	1854	rBV	3410492	4687018	45.49%	5.376%
22	14.010	1854	1857	1863	rVB8	8419	14951	0.15%	0.017%
23	14.180	1876	1886	1904	rBV	4109692	5919726	57.46%	6.790%
24	14.486	1931	1938	1946	rBV	2810306	4060733	39.42%	4.658%
25	14.563	1946	1951	1957	rBV4	20162	48472	0.47%	0.056%
26	14.710	1970	1976	1997	rBV	201392	461264	4.48%	0.529%
27	14.898	2005	2008	2020	rVV	10539	30161	0.29%	0.035%
28	15.233	2061	2065	2069	rBV	20897	33612	0.33%	0.039%
29	15.274	2069	2072	2076	rVV	19532	29217	0.28%	0.034%
30	15.327	2076	2081	2085	rVB5	10456	18457	0.18%	0.021%
31	15.480	2100	2107	2116	rBV	5773980	7785708	75.57%	8.931%
32	15.604	2122	2128	2142	rBV	1772747	2309865	22.42%	2.650%
33	15.715	2142	2147	2154	rVB3	27760	51125	0.50%	0.059%
34	16.492	2275	2279	2282	rBV4	11965	17304	0.17%	0.020%
35	16.633	2300	2303	2309	rBV8	6278	10964	0.11%	0.013%
36	17.015	2365	2368	2376	rBV7	7938	17679	0.17%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037351.D
 Acq On : 03 Nov 2022 17:52
 Operator : CG/JU
 Sample : N5276-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	17.227	2398	2404	2414	rBV	3577136	4739807	46.01%	5.437%
38	17.327	2414	2421	2437	rVV	6638725	8865001	86.05%	10.169%
39	17.892	2513	2517	2523	rVB2	33579	46857	0.45%	0.054%
40	18.121	2551	2556	2564	rBV	108293	179131	1.74%	0.205%
41	18.192	2566	2568	2573	rVB3	10972	12626	0.12%	0.014%
42	19.180	2732	2736	2741	rVB2	66872	93086	0.90%	0.107%
43	19.250	2744	2748	2751	rBV2	74104	100203	0.97%	0.115%
44	19.398	2769	2773	2779	rBV5	49792	82506	0.80%	0.095%
45	19.615	2804	2810	2822	rBV	8324731	10302343	100.00%	11.818%
46	21.109	3061	3064	3071	rBV3	186863	351180	3.41%	0.403%
47	21.397	3108	3113	3124	rBV	4050682	5261798	51.07%	6.036%
48	23.597	3480	3487	3497	rBV2	4776821	8904904	86.44%	10.215%
49	23.744	3506	3512	3523	rVB2	2269717	4495875	43.64%	5.157%




Sum of corrected areas: 87177618

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037351.D
Acq On : 03 Nov 2022 17:52
Operator : CG/JU
Sample : N5276-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

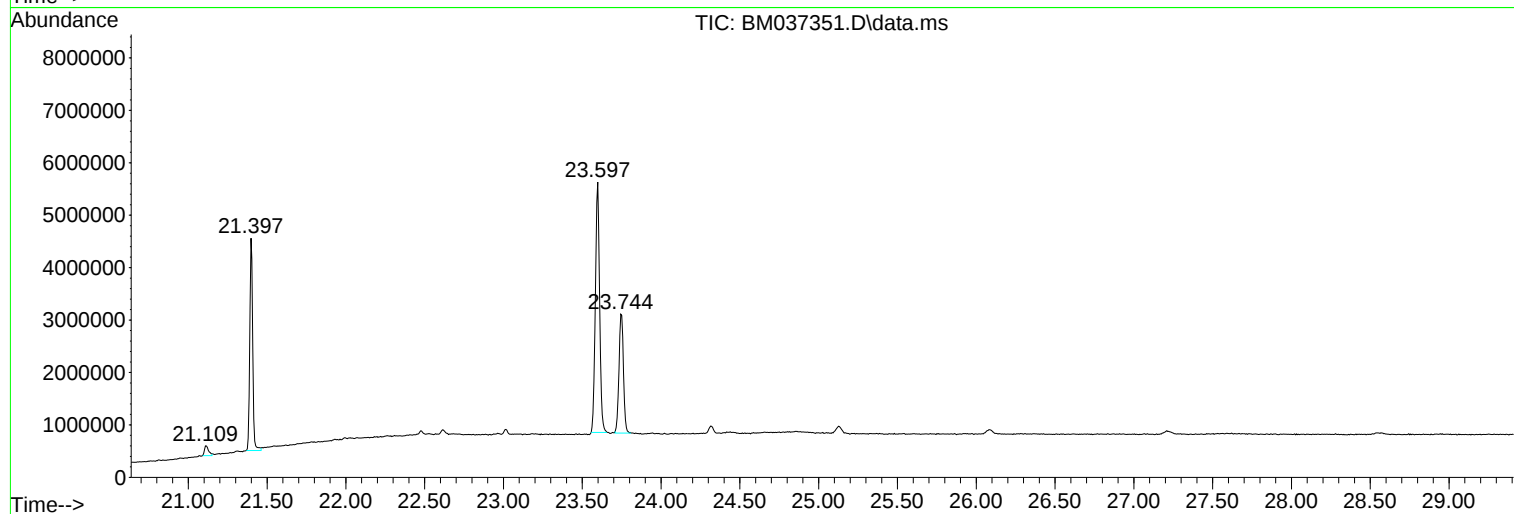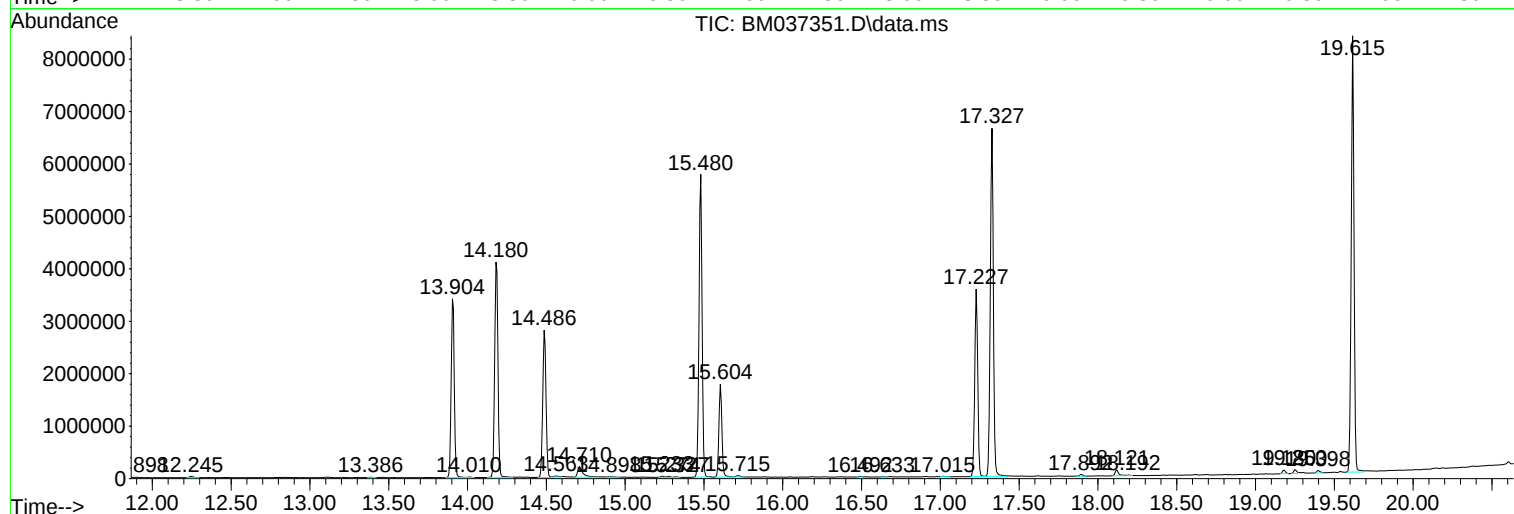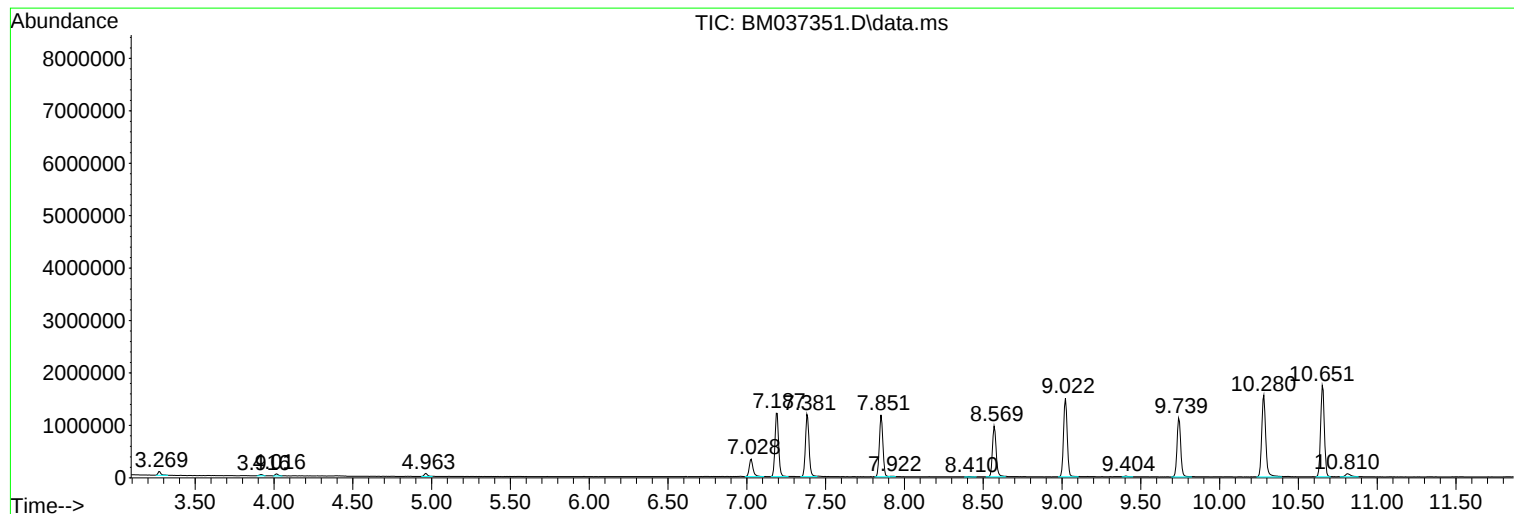

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037351.D
Acq On : 03 Nov 2022 17:52
Operator : CG/JU
Sample : N5276-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037351.D
Acq On : 03 Nov 2022 17:52
Operator : CG/JU
Sample : N5276-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
