

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037353.D
 Acq On : 03 Nov 2022 19:04
 Operator : CG/JU
 Sample : N5276-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rBV	55812	68124	0.65%	0.077%
2	3.916	137	141	149	rVB	23818	38277	0.36%	0.044%
3	4.016	153	158	164	rBV	35746	54123	0.51%	0.062%
4	4.963	316	319	328	rVB	20256	28760	0.27%	0.033%
5	7.028	663	670	684	rVB	300981	516204	4.89%	0.587%
6	7.193	691	698	711	rBV	1110624	1770123	16.77%	2.013%
7	7.381	724	730	740	rBV	1060967	1705652	16.16%	1.940%
8	7.851	803	810	818	rBV	1240457	1926574	18.26%	2.191%
9	7.922	818	822	829	rVB4	13615	24302	0.23%	0.028%
10	8.569	925	932	945	rBV	888430	1473961	13.97%	1.677%
11	9.022	1001	1009	1019	rBV	1368234	2216735	21.01%	2.521%
12	9.739	1124	1131	1148	rBV	1072532	1729749	16.39%	1.968%
13	10.281	1215	1223	1240	rBV	1452094	2626447	24.89%	2.987%
14	10.651	1279	1286	1294	rBV	1846956	3033459	28.75%	3.450%
15	10.816	1305	1314	1323	rBV	54703	126661	1.20%	0.144%
16	12.004	1512	1516	1523	rBV2	15838	25823	0.24%	0.029%
17	12.245	1549	1557	1563	rBV2	25629	47622	0.45%	0.054%
18	12.316	1565	1569	1574	rBV6	7663	16438	0.16%	0.019%
19	13.457	1760	1763	1770	rVB4	7708	12376	0.12%	0.014%
20	13.904	1832	1839	1851	rBV	3433879	4590540	43.50%	5.222%
21	14.180	1879	1886	1902	rBV	4105516	5789579	54.86%	6.585%
22	14.286	1902	1904	1910	rVB7	5631	10747	0.10%	0.012%
23	14.486	1931	1938	1952	rBV	3125956	4382178	41.53%	4.985%
24	14.710	1970	1976	1987	rBV	203766	442343	4.19%	0.503%
25	15.274	2062	2072	2074	rBV4	10219	21183	0.20%	0.024%
26	15.310	2074	2078	2084	rVB3	16593	30333	0.29%	0.035%
27	15.480	2096	2107	2121	rBV	5579950	7716208	73.12%	8.777%
28	15.604	2121	2128	2141	rVV	1784861	2353695	22.30%	2.677%
29	15.715	2143	2147	2155	rVB3	27254	52913	0.50%	0.060%
30	16.351	2250	2255	2259	rBV6	6123	12050	0.11%	0.014%
31	16.633	2298	2303	2308	rBV9	5486	11670	0.11%	0.013%
32	16.733	2317	2320	2327	rBV2	15842	32234	0.31%	0.037%
33	16.904	2347	2349	2355	rVB7	10705	15000	0.14%	0.017%
34	17.015	2365	2368	2373	rVB5	8798	12332	0.12%	0.014%
35	17.227	2397	2404	2414	rBV	3750698	5166552	48.96%	5.877%
36	17.327	2414	2421	2435	rVV	6641935	9035310	85.62%	10.277%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037353.D
 Acq On : 03 Nov 2022 19:04
 Operator : CG/JU
 Sample : N5276-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	17.892	2514	2517	2523	rBV7	15190	19220	0.18%	0.022%
38	18.115	2551	2555	2563	rBV	76650	125534	1.19%	0.143%
39	18.968	2698	2700	2706	rVB5	16915	17539	0.17%	0.020%
40	19.180	2732	2736	2743	rVB	75681	104603	0.99%	0.119%
41	19.251	2744	2748	2752	rBV	71270	106662	1.01%	0.121%
42	19.392	2769	2772	2777	rBV2	60182	84528	0.80%	0.096%
43	19.615	2804	2810	2826	rBV	8215428	10552420	100.00%	12.003%
44	21.397	3108	3113	3120	rBV	4479908	5551158	52.61%	6.314%
45	23.591	3479	3486	3499	rVB	4659583	9295846	88.09%	10.574%
46	23.744	3506	3512	3523	rVB2	2618569	4941359	46.83%	5.621%




Sum of corrected areas: 87915146

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037353.D
Acq On : 03 Nov 2022 19:04
Operator : CG/JU
Sample : N5276-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

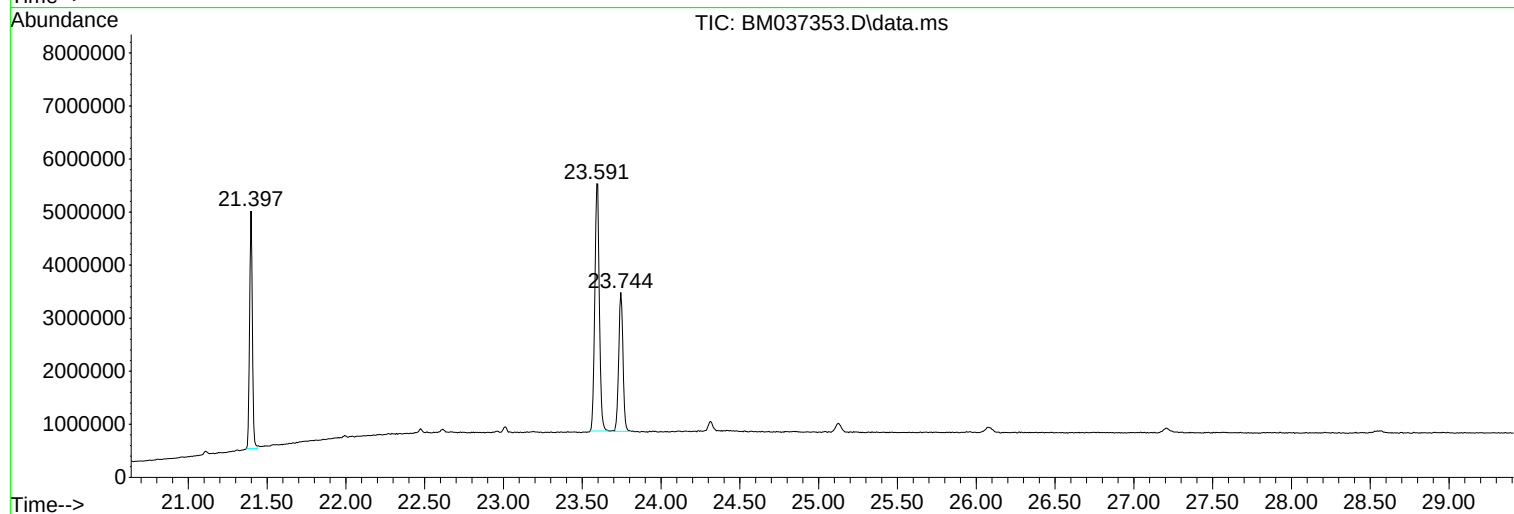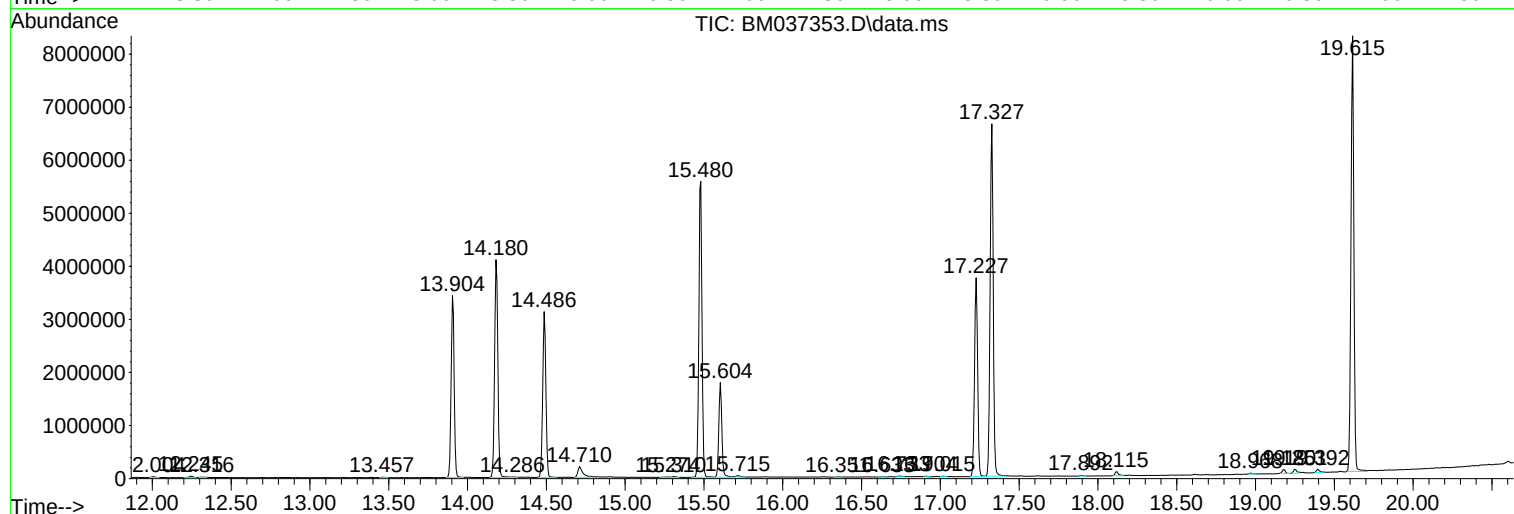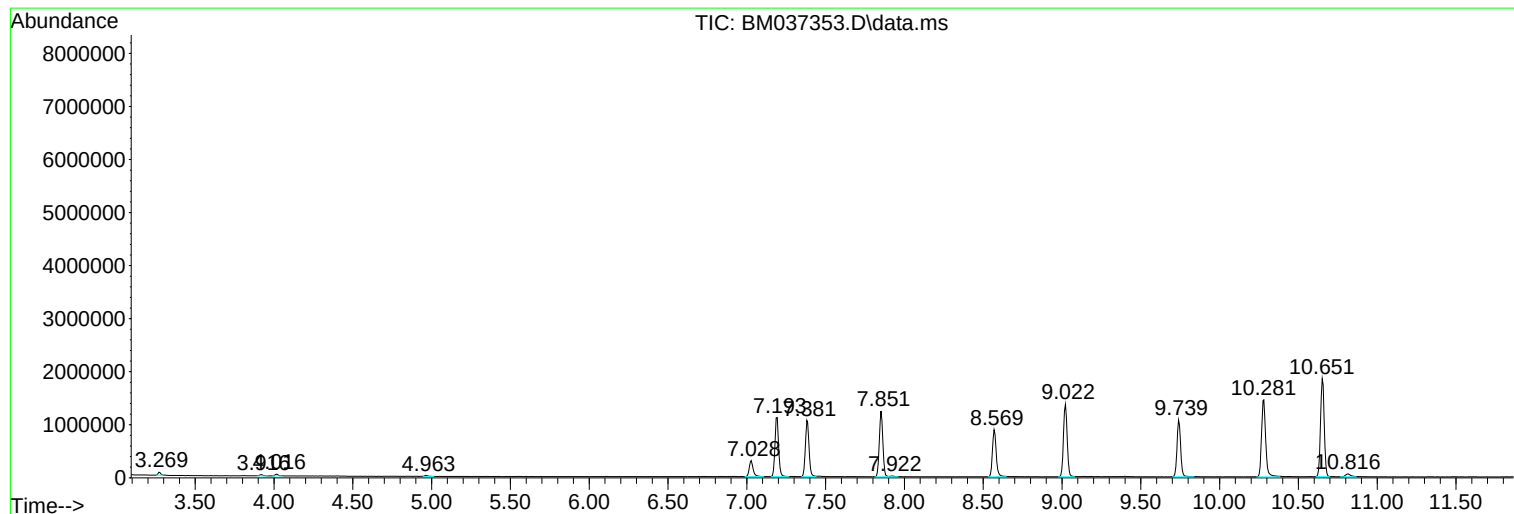

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037353.D
Acq On : 03 Nov 2022 19:04
Operator : CG/JU
Sample : N5276-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037353.D
Acq On : 03 Nov 2022 19:04
Operator : CG/JU
Sample : N5276-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
