

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037354.D
 Acq On : 03 Nov 2022 19:40
 Operator : CG/JU
 Sample : N5276-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	42	rVB	68839	96784	1.04%	0.114%
2	3.916	136	141	146	rVB	27302	42114	0.45%	0.049%
3	4.016	154	158	163	rBV	43188	58181	0.63%	0.068%
4	4.963	313	319	325	rBV	32678	52013	0.56%	0.061%
5	7.028	663	670	682	rBV	359896	604116	6.52%	0.709%
6	7.187	691	697	711	rBV	1433213	2232692	24.10%	2.621%
7	7.381	723	730	740	rBV	1386875	2145258	23.15%	2.518%
8	7.851	803	810	819	rBV	1281237	1967492	21.23%	2.310%
9	8.569	924	932	946	rBV	1088486	1759454	18.99%	2.065%
10	9.022	1001	1009	1025	rBV	1733272	2772957	29.93%	3.255%
11	9.398	1069	1073	1078	rVB7	7843	13376	0.14%	0.016%
12	9.739	1124	1131	1144	rBV	1359476	2179849	23.53%	2.559%
13	10.275	1214	1222	1246	rBV	1820602	3220657	34.76%	3.781%
14	10.451	1246	1252	1262	rVV4	16396	47002	0.51%	0.055%
15	10.651	1279	1286	1294	rBV	1866838	2999777	32.38%	3.522%
16	10.810	1307	1313	1323	rBV2	31997	70138	0.76%	0.082%
17	11.898	1494	1498	1503	rVB8	5647	9478	0.10%	0.011%
18	12.010	1512	1517	1522	rVB4	8746	16385	0.18%	0.019%
19	12.245	1550	1557	1562	rBV	31615	59939	0.65%	0.070%
20	12.304	1562	1567	1583	rVV	52234	147000	1.59%	0.173%
21	12.445	1587	1591	1597	rVB9	4074	10153	0.11%	0.012%
22	12.780	1642	1648	1652	rBV6	5797	11830	0.13%	0.014%
23	13.304	1730	1737	1740	rBV9	3706	9581	0.10%	0.011%
24	13.380	1746	1750	1757	rVB6	9414	15380	0.17%	0.018%
25	13.463	1757	1764	1767	rBV4	7548	12865	0.14%	0.015%
26	13.904	1831	1839	1851	rBV	3825504	5122504	55.29%	6.014%
27	14.010	1854	1857	1863	rVB8	9952	14949	0.16%	0.018%
28	14.180	1879	1886	1903	rBV	4670770	6645870	71.73%	7.802%
29	14.357	1913	1916	1923	rVB9	5733	11159	0.12%	0.013%
30	14.486	1931	1938	1948	rBV	2906795	4137088	44.65%	4.857%
31	14.710	1971	1976	1990	rBV	189552	419502	4.53%	0.492%
32	15.274	2068	2072	2074	rBV2	10401	13357	0.14%	0.016%
33	15.310	2074	2078	2084	rVB	114215	155350	1.68%	0.182%
34	15.474	2093	2106	2121	rBV	5987571	8420118	90.88%	9.885%
35	15.604	2122	2128	2141	rVV	1669942	2329823	25.15%	2.735%
36	15.715	2143	2147	2151	rVB3	28050	40351	0.44%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037354.D
 Acq On : 03 Nov 2022 19:40
 Operator : CG/JU
 Sample : N5276-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	16.180	2222	2226	2230	rBV7	8106	13753	0.15%	0.016%
38	16.257	2235	2239	2242	rVV6	8314	10023	0.11%	0.012%
39	16.733	2315	2320	2333	rBV	88015	197527	2.13%	0.232%
40	16.974	2358	2361	2365	rBV6	10006	14764	0.16%	0.017%
41	17.227	2397	2404	2414	rBV	3353861	4501742	48.59%	5.285%
42	17.327	2414	2421	2432	rBV	6302570	8718618	94.10%	10.235%
43	17.615	2466	2470	2474	rBV5	11409	21705	0.23%	0.025%
44	17.892	2514	2517	2521	rBV5	10924	13824	0.15%	0.016%
45	18.115	2551	2555	2561	rBV2	74643	116243	1.25%	0.136%
46	19.180	2732	2736	2741	rVB	66625	89162	0.96%	0.105%
47	19.250	2744	2748	2752	rBV	70841	98381	1.06%	0.115%
48	19.392	2769	2772	2777	rBV3	57068	84208	0.91%	0.099%
49	19.615	2804	2810	2825	rBV	7083291	9265394	100.00%	10.877%
50	21.397	3108	3113	3121	rBV	3160586	3867032	41.74%	4.540%
51	23.591	3479	3486	3496	rVB2	3575277	6922790	74.72%	8.127%
52	23.744	3506	3512	3525	rVB	1748525	3383646	36.52%	3.972%




Sum of corrected areas: 85183354

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037354.D
Acq On : 03 Nov 2022 19:40
Operator : CG/JU
Sample : N5276-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

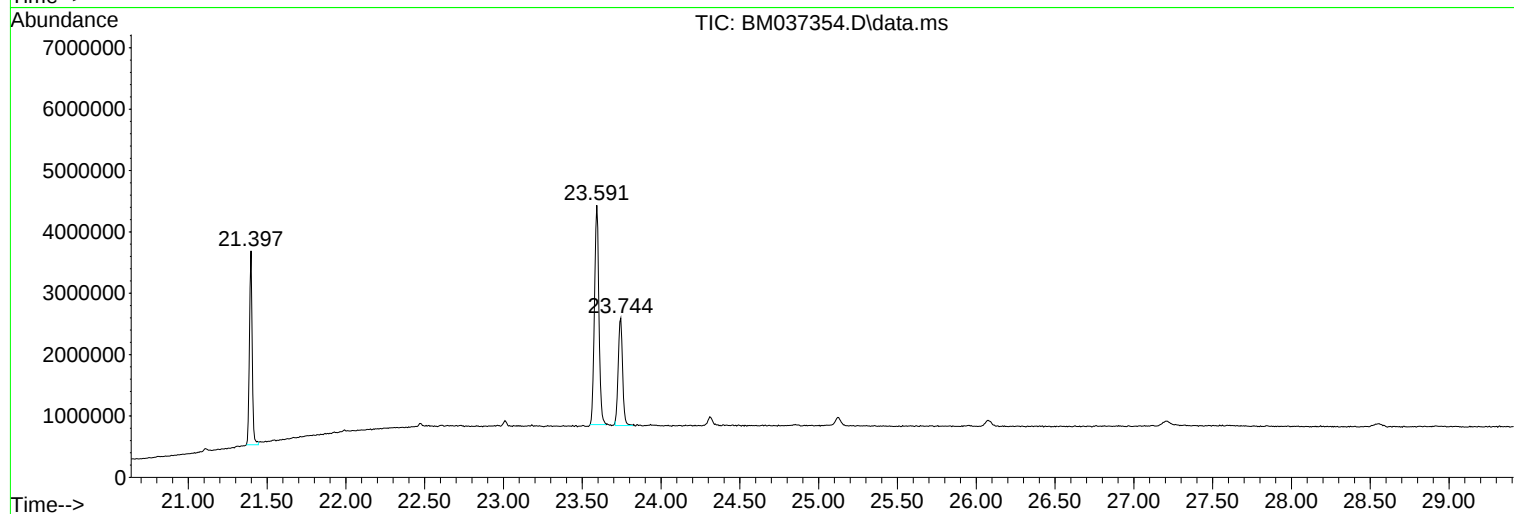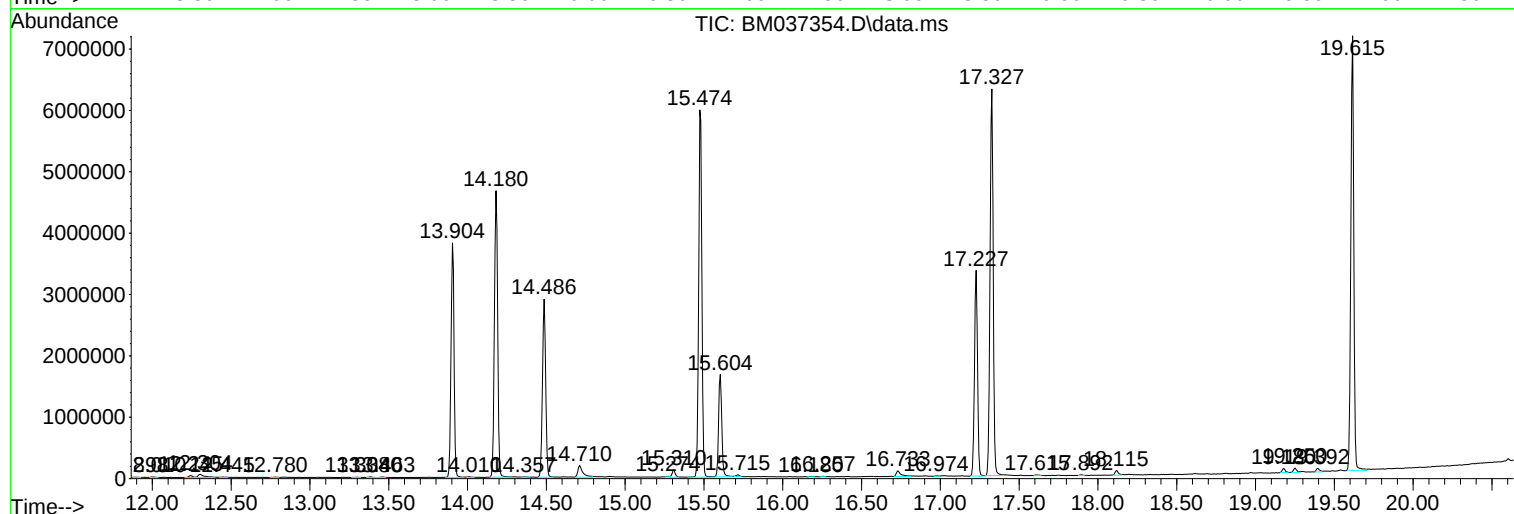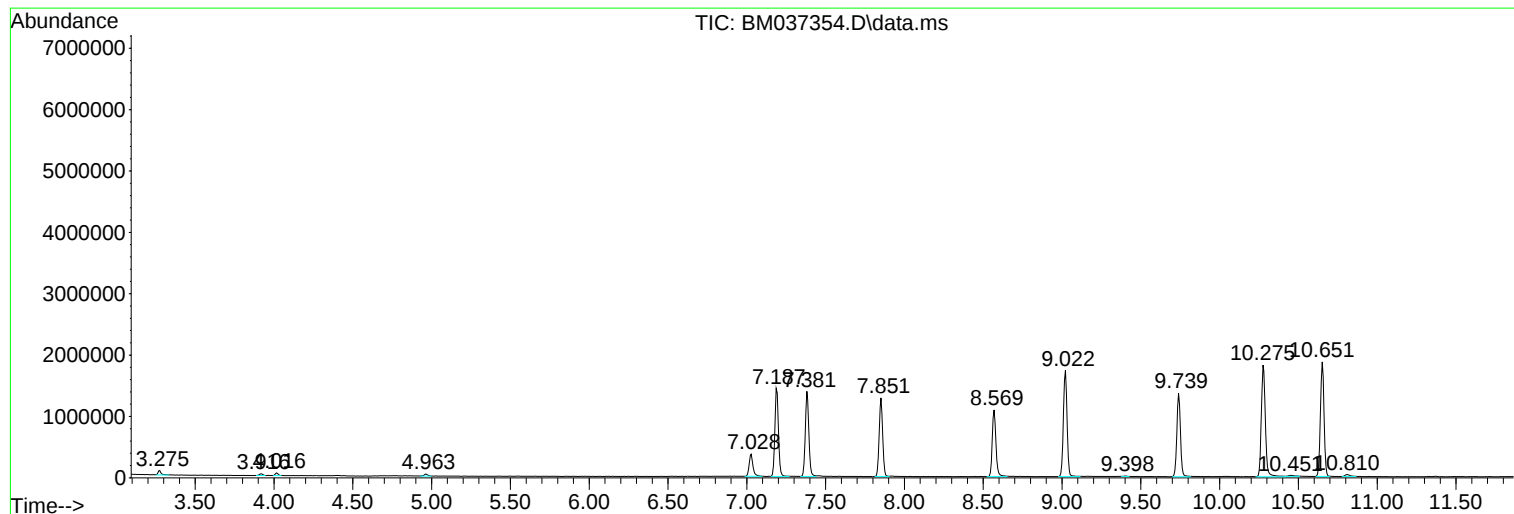

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037354.D
Acq On : 03 Nov 2022 19:40
Operator : CG/JU
Sample : N5276-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037354.D
Acq On : 03 Nov 2022 19:40
Operator : CG/JU
Sample : N5276-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc